

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030528.D
 Acq On : 09 Aug 2022 15:36
 Operator : JC/MD
 Sample : N4110-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	100657	105168	11.39%	1.349%
2	1.666	91	95	105	rVB	89267	108791	11.78%	1.395%
3	2.307	194	200	209	rVB	163316	258632	28.01%	3.317%
4	2.508	231	233	235	rBV2	588	568	0.06%	0.007%
5	2.624	250	252	253	rVB	898	483	0.05%	0.006%
6	2.666	257	259	264	rBV3	605	930	0.10%	0.012%
7	2.788	275	279	283	rBV2	1976	2947	0.32%	0.038%
8	2.867	288	292	295	rVB2	378	491	0.05%	0.006%
9	2.953	302	306	308	rBV3	579	826	0.09%	0.011%
10	3.050	320	322	325	rBV2	548	543	0.06%	0.007%
11	3.197	343	346	349	rBV2	416	608	0.07%	0.008%
12	3.337	368	369	372	rBV2	805	684	0.07%	0.009%
13	3.440	382	386	389	rBV2	657	1018	0.11%	0.013%
14	3.520	397	399	404	rBV	410	827	0.09%	0.011%
15	3.751	434	437	439	rBV2	457	464	0.05%	0.006%
16	3.928	461	466	467	rBV3	390	501	0.05%	0.006%
17	4.160	500	504	505	rBV2	383	474	0.05%	0.006%
18	4.471	547	555	569	rBV	89933	267785	29.00%	3.434%
19	4.702	591	593	594	rBV	957	561	0.06%	0.007%
20	5.062	639	652	673	rBV	120662	396599	42.96%	5.086%
21	5.257	682	684	688	rVB	653	725	0.08%	0.009%
22	5.452	715	716	720	rVB3	614	493	0.05%	0.006%
23	5.562	724	734	741	rBV8	2938	8491	0.92%	0.109%
24	5.702	755	757	760	rVB2	464	532	0.06%	0.007%
25	5.977	790	802	819	rBV2	323210	923256	100.00%	11.840%
26	6.294	851	854	855	rBV2	464	537	0.06%	0.007%
27	6.355	860	864	866	rBV2	709	943	0.10%	0.012%
28	6.538	891	894	900	rBV3	688	1173	0.13%	0.015%
29	6.769	922	932	944	rBV	301095	719454	77.93%	9.226%
30	6.946	957	961	965	rBV2	533	775	0.08%	0.010%
31	7.117	981	989	1000	rVB5	11390	27551	2.98%	0.353%
32	7.312	1013	1021	1034	rBV	199975	432356	46.83%	5.545%
33	7.927	1117	1122	1123	rBV3	463	725	0.08%	0.009%
34	8.080	1144	1147	1150	rVB	585	862	0.09%	0.011%
35	8.330	1180	1188	1199	rBV	132727	215697	23.36%	2.766%
36	8.482	1210	1213	1216	rVV3	606	956	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030528.D
 Acq On : 09 Aug 2022 15:36
 Operator : JC/MD
 Sample : N4110-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.586	1225	1230	1234	rBV3	2799	4518	0.49%	0.058%
38	8.653	1234	1241	1250	rBV	459164	708105	76.70%	9.081%
39	8.799	1263	1265	1267	rBV2	513	560	0.06%	0.007%
40	8.952	1284	1290	1303	rBV	95754	146551	15.87%	1.879%
41	9.092	1312	1313	1318	rVB4	583	483	0.05%	0.006%
42	9.196	1328	1330	1334	rBV	437	718	0.08%	0.009%
43	9.281	1339	1344	1347	rBV3	1704	2441	0.26%	0.031%
44	9.342	1352	1354	1356	rBV2	514	621	0.07%	0.008%
45	9.391	1356	1362	1379	rBV	411370	584680	63.33%	7.498%
46	9.525	1379	1384	1391	rVV2	20458	30918	3.35%	0.396%
47	9.586	1391	1394	1399	rVB2	4397	6785	0.73%	0.087%
48	9.659	1404	1406	1410	rVB2	598	567	0.06%	0.007%
49	9.732	1416	1418	1422	rBV	584	766	0.08%	0.010%
50	10.055	1465	1471	1481	rBV	612622	847953	91.84%	10.874%
51	10.269	1505	1506	1509	rBV2	437	540	0.06%	0.007%
52	10.378	1521	1524	1525	rBV2	642	654	0.07%	0.008%
53	10.647	1563	1568	1576	rBV	15089	21091	2.28%	0.270%
54	10.768	1583	1588	1594	rBV4	2977	5697	0.62%	0.073%
55	10.860	1600	1603	1608	rVV4	3812	4514	0.49%	0.058%
56	10.994	1624	1625	1627	rBV	733	536	0.06%	0.007%
57	11.018	1627	1629	1630	rBV2	672	554	0.06%	0.007%
58	11.037	1630	1632	1635	rVB2	1396	1190	0.13%	0.015%
59	11.073	1635	1638	1639	rBV2	609	671	0.07%	0.009%
60	11.140	1645	1649	1652	rVB3	612	846	0.09%	0.011%
61	11.195	1652	1658	1666	rBV	359488	455187	49.30%	5.837%
62	11.299	1673	1675	1677	rBV2	597	515	0.06%	0.007%
63	11.415	1690	1694	1695	rBV2	587	641	0.07%	0.008%
64	11.628	1727	1729	1732	rVV3	776	645	0.07%	0.008%
65	11.689	1738	1739	1742	rVB	750	526	0.06%	0.007%
66	11.732	1744	1746	1748	rBV2	469	554	0.06%	0.007%
67	11.756	1748	1750	1758	rVB3	2186	3534	0.38%	0.045%
68	11.933	1775	1779	1784	rVB2	3863	4511	0.49%	0.058%
69	11.976	1784	1786	1788	rVB2	1106	887	0.10%	0.011%
70	12.024	1789	1794	1802	rBV	636707	765748	82.94%	9.820%
71	12.219	1822	1826	1837	rBV2	14730	27750	3.01%	0.356%
72	12.323	1837	1843	1852	rVV	508719	626930	67.90%	8.040%
73	12.524	1872	1876	1877	rBV3	655	802	0.09%	0.010%
74	12.597	1884	1888	1892	rVB4	3390	5299	0.57%	0.068%
75	12.732	1908	1910	1913	rVB2	738	592	0.06%	0.008%
76	12.774	1913	1917	1921	rBV3	838	1573	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030528.D
 Acq On : 09 Aug 2022 15:36
 Operator : JC/MD
 Sample : N4110-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.817	1921	1924	1927	rBV3	1774	2454	0.27%	0.031%
78	12.860	1927	1931	1935	rVB2	8708	10846	1.17%	0.139%
79	13.073	1964	1966	1968	rBV2	551	538	0.06%	0.007%
80	13.103	1968	1971	1975	rBV3	928	1596	0.17%	0.020%
81	13.366	2011	2014	2019	rBV2	461	759	0.08%	0.010%
82	13.420	2020	2023	2025	rBV	808	653	0.07%	0.008%
83	13.469	2027	2031	2035	rVB3	1997	2788	0.30%	0.036%
84	13.585	2047	2050	2051	rBV2	1081	1273	0.14%	0.016%
85	13.756	2072	2078	2089	rBV7	6117	13164	1.43%	0.169%
86	13.908	2101	2103	2104	rBV2	812	565	0.06%	0.007%
87	13.945	2108	2109	2112	rBV2	664	564	0.06%	0.007%
88	14.122	2136	2138	2142	rVV2	528	565	0.06%	0.007%
89	14.256	2157	2160	2164	rVB3	1250	1729	0.19%	0.022%
90	14.536	2205	2206	2210	rVB2	499	528	0.06%	0.007%
91	14.585	2210	2214	2215	rBV	580	570	0.06%	0.007%
92	14.688	2229	2231	2233	rBV3	634	632	0.07%	0.008%
93	14.719	2233	2236	2240	rBV4	1520	2294	0.25%	0.029%
94	14.926	2269	2270	2273	rBV2	749	489	0.05%	0.006%
95	14.999	2279	2282	2286	rBV4	1119	1566	0.17%	0.020%
96	15.085	2295	2296	2298	rBV2	760	691	0.07%	0.009%
97	15.188	2311	2313	2314	rBV	818	548	0.06%	0.007%
98	15.335	2335	2337	2339	rBV	701	515	0.06%	0.007%
99	15.841	2418	2420	2423	rVB2	691	511	0.06%	0.007%
100	16.078	2458	2459	2462	rBV2	864	831	0.09%	0.011%


Sum of corrected areas: 7797748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030528.D
Acq On : 09 Aug 2022 15:36
Operator : JC/MD
Sample : N4110-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

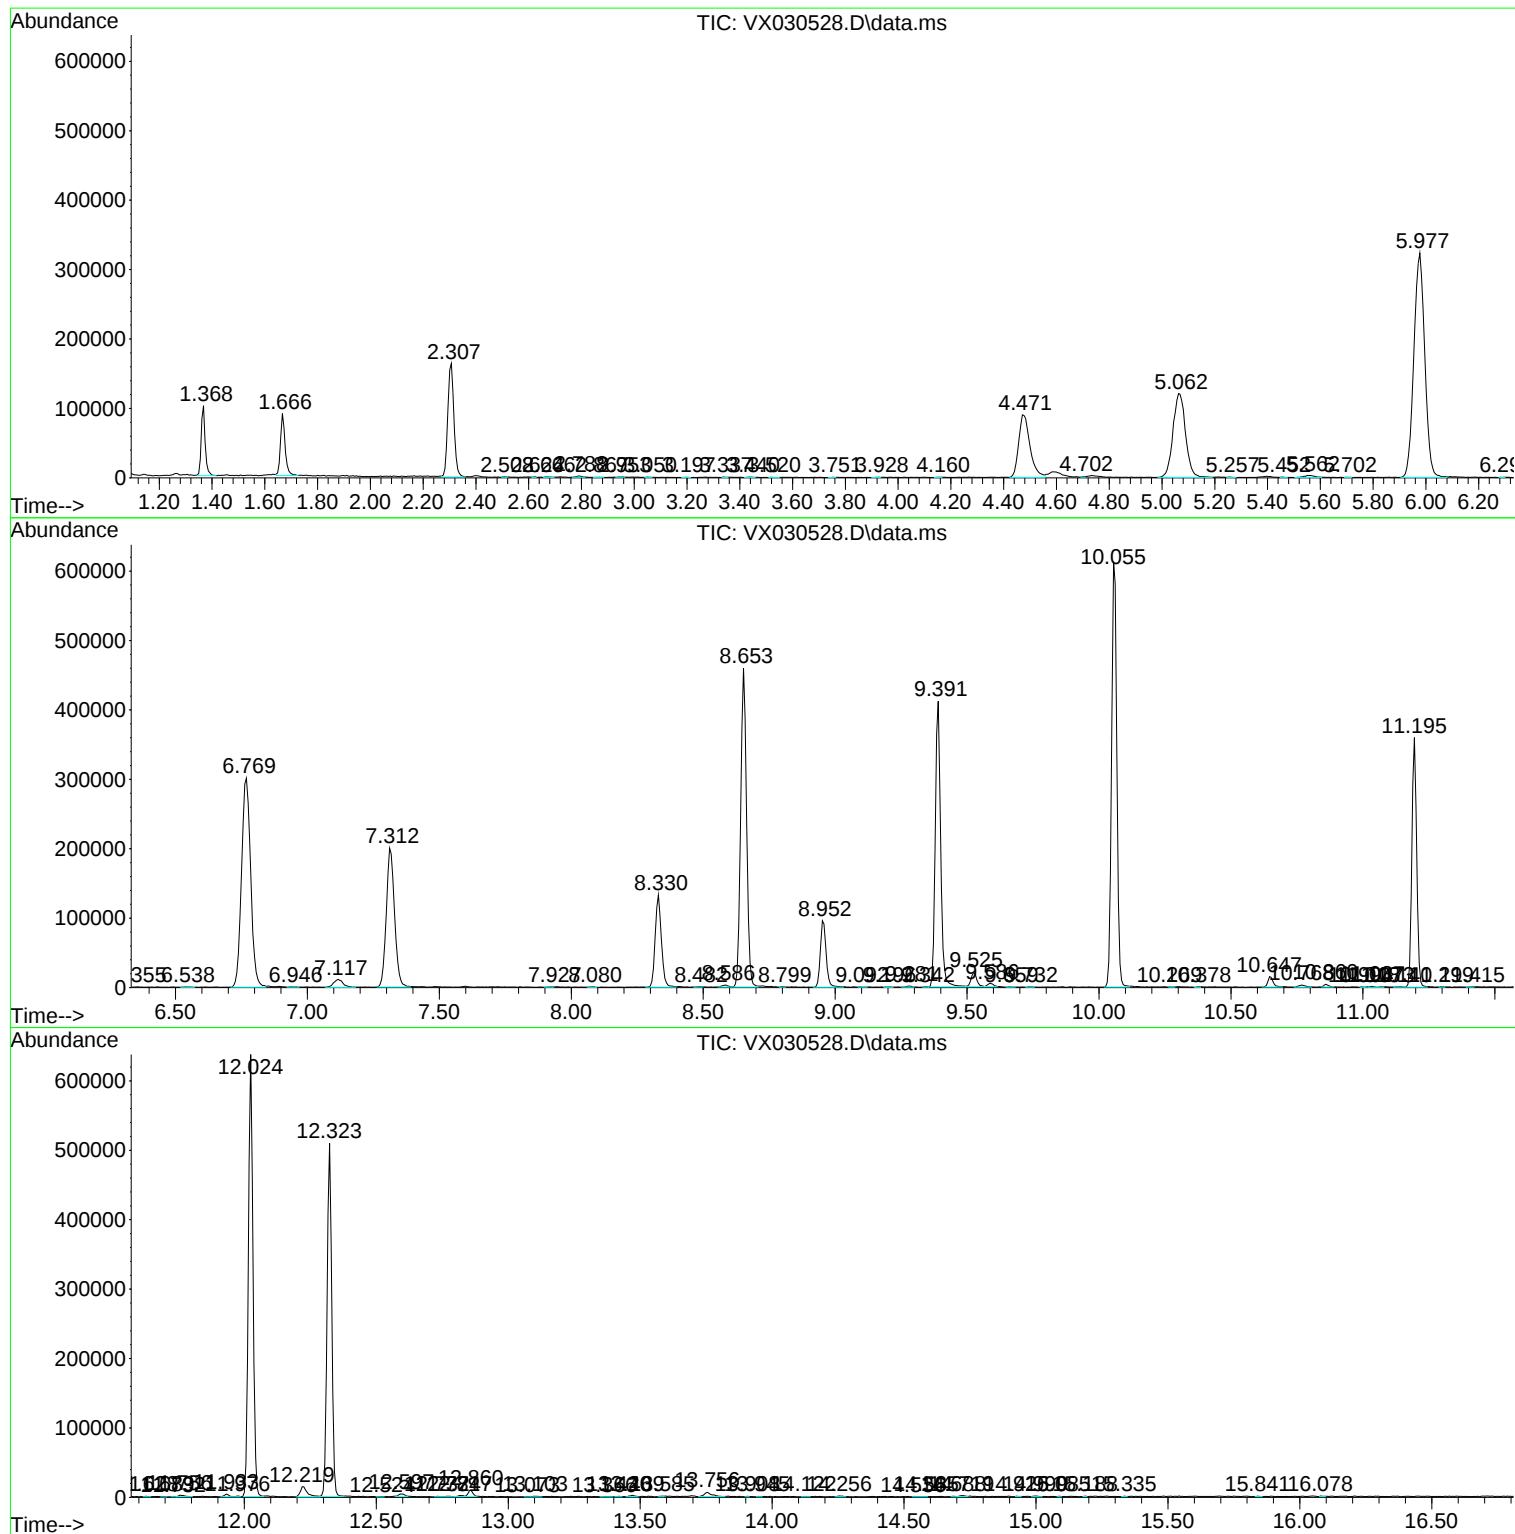

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030528.D
Acq On : 09 Aug 2022 15:36
Operator : JC/MD
Sample : N4110-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030528.D
Acq On : 09 Aug 2022 15:36
Operator : JC/MD
Sample : N4110-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc