

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030529.D
 Acq On : 09 Aug 2022 15:59
 Operator : JC/MD
 Sample : N4114-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	197737	216182	14.83%	2.380%
2	1.666	91	95	104	rVB	86474	104868	7.19%	1.154%
3	2.306	193	200	209	rVB	174506	263379	18.06%	2.899%
4	2.855	288	290	293	rBV2	421	442	0.03%	0.005%
5	2.965	305	308	311	rVB2	520	450	0.03%	0.005%
6	2.989	311	312	314	rBV	427	360	0.02%	0.004%
7	3.050	320	322	324	rBV2	472	542	0.04%	0.006%
8	3.093	324	329	337	rVB	9941	18277	1.25%	0.201%
9	3.154	337	339	341	rBV	323	326	0.02%	0.004%
10	3.300	360	363	365	rBV2	420	529	0.04%	0.006%
11	3.343	369	370	372	rVB2	520	356	0.02%	0.004%
12	3.373	372	375	378	rBV2	519	871	0.06%	0.010%
13	3.562	405	406	412	rVB2	640	938	0.06%	0.010%
14	3.642	417	419	422	rVV	324	328	0.02%	0.004%
15	3.977	472	474	478	rBV2	467	403	0.03%	0.004%
16	4.026	478	482	483	rVB2	407	397	0.03%	0.004%
17	4.117	494	497	500	rBV2	497	736	0.05%	0.008%
18	4.196	508	510	511	rBV	592	379	0.03%	0.004%
19	4.489	546	558	575	rBV2	497306	1458194	100.00%	16.050%
20	4.794	606	608	611	rVB2	445	409	0.03%	0.005%
21	4.830	612	614	617	rVV	443	497	0.03%	0.005%
22	5.068	641	653	670	rBV	125671	384508	26.37%	4.232%
23	5.306	690	692	695	rBV2	411	525	0.04%	0.006%
24	5.367	699	702	703	rBV3	683	825	0.06%	0.009%
25	5.385	703	705	706	rBV2	944	874	0.06%	0.010%
26	5.568	727	735	747	rBV4	2520	7096	0.49%	0.078%
27	5.702	754	757	758	rBV2	557	536	0.04%	0.006%
28	5.769	767	768	772	rVB2	459	470	0.03%	0.005%
29	5.812	772	775	778	rBV2	358	466	0.03%	0.005%
30	5.873	782	785	786	rVB2	429	374	0.03%	0.004%
31	5.891	786	788	789	rBV2	584	473	0.03%	0.005%
32	5.977	790	802	818	rBV2	311573	927466	63.60%	10.209%
33	6.269	848	850	853	rVV2	616	627	0.04%	0.007%
34	6.483	881	885	887	rBV	478	473	0.03%	0.005%
35	6.537	892	894	896	rBV2	371	331	0.02%	0.004%
36	6.635	908	910	912	rBV2	592	504	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030529.D
 Acq On : 09 Aug 2022 15:59
 Operator : JC/MD
 Sample : N4114-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.659	912	914	917	rVB	488	476	0.03%	0.005%
38	6.690	917	919	920	rBV	421	336	0.02%	0.004%
39	6.769	922	932	944	rBV	313226	728429	49.95%	8.018%
40	7.135	982	992	1002	rVB4	27686	72358	4.96%	0.796%
41	7.312	1013	1021	1037	rBV	190705	430572	29.53%	4.739%
42	7.488	1046	1050	1051	rBV2	734	765	0.05%	0.008%
43	7.513	1052	1054	1055	rVV	571	399	0.03%	0.004%
44	7.684	1079	1082	1083	rBV	279	331	0.02%	0.004%
45	7.757	1092	1094	1098	rVB2	388	372	0.03%	0.004%
46	7.848	1106	1109	1112	rBV2	282	432	0.03%	0.005%
47	8.049	1140	1142	1145	rBV	509	555	0.04%	0.006%
48	8.330	1182	1188	1200	rVV	133002	217286	14.90%	2.392%
49	8.580	1227	1229	1231	rVB	521	348	0.02%	0.004%
50	8.653	1234	1241	1257	rBV	458938	709298	48.64%	7.807%
51	8.836	1269	1271	1272	rBV	474	328	0.02%	0.004%
52	8.952	1285	1290	1301	rBV	92130	144795	9.93%	1.594%
53	9.275	1341	1343	1347	rVB3	1280	1539	0.11%	0.017%
54	9.391	1356	1362	1374	rBV	400547	569806	39.08%	6.272%
55	9.519	1381	1383	1387	rVB2	1022	1134	0.08%	0.012%
56	9.586	1391	1394	1395	rBV2	547	563	0.04%	0.006%
57	9.622	1398	1400	1405	rBV3	589	522	0.04%	0.006%
58	10.055	1466	1471	1482	rBV	605259	837613	57.44%	9.220%
59	10.238	1499	1501	1502	rBV	646	470	0.03%	0.005%
60	10.549	1550	1552	1555	rVB2	408	383	0.03%	0.004%
61	10.640	1566	1567	1569	rBV	566	388	0.03%	0.004%
62	10.866	1602	1604	1606	rVB2	437	375	0.03%	0.004%
63	11.092	1639	1641	1643	rVB2	756	407	0.03%	0.004%
64	11.195	1653	1658	1666	rBV	375236	474671	32.55%	5.225%
65	11.317	1676	1678	1680	rVV	583	447	0.03%	0.005%
66	11.390	1688	1690	1692	rBV	561	418	0.03%	0.005%
67	11.476	1703	1704	1709	rVB3	423	525	0.04%	0.006%
68	11.585	1720	1722	1725	rBV2	557	676	0.05%	0.007%
69	11.634	1729	1730	1732	rVB	706	330	0.02%	0.004%
70	11.860	1765	1767	1768	rBV2	390	324	0.02%	0.004%
71	11.902	1771	1774	1777	rBV	349	596	0.04%	0.007%
72	11.975	1784	1786	1789	rBV2	380	350	0.02%	0.004%
73	12.024	1789	1794	1802	rVV	648719	796121	54.60%	8.763%
74	12.323	1837	1843	1854	rBV	553234	682058	46.77%	7.507%
75	12.488	1868	1870	1871	rVB	598	410	0.03%	0.005%
76	12.756	1913	1914	1917	rBV2	440	489	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030529.D
 Acq On : 09 Aug 2022 15:59
 Operator : JC/MD
 Sample : N4114-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.853	1927	1930	1935	rBV4	778	1309	0.09%	0.014%
78	12.902	1935	1938	1940	rVV3	417	414	0.03%	0.005%
79	13.055	1961	1963	1967	rVB2	569	640	0.04%	0.007%
80	13.103	1967	1971	1972	rBV	537	534	0.04%	0.006%
81	13.122	1972	1974	1975	rBV	502	384	0.03%	0.004%
82	13.140	1975	1977	1979	rBV2	677	729	0.05%	0.008%
83	13.250	1994	1995	1999	rBV2	564	572	0.04%	0.006%
84	13.372	2013	2015	2018	rBV	836	640	0.04%	0.007%
85	13.402	2018	2020	2021	rBV2	604	412	0.03%	0.005%
86	13.591	2049	2051	2053	rBV	458	330	0.02%	0.004%
87	13.932	2105	2107	2108	rBV	1094	720	0.05%	0.008%
88	13.951	2108	2110	2112	rVV	467	512	0.04%	0.006%
89	14.103	2131	2135	2136	rBV2	463	554	0.04%	0.006%
90	14.176	2145	2147	2149	rVB2	522	321	0.02%	0.004%
91	14.262	2159	2161	2163	rBV	428	417	0.03%	0.005%
92	14.377	2178	2180	2184	rVB2	538	477	0.03%	0.005%
93	14.512	2200	2202	2204	rBV2	424	413	0.03%	0.005%
94	14.743	2239	2240	2241	rBV	522	320	0.02%	0.004%
95	14.865	2258	2260	2262	rBV2	530	401	0.03%	0.004%
96	14.896	2262	2265	2266	rBV2	561	659	0.05%	0.007%
97	15.066	2291	2293	2295	rVB2	720	398	0.03%	0.004%
98	15.487	2360	2362	2363	rBV	656	436	0.03%	0.005%
99	15.731	2400	2402	2404	rBV3	820	799	0.05%	0.009%
100	16.731	2564	2566	2568	rBV2	689	679	0.05%	0.007%




Sum of corrected areas: 9085176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030529.D
Acq On : 09 Aug 2022 15:59
Operator : JC/MD
Sample : N4114-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

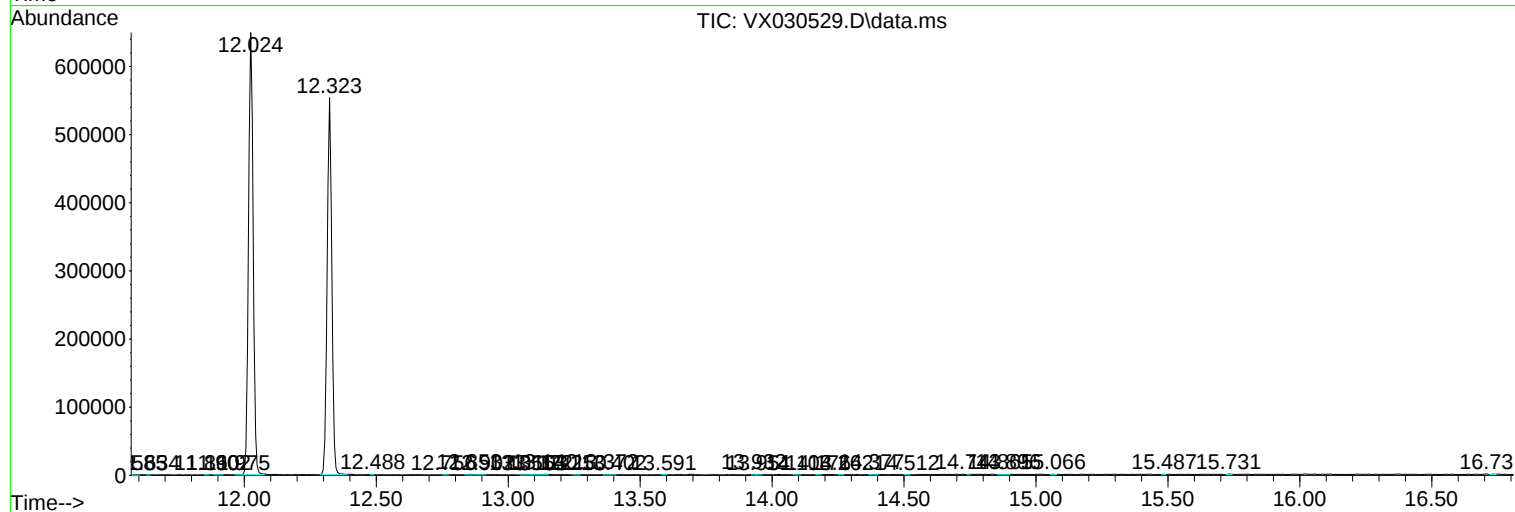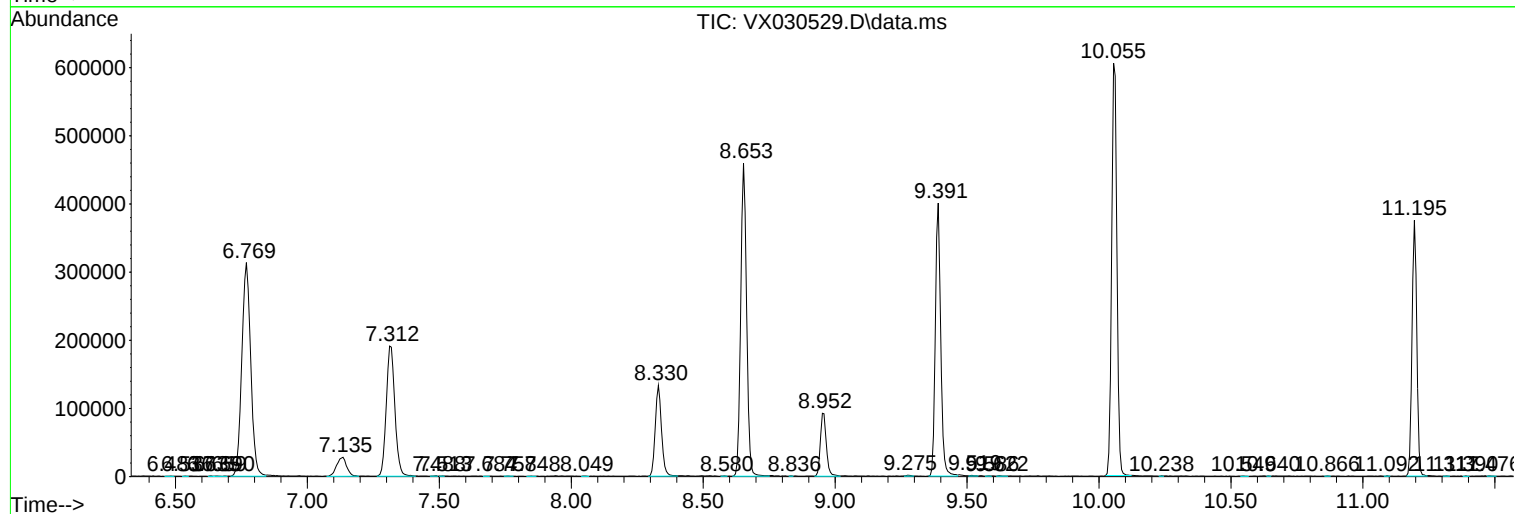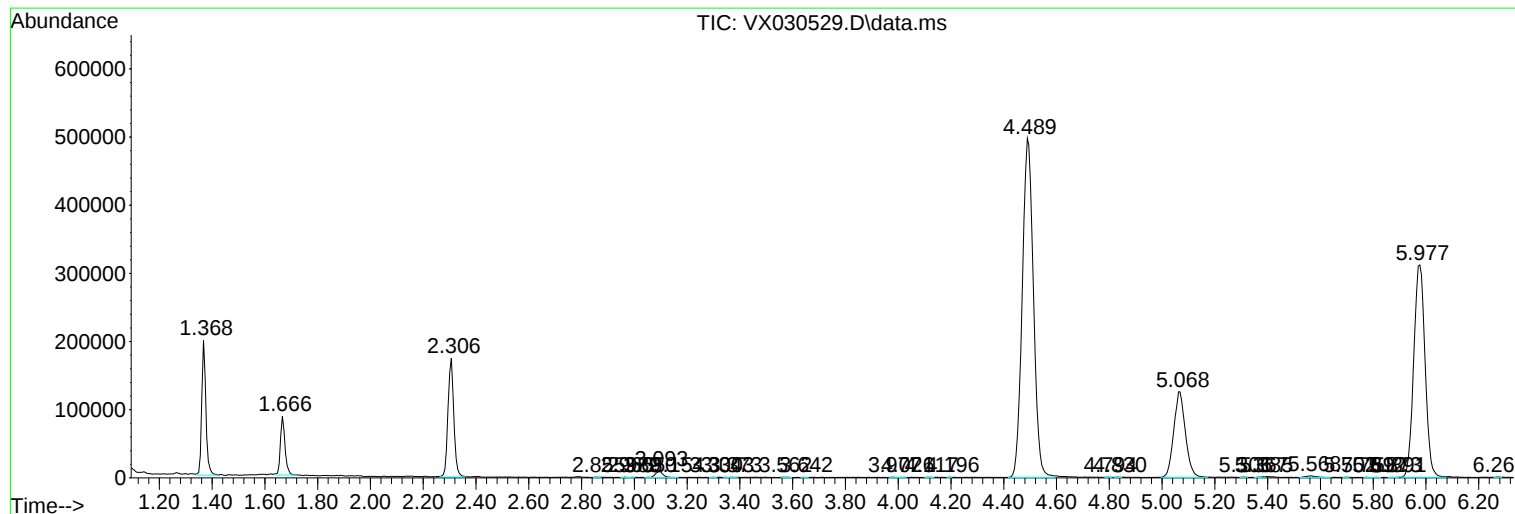

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030529.D
Acq On : 09 Aug 2022 15:59
Operator : JC/MD
Sample : N4114-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030529.D
Acq On : 09 Aug 2022 15:59
Operator : JC/MD
Sample : N4114-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc