

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030531.D
 Acq On : 09 Aug 2022 16:46
 Operator : JC/MD
 Sample : N4114-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB2	858510	982673	12.47%	3.995%
2	1.666	91	95	106	rVB2	85148	170077	2.16%	0.691%
3	2.313	194	201	211	rVB2	205474	386843	4.91%	1.573%
4	2.502	229	232	234	rBV3	660	724	0.01%	0.003%
5	2.648	255	256	260	rBV2	407	354	0.00%	0.001%
6	2.855	287	290	292	rBV2	754	885	0.01%	0.004%
7	2.953	302	306	309	rBV3	502	544	0.01%	0.002%
8	2.983	309	311	315	rVV3	349	399	0.01%	0.002%
9	3.099	322	330	341	rBV	49100	98044	1.24%	0.399%
10	3.440	385	386	391	rVB2	850	750	0.01%	0.003%
11	3.666	421	423	425	rVB	741	444	0.01%	0.002%
12	3.904	459	462	463	rVB2	362	376	0.00%	0.002%
13	3.959	470	471	474	rVB2	587	377	0.00%	0.002%
14	4.074	488	490	491	rBV	364	345	0.00%	0.001%
15	4.105	493	495	498	rBV2	299	449	0.01%	0.002%
16	4.160	502	504	507	rBV2	345	538	0.01%	0.002%
17	4.263	520	521	523	rVV2	435	381	0.00%	0.002%
18	4.288	523	525	530	rVV2	542	693	0.01%	0.003%
19	4.355	532	536	537	rBV2	540	642	0.01%	0.003%
20	4.501	546	560	577	rBV	2529519	6878066	87.28%	27.960%
21	4.928	628	630	634	rBV4	935	898	0.01%	0.004%
22	5.074	641	654	668	rBV	127942	395114	5.01%	1.606%
23	5.196	673	674	677	rVV2	534	474	0.01%	0.002%
24	5.227	677	679	681	rVV	576	451	0.01%	0.002%
25	5.251	681	683	686	rVB2	742	606	0.01%	0.002%
26	5.318	693	694	697	rBV2	486	449	0.01%	0.002%
27	5.464	716	718	719	rBV2	661	395	0.01%	0.002%
28	5.562	727	734	743	rBV6	2981	7822	0.10%	0.032%
29	5.757	764	766	769	rVB	499	422	0.01%	0.002%
30	5.977	789	802	821	rBV2	327178	952351	12.09%	3.871%
31	6.196	835	838	839	rBV2	428	339	0.00%	0.001%
32	6.257	846	848	851	rBV2	566	364	0.00%	0.001%
33	6.373	865	867	869	rVV2	948	714	0.01%	0.003%
34	6.403	869	872	874	rVV2	450	420	0.01%	0.002%
35	6.434	874	877	880	rVB2	424	676	0.01%	0.003%
36	6.464	880	882	885	rBV3	559	646	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030531.D
 Acq On : 09 Aug 2022 16:46
 Operator : JC/MD
 Sample : N4114-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.629	905	909	911	rBV2	397	556	0.01%	0.002%
38	6.769	923	932	945	rBV	295384	717174	9.10%	2.915%
39	6.958	960	963	968	rVB3	601	748	0.01%	0.003%
40	7.135	981	992	1013	rBV	3675002	7880018	100.00%	32.033%
41	7.318	1014	1022	1032	rVB	206189	432115	5.48%	1.757%
42	7.751	1090	1093	1096	rVB2	462	469	0.01%	0.002%
43	7.799	1099	1101	1104	rBV2	488	634	0.01%	0.003%
44	7.952	1122	1126	1129	rBV3	854	1185	0.02%	0.005%
45	8.031	1137	1139	1144	rVB3	335	554	0.01%	0.002%
46	8.080	1144	1147	1148	rBV	457	480	0.01%	0.002%
47	8.330	1181	1188	1199	rBV	132722	219225	2.78%	0.891%
48	8.494	1211	1215	1217	rBV3	883	1028	0.01%	0.004%
49	8.653	1235	1241	1251	rBV	456608	715290	9.08%	2.908%
50	8.818	1266	1268	1269	rBV2	495	449	0.01%	0.002%
51	8.958	1285	1291	1300	rBV	96875	145090	1.84%	0.590%
52	9.061	1307	1308	1312	rVB2	866	710	0.01%	0.003%
53	9.116	1315	1317	1321	rVB2	592	471	0.01%	0.002%
54	9.153	1321	1323	1328	rBV3	605	1040	0.01%	0.004%
55	9.281	1337	1344	1355	rBV	818737	1226285	15.56%	4.985%
56	9.391	1356	1362	1375	rBV	425203	586656	7.44%	2.385%
57	9.531	1384	1385	1387	rBV2	734	618	0.01%	0.003%
58	9.702	1410	1413	1415	rBV2	809	902	0.01%	0.004%
59	9.866	1438	1440	1444	rBV3	590	669	0.01%	0.003%
60	9.921	1447	1449	1452	rBV3	724	734	0.01%	0.003%
61	9.982	1457	1459	1462	rBV2	459	526	0.01%	0.002%
62	10.061	1466	1472	1479	rBV	575207	806278	10.23%	3.278%
63	10.317	1513	1514	1517	rBV2	638	425	0.01%	0.002%
64	10.366	1520	1522	1524	rVB	588	345	0.00%	0.001%
65	10.390	1524	1526	1528	rBV2	504	391	0.00%	0.002%
66	10.653	1567	1569	1573	rBV3	402	534	0.01%	0.002%
67	10.720	1578	1580	1582	rVB2	618	400	0.01%	0.002%
68	10.854	1601	1602	1607	rBV3	607	697	0.01%	0.003%
69	11.006	1624	1627	1628	rBV2	390	393	0.00%	0.002%
70	11.085	1638	1640	1642	rBV2	749	710	0.01%	0.003%
71	11.195	1653	1658	1670	rBV	383245	473020	6.00%	1.923%
72	11.433	1694	1697	1698	rBV	324	357	0.00%	0.001%
73	11.457	1699	1701	1705	rVB2	510	744	0.01%	0.003%
74	11.616	1725	1727	1732	rVB4	521	579	0.01%	0.002%
75	11.658	1732	1734	1736	rVB2	463	392	0.00%	0.002%
76	11.683	1736	1738	1741	rBV	547	635	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030531.D
 Acq On : 09 Aug 2022 16:46
 Operator : JC/MD
 Sample : N4114-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.969	1784	1785	1788	rBV3	814	578	0.01%	0.002%
78	12.024	1789	1794	1805	rVV	645342	793423	10.07%	3.225%
79	12.152	1814	1815	1823	rVB3	812	918	0.01%	0.004%
80	12.225	1824	1827	1831	rVB3	700	998	0.01%	0.004%
81	12.262	1831	1833	1836	rBV3	341	365	0.00%	0.001%
82	12.323	1838	1843	1851	rVB	552535	687329	8.72%	2.794%
83	12.408	1856	1857	1858	rBV	730	385	0.00%	0.002%
84	12.500	1870	1872	1874	rBV	499	443	0.01%	0.002%
85	12.567	1881	1883	1886	rVB3	560	465	0.01%	0.002%
86	13.030	1954	1959	1961	rBV	614	904	0.01%	0.004%
87	13.134	1974	1976	1978	rBV2	677	660	0.01%	0.003%
88	13.335	2007	2009	2012	rBV3	496	786	0.01%	0.003%
89	13.506	2034	2037	2041	rBV2	460	756	0.01%	0.003%
90	13.689	2064	2067	2070	rBV3	656	705	0.01%	0.003%
91	13.774	2079	2081	2085	rBB2	554	654	0.01%	0.003%
92	14.054	2125	2127	2130	rVB2	408	346	0.00%	0.001%
93	14.091	2130	2133	2134	rBV2	657	643	0.01%	0.003%
94	14.164	2143	2145	2148	rVB3	534	413	0.01%	0.002%
95	14.445	2190	2191	2194	rBV2	448	514	0.01%	0.002%
96	14.469	2194	2195	2197	rVB	763	392	0.00%	0.002%
97	14.493	2197	2199	2200	rBV2	608	474	0.01%	0.002%
98	14.731	2236	2238	2240	rBV2	623	610	0.01%	0.002%
99	14.914	2266	2268	2271	rBV2	543	508	0.01%	0.002%
100	15.274	2325	2327	2330	rVB2	962	888	0.01%	0.004%




Sum of corrected areas: 24599428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030531.D
Acq On : 09 Aug 2022 16:46
Operator : JC/MD
Sample : N4114-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

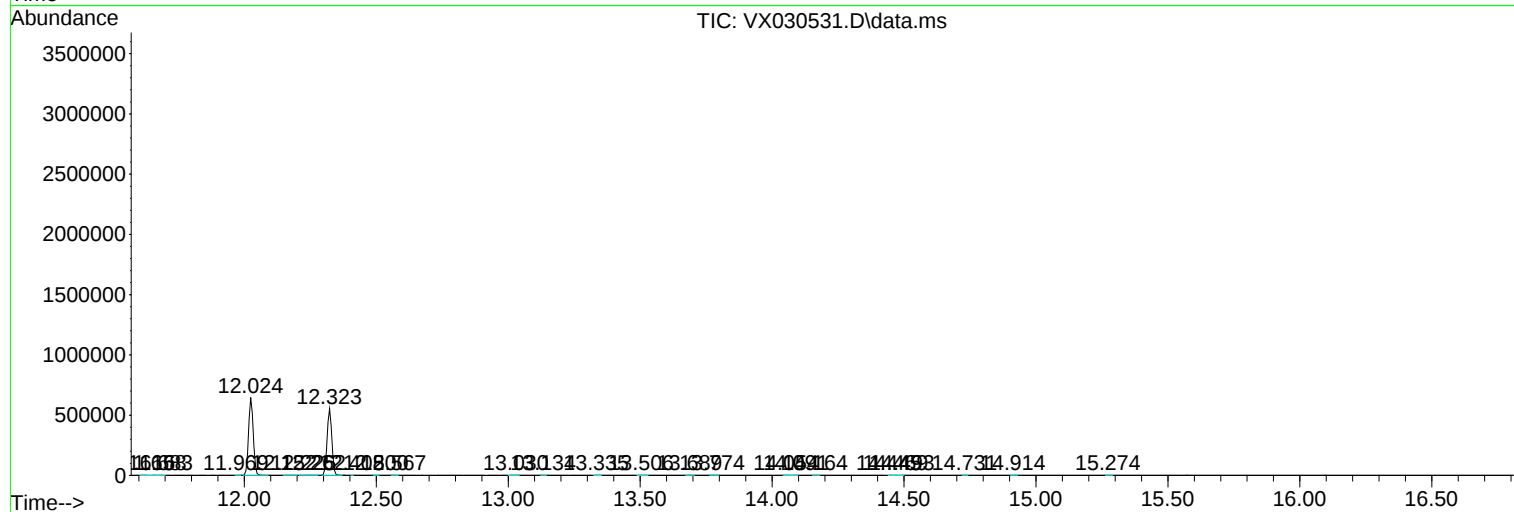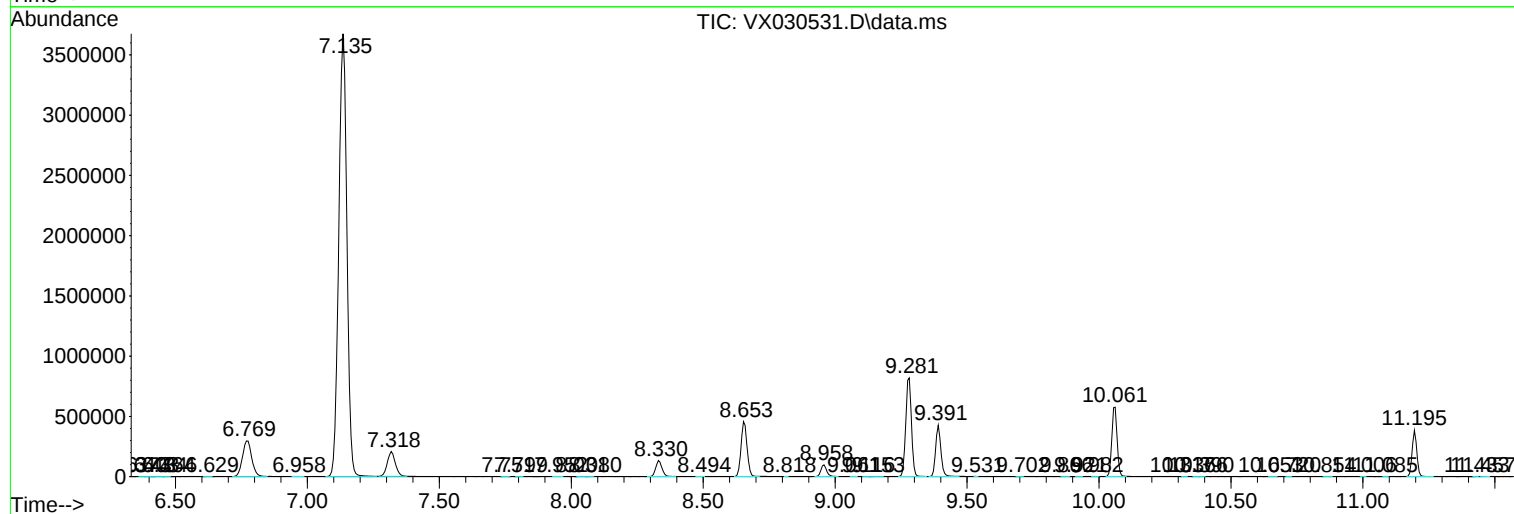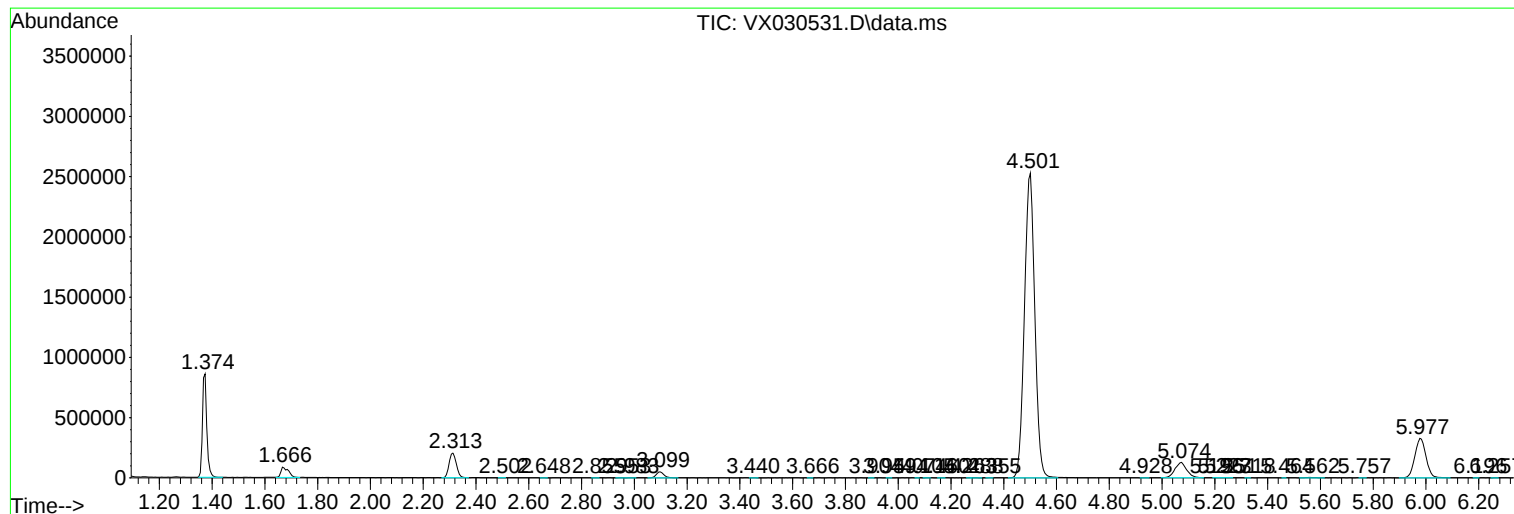

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030531.D
Acq On : 09 Aug 2022 16:46
Operator : JC/MD
Sample : N4114-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030531.D
Acq On : 09 Aug 2022 16:46
Operator : JC/MD
Sample : N4114-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc