

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030534.D
 Acq On : 09 Aug 2022 17:58
 Operator : JC/MD
 Sample : N4114-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB2	498904	554937	18.26%	5.026%
2	1.672	91	96	106	rVB	78450	103023	3.39%	0.933%
3	2.306	195	200	212	rVB	167503	259936	8.55%	2.354%
4	2.404	212	216	218	rBV4	1626	2472	0.08%	0.022%
5	2.611	248	250	252	rBV2	476	443	0.01%	0.004%
6	2.794	277	280	281	rBV3	863	829	0.03%	0.008%
7	3.001	311	314	318	rBV3	416	680	0.02%	0.006%
8	3.099	323	330	338	rVB	35541	65964	2.17%	0.597%
9	3.215	347	349	350	rBV	618	389	0.01%	0.004%
10	3.453	385	388	391	rBV3	809	747	0.02%	0.007%
11	3.507	395	397	400	rBV2	456	515	0.02%	0.005%
12	3.672	421	424	425	rBV2	441	367	0.01%	0.003%
13	3.745	433	436	439	rBV2	271	374	0.01%	0.003%
14	4.050	484	486	488	rBV2	320	342	0.01%	0.003%
15	4.093	491	493	496	rBV2	436	434	0.01%	0.004%
16	4.135	498	500	504	rVB2	487	485	0.02%	0.004%
17	4.190	504	509	511	rBV2	438	749	0.02%	0.007%
18	4.233	514	516	518	rVB2	492	366	0.01%	0.003%
19	4.501	548	560	583	rBV2	1082463	3038531	100.00%	27.521%
20	4.964	633	636	637	rBV3	594	532	0.02%	0.005%
21	5.074	642	654	668	rBV	124431	385326	12.68%	3.490%
22	5.397	705	707	712	rVB4	977	1451	0.05%	0.013%
23	5.556	729	733	734	rBV2	1920	2294	0.08%	0.021%
24	5.702	755	757	759	rBV2	327	404	0.01%	0.004%
25	5.787	769	771	776	rBV5	535	914	0.03%	0.008%
26	5.983	791	803	817	rVV2	332011	943455	31.05%	8.545%
27	6.092	819	821	826	rVV5	837	1078	0.04%	0.010%
28	6.318	856	858	860	rBV2	545	364	0.01%	0.003%
29	6.422	872	875	879	rBV3	722	1002	0.03%	0.009%
30	6.476	883	884	887	rVB2	530	416	0.01%	0.004%
31	6.641	909	911	914	rBV2	335	439	0.01%	0.004%
32	6.775	922	933	945	rBV	307302	718893	23.66%	6.511%
33	7.080	981	983	984	rVV	409	367	0.01%	0.003%
34	7.129	984	991	1002	rVB8	11776	30129	0.99%	0.273%
35	7.318	1013	1022	1036	rBV	200968	439914	14.48%	3.984%
36	7.494	1047	1051	1054	rBV4	708	1059	0.03%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030534.D
 Acq On : 09 Aug 2022 17:58
 Operator : JC/MD
 Sample : N4114-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.732	1088	1090	1092	rVV3	468	402	0.01%	0.004%
38	7.769	1094	1096	1099	rVB3	500	403	0.01%	0.004%
39	7.818	1101	1104	1106	rVB3	448	555	0.02%	0.005%
40	7.952	1124	1126	1129	rVB2	665	492	0.02%	0.004%
41	8.330	1182	1188	1200	rBV	128962	216360	7.12%	1.960%
42	8.488	1210	1214	1217	rBV5	688	1111	0.04%	0.010%
43	8.549	1221	1224	1227	rBV4	515	811	0.03%	0.007%
44	8.653	1235	1241	1251	rBV	446271	705584	23.22%	6.391%
45	8.854	1272	1274	1276	rBV2	696	723	0.02%	0.007%
46	8.891	1278	1280	1282	rVB2	956	700	0.02%	0.006%
47	8.958	1285	1291	1302	rBV	94883	142637	4.69%	1.292%
48	9.104	1312	1315	1317	rBV3	455	582	0.02%	0.005%
49	9.183	1326	1328	1331	rVB2	425	508	0.02%	0.005%
50	9.214	1331	1333	1336	rBV2	500	718	0.02%	0.007%
51	9.275	1341	1343	1349	rVB6	1967	2884	0.09%	0.026%
52	9.390	1356	1362	1375	rBV	428322	599879	19.74%	5.433%
53	9.653	1402	1405	1407	rBV	613	619	0.02%	0.006%
54	9.677	1407	1409	1412	rVV2	598	456	0.02%	0.004%
55	9.787	1425	1427	1428	rBV	590	342	0.01%	0.003%
56	9.866	1437	1440	1442	rVB3	574	654	0.02%	0.006%
57	9.896	1442	1445	1446	rBV2	454	338	0.01%	0.003%
58	10.061	1466	1472	1482	rBV	599739	816206	26.86%	7.393%
59	10.195	1492	1494	1497	rVB	686	523	0.02%	0.005%
60	10.293	1509	1510	1512	rBV	567	491	0.02%	0.004%
61	10.409	1528	1529	1532	rBV2	412	355	0.01%	0.003%
62	10.506	1542	1545	1546	rBV3	502	428	0.01%	0.004%
63	10.573	1554	1556	1558	rBV2	560	521	0.02%	0.005%
64	10.695	1572	1576	1579	rBV3	570	772	0.03%	0.007%
65	10.750	1582	1585	1588	rBV3	480	631	0.02%	0.006%
66	10.787	1588	1591	1594	rBV3	588	631	0.02%	0.006%
67	10.823	1596	1597	1600	rBV	552	428	0.01%	0.004%
68	10.927	1611	1614	1618	rBV3	679	952	0.03%	0.009%
69	11.000	1625	1626	1629	rBV	471	454	0.01%	0.004%
70	11.061	1634	1636	1638	rVB3	475	405	0.01%	0.004%
71	11.097	1638	1642	1643	rBV2	443	510	0.02%	0.005%
72	11.195	1653	1658	1666	rBV	379231	480890	15.83%	4.356%
73	11.640	1729	1731	1734	rVB	722	762	0.03%	0.007%
74	11.671	1734	1736	1737	rBV2	521	370	0.01%	0.003%
75	11.756	1748	1750	1751	rBV2	589	437	0.01%	0.004%
76	11.768	1751	1752	1754	rBV	473	424	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030534.D
 Acq On : 09 Aug 2022 17:58
 Operator : JC/MD
 Sample : N4114-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.847	1762	1765	1767	rBV2	485	575	0.02%	0.005%
78	12.024	1789	1794	1804	rBV	643977	787886	25.93%	7.136%
79	12.231	1824	1828	1831	rBV3	621	1194	0.04%	0.011%
80	12.323	1838	1843	1850	rVB	566626	697689	22.96%	6.319%
81	12.555	1879	1881	1882	rBV	515	411	0.01%	0.004%
82	12.689	1901	1903	1905	rBV2	547	489	0.02%	0.004%
83	13.146	1973	1978	1981	rBV4	616	1098	0.04%	0.010%
84	13.286	1999	2001	2002	rBV2	582	391	0.01%	0.004%
85	13.396	2016	2019	2021	rBV2	363	387	0.01%	0.004%
86	13.743	2075	2076	2079	rVB	761	617	0.02%	0.006%
87	13.780	2079	2082	2083	rBV2	565	657	0.02%	0.006%
88	13.877	2096	2098	2100	rBV2	416	407	0.01%	0.004%
89	14.018	2119	2121	2123	rBV2	508	510	0.02%	0.005%
90	14.042	2123	2125	2127	rVV	509	368	0.01%	0.003%
91	14.353	2174	2176	2178	rBV	610	394	0.01%	0.004%
92	14.396	2181	2183	2186	rVB2	462	367	0.01%	0.003%
93	14.566	2209	2211	2213	rBV	621	560	0.02%	0.005%
94	14.816	2250	2252	2255	rBV2	730	476	0.02%	0.004%
95	14.883	2261	2263	2266	rBV3	640	777	0.03%	0.007%
96	14.987	2279	2280	2282	rVB	919	471	0.02%	0.004%
97	15.018	2283	2285	2287	rVV2	633	404	0.01%	0.004%
98	15.548	2370	2372	2374	rBV3	804	942	0.03%	0.009%
99	16.657	2552	2554	2556	rBV	846	576	0.02%	0.005%
100	16.688	2557	2559	2561	rBV	1088	756	0.02%	0.007%




Sum of corrected areas: 11040970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030534.D
Acq On : 09 Aug 2022 17:58
Operator : JC/MD
Sample : N4114-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

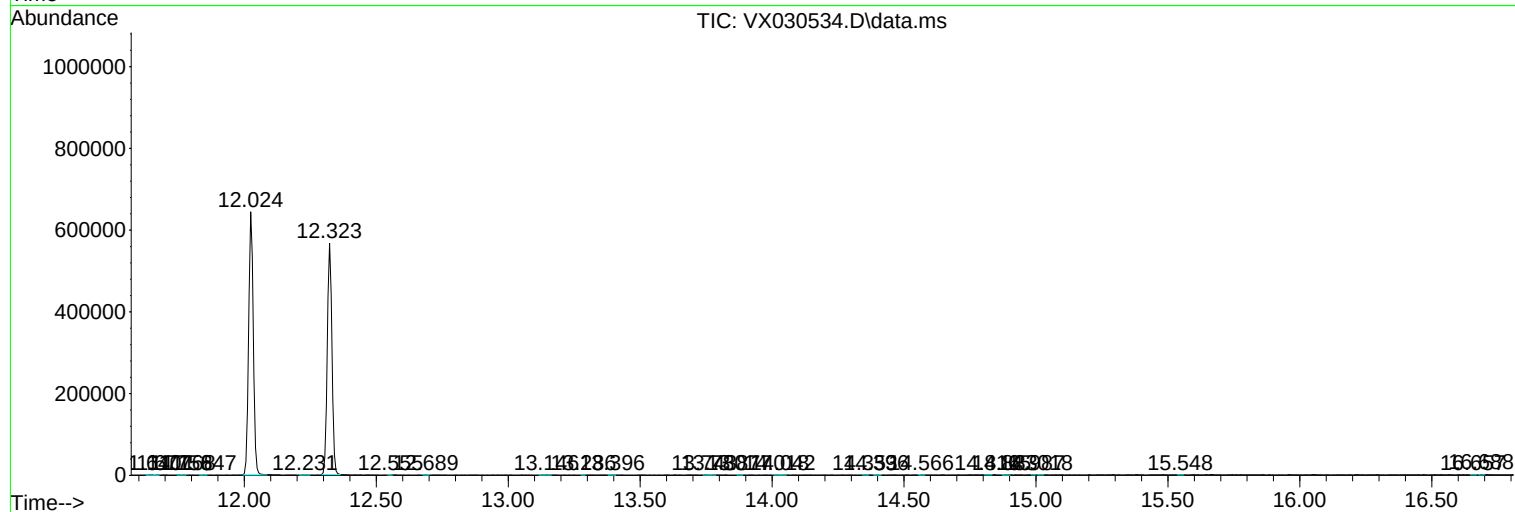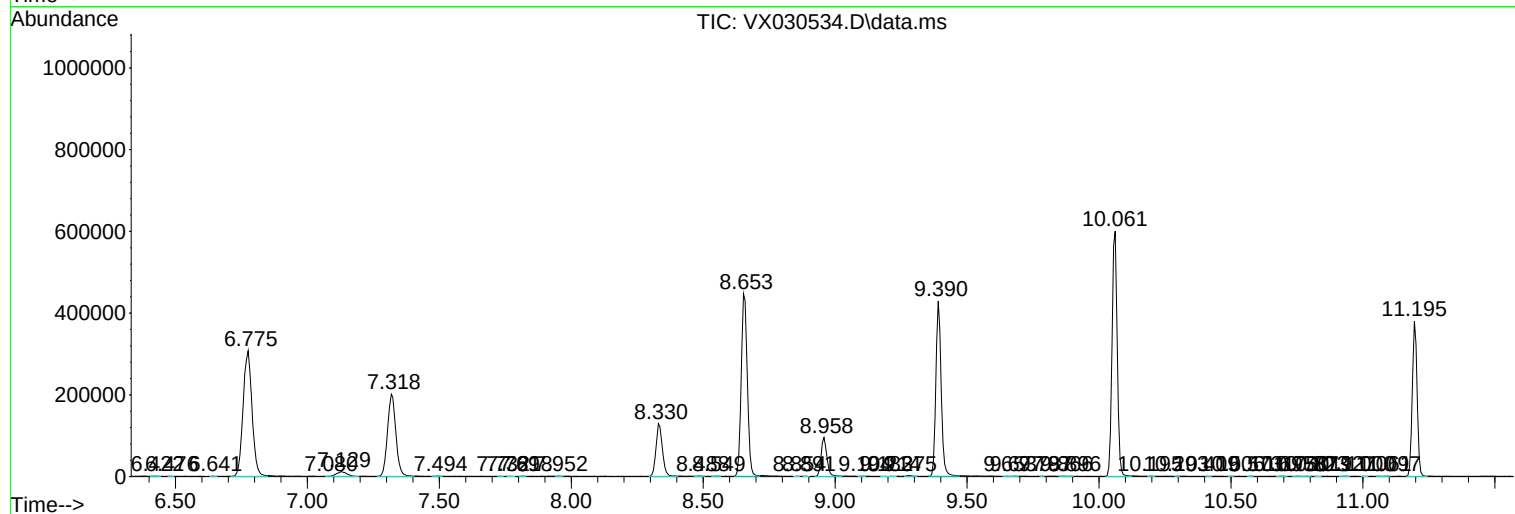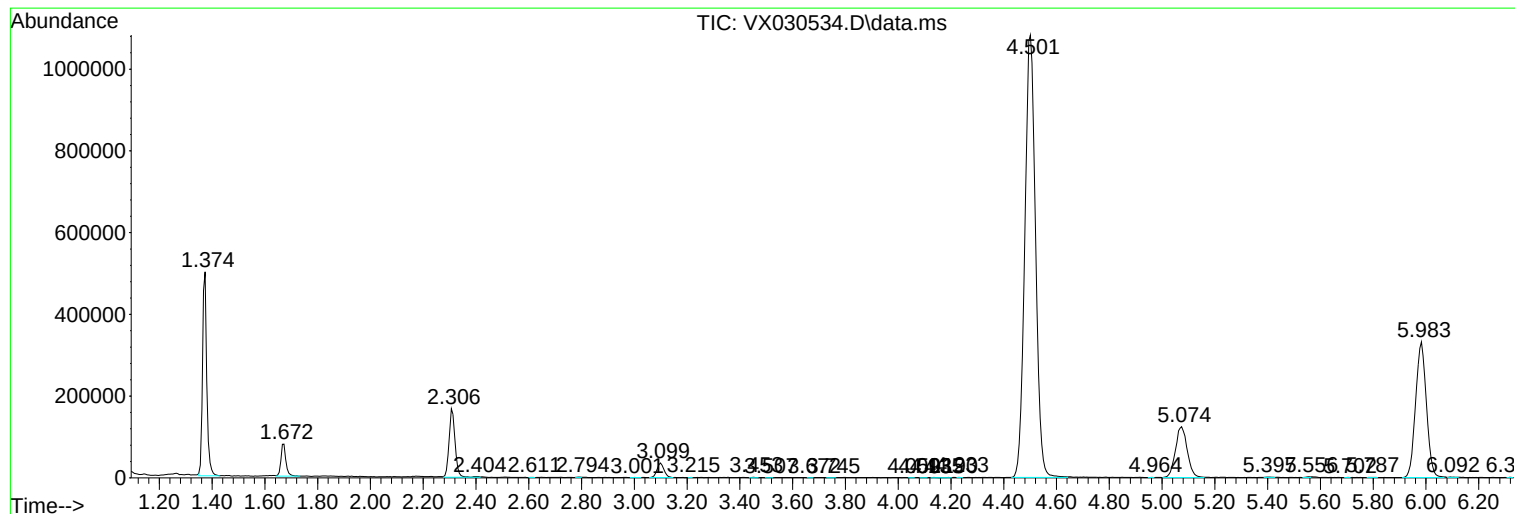

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030534.D
Acq On : 09 Aug 2022 17:58
Operator : JC/MD
Sample : N4114-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030534.D
Acq On : 09 Aug 2022 17:58
Operator : JC/MD
Sample : N4114-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------