
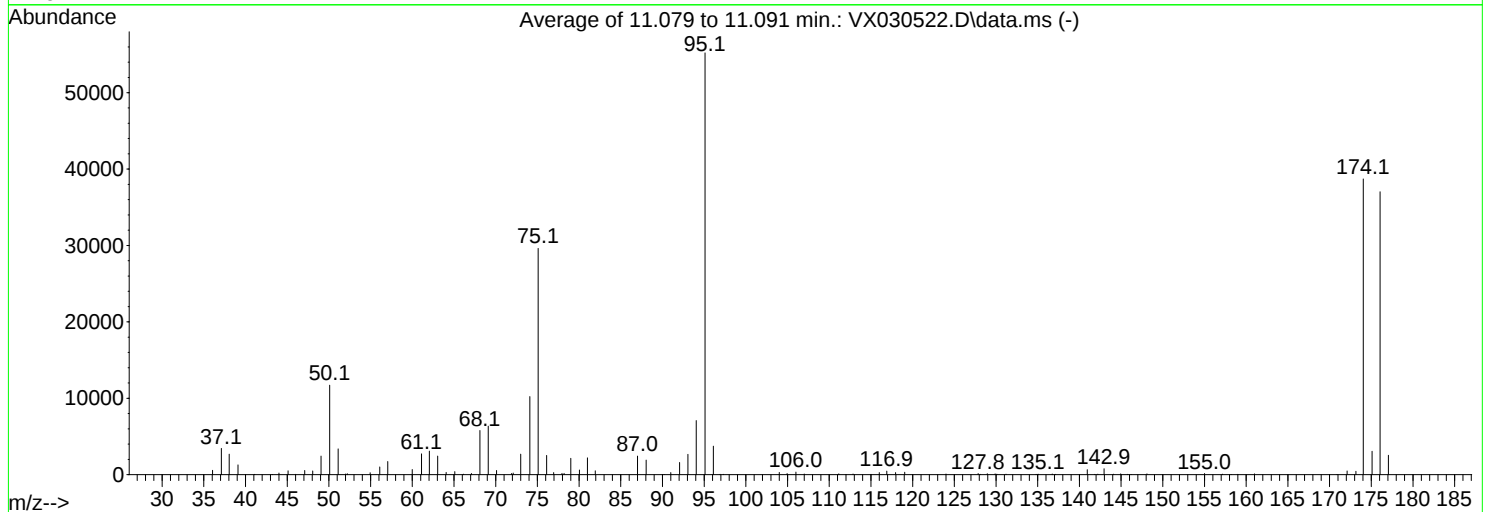


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030522.D
 Acq On : 09 Aug 2022 10:05
 Operator : JC/MD
 Sample : BFB674
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB674

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 10 01:21:25 2022

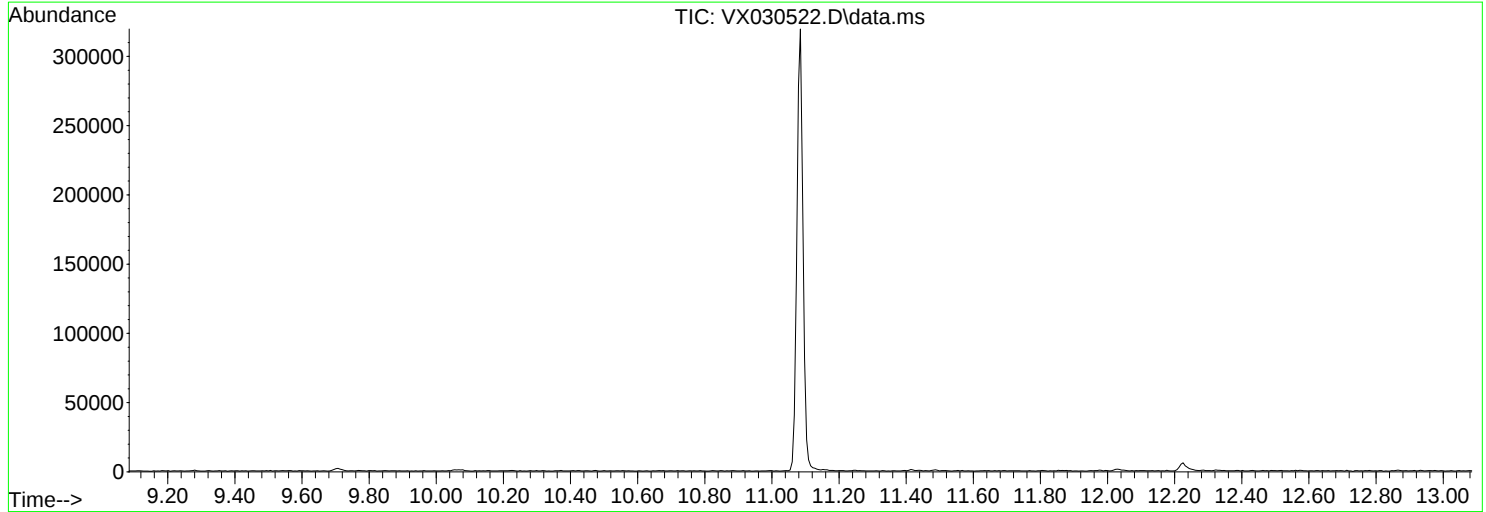

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	11716	PASS
75	95	30	80	53.6	29621	PASS
95	95	100	100	100.0	55219	PASS
96	95	5	9	6.8	3739	PASS
173	174	0.00	2	1.1	436	PASS
174	95	50	120	70.1	38720	PASS
175	174	5	9	7.9	3050	PASS
176	174	95	101	95.6	37024	PASS
177	176	5	9	6.8	2535	PASS

m/z	Abundance
40.10	439.0
44.00	440.0
65.60	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB674

m/z	Abundance
36.00	705.0
37.10	3825.0
38.10	2955.0
39.10	1509.0
40.10	387.0
41.10	53.0
44.00	878.0
45.10	594.0
47.20	498.0
48.00	495.0
49.10	2786.0
50.10	13904.0
51.10	4110.0
52.00	271.0
54.90	174.0
56.10	1209.0
57.00	1928.0
60.00	759.0
61.10	3002.0
62.00	3417.0
63.10	2834.0
64.00	240.0
65.00	200.0
66.10	88.0
67.10	184.0
68.10	6697.0
69.10	7530.0
70.10	611.0
71.90	307.0
73.00	2683.0
74.10	11139.0
75.10	32824.0
76.10	3307.0
76.90	371.0
77.90	325.0
79.00	2322.0
80.00	661.0
81.00	2491.0
81.90	533.0
87.00	2768.0
88.10	2054.0
90.20	60.0
91.00	299.0
92.00	1634.0
93.00	2891.0
94.00	7587.0
95.10	57656.0
96.10	3850.0
96.90	112.0
104.10	289.0
104.90	133.0
106.00	402.0
111.20	144.0
112.00	54.0
112.80	93.0
116.00	301.0
116.90	649.0
117.90	233.0
119.00	234.0
124.00	72.0
127.80	264.0
129.00	82.0
129.90	112.0
135.10	90.0
136.70	80.0
137.20	72.0
140.90	609.0
141.90	56.0
143.00	767.0
144.10	109.0
145.00	172.0
146.20	51.0
148.10	63.0
155.10	79.0
161.00	63.0
170.90	66.0
172.20	398.0
173.20	444.0
174.10	35448.0
175.10	2889.0
176.10	33992.0
177.00	2239.0

Instrument :
MSVOA_X
ClientSampleId :
BFB674

m/z	Abundance
36.10	676.0
37.10	4246.0
38.00	3015.0
39.10	1587.0
40.00	452.0
41.10	55.0
44.00	545.0
45.10	632.0
46.00	111.0
47.10	766.0
48.00	573.0
49.00	2990.0
50.10	13836.0
51.10	3985.0
52.20	179.0
54.90	200.0
56.10	1214.0
57.10	2029.0
60.00	810.0
61.10	3122.0
62.10	3672.0
63.00	2623.0
64.10	433.0
65.10	750.0
66.20	74.0
67.10	97.0
68.10	6302.0
69.10	7191.0
70.10	739.0
72.10	607.0
73.00	3677.0
74.10	12876.0
75.10	35320.0
76.10	2765.0
77.00	325.0
78.20	520.0
79.00	2324.0
80.10	638.0
81.00	2662.0
82.00	572.0
87.00	3111.0
88.00	2245.0
91.00	372.0
92.00	1922.0
93.10	2867.0
94.10	7999.0
95.10	65448.0
96.10	4497.0
97.30	145.0
103.90	370.0
105.00	188.0
106.00	406.0
107.00	158.0
111.10	156.0
112.90	117.0
115.10	61.0
116.00	282.0
116.90	391.0
118.00	373.0
119.00	394.0
124.00	170.0
127.90	178.0
128.90	168.0
130.10	196.0
131.20	94.0
135.00	130.0
137.00	88.0
141.00	638.0
141.80	96.0
142.20	83.0
142.90	943.0
144.10	79.0
144.90	145.0
148.10	165.0
155.00	227.0
157.20	89.0
159.00	65.0
161.00	134.0
172.00	645.0
173.10	580.0
174.00	46904.0
175.10	3483.0
176.00	44808.0
177.10	2958.0

Instrument :
MSVOA_X
ClientSampleId :
BFB674

m/z	Abundance
36.10	331.0
37.00	2206.0
38.10	2084.0
39.00	722.0
40.00	350.0
43.20	81.0
44.10	521.0
45.00	260.0
47.00	398.0
48.10	397.0
49.10	1510.0
50.10	7408.0
51.00	2012.0
52.20	202.0
55.00	357.0
56.00	606.0
57.00	1218.0
60.00	445.0
61.10	2031.0
62.00	2125.0
63.00	1839.0
64.00	185.0
65.10	263.0
67.10	164.0
68.10	4349.0
69.10	4295.0
70.00	296.0
71.90	106.0
73.00	1663.0
74.10	6682.0
75.10	20720.0
76.00	1474.0
77.00	137.0
78.00	196.0
79.00	1766.0
80.00	533.0
81.00	1422.0
82.00	388.0
86.90	1384.0
88.00	1446.0
90.90	179.0
92.10	1219.0
93.00	2219.0
94.10	5687.0
95.10	42552.0
96.10	2869.0
104.00	223.0
105.00	121.0
105.90	203.0
107.00	90.0
112.90	54.0
114.90	59.0
116.00	264.0
116.90	320.0
118.00	192.0
119.10	322.0
128.10	107.0
129.00	105.0
129.90	195.0
131.20	72.0
134.80	103.0
136.80	160.0
140.90	724.0
142.20	94.0
142.90	618.0
145.80	132.0
148.10	64.0
154.90	139.0
157.10	113.0
158.20	87.0
159.00	55.0
161.00	99.0
172.10	417.0
173.10	283.0
174.10	33808.0
175.10	2778.0
176.10	32272.0
177.00	2407.0

Instrument :
MSVOA_X
ClientSampleId :
BFB674