

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080923\
 Data File : VX036890.D
 Acq On : 09 Aug 2023 16:20
 Operator : JC/MD
 Sample : 03903-01ME
 Misc : 5.00g/10mL100uL/5.00mLMSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01ME


Quant Time: Aug 10 01:18:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	106545	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	194555	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	186518	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	92395	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	72570	46.033	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.060%
35) Dibromofluoromethane	5.391	113	61229	45.787	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.580%
50) Toluene-d8	8.647	98	235056	49.567	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.140%
62) 4-Bromofluorobenzene	11.079	95	96167	53.750	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.500%
Target Compounds						
					Qvalue	
5) Bromomethane	1.605	94	287	0.369	ug/l #	60
11) Tert butyl alcohol	2.959	59	159	0.426	ug/l #	78
13) Acrolein	2.246	56	177	0.831	ug/l #	43
15) Acrylonitrile	3.093	53	158	0.211	ug/l #	66
17) Carbon Disulfide	2.477	76	820	0.249	ug/l #	84
18) Methyl Acetate	2.721	43	609	0.221	ug/l #	53
20) Methylene Chloride	2.776	84	2417	1.661	ug/l	90
25) 2-Butanone	4.605	43	304	0.286	ug/l #	51
29) Tetrahydrofuran	5.038	42	408	0.596	ug/l #	38
36) 1,1-Dichloropropene	5.550	75	9015	4.523	ug/l #	51
38) Carbon Tetrachloride	5.550	117	11163	5.268	ug/l #	15
39) Methylcyclohexane	7.367	83	555	0.224	ug/l #	89
51) 4-Methyl-2-Pentanone	8.604	43	1113	0.518	ug/l #	65
55) 1,1,2-Trichloroethane	9.098	97	1347	0.882	ug/l #	22
59) 2-Hexanone	9.446	43	407	0.255	ug/l #	26
68) m/p-Xylenes	10.299	106	1078	0.385	ug/l	90
74) N-amyl acetate	10.854	43	2752	0.772	ug/l #	5
76) 1,2,3-Trichloropropane	11.079	75	49581	22.814	ug/l #	39
78) n-propylbenzene	11.305	91	1816	0.205	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.079	75	49581	51.710	ug/l #	6
84) 1,2,4-Trimethylbenzene	11.750	105	2392	0.374	ug/l	100
85) sec-Butylbenzene	11.890	105	4870	0.621	ug/l	100
88) 1,4-Dichlorobenzene	12.037	146	809	0.253	ug/l #	1
89) n-Butylbenzene	12.329	91	7580	1.313	ug/l #	75
90) Hexachloroethane	12.616	117	3953	3.024	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.914	75	243	0.405	ug/l #	9
93) 1,2,4-Trichlorobenzene	13.585	180	944	0.492	ug/l #	2
94) Hexachlorobutadiene	13.719	225	457	0.576	ug/l	88
95) Naphthalene	13.774	128	4024	0.602	ug/l #	80
96) 1,2,3-Trichlorobenzene	13.963	180	825	0.437	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 10 01:18:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:168 Resp: 106545
Ion Ratio Lower Upper
168 100
99 64.0 56.6 85.0

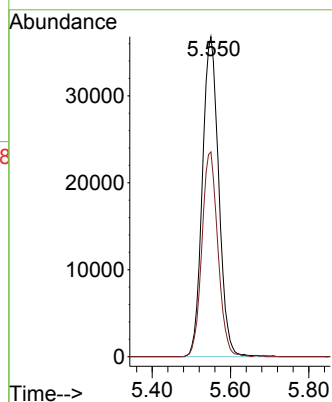

#5
Bromomethane
Concen: 0.369 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.012 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 94 Resp: 287
Ion Ratio Lower Upper
94 100
96 55.2 74.6 111.8#


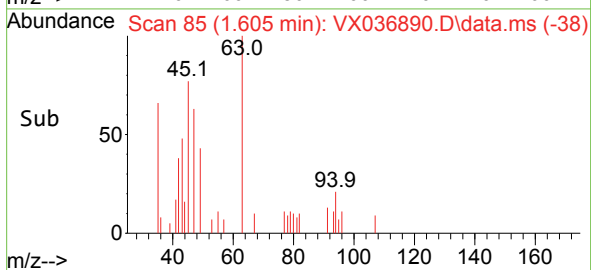
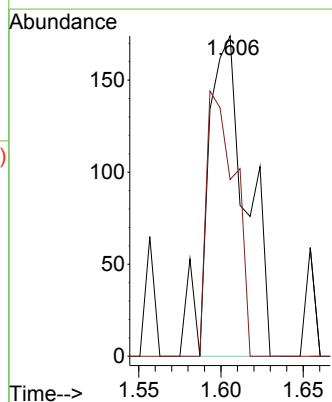
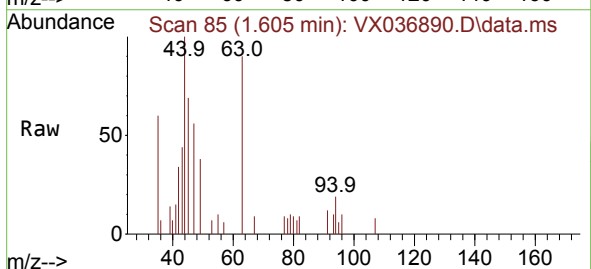




#11
Tert butyl alcohol
Concen: 0.426 ug/l
RT: 2.959 min Scan# 30
Delta R.T. -0.030 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 59 Resp: 159
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

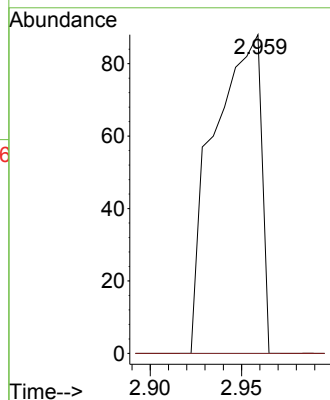

#13
Acrolein
Concen: 0.831 ug/l
RT: 2.246 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 56 Resp: 177
Ion Ratio Lower Upper
56 100
55 24.3 57.1 85.7#


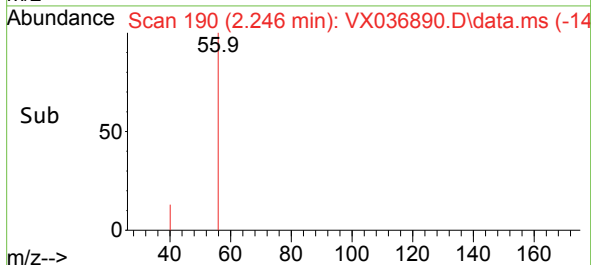
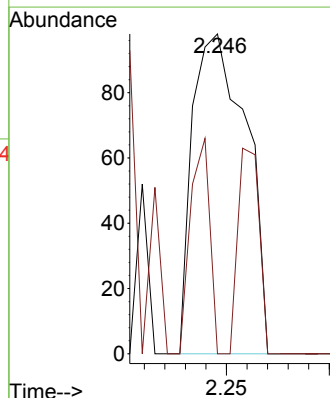
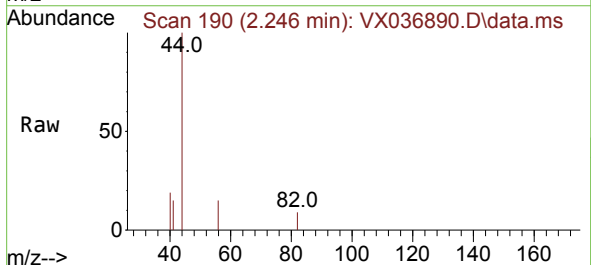




#15
Acrylonitrile
Concen: 0.211 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.025 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 53 Resp: 158
Ion Ratio Lower Upper
53 100
52 110.1 66.0 99.0#
51 12.0 29.8 44.6#

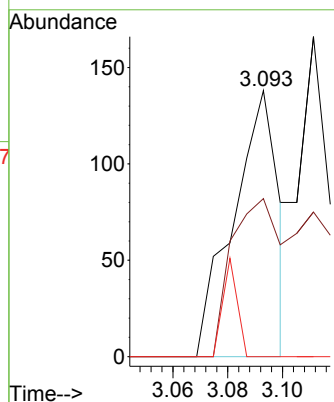

#17
Carbon Disulfide
Concen: 0.249 ug/l
RT: 2.477 min Scan# 228
Delta R.T. -0.036 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 76 Resp: 820
Ion Ratio Lower Upper
76 100
78 14.6 7.0 10.6#

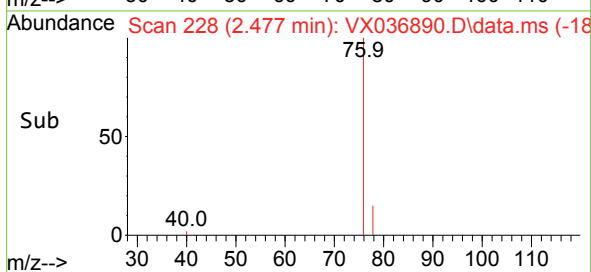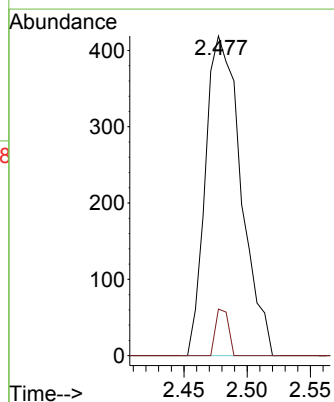



#18

Methyl Acetate

Concen: 0.221 ug/l

RT: 2.721 min Scan# 2

Delta R.T. 0.012 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20

Instrument :

MSVOA_X

ClientSampleId :





MW-01ME

Tgt Ion: 43 Resp: 609

Ion Ratio Lower Upper

43 100

74 0.0 17.8 26.8#

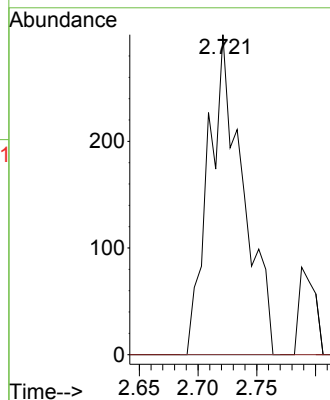

#20

Methylene Chloride

Concen: 1.661 ug/l

RT: 2.776 min Scan# 277

Delta R.T. -0.012 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20

Tgt Ion: 84 Resp: 2417




Ion Ratio Lower Upper


84 100

49 111.1 103.6 155.4

51 39.8 33.8 50.6

86 63.4 49.4 74.0


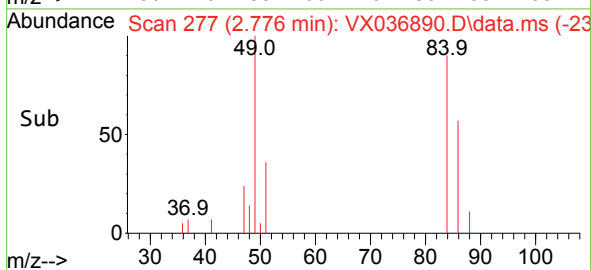
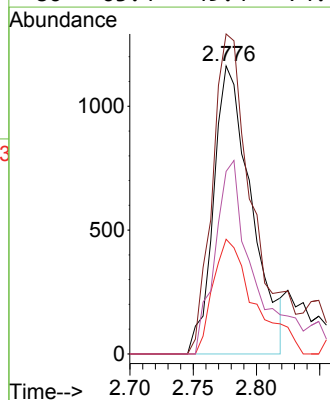





#25
2-Butanone
Concen: 0.286 ug/l
RT: 4.605 min Scan# 51
Delta R.T. 0.043 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 43 Resp: 304
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#

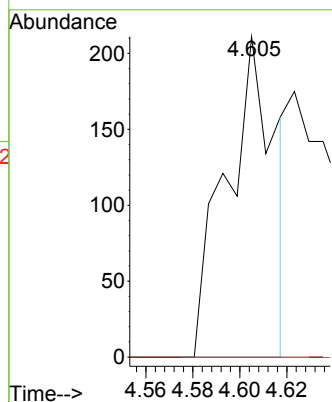

#29
Tetrahydrofuran
Concen: 0.596 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.031 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 42 Resp: 408
Ion Ratio Lower Upper
42 100
72 4.9 34.2 51.4#
71 0.0 32.2 48.2#


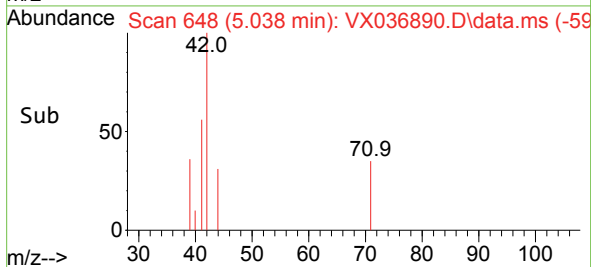

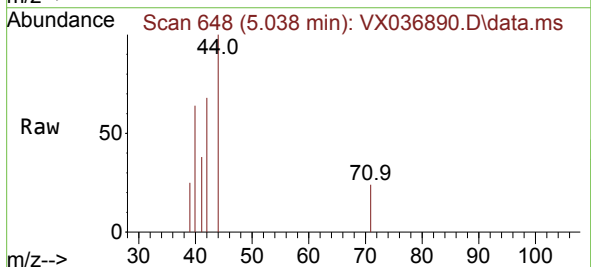




#33
 1,2-Dichloroethane-d4
 Concen: 46.033 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX036890.D
 Acq: 09 Aug 2023 16:20




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01ME


Tgt Ion: 65 Resp: 72570
 Ion Ratio Lower Upper
 65 100
 67 51.0 0.0 100.2

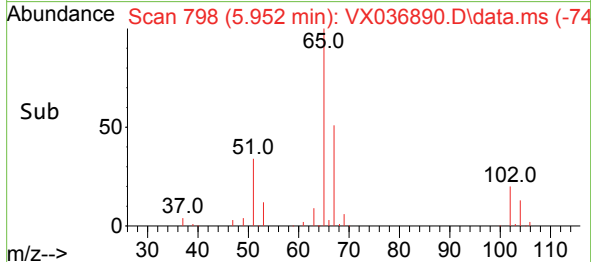

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.006 min
 Lab File: VX036890.D
 Acq: 09 Aug 2023 16:20

Tgt Ion: 114 Resp: 194555
 Ion Ratio Lower Upper
 114 100
 63 21.7 0.0 45.0
 88 16.6 0.0 36.6


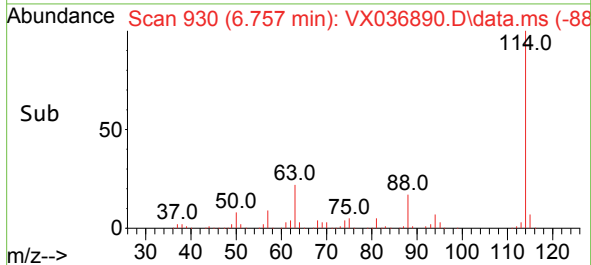

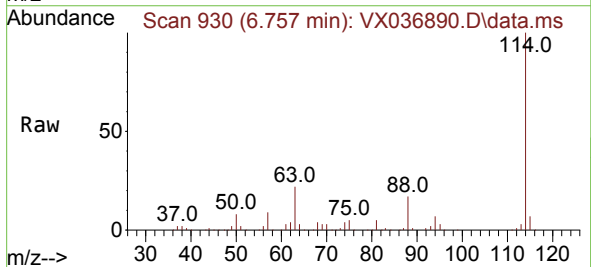


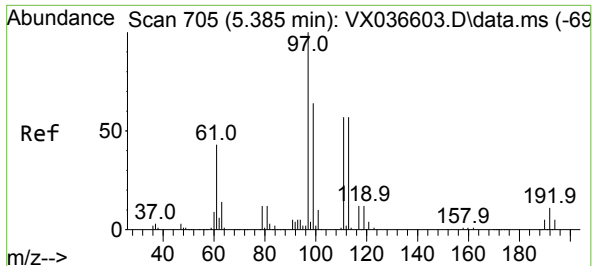

#35
Dibromofluoromethane
Concen: 45.787 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:113 Resp: 61229
Ion Ratio Lower Upper
113 100
111 101.3 82.9 124.3
192 18.4 13.3 19.9

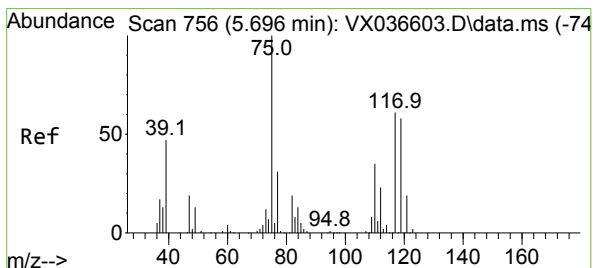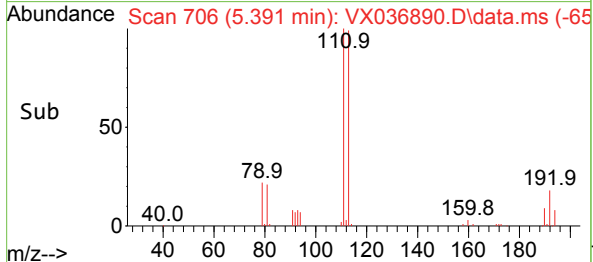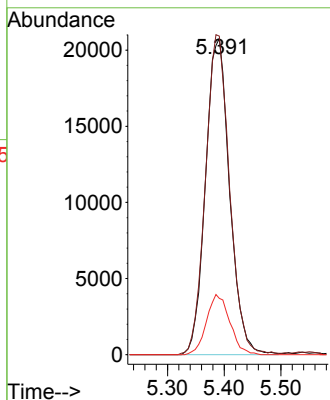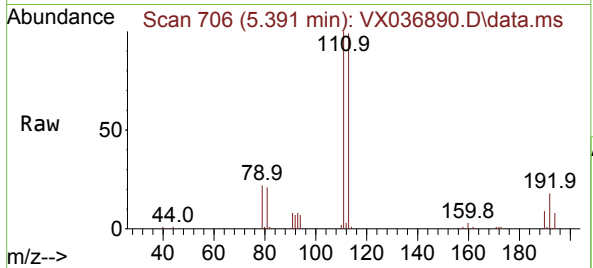

#36
1,1-Dichloropropene
Concen: 4.523 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20


Tgt Ion: 75 Resp: 9015
Ion Ratio Lower Upper
75 100
110 9.2 17.0 50.9#
77 0.0 24.7 37.1#

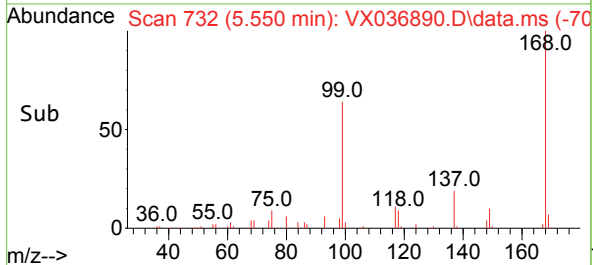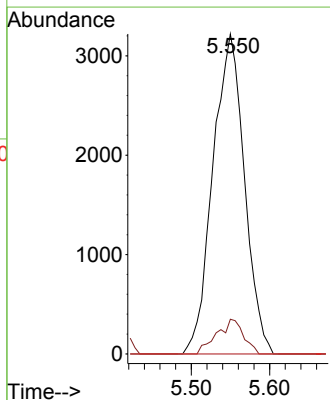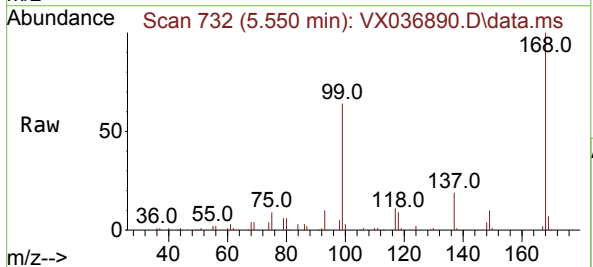






#38
Carbon Tetrachloride
Concen: 5.268 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Instrument :
MSVOA_X
ClientSampleId :
MW-01ME



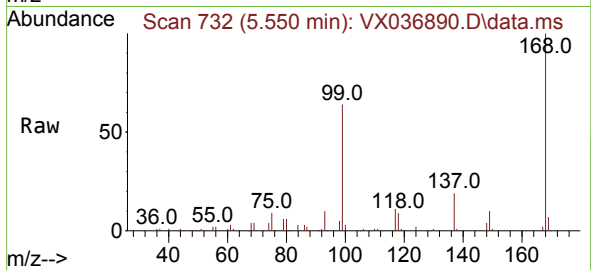



Tgt Ion:117 Resp: 11163
Ion Ratio Lower Upper
117 100
119 4.7 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.224 ug/l
RT: 7.367 min Scan# 1030
Delta R.T. -0.018 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 83 Resp: 555
Ion Ratio Lower Upper
83 100
55 77.5 64.6 97.0
98 29.4 36.7 55.1#


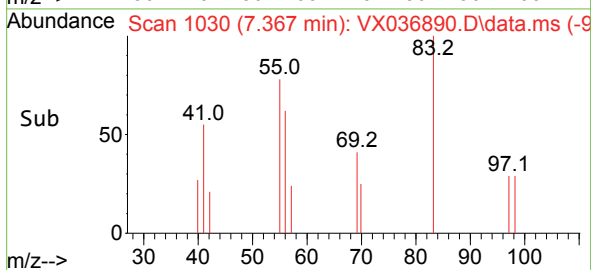

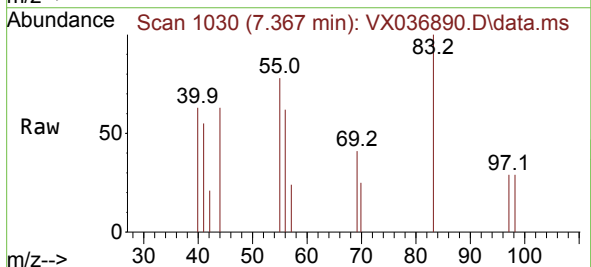




#50
Toluene-d8
Concen: 49.567 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 98 Resp: 235056
Ion Ratio Lower Upper
98 100
100 66.1 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 0.518 ug/l
RT: 8.604 min Scan# 1233
Delta R.T. 0.031 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 43 Resp: 1113
Ion Ratio Lower Upper
43 100
58 16.7 30.4 45.6#


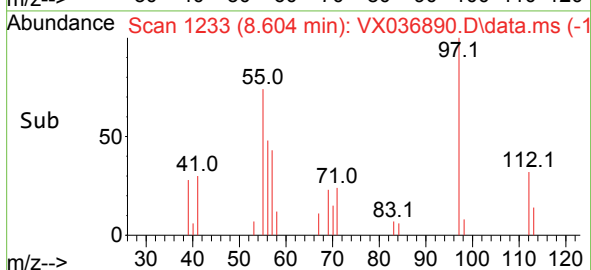






#55
 1,1,2-Trichloroethane
 Concen: 0.882 ug/l
 RT: 9.098 min Scan# 1314
 Delta R.T. -0.055 min
 Lab File: VX036890.D
 Acq: 09 Aug 2023 16:20




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01ME


Tgt Ion: 97	Resp:	1347
Ion	Ratio	Lower Upper
97	100	
83	10.8	65.8 98.8#
85	0.0	41.6 62.4#
99	0.0	47.8 71.8#



#59
 2-Hexanone
 Concen: 0.255 ug/l
 RT: 9.446 min Scan# 1371
 Delta R.T. 0.018 min
 Lab File: VX036890.D
 Acq: 09 Aug 2023 16:20

Tgt Ion: 43	Resp:	407
Ion	Ratio	Lower Upper
43	100	
58	0.0	26.2 78.5#


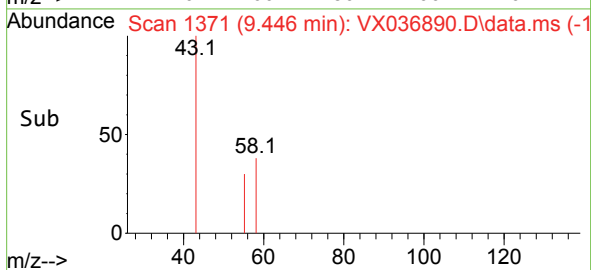

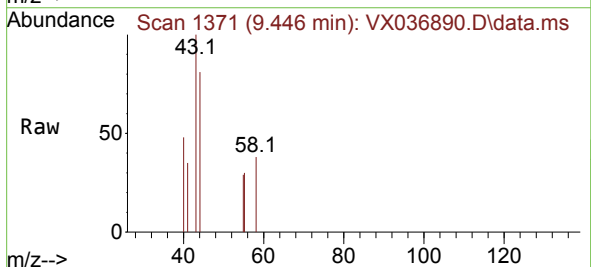




#62
4-Bromofluorobenzene
Concen: 53.750 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 95 Resp: 96167
Ion Ratio Lower Upper
95 100
174 73.0 0.0 135.6
176 69.7 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 117 Resp: 186518
Ion Ratio Lower Upper
117 100
82 56.3 46.2 69.4
119 32.6 25.5 38.3


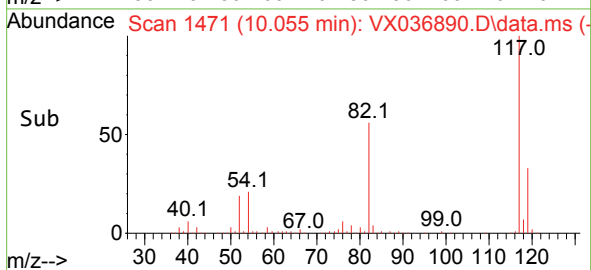




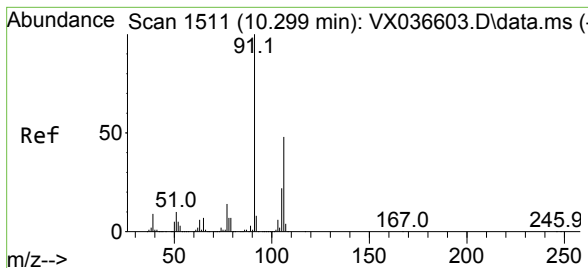

#68
m/p-Xylenes
Concen: 0.385 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:106 Resp: 1078
Ion Ratio Lower Upper
106 100
91 222.3 165.5 248.3

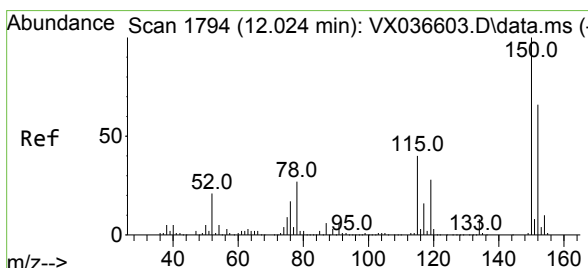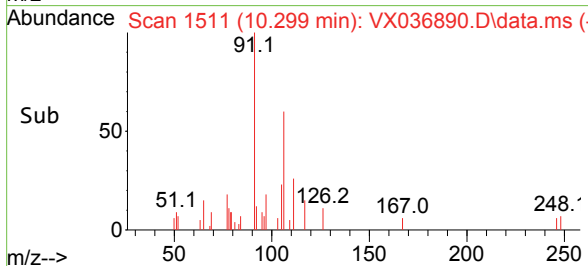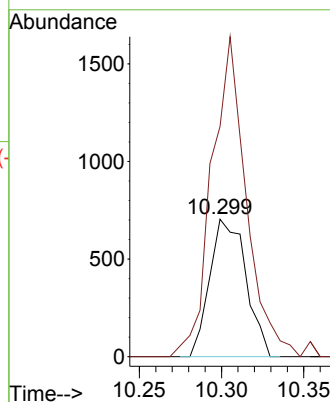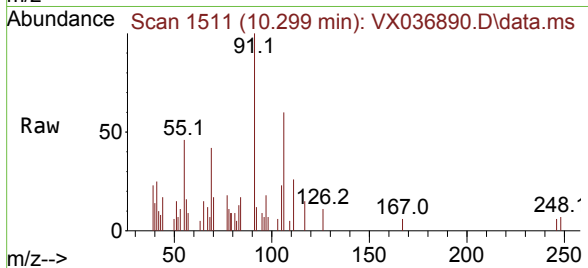

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion:152 Resp: 92395
Ion Ratio Lower Upper
152 100
115 63.2 43.3 129.9
150 156.3 0.0 345.0


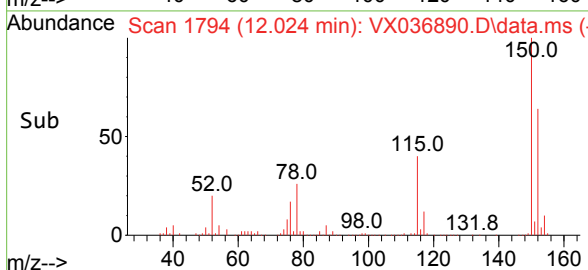
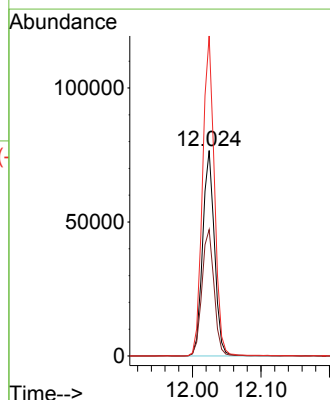
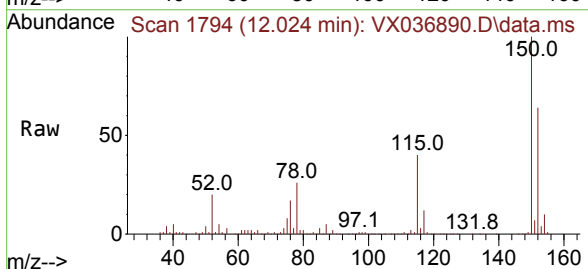




#74
N-amy1 acetate
Concen: 0.772 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.012 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:	43	Resp:	2752
Ion	Ratio	Lower	Upper
43	100		
70	18.2	32.9	49.3#
55	143.2	19.3	28.9#
61	0.0	18.8	28.2#

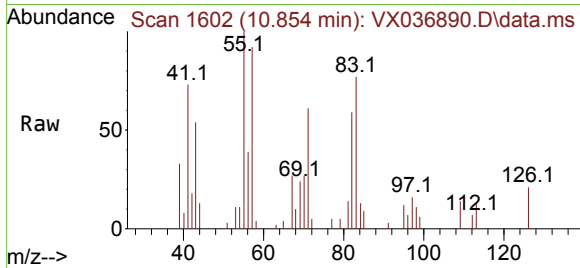

#76
1,2,3-Trichloropropane
Concen: 22.814 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion:	75	Resp:	49581
Ion	Ratio	Lower	Upper
75	100		
77	1.6	19.1	57.5#


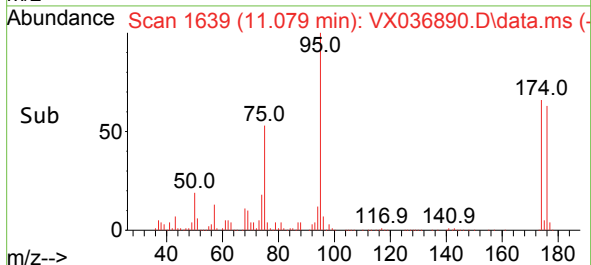

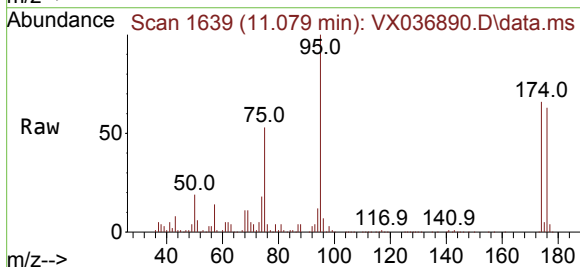


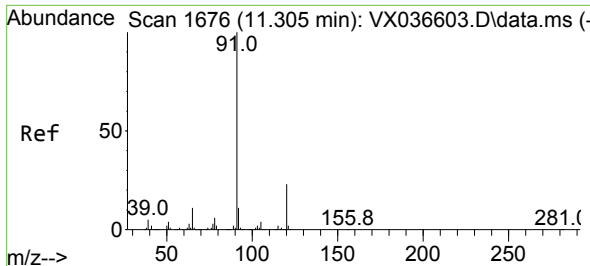

#78
n-propylbenzene
Concen: 0.205 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion: 91 Resp: 1816
Ion Ratio Lower Upper
91 100
120 18.2 11.5 34.4

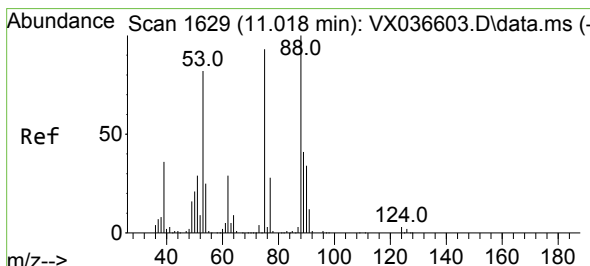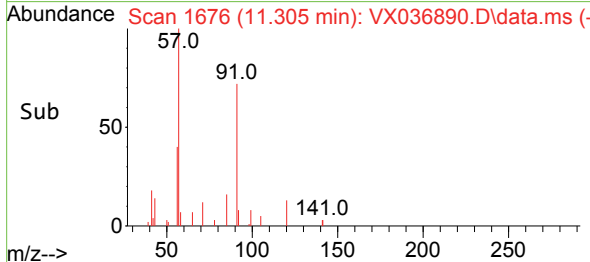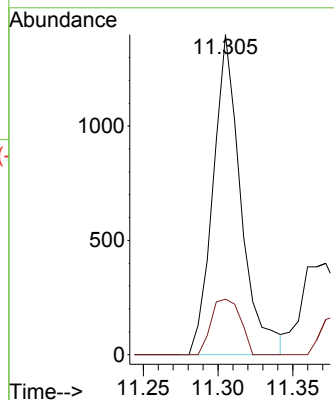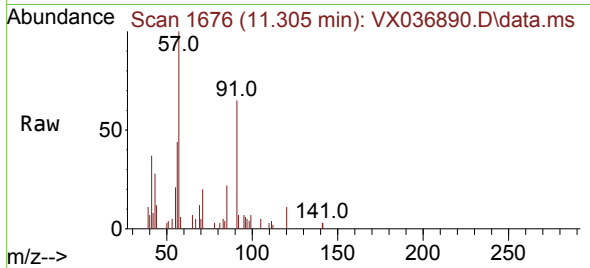

#81
trans-1,4-Dichloro-2-butene
Concen: 51.710 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 75 Resp: 49581
Ion Ratio Lower Upper
75 100
53 1.0 90.5 135.7#
89 0.0 36.9 55.3#


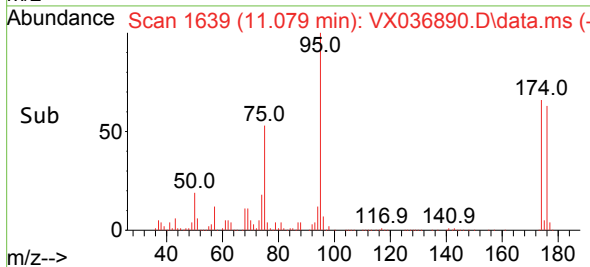
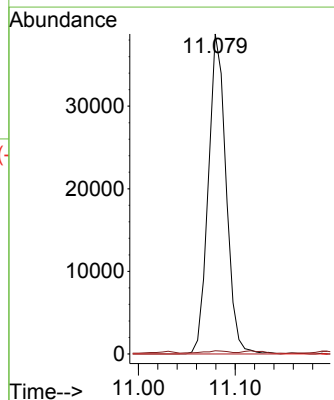
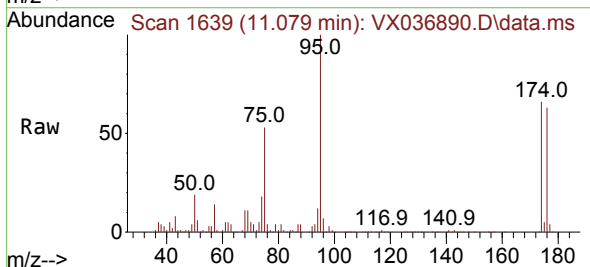




#84
1,2,4-Trimethylbenzene
Concen: 0.374 ug/l
RT: 11.750 min Scan# 11749
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:105 Resp: 2392
Ion Ratio Lower Upper
105 100
120 42.6 21.2 63.6

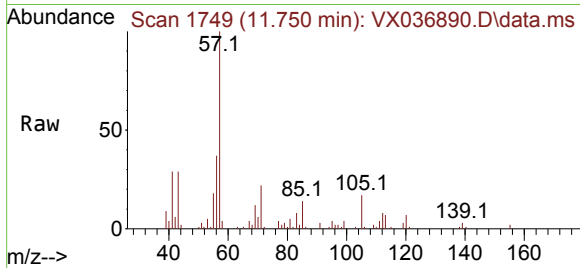

#85
sec-Butylbenzene
Concen: 0.621 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion:105 Resp: 4870
Ion Ratio Lower Upper
105 100
134 19.7 9.8 29.4



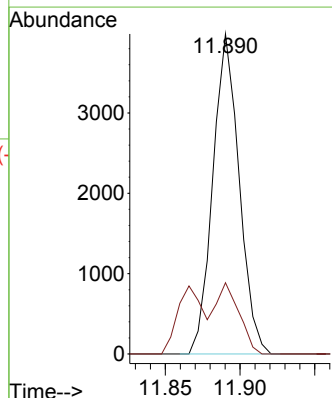
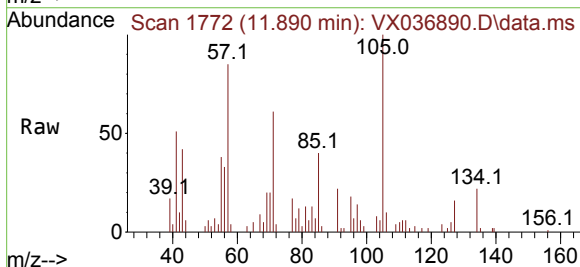




#88
1,4-Dichlorobenzene
Concen: 0.253 ug/l
RT: 12.037 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20




Instrument :
MSVOA_X
ClientSampleId :
MW-01ME


Tgt Ion:146 Resp: 809
Ion Ratio Lower Upper
146 100
111 236.8 21.3 63.7#
148 96.5 31.8 95.4#

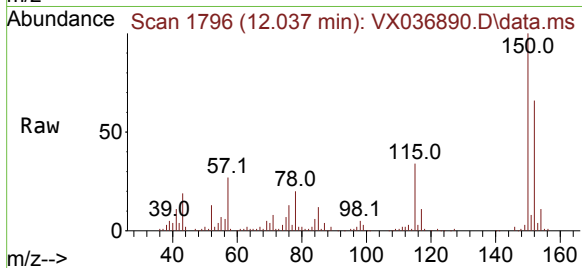

#89
n-Butylbenzene
Concen: 1.313 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion: 91 Resp: 7580
Ion Ratio Lower Upper
91 100
92 43.9 27.4 82.0
134 48.2 12.6 37.8#

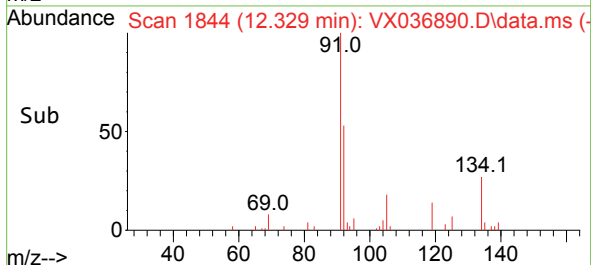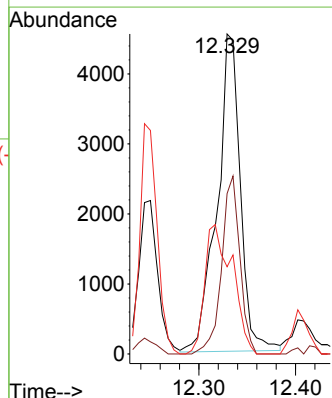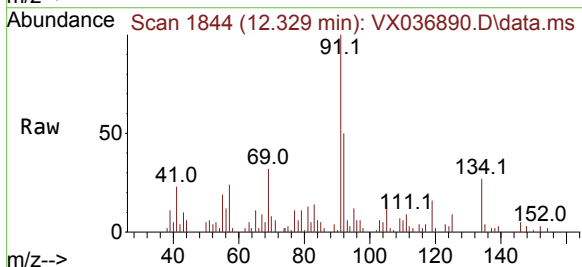



#90

Hexachloroethane

Concen: 3.024 ug/l

RT: 12.616 min Scan# 117

Delta R.T. 0.079 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20

Instrument :

MSVOA_X

ClientSampleId :





MW-01ME

Tgt Ion:117 Resp: 3953

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

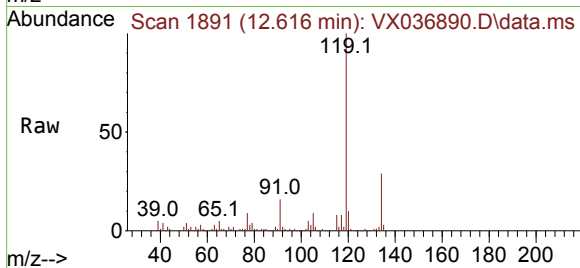

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.405 ug/l

RT: 12.914 min Scan# 1940

Delta R.T. -0.024 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20




Tgt Ion: 75 Resp: 243


Ion Ratio Lower Upper

75 100

155 0.0 36.1 108.5#

157 0.0 44.9 134.7#

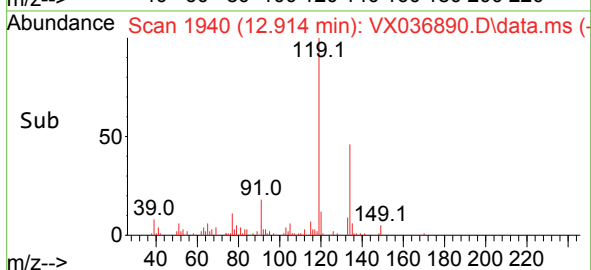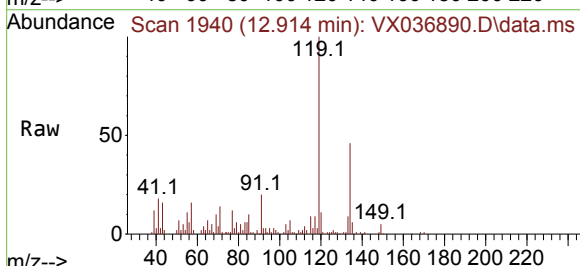



#93

1,2,4-Trichlorobenzene

Concen: 0.492 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. 0.000 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20





Instrument :

MSVOA_X

ClientSampleId :

MW-01ME

Tgt Ion:180	Resp:	944
Ion Ratio	Lower	Upper
180	100	
182	82.0	48.3 144.8
145	225.0	18.0 54.0#

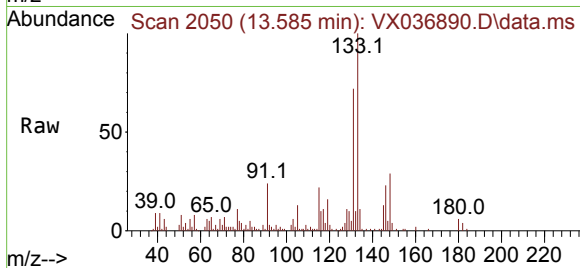

#94

Hexachlorobutadiene

Concen: 0.576 ug/l




RT: 13.719 min Scan# 2072


Delta R.T. -0.006 min

Lab File: VX036890.D

Acq: 09 Aug 2023 16:20

Tgt Ion:225	Resp:	457
Ion Ratio	Lower	Upper
225	100	
223	46.6	31.1 93.2
227	61.9	32.5 97.5




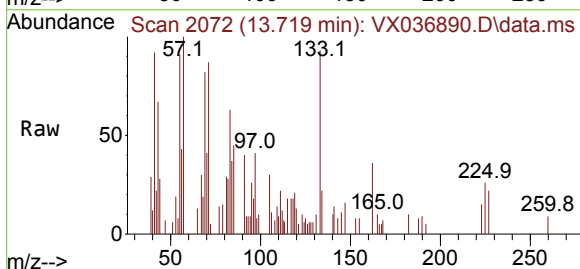


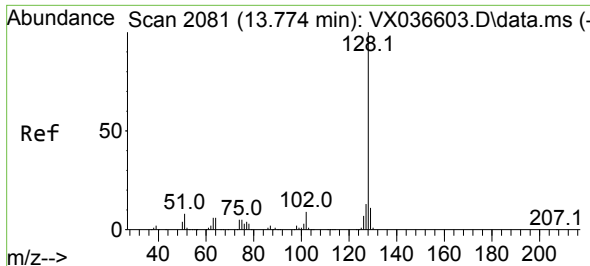

#95
Naphthalene
Concen: 0.602 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Instrument :
MSVOA_X
ClientSampleId :
MW-01ME

Tgt Ion:128 Resp: 4024
Ion Ratio Lower Upper
128 100
127 21.6 10.3 15.5#
129 4.4 8.8 13.2#

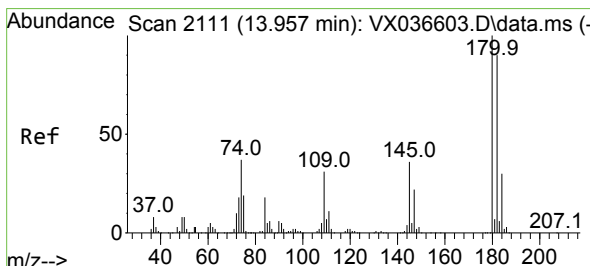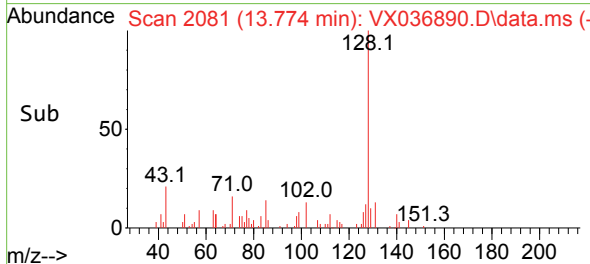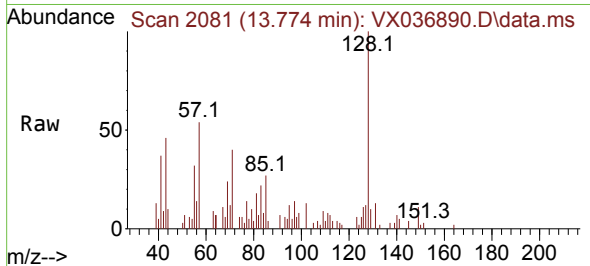

#96
1,2,3-Trichlorobenzene
Concen: 0.437 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX036890.D
Acq: 09 Aug 2023 16:20

Tgt Ion:180 Resp: 825
Ion Ratio Lower Upper
180 100
182 98.8 46.9 140.6
145 256.1 17.8 53.5#

