

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080924\
 Data File : VX043000.D
 Acq On : 09 Aug 2024 17:01
 Operator : JC/MD
 Sample : P3430-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 927-K1-WPO-0-0.25-073124-FD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M

Title : SW846 8260

Signal : TIC: VX043000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rBV	41820	34211	4.39%	0.776%
2	1.173	12	14	20	rVB3	9094	12729	1.63%	0.289%
3	1.374	44	47	51	rBV	22656	24459	3.14%	0.555%
4	1.599	70	84	85	rBV8	14858	45005	5.78%	1.021%
5	1.636	85	90	95	rVB6	20217	39558	5.08%	0.898%
6	2.136	166	172	180	rVB2	19091	32248	4.14%	0.732%
7	2.386	207	213	221	rBV2	7163	13695	1.76%	0.311%
8	3.093	323	329	338	rVB4	5475	10124	1.30%	0.230%
9	4.495	549	559	570	rBV2	8870	24957	3.20%	0.566%
10	5.032	640	647	659	rBV5	6006	18687	2.40%	0.424%
11	5.391	693	706	721	rBV	91138	271254	34.81%	6.155%
12	5.556	721	733	750	rVV	159530	457416	58.70%	10.378%
13	5.958	789	799	816	rBV	108368	284391	36.49%	6.453%
14	6.763	922	931	944	rBV	236421	569456	73.07%	12.920%
15	8.647	1234	1240	1248	rBV	487354	779307	100.00%	17.682%
16	8.720	1248	1252	1263	rVB	20761	38669	4.96%	0.877%
17	10.055	1465	1471	1482	rBV	483327	667325	85.63%	15.141%
18	11.079	1634	1639	1654	rBV	345008	482066	61.86%	10.938%
19	12.024	1788	1794	1806	rBV	444694	577929	74.16%	13.113%
20	13.122	1970	1974	1980	rBV2	8849	11590	1.49%	0.263%
21	13.780	2077	2082	2087	rBV	8813	12323	1.58%	0.280%




Sum of corrected areas: 4407399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080924\
Data File : VX043000.D
Acq On : 09 Aug 2024 17:01
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

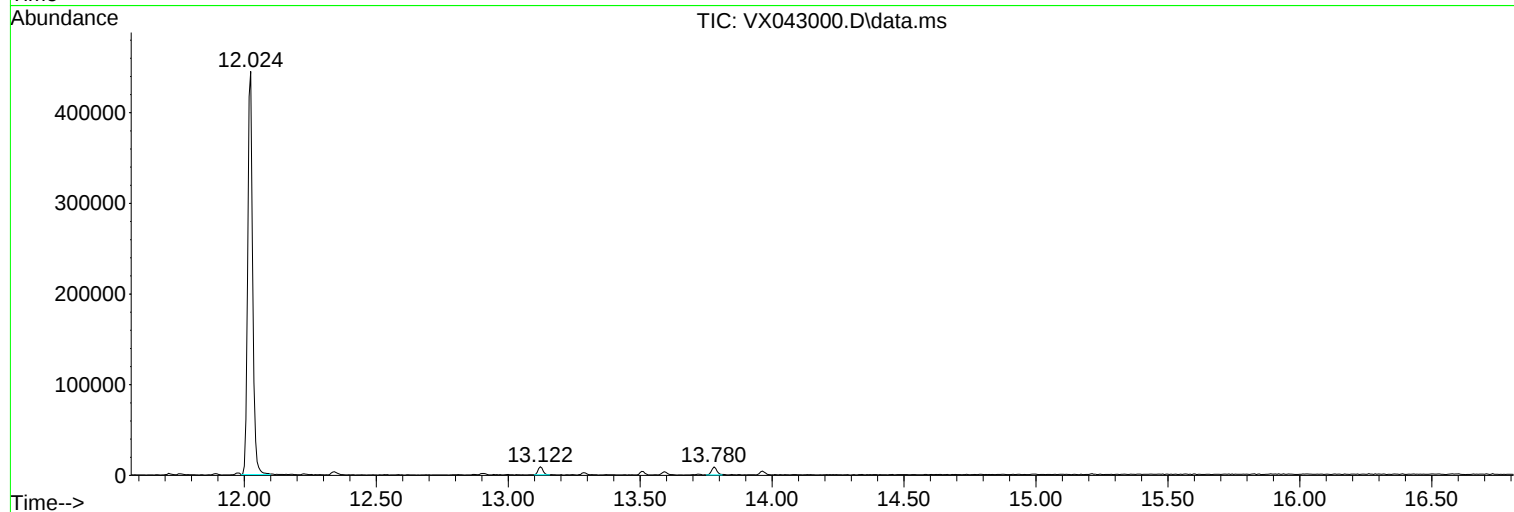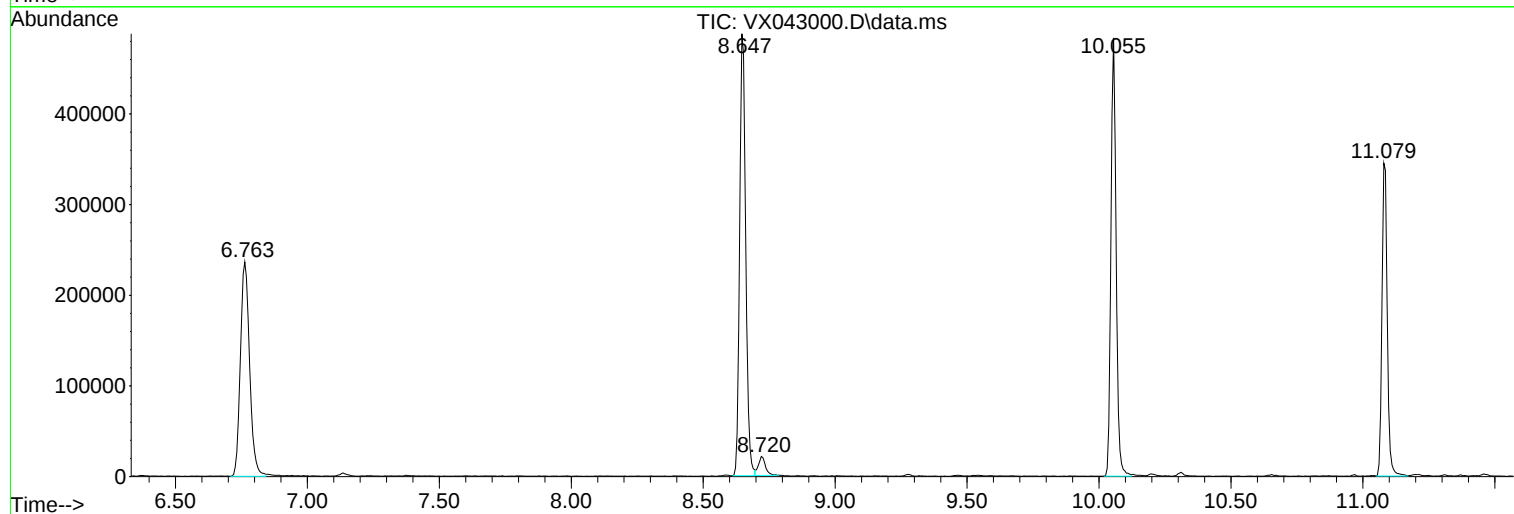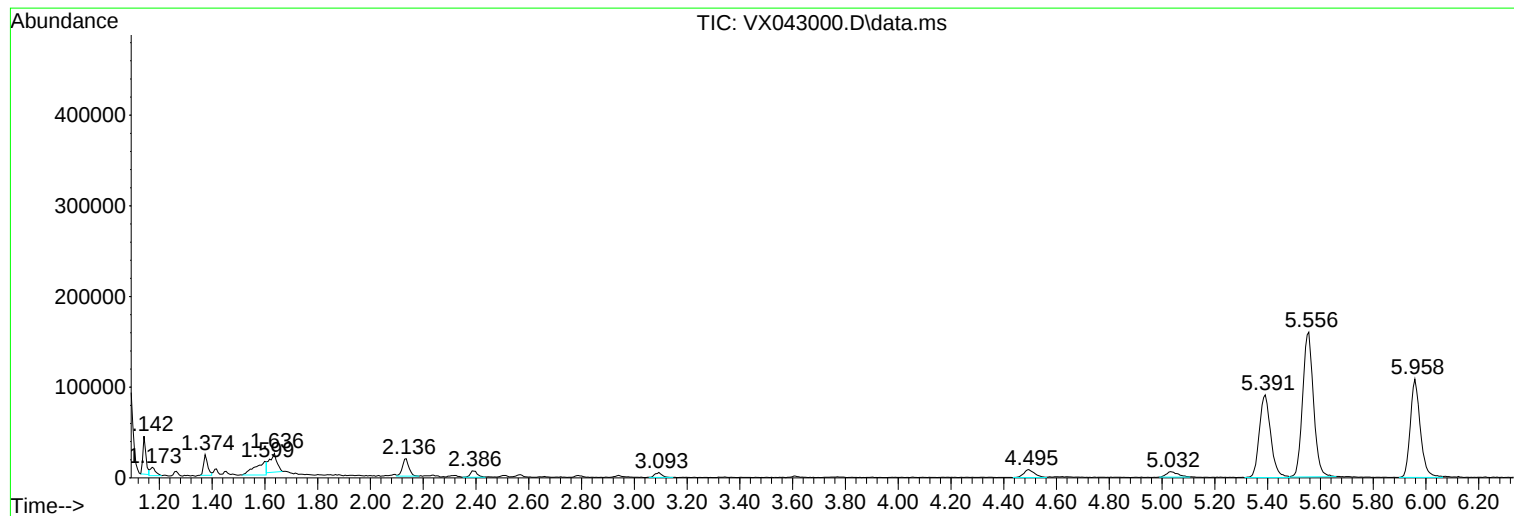

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080924\
Data File : VX043000.D
Acq On : 09 Aug 2024 17:01
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080924\
Data File : VX043000.D
Acq On : 09 Aug 2024 17:01
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------