
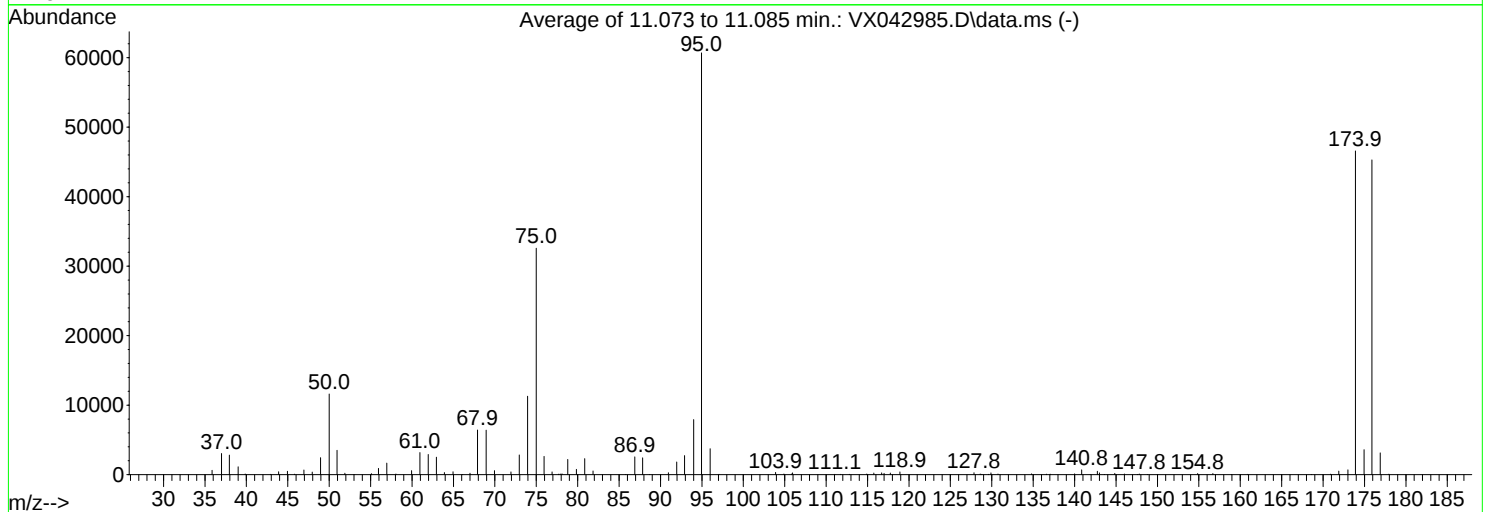


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080924\
Data File : VX042985.D
Acq On : 09 Aug 2024 10:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Title : SW846 8260
Last Update : Wed Aug 07 02:55:22 2024

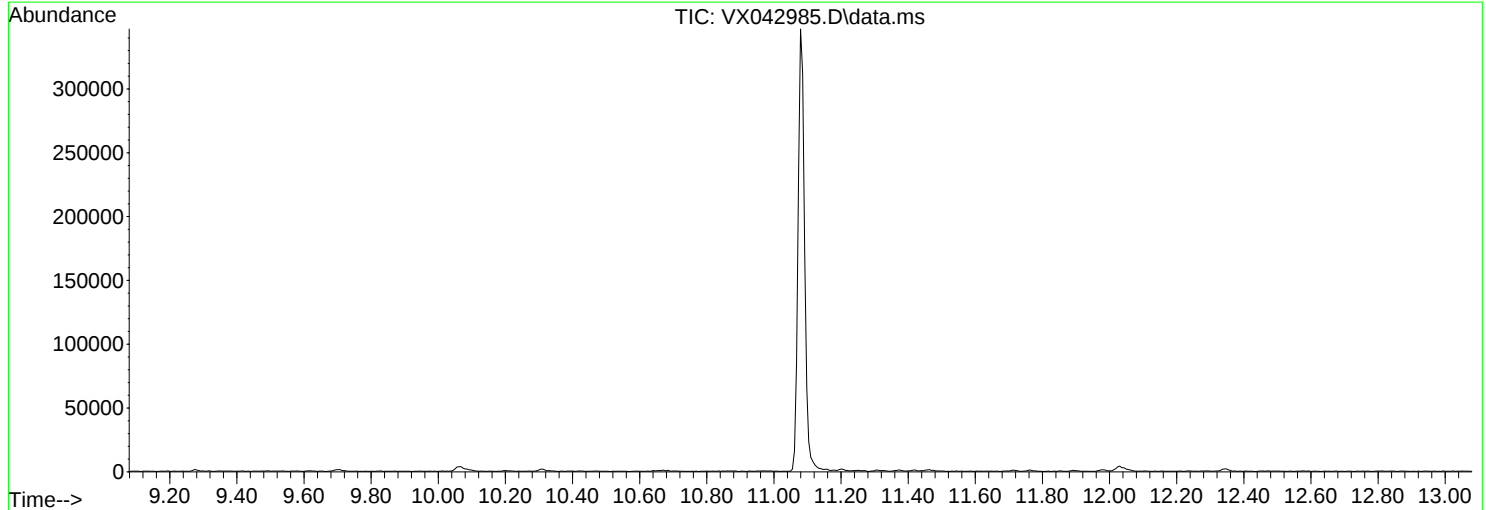

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	11610	PASS
75	95	30	60	53.7	32587	PASS
95	95	100	100	100.0	60691	PASS
96	95	5	9	6.1	3721	PASS
173	174	0.00	2	1.5	692	PASS
174	95	50	100	76.8	46584	PASS
175	174	5	9	7.7	3602	PASS
176	174	95	101	97.2	45277	PASS
177	176	5	9	6.9	3138	PASS