


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081018\
 Data File : VX003964.D
 Acq On : 10 Aug 2018 08:57
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
 Title : SW846 8260
 Last Update : Mon Aug 13 01:34:27 2018

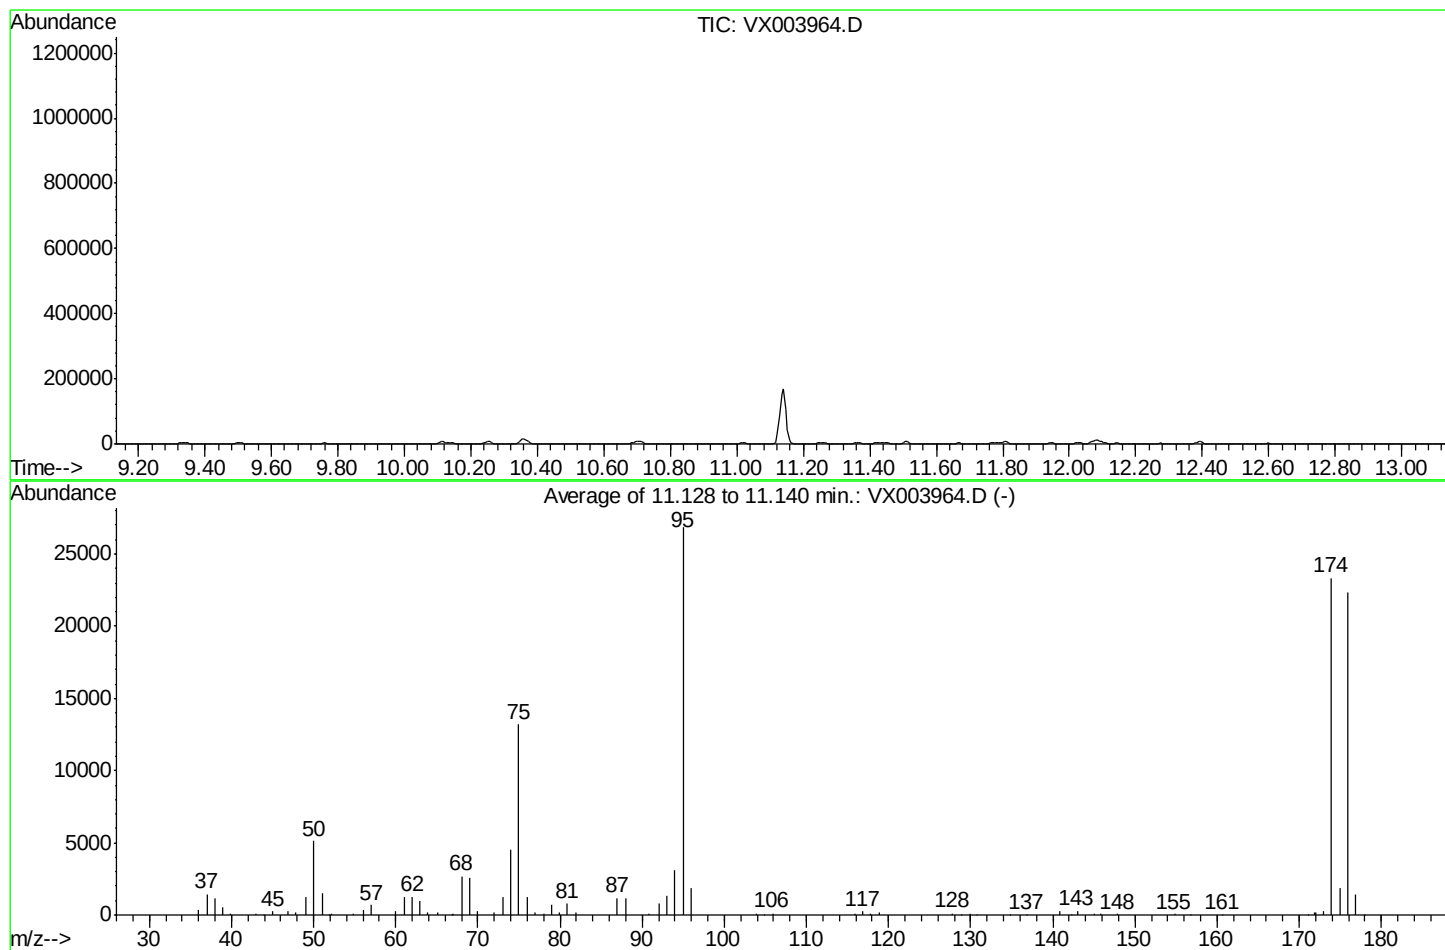

AutoFind: Scans 1729, 1730, 1731; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	5140	PASS
75	95	30	60	49.1	13186	PASS
95	95	100	100	100.0	26848	PASS
96	95	5	9	6.9	1861	PASS
173	174	0.00	2	1.0	242	PASS
174	95	50	100	87.0	23361	PASS
175	174	5	9	7.8	1829	PASS
176	174	95	101	95.5	22303	PASS
177	176	5	9	6.2	1387	PASS