

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081020\
 Data File : VX017841.D
 Acq On : 10 Aug 2020 11:21
 Operator : JC/SP
 Sample : VX0810WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK64

Quant Time: Aug 11 07:20:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 11 07:12:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	298951	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	275064	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	140759	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	95757	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	1.69	69	86276	5.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.20%
11) 1,1-Dichloroethene-d2	2.34	63	135339	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	4.53	46	292105	53.24	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.48%
24) Chloroform-d	5.14	84	213096	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	6.03	65	122188	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
32) Benzene-d6	6.04	84	362307	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	7.37	67	129465	5.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.00%
41) Toluene-d8	8.70	98	292041	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.20%
45) trans-1,3-Dichloropropene-	8.99	79	52878	5.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.60%
48) 2-Hexanone-d5	9.43	63	212275	50.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.04%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	96028	5.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.20%
65) 1,2-Dichlorobenzene-d4	12.36	152	143692	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds				Ovalue
16) Methylene chloride	2.83	84	12728	0.402 ug/L 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081020\
Data File : VX017841.D
Acq On : 10 Aug 2020 11:21
Operator : JC/SP
Sample : VX0810WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK64

Quant Time: Aug 11 07:20:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 11 07:12:14 2020
Response via : Initial Calibration

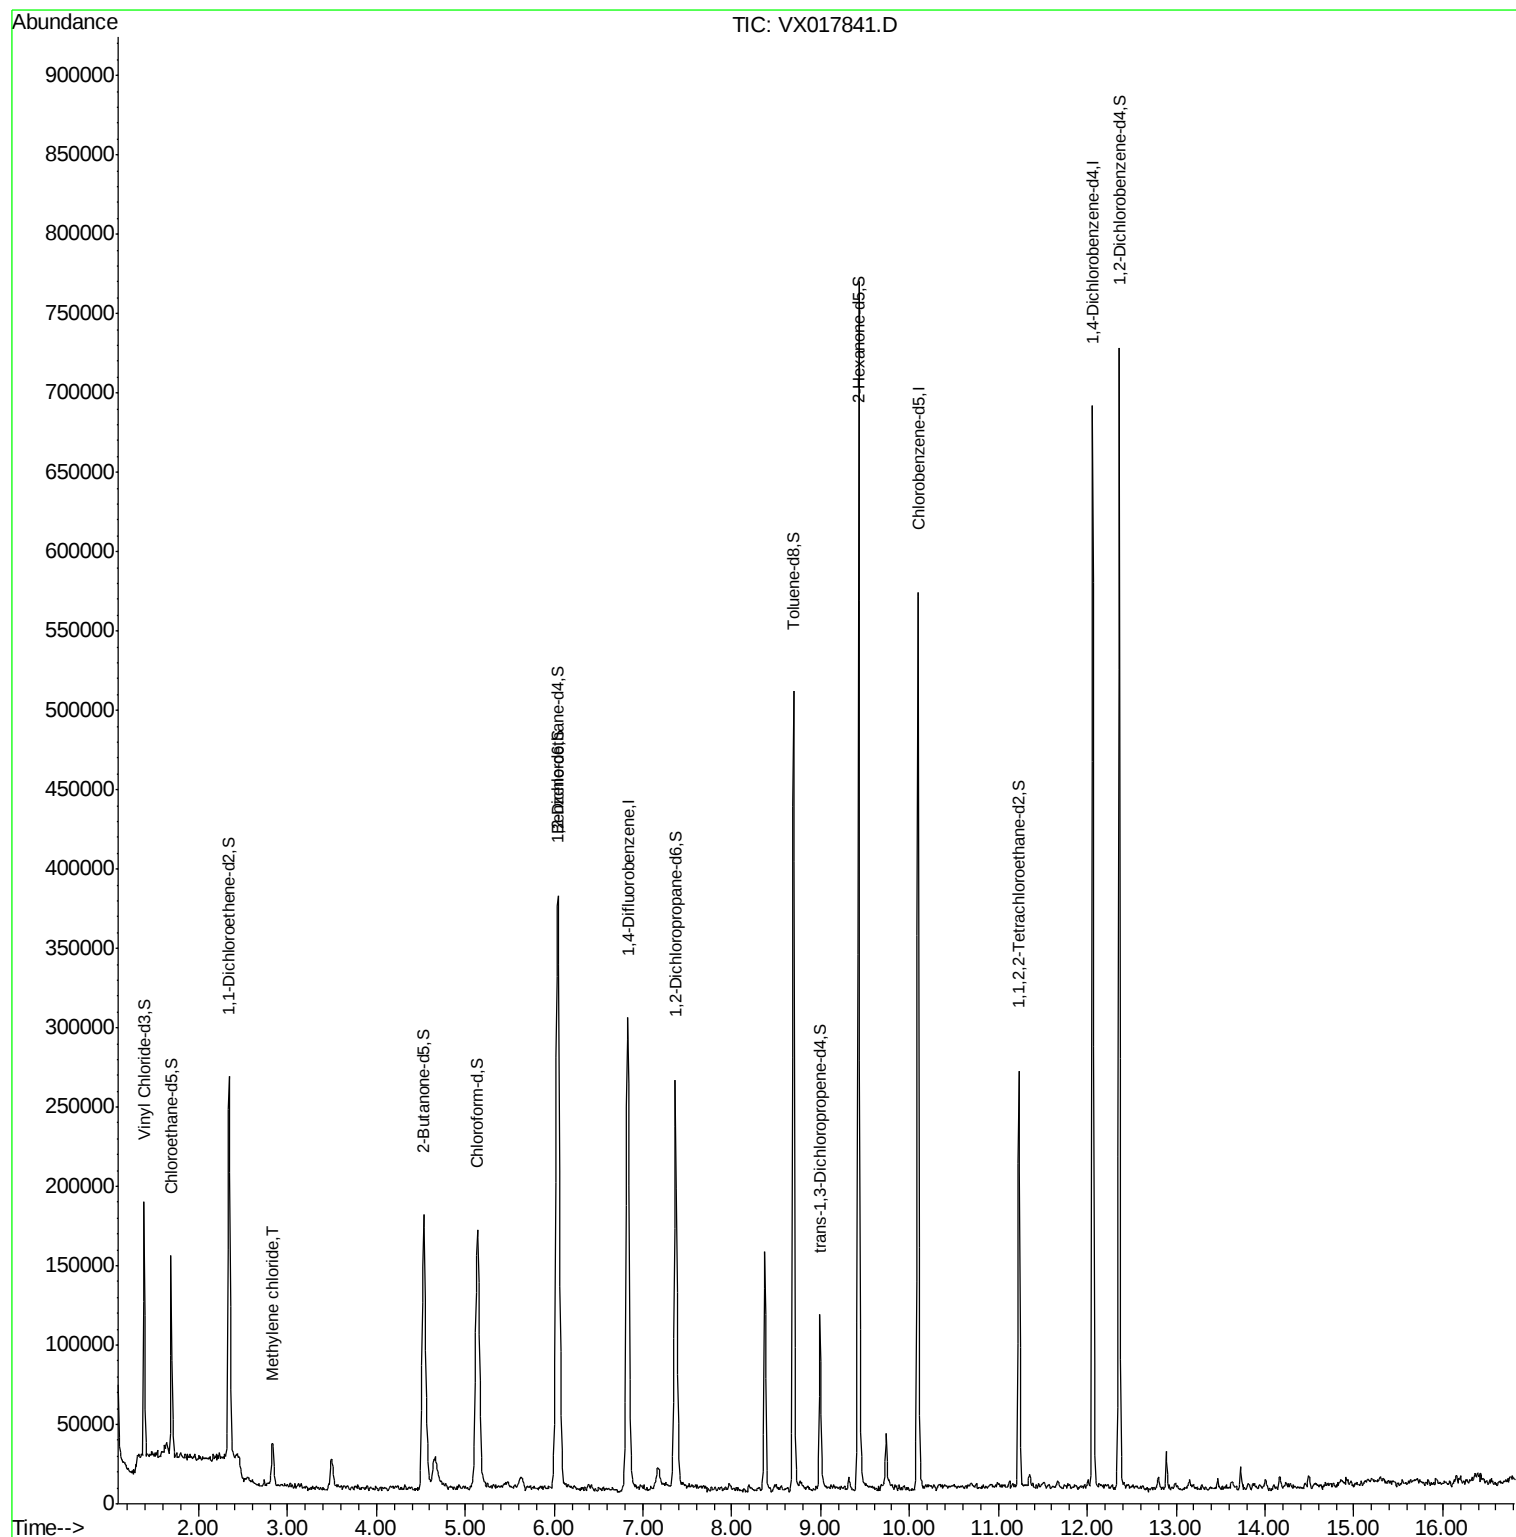

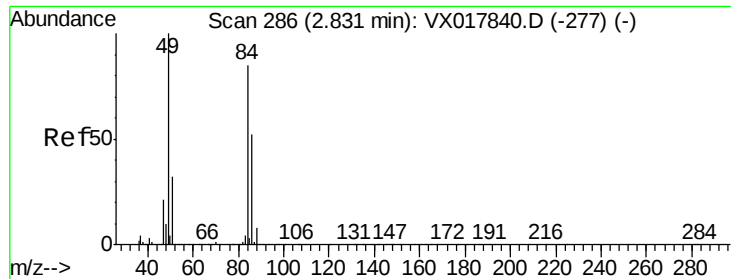

#16
 Methvlene chloride
 Concen: 0.402 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. -0.00 min
 Lab File: VX017841.D
 Acq: 10 Aug 2020 11:21

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK64

Tot Ion: 84 Resp: 12728
 Ion Ratio Lower Upper
 84 100
 86 71.0 43.0 80.0
 49 121.5 86.9 161.3

