


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081020\
 Data File : VX017839.D
 Acq On : 10 Aug 2020 08:51
 Operator : JC/SP
 Sample : BFB66
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB66

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 11 07:12:14 2020

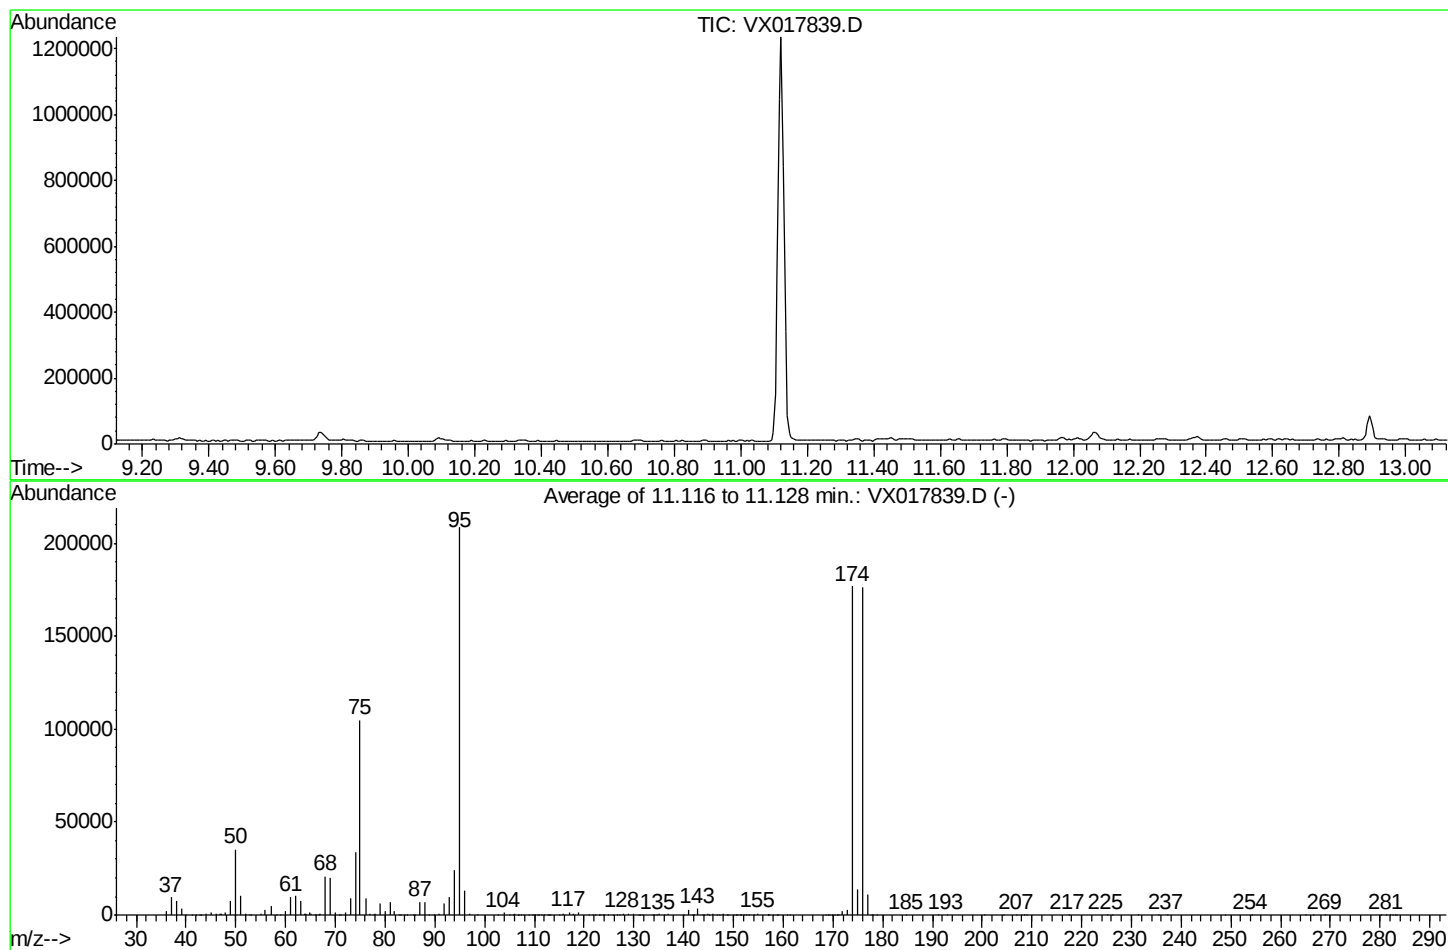

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	35408	PASS
75	95	30	80	50.2	104741	PASS
95	95	100	100	100.0	208546	PASS
96	95	5	9	6.4	13410	PASS
173	174	0.00	2	1.4	2556	PASS
174	95	50	120	84.7	176661	PASS
175	174	5	9	7.7	13677	PASS
176	174	95	101	99.8	176320	PASS
177	176	5	9	6.3	11133	PASS

m/z	Abundance
36.00	2454.0
37.00	11122.0
38.00	8699.0
39.00	4342.0
40.00	404.0
41.00	211.0
42.10	315.0
43.10	619.0
43.90	1698.0
45.10	1959.0
46.10	292.0
46.90	1615.0
48.00	1538.0
49.00	8110.0
50.00	40424.0
51.10	12318.0
52.00	536.0
52.70	226.0
53.10	226.0
54.10	177.0
54.90	586.0
56.00	3235.0
57.00	6137.0
58.00	123.0
59.00	93.0
60.10	1894.0
61.00	10695.0
62.00	11365.0
63.00	8864.0
63.90	961.0
64.30	967.0
65.00	1957.0
66.40	121.0
67.00	608.0
68.00	23336.0
69.00	21152.0
70.00	2240.0
70.80	206.0
72.10	1240.0
73.00	10634.0
74.00	36568.0
75.00	109808.0
76.10	9880.0
77.10	942.0
77.80	1152.0
78.90	6746.0
79.80	2109.0
80.90	7444.0
81.90	2099.0
82.90	155.0
86.10	642.0
87.00	7822.0
88.00	7558.0
90.90	926.0
92.00	6607.0
93.00	10067.0
94.00	26032.0
95.00	211520.0
96.00	13876.0
97.10	1048.0
98.50	56.0
102.90	128.0
103.80	1316.0
104.90	357.0
105.70	982.0
106.70	242.0
107.20	65.0
107.90	102.0
109.90	213.0
110.70	276.0
111.30	146.0
111.80	312.0
113.10	92.0
115.10	314.0
115.80	693.0
117.00	1734.0
117.80	812.0
118.80	1487.0
121.80	164.0
122.90	212.0
123.70	83.0
125.80	174.0
126.70	118.0
127.90	879.0
128.80	425.0
129.90	978.0
131.10	260.0
131.80	125.0
132.90	147.0
134.10	242.0
134.90	739.0
136.10	127.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

137.00	394.0
141.00	2465.0
142.10	521.0
142.90	2837.0
143.90	300.0
145.00	983.0
145.90	485.0
146.80	460.0
148.10	528.0
149.00	217.0
150.00	302.0
150.50	108.0
152.10	177.0
152.60	139.0
153.00	125.0
154.10	248.0
154.90	811.0
156.80	363.0
158.80	255.0
159.10	245.0
160.80	328.0
169.00	109.0
169.30	112.0
170.30	393.0
171.20	289.0
171.90	2272.0
173.00	2454.0
174.00	162816.0
175.00	12644.0
176.00	158528.0
177.00	9318.0
178.10	436.0
178.70	84.0
184.80	108.0
191.10	98.0
192.90	182.0
200.40	111.0
207.00	449.0
208.30	128.0
225.10	65.0
254.10	103.0
268.90	82.0
281.30	365.0
282.20	100.0
283.30	103.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
36.00	1948.0
37.00	11460.0
38.00	9640.0
39.00	3734.0
39.90	373.0
40.80	235.0
41.60	132.0
42.30	129.0
42.80	341.0
44.00	2100.0
45.00	1954.0
46.00	474.0
47.10	2185.0
47.90	1318.0
49.00	9238.0
50.00	40176.0
51.00	11873.0
51.90	231.0
52.20	273.0
52.90	303.0
55.00	852.0
56.00	3222.0
57.00	6096.0
58.10	254.0
58.90	215.0
59.90	2522.0
61.00	12244.0
62.00	11523.0
63.00	8726.0
64.10	1633.0
65.20	1690.0
65.90	385.0
67.00	1185.0
68.00	24792.0
69.00	25496.0
69.90	1623.0
71.00	264.0
72.00	1374.0
73.00	11672.0
74.00	39912.0
75.00	126568.0
76.10	10280.0
76.90	1322.0
78.00	537.0
79.00	7578.0
79.90	2134.0
81.00	8565.0
81.90	2232.0
83.00	330.0
83.80	180.0
86.00	360.0
87.00	8232.0
88.00	7004.0
88.80	572.0
89.70	62.0
90.80	1183.0
91.90	8241.0
93.00	10372.0
94.00	29384.0
95.00	250432.0
96.00	15231.0
97.00	437.0
102.70	246.0
103.90	1038.0
104.70	214.0
106.00	1421.0
106.90	367.0
107.90	69.0
109.60	161.0
110.10	234.0
110.90	290.0
111.70	261.0
112.90	463.0
115.00	462.0
115.90	1171.0
116.90	1606.0
117.90	1216.0
118.90	1758.0
122.20	59.0
123.20	194.0
124.00	118.0
124.90	106.0
125.80	189.0
126.70	76.0
127.80	1279.0
128.80	525.0
129.90	1181.0
130.80	471.0
131.80	149.0
132.90	88.0
134.00	120.0
135.00	566.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

136.00	221.0
136.90	578.0
139.80	289.0
141.00	2975.0
142.90	4525.0
143.80	220.0
144.20	197.0
144.90	650.0
145.90	672.0
147.10	353.0
148.10	736.0
148.70	238.0
149.90	366.0
150.70	93.0
151.70	70.0
152.60	109.0
153.90	362.0
154.90	867.0
155.70	61.0
156.90	502.0
157.20	504.0
157.90	63.0
158.90	460.0
160.70	292.0
168.40	157.0
169.20	114.0
169.90	148.0
170.90	278.0
171.80	2619.0
172.90	2651.0
174.00	204608.0
175.00	17000.0
176.00	213888.0
177.00	14222.0
178.20	228.0
178.70	100.0
191.10	74.0
192.80	142.0
193.30	72.0
200.40	69.0
204.30	102.0
207.00	728.0
207.90	140.0
231.30	84.0
237.20	101.0
248.90	58.0
254.10	78.0
266.60	76.0
267.50	50.0
281.20	424.0
282.60	82.0
283.00	148.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
36.00	1030.0
37.00	6890.0
38.00	5227.0
39.00	2747.0
40.00	583.0
41.10	248.0
42.00	132.0
43.00	241.0
44.00	1941.0
45.10	1111.0
46.00	458.0
46.90	1315.0
47.80	1009.0
49.00	5485.0
50.00	26000.0
51.00	7374.0
51.90	359.0
53.10	252.0
55.10	384.0
56.00	2242.0
57.00	3549.0
57.80	216.0
58.80	211.0
59.90	1743.0
61.00	7063.0
62.00	7396.0
63.00	5920.0
63.80	628.0
64.90	1230.0
66.20	341.0
66.60	234.0
67.10	185.0
68.00	14738.0
69.00	14349.0
70.10	1066.0
71.10	212.0
72.10	1177.0
72.90	6422.0
74.00	24896.0
75.00	77848.0
76.00	6447.0
77.00	795.0
77.90	776.0
78.90	4683.0
80.00	1522.0
80.90	5206.0
82.00	1196.0
83.20	246.0
83.80	246.0
84.30	65.0
85.70	157.0
87.00	5470.0
87.90	5165.0
90.20	94.0
90.90	1086.0
92.00	4317.0
93.00	7618.0
94.00	17024.0
95.00	164032.0
96.00	11123.0
97.00	318.0
102.60	124.0
103.90	885.0
104.90	274.0
105.90	671.0
106.80	284.0
107.90	92.0
108.80	58.0
109.90	172.0
110.90	243.0
111.90	209.0
112.70	292.0
113.20	127.0
114.90	305.0
116.00	798.0
116.90	1651.0
117.70	679.0
118.90	1472.0
121.00	70.0
121.80	109.0
124.00	64.0
125.90	309.0
126.70	84.0
127.10	210.0
127.80	855.0
128.90	356.0
129.90	667.0
130.90	400.0
131.90	67.0
132.90	74.0
133.80	180.0
134.60	287.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

135.00	275.0
135.90	73.0
136.80	536.0
139.90	292.0
140.90	2459.0
141.70	296.0
142.10	162.0
142.90	2837.0
143.90	319.0
145.20	350.0
146.00	441.0
146.60	215.0
147.90	612.0
149.10	103.0
149.80	373.0
151.30	63.0
151.60	74.0
153.00	167.0
154.00	221.0
155.00	648.0
155.70	83.0
157.00	419.0
158.90	246.0
160.70	175.0
161.20	184.0
168.40	94.0
169.70	223.0
170.70	345.0
171.90	1967.0
173.10	2565.0
174.00	162560.0
175.00	11388.0
176.00	156544.0
177.00	9859.0
177.90	250.0
178.10	241.0
178.80	80.0
190.70	61.0
191.10	161.0
192.80	220.0
206.90	433.0
207.90	228.0
208.80	72.0
217.30	58.0
226.10	59.0
235.30	60.0
248.90	82.0
265.10	55.0
280.20	102.0
281.00	447.0
282.00	68.0
282.90	176.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
35.70	85.0
36.50	169.0
37.20	209.0
38.10	200.0
39.10	253.0
39.80	297.0
41.00	228.0
41.50	174.0
42.50	248.0
43.00	197.0
44.00	879.0
45.00	151.0
45.80	85.0
46.80	144.0
47.80	228.0
48.80	97.0
49.30	57.0
50.20	125.0
51.00	180.0
52.10	109.0
54.30	160.0
54.70	145.0
55.80	111.0
57.10	81.0
57.80	78.0
59.70	61.0
62.20	81.0
64.70	102.0
67.00	67.0
70.00	80.0
73.10	367.0
74.10	172.0
75.30	63.0
77.10	149.0
77.70	97.0
78.40	81.0
80.20	83.0
81.00	80.0
86.30	65.0
87.30	55.0
90.00	96.0
90.90	75.0
94.80	64.0
95.20	51.0
102.70	131.0
107.00	78.0
116.30	117.0
117.80	92.0
119.30	63.0
131.60	80.0
132.80	150.0
133.10	144.0
155.60	72.0
176.40	65.0
178.80	59.0
181.40	52.0
190.90	83.0
192.30	51.0
193.20	96.0
195.00	62.0
207.00	397.0
207.90	77.0
209.10	96.0
228.80	82.0
230.00	70.0
254.50	64.0
267.30	233.0
280.80	182.0
281.50	244.0
296.10	56.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66