

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081021\
 Data File : VX023634.D
 Acq On : 10 Aug 2021 14:13
 Operator : JC/MD
 Sample : M3326-01ME
 Misc : 6.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 11 03:00:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	156136	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	264255	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	235712	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	89870	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	103088	52.929	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 105.860%			
35) Dibromofluoromethane	5.397	113	82167	49.731	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.460%			
50) Toluene-d8	8.653	98	319093	52.566	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 105.140%			
62) 4-Bromofluorobenzene	11.085	95	105756	51.234	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 102.460%			
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	445	0.266	ug/l	97
5) Bromomethane	1.611	94	621	0.618	ug/l #	55
10) Methyl Iodide	2.465	142	1147	0.592	ug/l #	88
11) Tert butyl alcohol	2.959	59	586	1.317	ug/l #	73
13) Acrolein	2.227	56	59	1.623	ug/l #	14
16) Acetone	2.392	43	1689	1.768	ug/l #	84
17) Carbon Disulfide	2.514	76	798	0.211	ug/l #	88
20) Methylene Chloride	2.794	84	1500	0.807	ug/l #	83
31) Cyclohexane	5.507	56	2271	0.787	ug/l #	41
36) 1,1-Dichloropropene	5.556	75	12281	5.137	ug/l #	50
38) Carbon Tetrachloride	5.562	117	16236	6.679	ug/l #	16
39) Methylcyclohexane	7.391	83	3203	1.061	ug/l	88
53) t-1,3-Dichloropropene	8.988	75	138	1.863	ug/l #	44
55) 1,1,2-Trichloroethane	9.110	97	650	0.366	ug/l #	15
59) 2-Hexanone	9.439	43	502	0.231	ug/l	61
67) Ethyl Benzene	10.195	91	20181	2.412	ug/l	100
68) m/p-Xylenes	10.305	106	26203	8.143	ug/l	97
69) o-Xylene	10.640	106	671	0.210	ug/l	90
73) Isopropylbenzene	10.963	105	8372	1.235	ug/l	99
76) 1,2,3-Trichloropropane	11.085	75	55658	28.143	ug/l #	39
78) n-propylbenzene	11.305	91	13086	1.705	ug/l	99
79) 2-Chlorotoluene	11.402	91	11161	2.434	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	88626	16.048	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	55658	75.674	ug/l #	12
82) 4-Chlorotoluene	11.457	91	10486	2.021	ug/l #	48
83) tert-Butylbenzene	11.756	119	17088	3.154	ug/l #	53
84) 1,2,4-Trimethylbenzene	11.756	105	137513	25.033	ug/l	97
85) sec-Butylbenzene	11.896	105	6609	0.941	ug/l	98
86) p-Isopropyltoluene	11.969	119	4904	0.865	ug/l	95
89) n-Butylbenzene	12.323	91	15938	3.104	ug/l #	1
90) Hexachloroethane	12.536	117	5232	6.853	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.963	75	338	2.723	ug/l #	1
93) 1,2,4-Trichlorobenzene	13.591	180	392	0.213	ug/l #	72
94) Hexachlorobutadiene	13.725	225	167	0.202	ug/l #	47
95) Naphthalene	13.780	128	6847	1.082	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081021\
Data File : VX023634.D
Acq On : 10 Aug 2021 14:13
Operator : JC/MD
Sample : M3326-01ME
Misc : 6.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Aug 11 03:00:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081021\
Data File : VX023634.D
Acq On : 10 Aug 2021 14:13
Operator : JC/MD
Sample : M3326-01ME
Misc : 6.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Aug 11 03:00:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




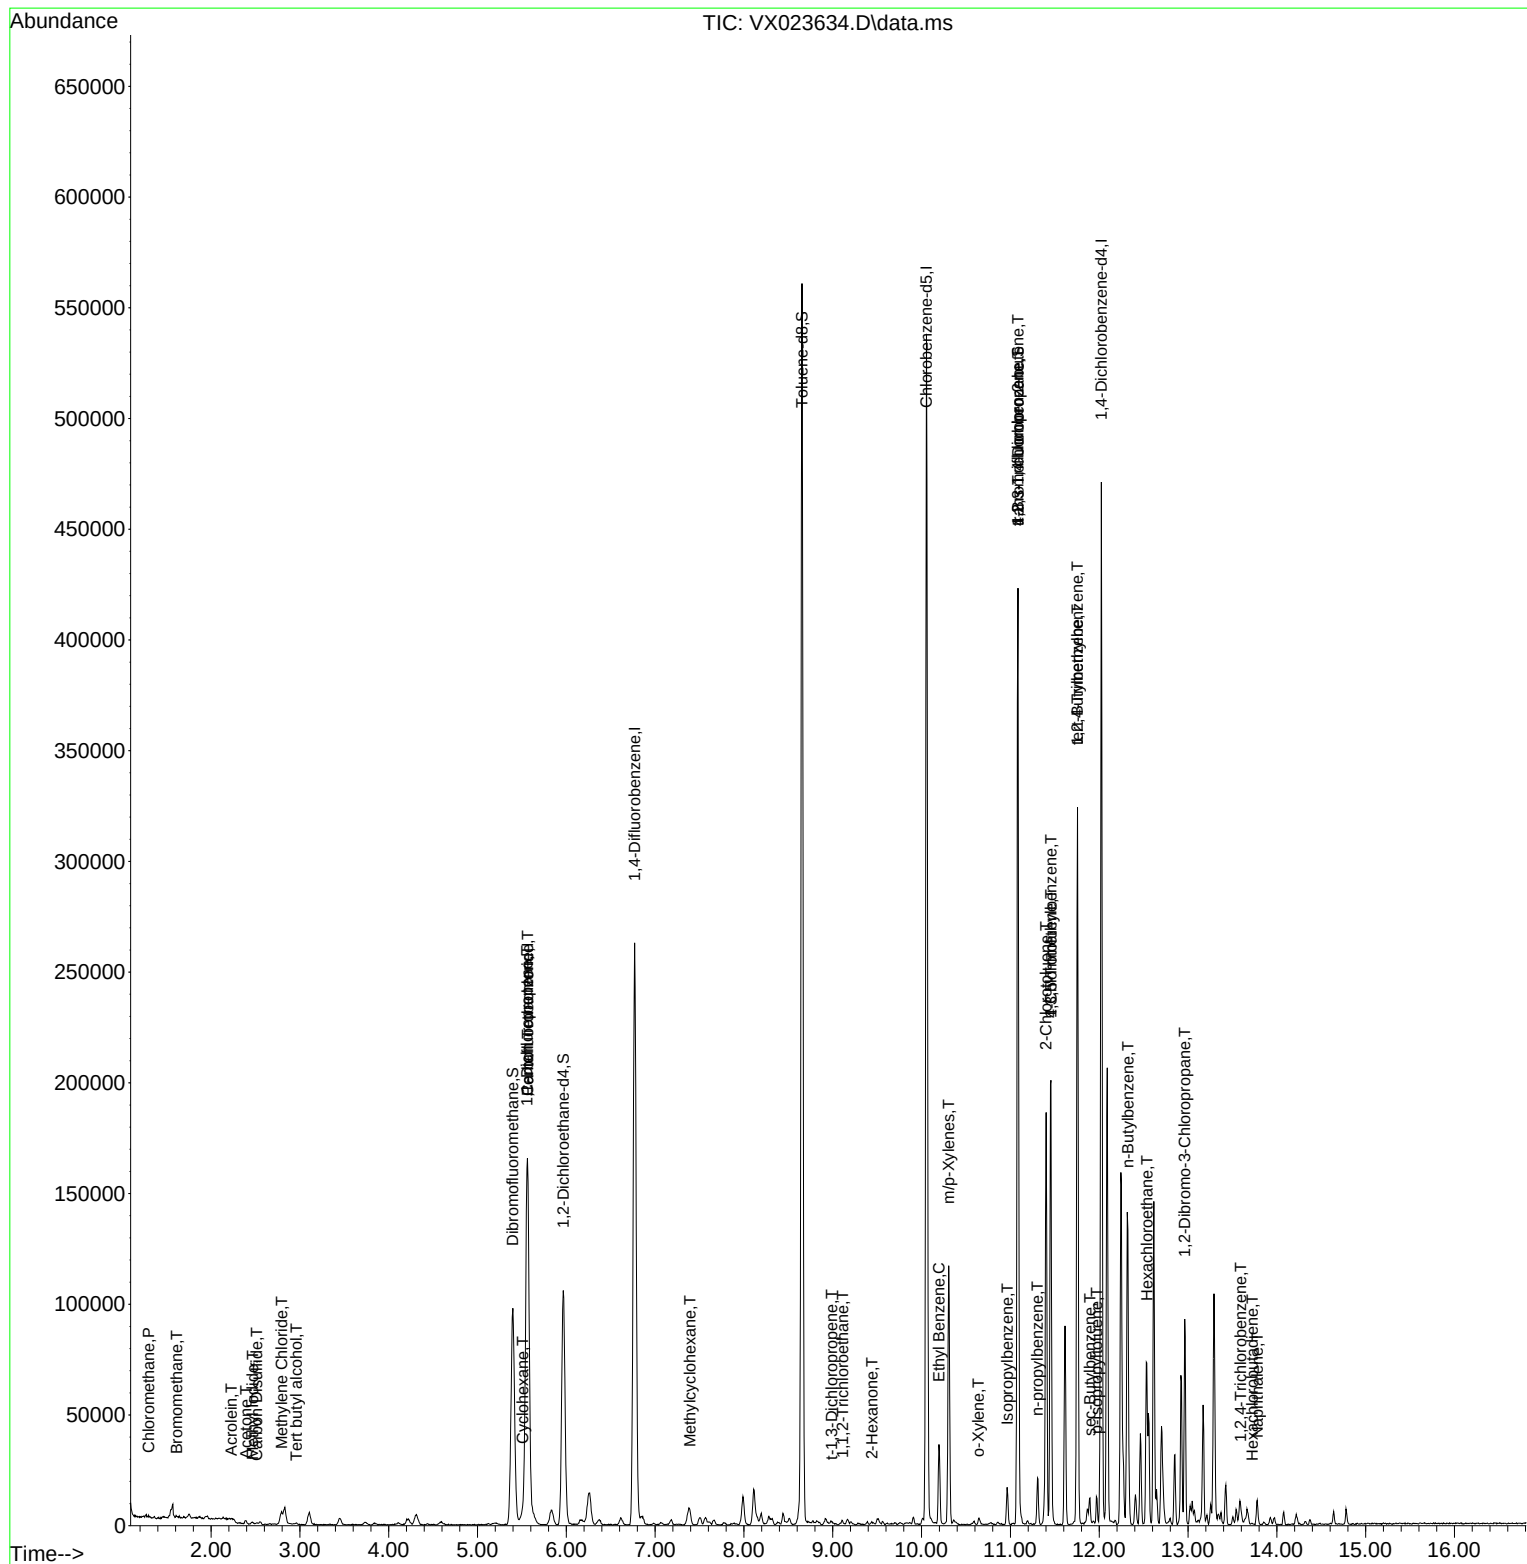




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 156136
Ion Ratio Lower Upper
168 100
99 57.2 45.8 68.6

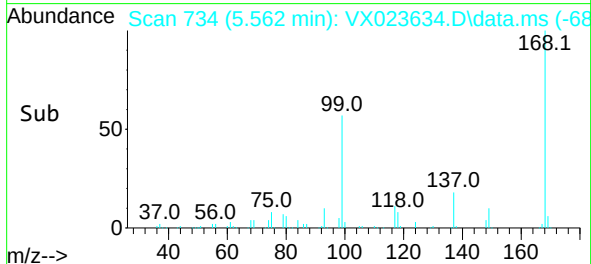

#3
Chloromethane
Concen: 0.266 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 50 Resp: 445
Ion Ratio Lower Upper
50 100
52 34.9 26.4 39.6




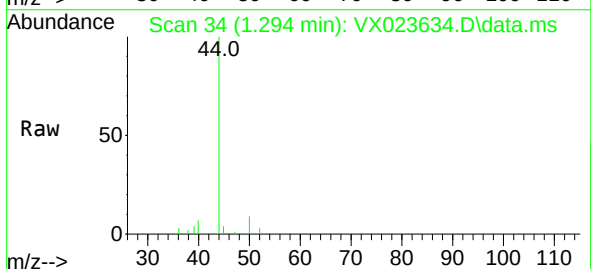


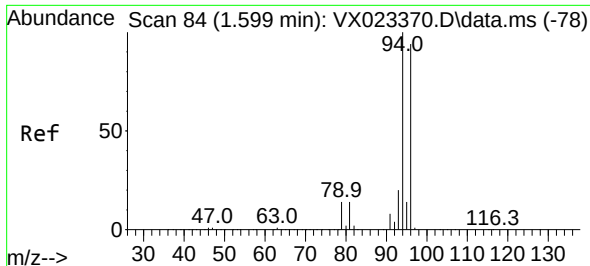

#5
Bromomethane
Concen: 0.618 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 621
Ion Ratio Lower Upper
94 100
96 51.2 76.4 114.6#

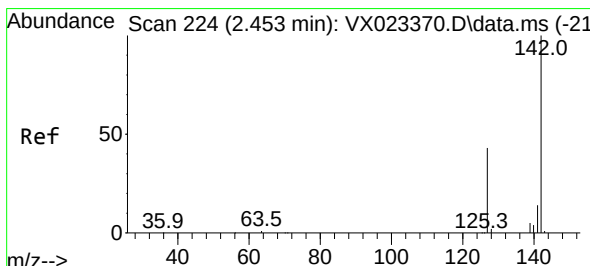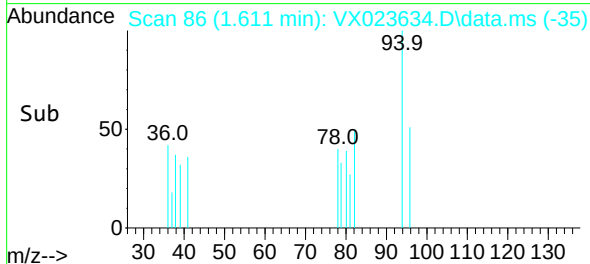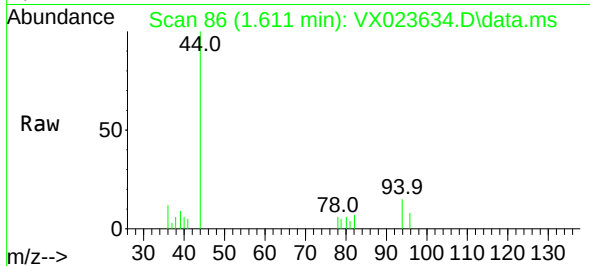

#10
Methyl Iodide
Concen: 0.592 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 142 Resp: 1147
Ion Ratio Lower Upper
142 100
127 35.0 33.3 49.9
141 6.7 11.4 17.0#

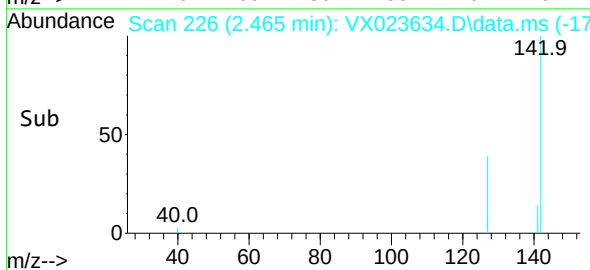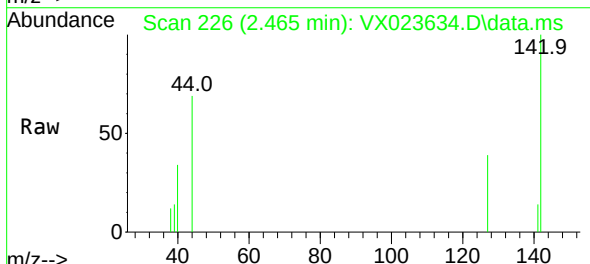







#11

Tert butyl alcohol
Concen: 1.317 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.024 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 59 Resp: 586
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#






#13

Acrolein
Concen: 1.623 ug/l
RT: 2.227 min Scan# 187
Delta R.T. -0.012 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13



Tgt Ion: 56 Resp: 59
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#



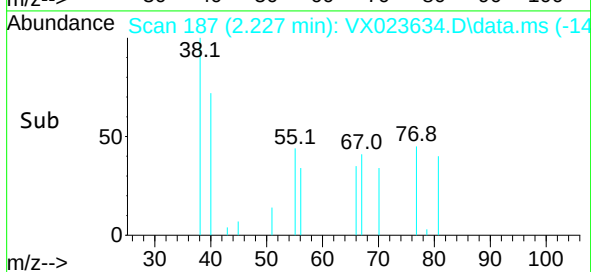



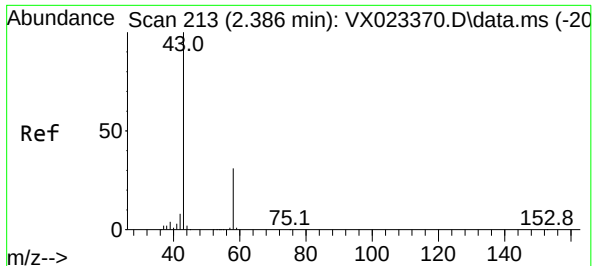

#16
Acetone
Concen: 1.768 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1689
Ion Ratio Lower Upper
43 100
58 25.3 27.8 41.8#

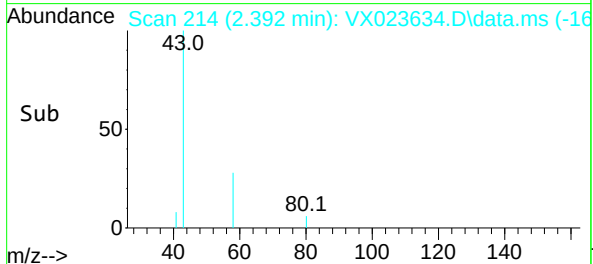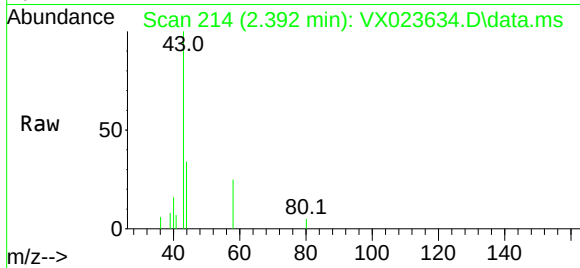

#17
Carbon Disulfide
Concen: 0.211 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13


Tgt Ion: 76 Resp: 798
Ion Ratio Lower Upper
76 100
78 13.2 7.2 10.8#

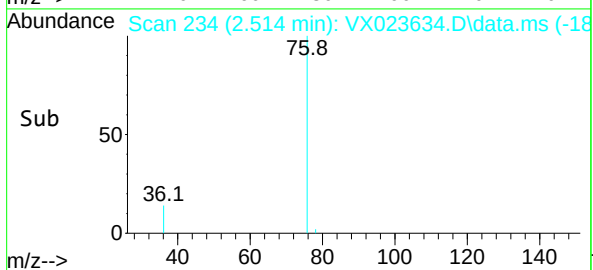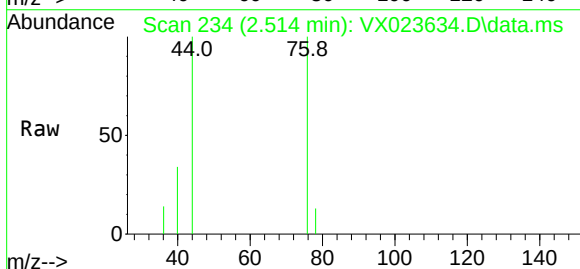



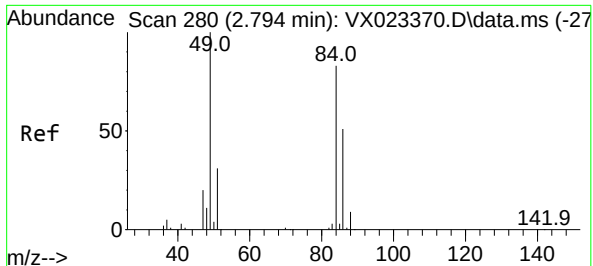


#20
Methylene Chloride
Concen: 0.807 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion:	84	Resp:	1500
Ion	Ratio	Lower	Upper
84	100		
49	128.5	88.6	132.8
51	47.6	27.0	40.6#
86	73.0	50.3	75.5

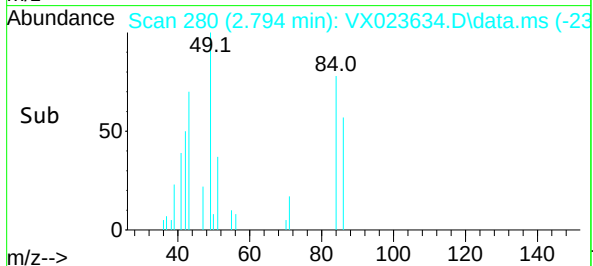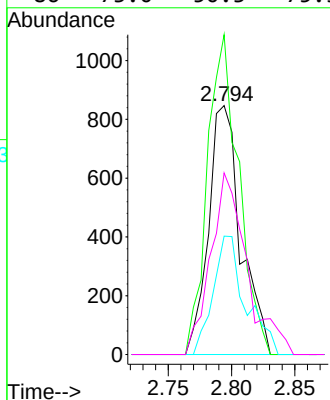

#31
Cyclohexane
Concen: 0.787 ug/l
RT: 5.507 min Scan# 725
Delta R.T. 0.030 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion:	56	Resp:	2271
Ion	Ratio	Lower	Upper
56	100		
69	13.2	25.3	37.9#
84	25.2	71.4	107.0#

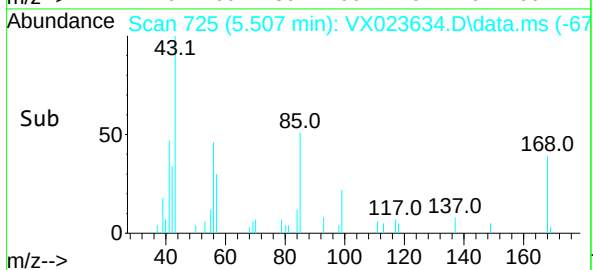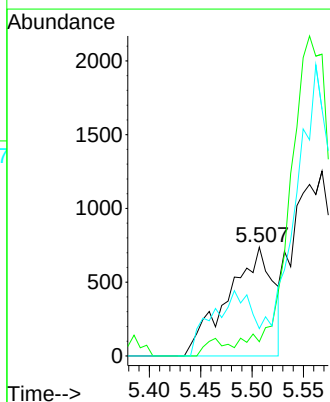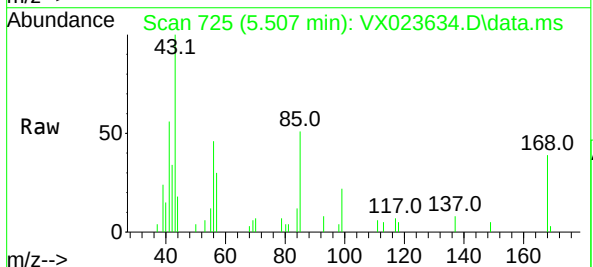

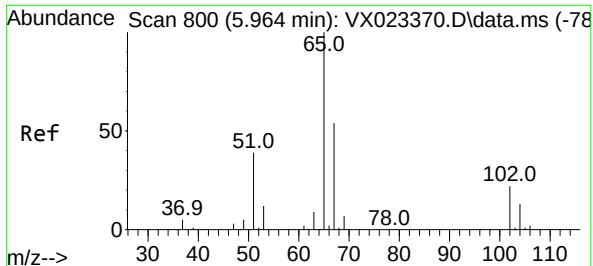

#33

1,2-Dichloroethane-d4

Concen: 52.929 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX023634.D





Acq: 10 Aug 2021 14:13

Tgt Ion: 65 Resp: 103088

Ion Ratio Lower Upper

65 100

67 51.0 0.0 105.4

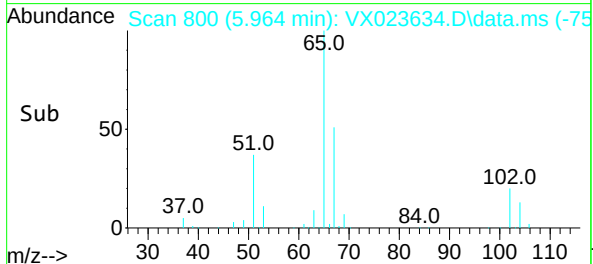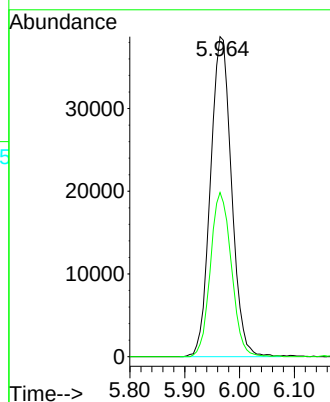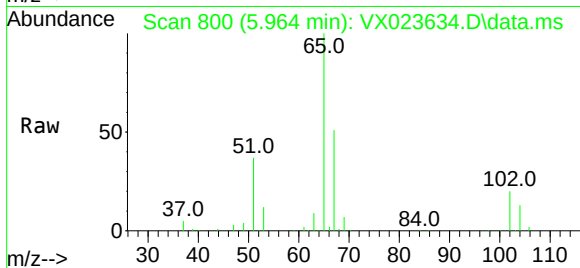

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX023634.D

Acq: 10 Aug 2021 14:13




Tgt Ion: 114 Resp: 264255


Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.8

88 15.2 0.0 32.8

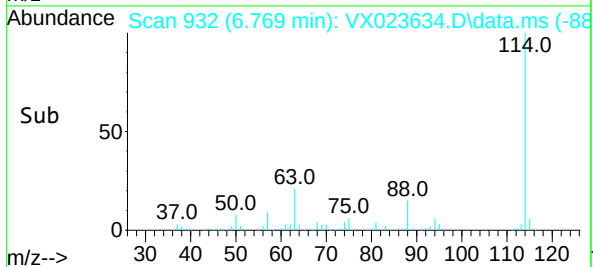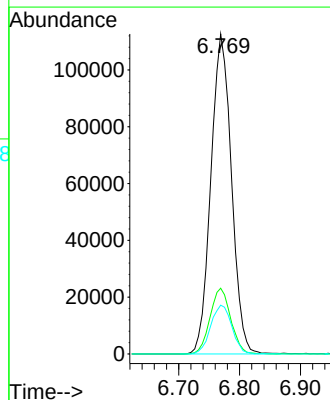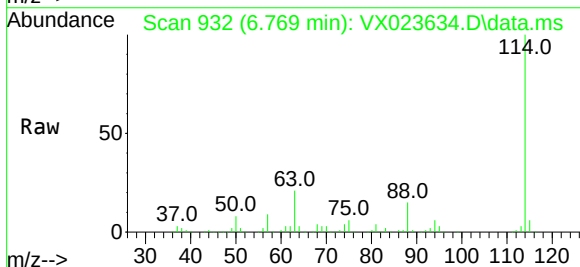

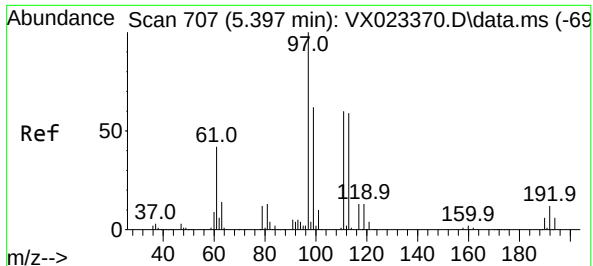

#35

Dibromofluoromethane

Concen: 49.731 ug/l

RT: 5.397 min Scan# 707





Delta R.T. 0.000 min

Lab File: VX023634.D

Acq: 10 Aug 2021 14:13

Tgt Ion:	113	Resp:	82167
Ion	Ratio	Lower	Upper
113	100		
111	101.5	81.9	122.9
192	19.5	16.7	25.1

Instrument :
MSVOA_X
ClientSampleId :

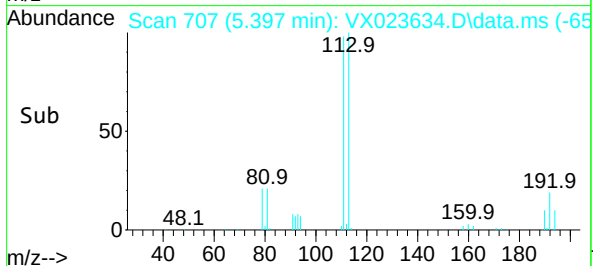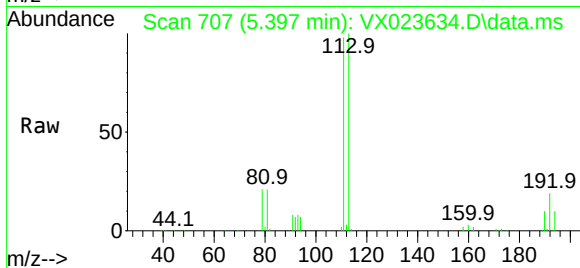

#36

1,1-Dichloropropene

Concen: 5.137 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.140 min

Lab File: VX023634.D

Acq: 10 Aug 2021 14:13


Tgt Ion:	75	Resp:	12281
Ion	Ratio	Lower	Upper
75	100		
110	10.5	18.1	54.4#
77	0.0	25.3	37.9#

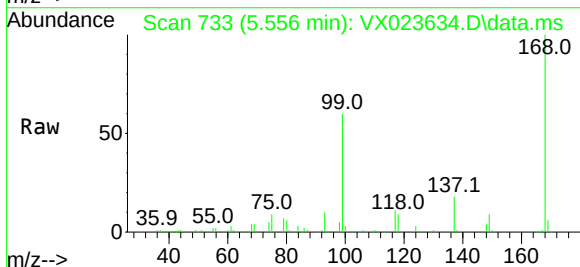



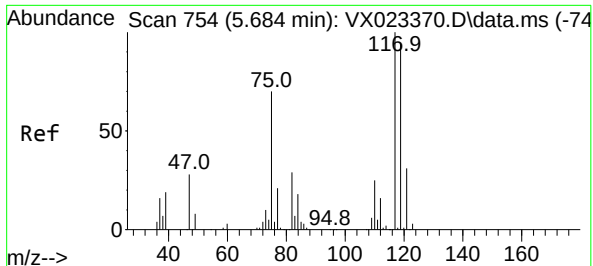


#38
Carbon Tetrachloride
Concen: 6.679 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13


Instrument :
MSVOA_X
ClientSampled :

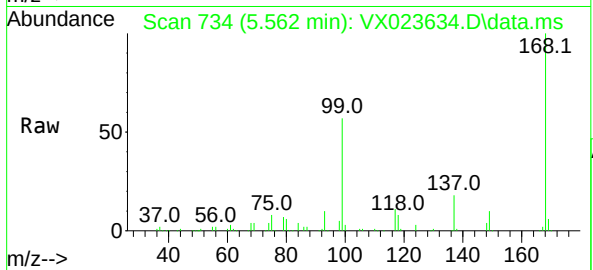



Tgt Ion:117 Resp: 16236
Ion Ratio Lower Upper
117 100
119 5.2 76.2 114.2#
121 0.0 24.8 37.2#

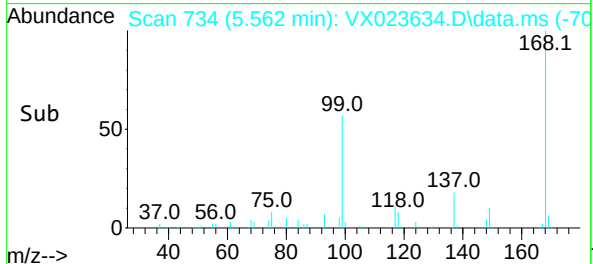


#39
Methylcyclohexane
Concen: 1.061 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

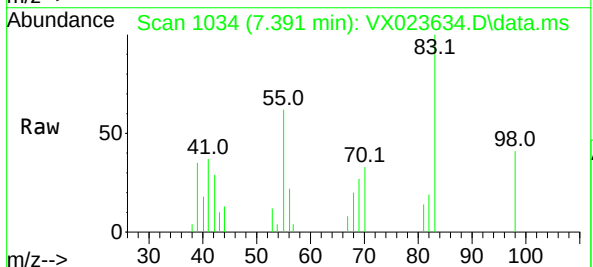

Tgt Ion: 83 Resp: 3203
Ion Ratio Lower Upper
83 100
55 62.4 58.9 88.3
98 40.8 38.1 57.1









#50
Toluene-d8
Concen: 52.566 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 319093
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9

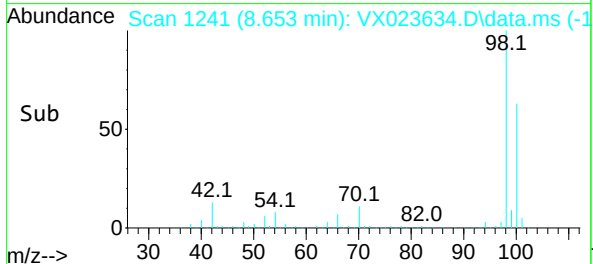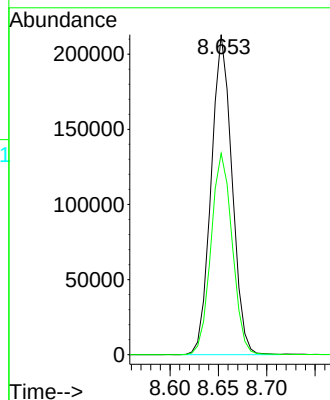

#53
t-1,3-Dichloropropene
Concen: 1.863 ug/l
RT: 8.988 min Scan# 1296
Delta R.T. 0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 75 Resp: 138
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#

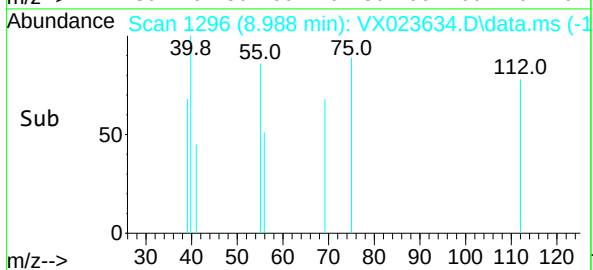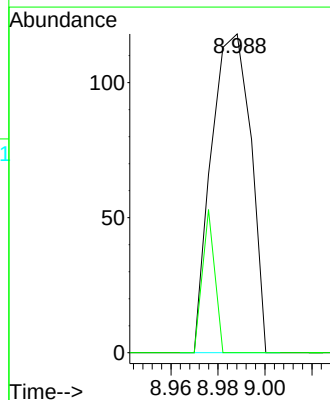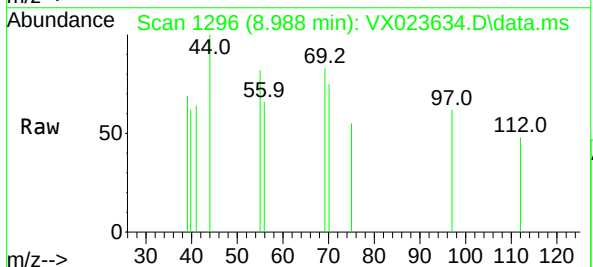




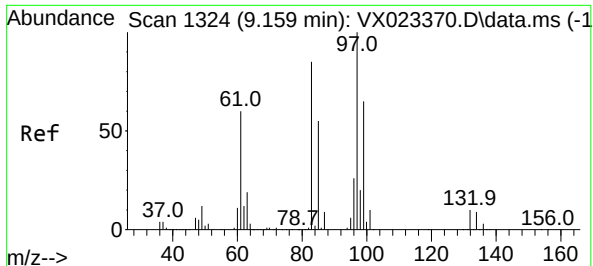


#55
 1,1,2-Trichloroethane
 Concen: 0.366 ug/l
 RT: 9.110 min Scan# 1316
 Delta R.T. -0.049 min
 Lab File: VX023634.D
 Acq: 10 Aug 2021 14:13

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 97 Resp: 650




Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#

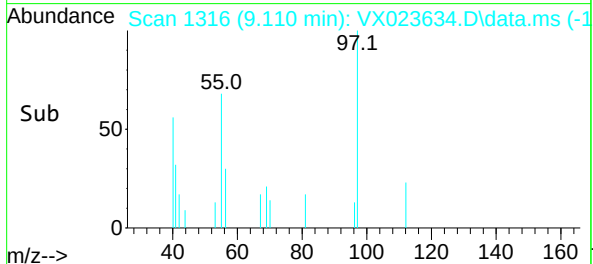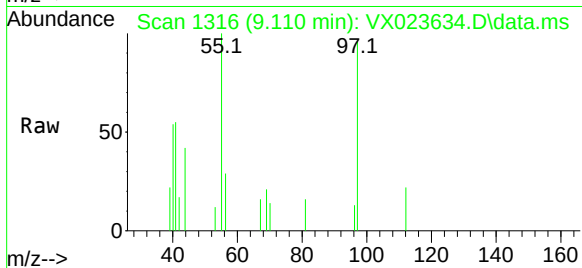


#59
 2-Hexanone
 Concen: 0.231 ug/l
 RT: 9.439 min Scan# 1370
 Delta R.T. 0.006 min
 Lab File: VX023634.D
 Acq: 10 Aug 2021 14:13

Tgt Ion: 43 Resp: 502

Ion	Ratio	Lower	Upper
43	100		
58	32.3	30.9	92.8


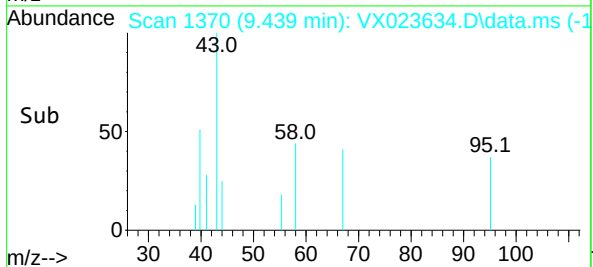

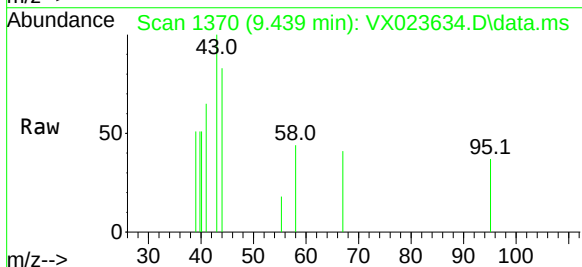




#62
4-Bromofluorobenzene
Concen: 51.234 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 105756
Ion Ratio Lower Upper
95 100
174 79.2 0.0 154.6
176 78.1 0.0 155.8

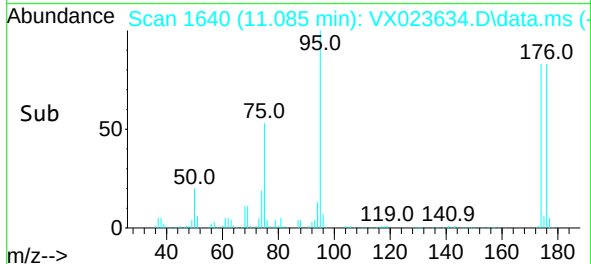

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 117 Resp: 235712
Ion Ratio Lower Upper
117 100
82 57.1 47.4 71.2
119 33.3 26.6 39.8


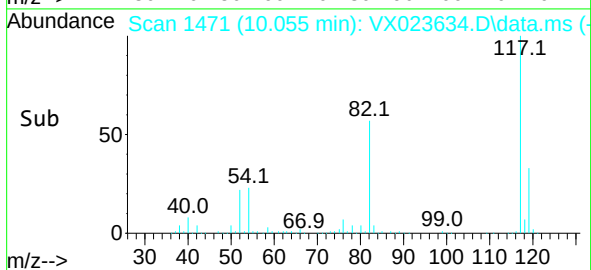

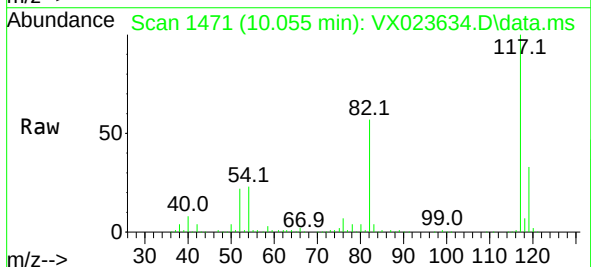




#67
Ethyl Benzene
Concen: 2.412 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 20181
Ion Ratio Lower Upper
91 100
106 30.7 24.6 37.0

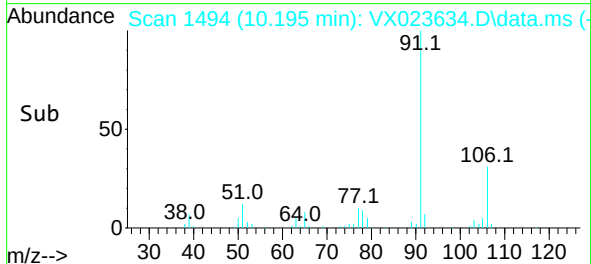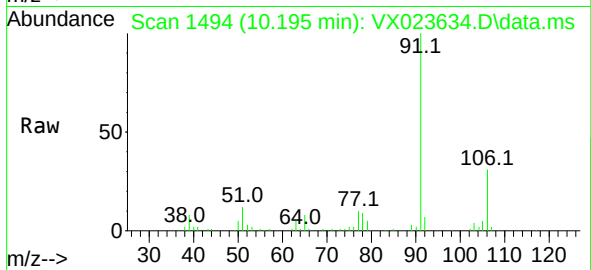

#68
m/p-Xylenes
Concen: 8.143 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 106 Resp: 26203
Ion Ratio Lower Upper
106 100
91 208.3 162.8 244.2




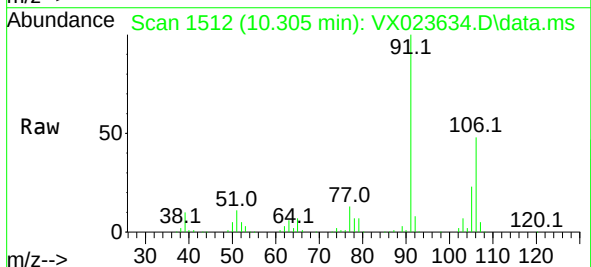




#69
o-Xylene
Concen: 0.210 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 671
Ion Ratio Lower Upper
106 100
91 200.7 108.1 324.2

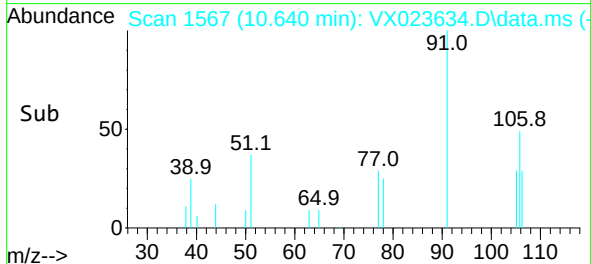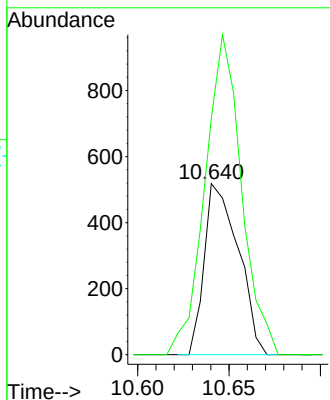

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion:152 Resp: 89870
Ion Ratio Lower Upper
152 100
115 60.4 41.1 123.3
150 158.8 0.0 349.0

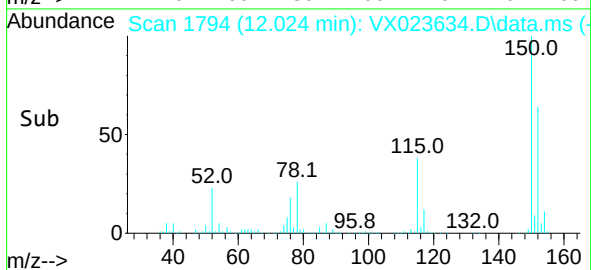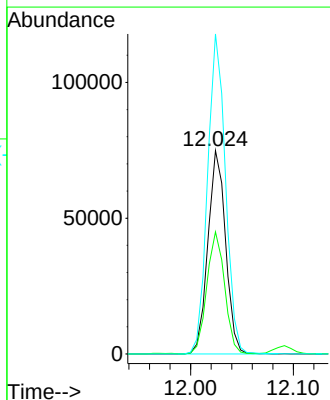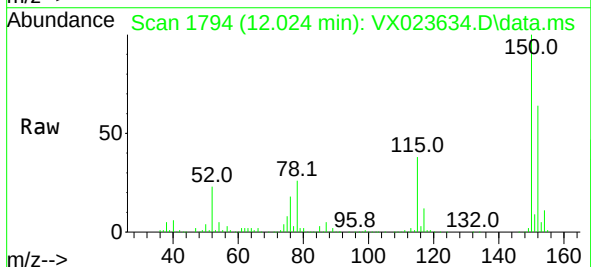

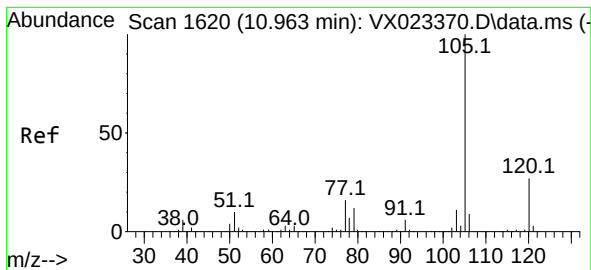

#73

Isopropylbenzene

Concen: 1.235 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX023634.D





Acq: 10 Aug 2021 14:13

Tgt Ion: 105 Resp: 8372

Ion Ratio Lower Upper

105 100

120 25.7 13.2 39.6

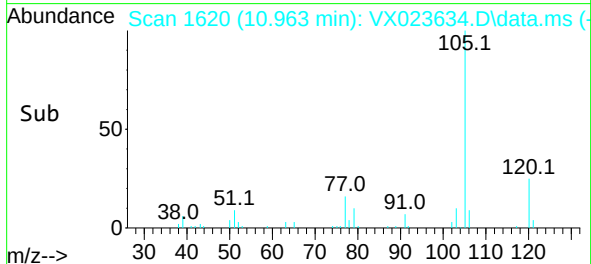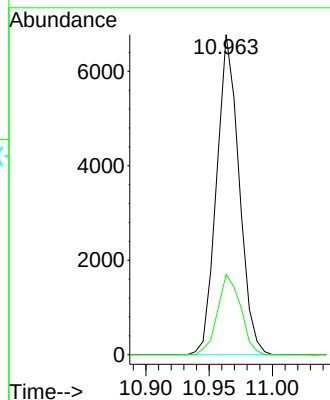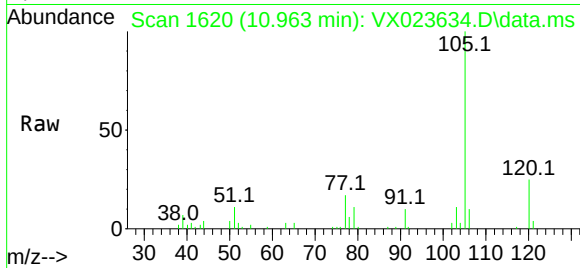

#76

1,2,3-Trichloropropane

Concen: 28.143 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min

Lab File: VX023634.D




Acq: 10 Aug 2021 14:13


Tgt Ion: 75 Resp: 55658

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#

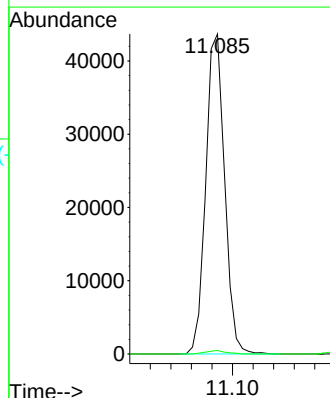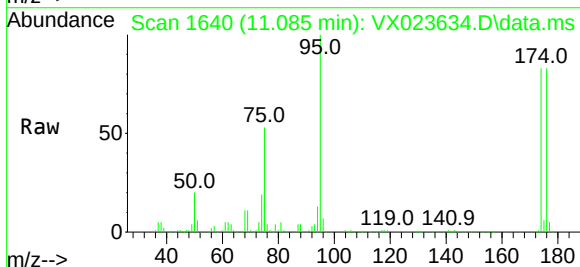



#78

n-propylbenzene

Concen: 1.705 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.006 min

Lab File: VX023634.D





Acq: 10 Aug 2021 14:13

Tgt Ion: 91 Resp: 13086

Ion Ratio Lower Upper

91 100

120 23.3 11.5 34.5

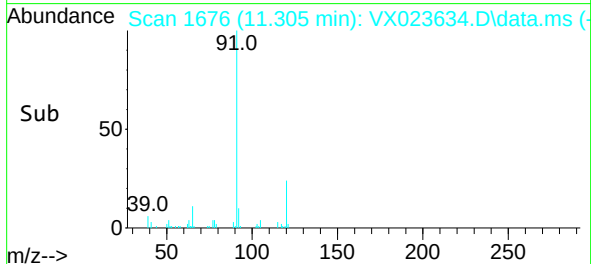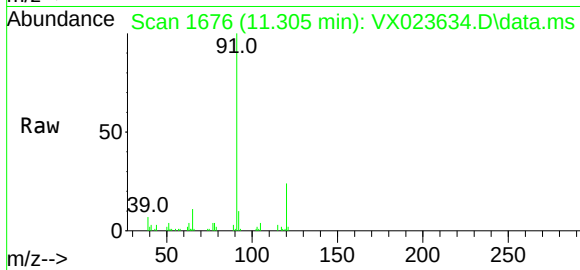

#79

2-Chlorotoluene

Concen: 2.434 ug/l

RT: 11.402 min Scan# 1692

Delta R.T. 0.036 min

Lab File: VX023634.D




Acq: 10 Aug 2021 14:13


Tgt Ion: 91 Resp: 11161

Ion Ratio Lower Upper

91 100

126 0.0 16.6 49.8#


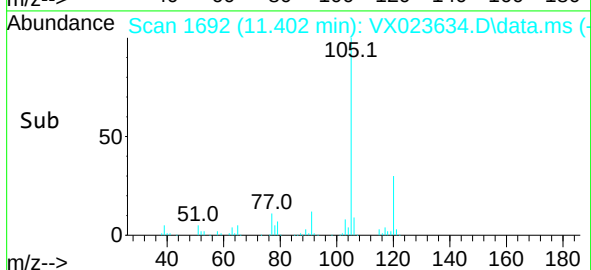

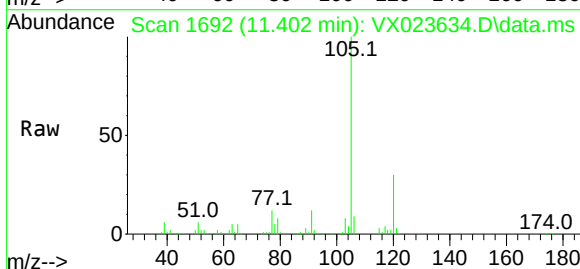




#80
1,3,5-Trimethylbenzene
Concen: 16.048 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 88626
Ion Ratio Lower Upper
105 100
120 47.3 23.8 71.5

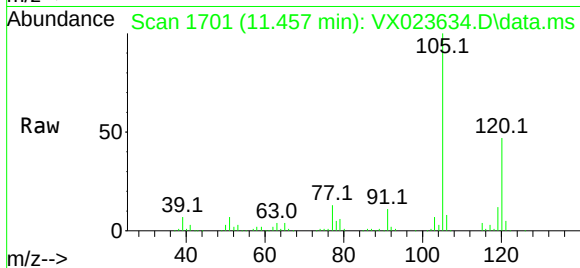

#81
trans-1,4-Dichloro-2-butene
Concen: 75.674 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 75 Resp: 55658
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


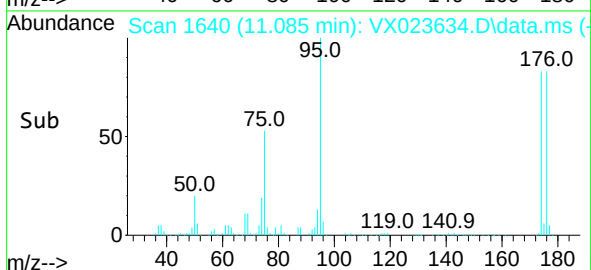

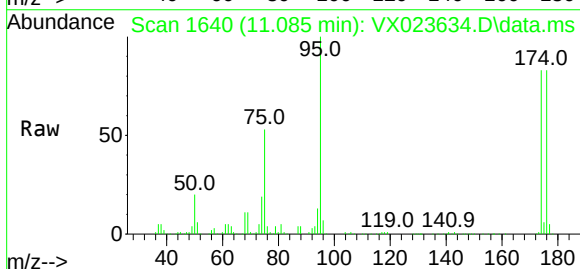




#82
4-Chlorotoluene
Concen: 2.021 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 10486
Ion Ratio Lower Upper
91 100
126 1.7 14.9 44.5#

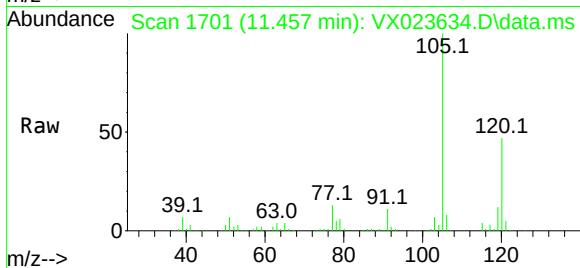

#83
tert-Butylbenzene
Concen: 3.154 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 119 Resp: 17088
Ion Ratio Lower Upper
119 100
91 89.7 27.9 83.7#
134 0.0 11.3 33.9#


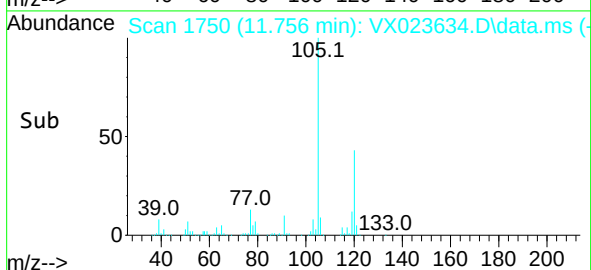

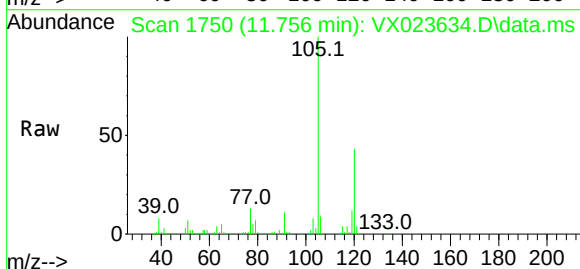




#84
1,2,4-Trimethylbenzene
Concen: 25.033 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 137513
Ion Ratio Lower Upper
105 100
120 43.1 22.4 67.3

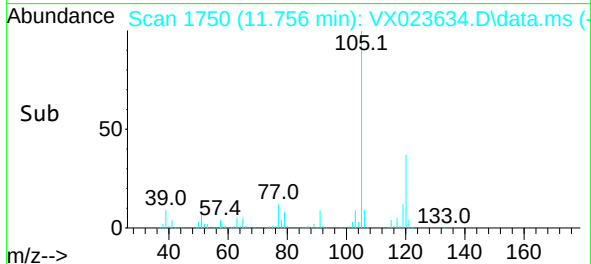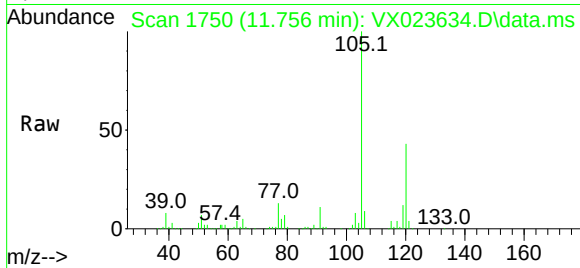

#85
sec-Butylbenzene
Concen: 0.941 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion:105 Resp: 6609
Ion Ratio Lower Upper
105 100
134 20.7 10.0 29.8


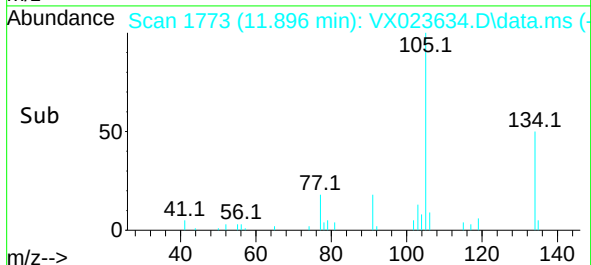

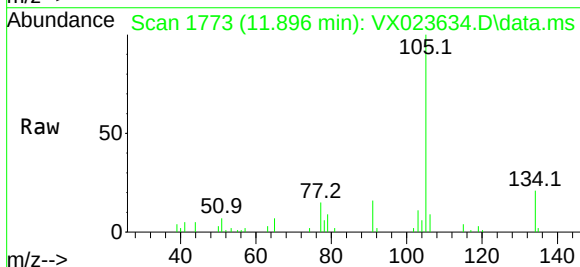


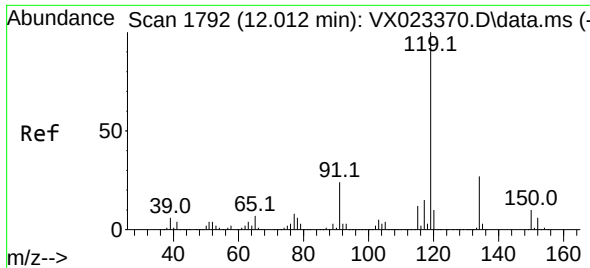

#86
p-Isopropyltoluene
Concen: 0.865 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.043 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 4904
Ion Ratio Lower Upper
119 100
134 27.8 12.9 38.7
91 26.5 11.7 35.0

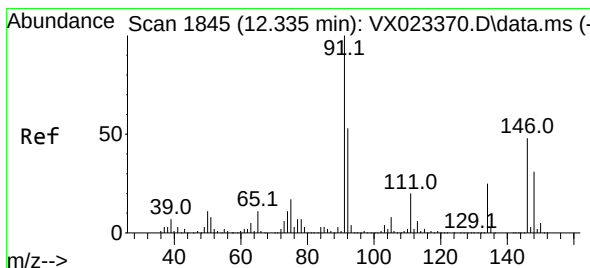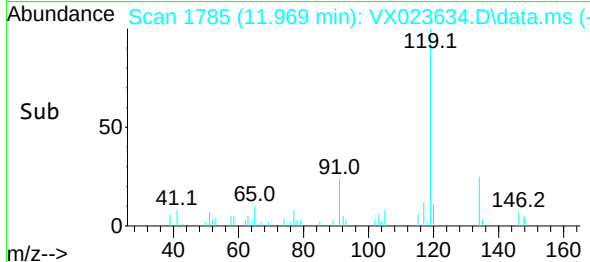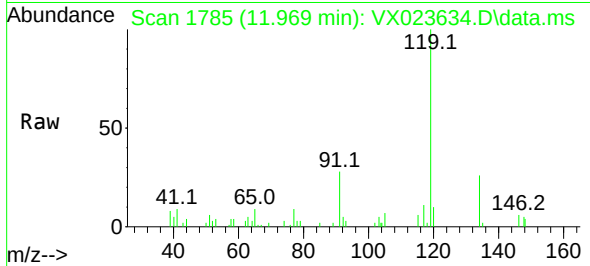

#89
n-Butylbenzene
Concen: 3.104 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 91 Resp: 15938
Ion Ratio Lower Upper
91 100
92 22.8 27.4 82.0#
134 135.3 13.2 39.5#


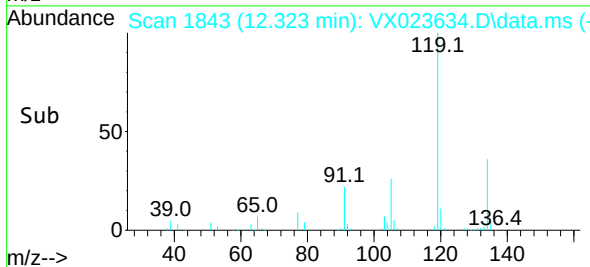

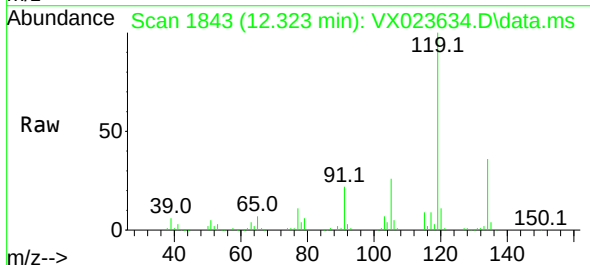




#90
Hexachloroethane
Concen: 6.853 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 5232
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

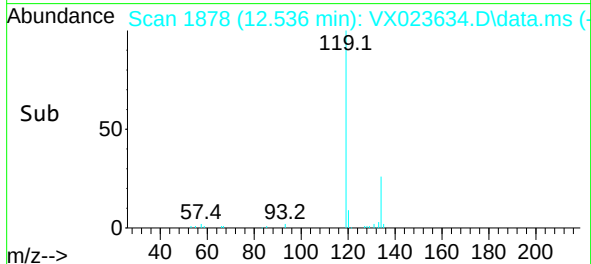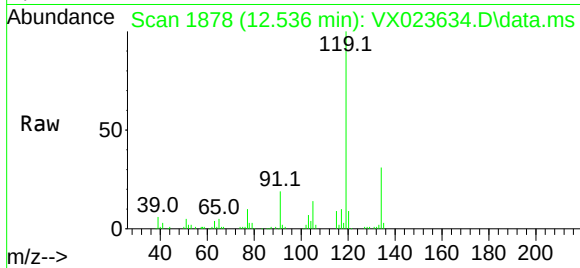

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.723 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Tgt Ion: 75 Resp: 338
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#


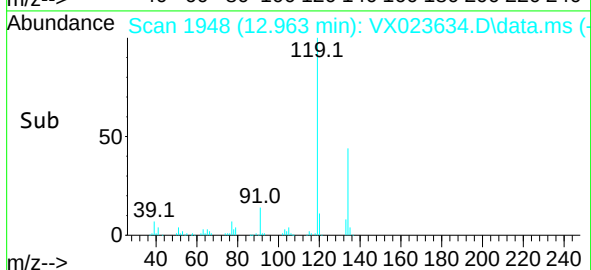






#93
1,2,4-Trichlorobenzene
Concen: 0.213 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:180 Resp: 392
Ion Ratio Lower Upper
180 100
182 90.6 47.7 143.1
145 84.4 15.0 45.0#

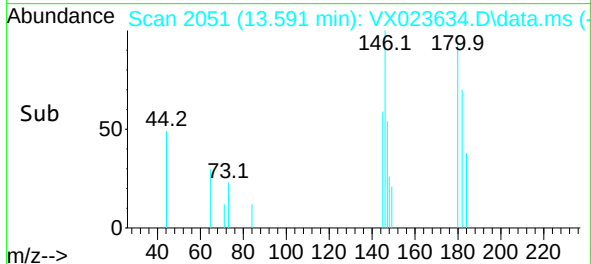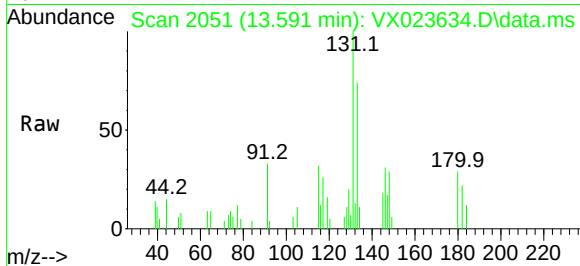

#94
Hexachlorobutadiene
Concen: 0.202 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.006 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13


Tgt Ion:225 Resp: 167
Ion Ratio Lower Upper
225 100
223 30.5 31.1 93.2#
227 13.2 31.6 95.0#

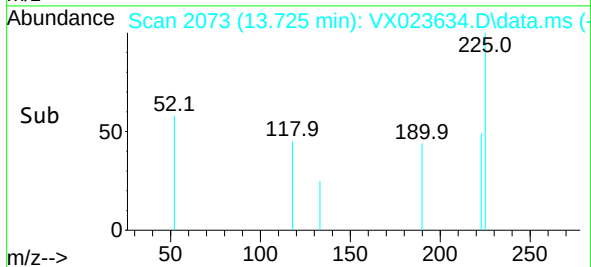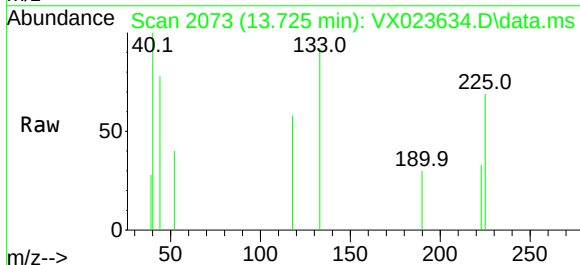

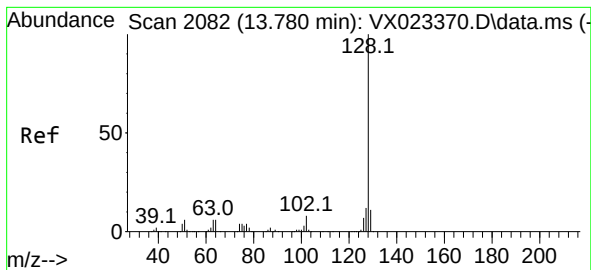

#95
Naphthalene
Concen: 1.082 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX023634.D
Acq: 10 Aug 2021 14:13

Instrument :
MSVOA_X
ClientSampleId :

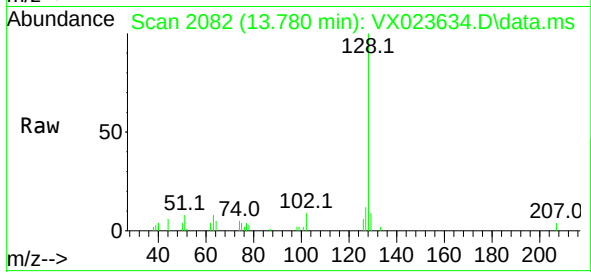

Tgt Ion:128 Resp: 6847
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 12.0 8.8 13.2

