

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
 Data File : VX030540.D
 Acq On : 10 Aug 2022 09:44
 Operator : JC/MD
 Sample : VX0810MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK677

Quant Time: Aug 10 12:50:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 10 01:21:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	300437	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	266143	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	120553	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	92936	48.169	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.340%
7) Chloroethane-d5	1.672	69	71862	52.836	ug/L	0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.680%
11) 1,1-Dichloroethene-d2	2.307	63	137905	37.787	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.580%
21) 2-Butanone-d5	4.471	46	209088	116.963	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.960%
24) Chloroform-d	5.062	84	204980	51.611	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.220%
26) 1,2-Dichloroethane-d4	5.958	65	145418	53.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.840%
32) Benzene-d6	5.971	84	395423	51.868	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.740%
36) 1,2-Dichloropropane-d6	7.312	67	131865	53.313	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.620%
41) Toluene-d8	8.647	98	348891	48.551	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.100%
43) trans-1,3-Dichloroprop...	8.952	79	61933	50.332	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.660%
47) 2-Hexanone-d5	9.385	63	136941	108.619	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.620%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	179390	55.209	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.420%
66) 1,2-Dichlorobenzene-d4	12.323	152	121771	52.078	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.160%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	4205	1.242	ug/L	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
Data File : VX030540.D
Acq On : 10 Aug 2022 09:44
Operator : JC/MD
Sample : VX0810MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK677

Quant Time: Aug 10 12:50:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 10 01:21:25 2022
Response via : Initial Calibration

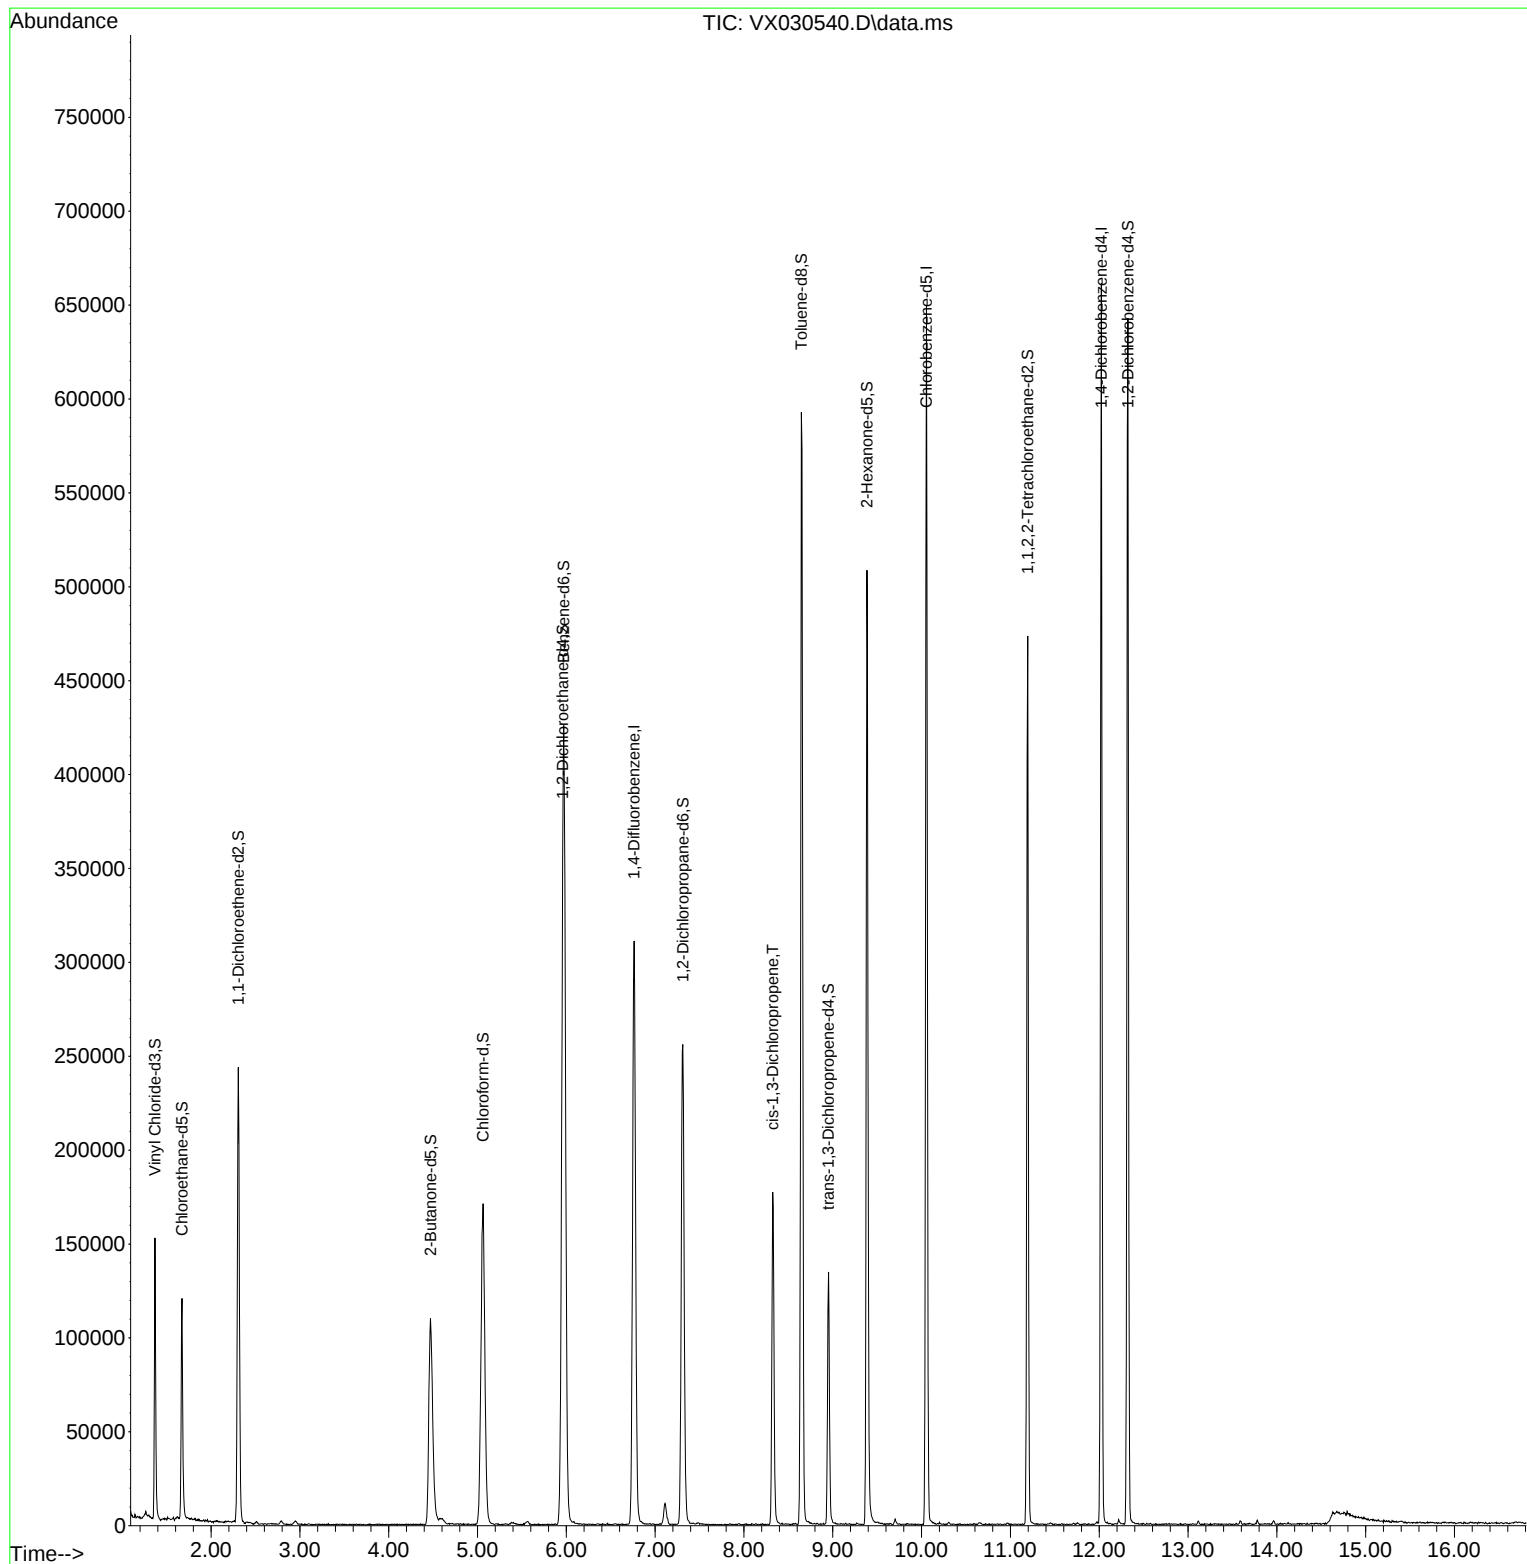

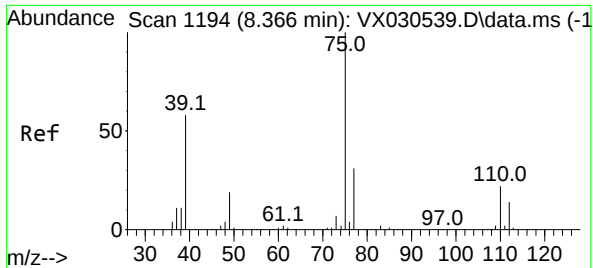

#39
 cis-1,3-Dichloropropene
 Concen: 1.242 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VX030540.D
 Acq: 10 Aug 2022 09:44

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK677

Tgt Ion: 75 Resp: 4205
 Ion Ratio Lower Upper
 75 100
 77 52.1 22.4 41.6#

