

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
 Data File : VX030548.D
 Acq On : 10 Aug 2022 13:36
 Operator : JC/MD
 Sample : N4114-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	27	31	39	rBV3	9932	24956	1.89%	0.219%
2	1.368	42	46	56	rVB2	233484	256158	19.36%	2.243%
3	1.666	91	95	103	rBV	125393	162265	12.27%	1.421%
4	2.306	194	200	210	rVB	265098	424369	32.08%	3.716%
5	2.666	258	259	261	rBV2	541	360	0.03%	0.003%
6	2.794	274	280	288	rVB6	2001	4526	0.34%	0.040%
7	2.947	299	305	316	rVB	8698	20397	1.54%	0.179%
8	3.099	323	330	335	rVB3	5142	9925	0.75%	0.087%
9	3.148	335	338	340	rBV2	420	399	0.03%	0.003%
10	3.696	426	428	432	rVB3	581	498	0.04%	0.004%
11	3.800	443	445	448	rBV	427	440	0.03%	0.004%
12	3.855	450	454	455	rBV2	345	461	0.03%	0.004%
13	4.300	525	527	530	rBV3	496	534	0.04%	0.005%
14	4.489	547	558	572	rBV3	301566	949745	71.79%	8.317%
15	5.068	642	653	667	rBV	169676	528090	39.92%	4.624%
16	5.556	727	733	737	rBV4	1701	3975	0.30%	0.035%
17	5.861	781	783	786	rVB2	708	514	0.04%	0.005%
18	5.891	786	788	790	rBV2	511	459	0.03%	0.004%
19	5.976	790	802	816	rBV2	459087	1322881	100.00%	11.584%
20	6.391	868	870	873	rVB2	695	710	0.05%	0.006%
21	6.446	877	879	881	rBV3	455	425	0.03%	0.004%
22	6.537	892	894	896	rBV2	500	474	0.04%	0.004%
23	6.769	922	932	942	rBV2	299151	725899	54.87%	6.356%
24	6.928	957	958	961	rVB3	880	619	0.05%	0.005%
25	6.958	961	963	966	rBV3	475	398	0.03%	0.003%
26	7.129	982	991	1009	rBV	363100	783742	59.25%	6.863%
27	7.312	1012	1021	1036	rBV	279716	608612	46.01%	5.329%
28	7.799	1099	1101	1103	rBV3	751	719	0.05%	0.006%
29	7.927	1120	1122	1124	rBV	441	403	0.03%	0.004%
30	8.110	1150	1152	1154	rBV3	368	424	0.03%	0.004%
31	8.183	1162	1164	1165	rBV	549	442	0.03%	0.004%
32	8.250	1172	1175	1180	rVB3	410	419	0.03%	0.004%
33	8.330	1182	1188	1201	rVV	187893	309253	23.38%	2.708%
34	8.482	1211	1213	1214	rBV2	673	524	0.04%	0.005%
35	8.653	1234	1241	1252	rBV	665170	1034628	78.21%	9.060%
36	8.952	1284	1290	1302	rBV	135398	209207	15.81%	1.832%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
 Data File : VX030548.D
 Acq On : 10 Aug 2022 13:36
 Operator : JC/MD
 Sample : N4114-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	9.098	1311	1314	1315	rBV2	614	594	0.04%	0.005%
38	9.275	1335	1343	1352	rBV	83934	122447	9.26%	1.072%
39	9.390	1356	1362	1377	rBV	519905	748394	56.57%	6.553%
40	9.628	1399	1401	1405	rVB3	905	879	0.07%	0.008%
41	9.671	1405	1408	1409	rBV	565	448	0.03%	0.004%
42	9.707	1409	1414	1418	rVB4	2827	4058	0.31%	0.036%
43	9.811	1429	1431	1433	rBV3	675	462	0.03%	0.004%
44	10.012	1462	1464	1465	rBV2	566	438	0.03%	0.004%
45	10.055	1466	1471	1481	rVV	622521	837138	63.28%	7.331%
46	10.238	1499	1501	1505	rVB	622	690	0.05%	0.006%
47	10.281	1505	1508	1510	rBV	531	379	0.03%	0.003%
48	10.415	1528	1530	1533	rBV	362	468	0.04%	0.004%
49	10.470	1538	1539	1543	rVB2	576	650	0.05%	0.006%
50	10.512	1543	1546	1550	rBV2	465	580	0.04%	0.005%
51	10.549	1550	1552	1555	rVB2	507	474	0.04%	0.004%
52	10.732	1579	1582	1584	rBV2	401	499	0.04%	0.004%
53	10.890	1605	1608	1610	rVB	682	569	0.04%	0.005%
54	10.915	1610	1612	1617	rVB2	503	490	0.04%	0.004%
55	10.969	1617	1621	1624	rBV	412	669	0.05%	0.006%
56	11.140	1646	1649	1651	rBV2	556	442	0.03%	0.004%
57	11.195	1652	1658	1666	rVV	504614	618561	46.76%	5.417%
58	11.335	1679	1681	1682	rBV2	698	553	0.04%	0.005%
59	11.482	1701	1705	1706	rVB3	343	484	0.04%	0.004%
60	11.640	1729	1731	1735	rBV2	385	541	0.04%	0.005%
61	11.707	1741	1742	1746	rVB2	538	484	0.04%	0.004%
62	11.738	1746	1747	1749	rBV	541	402	0.03%	0.004%
63	11.963	1781	1784	1788	rBV2	688	859	0.06%	0.008%
64	12.024	1789	1794	1805	rVV	656016	783308	59.21%	6.859%
65	12.195	1820	1822	1823	rBV	684	419	0.03%	0.004%
66	12.225	1823	1827	1830	rVB5	797	1047	0.08%	0.009%
67	12.323	1837	1843	1856	rBV	700351	883417	66.78%	7.736%
68	12.555	1879	1881	1883	rBV2	456	410	0.03%	0.004%
69	12.628	1889	1893	1894	rBV3	417	425	0.03%	0.004%
70	12.804	1920	1922	1923	rVB	701	397	0.03%	0.003%
71	12.835	1925	1927	1928	rBV	622	484	0.04%	0.004%
72	12.902	1936	1938	1941	rVB	495	418	0.03%	0.004%
73	12.933	1941	1943	1945	rVB	630	379	0.03%	0.003%
74	12.951	1945	1946	1949	rBV2	555	445	0.03%	0.004%
75	12.981	1949	1951	1954	rBV2	565	446	0.03%	0.004%
76	13.371	2012	2015	2018	rVV2	569	782	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
 Data File : VX030548.D
 Acq On : 10 Aug 2022 13:36
 Operator : JC/MD
 Sample : N4114-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.445	2025	2027	2029	rVV2	622	520	0.04%	0.005%
78	13.536	2040	2042	2045	rBV2	596	713	0.05%	0.006%
79	13.707	2068	2070	2073	rBV	551	449	0.03%	0.004%
80	13.835	2089	2091	2096	rVB	639	629	0.05%	0.006%
81	13.981	2113	2115	2118	rVB2	619	681	0.05%	0.006%
82	14.109	2130	2136	2137	rBV2	236	404	0.03%	0.004%
83	14.298	2164	2167	2170	rBV2	458	772	0.06%	0.007%
84	14.323	2170	2171	2174	rVB2	617	475	0.04%	0.004%
85	14.646	2222	2224	2226	rBV2	499	387	0.03%	0.003%
86	14.731	2236	2238	2239	rBV	822	529	0.04%	0.005%
87	14.853	2255	2258	2259	rBV2	753	755	0.06%	0.007%
88	15.042	2285	2289	2290	rBV2	647	985	0.07%	0.009%
89	15.219	2316	2318	2323	rBV2	612	691	0.05%	0.006%
90	15.402	2346	2348	2349	rVB	678	438	0.03%	0.004%
91	15.524	2364	2368	2371	rBV4	908	1421	0.11%	0.012%
92	15.609	2381	2382	2388	rVV4	806	1248	0.09%	0.011%
93	15.658	2388	2390	2393	rVB	835	832	0.06%	0.007%
94	15.780	2408	2410	2411	rBV	582	525	0.04%	0.005%
95	15.914	2430	2432	2434	rBV3	870	622	0.05%	0.005%
96	16.164	2471	2473	2476	rVB2	844	775	0.06%	0.007%
97	16.200	2476	2479	2480	rBV3	924	1091	0.08%	0.010%
98	16.310	2495	2497	2499	rVB2	929	649	0.05%	0.006%
99	16.334	2499	2501	2504	rBV	579	726	0.05%	0.006%
100	16.676	2555	2557	2558	rBV2	902	621	0.05%	0.005%


Sum of corrected areas: 11419817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
Data File : VX030548.D
Acq On : 10 Aug 2022 13:36
Operator : JC/MD
Sample : N4114-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

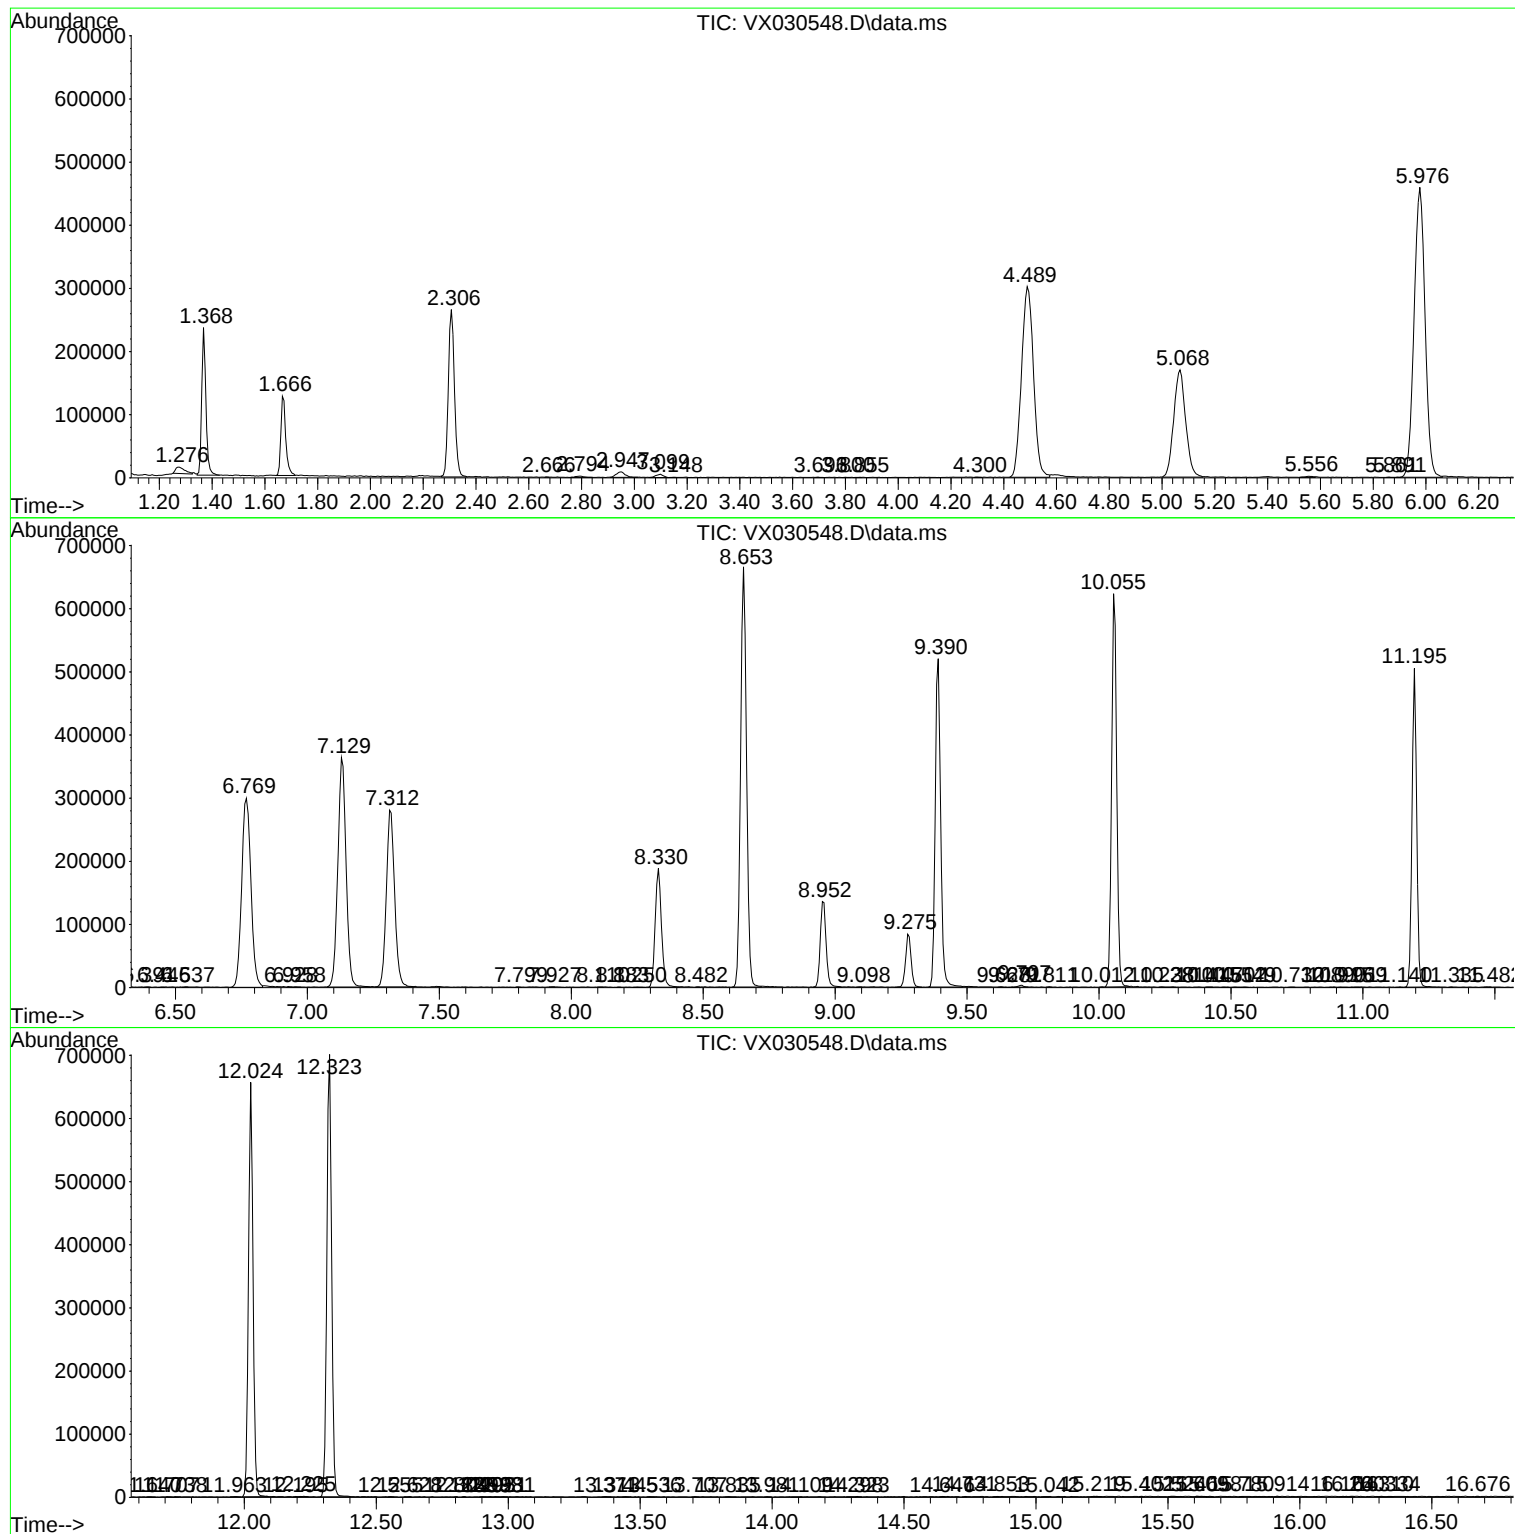

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
Data File : VX030548.D
Acq On : 10 Aug 2022 13:36
Operator : JC/MD
Sample : N4114-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
Data File : VX030548.D
Acq On : 10 Aug 2022 13:36
Operator : JC/MD
Sample : N4114-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc