
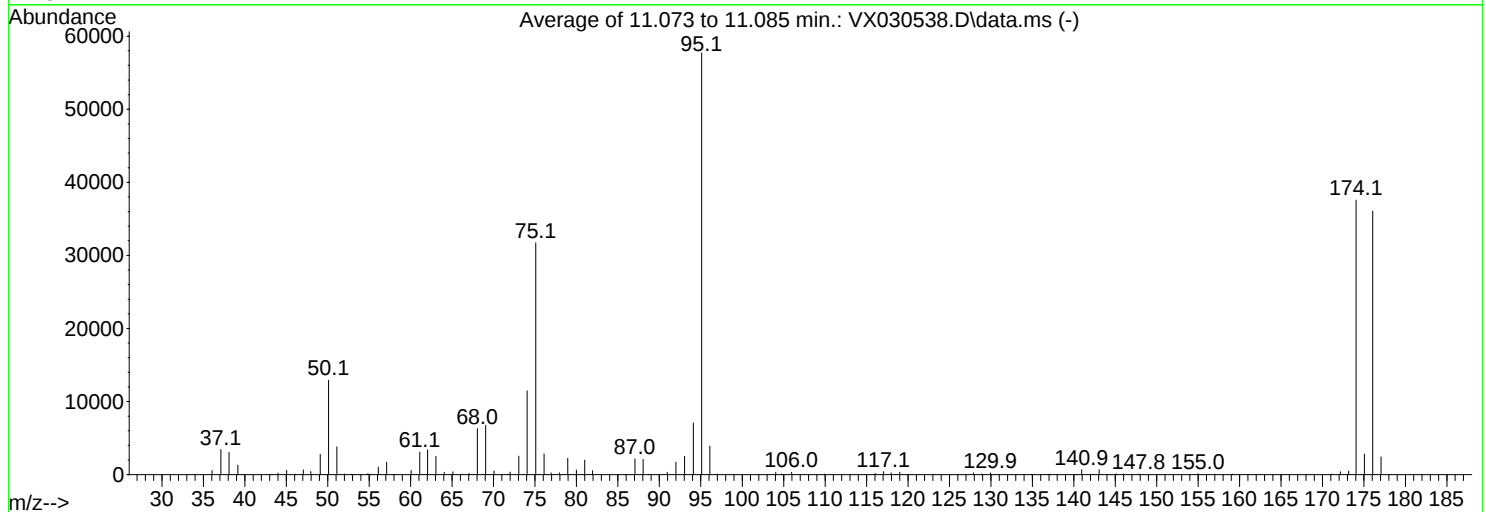


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081022\
 Data File : VX030538.D
 Acq On : 10 Aug 2022 08:05
 Operator : JC/MD
 Sample : BFB675
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB675

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 10 01:21:25 2022

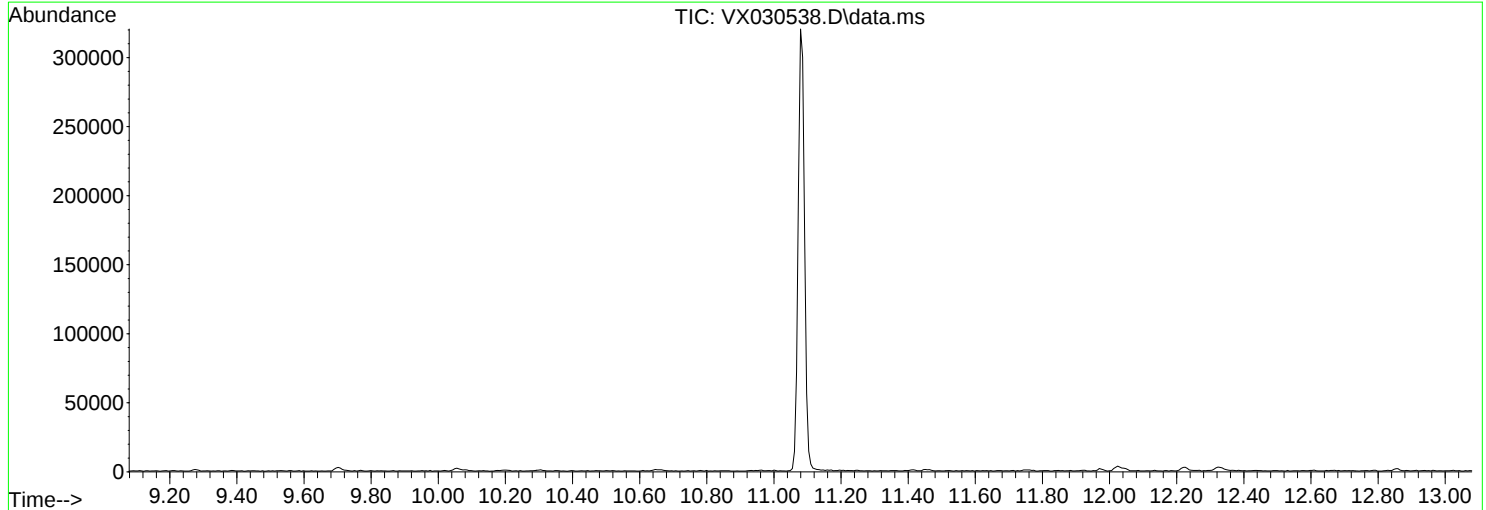

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	12912	PASS
75	95	30	80	55.0	31723	PASS
95	95	100	100	100.0	57717	PASS
96	95	5	9	6.7	3889	PASS
173	174	0.00	2	1.3	477	PASS
174	95	50	120	65.1	37579	PASS
175	174	5	9	7.4	2795	PASS
176	174	95	101	96.0	36069	PASS
177	176	5	9	6.8	2439	PASS

m/z	Abundance
40.00	287.0
44.00	367.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
36.10	530.0
37.10	3060.0
38.10	2730.0
39.10	1192.0
39.90	347.0
43.30	67.0
44.00	414.0
45.10	684.0
46.10	67.0
47.10	602.0
47.90	284.0
49.10	2461.0
50.10	10396.0
51.10	2998.0
53.20	68.0
55.20	183.0
56.10	744.0
57.10	1488.0
58.20	73.0
60.00	535.0
61.10	2342.0
62.10	2869.0
63.10	1972.0
64.10	328.0
65.10	350.0
67.10	83.0
68.10	5360.0
69.10	5476.0
70.10	480.0
71.80	205.0
73.10	2124.0
74.10	9450.0
75.10	26248.0
76.10	2142.0
77.10	103.0
77.90	189.0
79.00	1524.0
80.00	529.0
81.00	1487.0
82.00	477.0
83.10	51.0
87.00	1787.0
88.10	1631.0
91.10	255.0
92.00	1480.0
93.10	1989.0
94.10	5988.0
95.10	43104.0
96.10	3189.0
104.10	213.0
104.70	67.0
106.00	259.0
116.10	193.0
117.10	334.0
118.00	184.0
119.00	275.0
128.00	132.0
130.10	81.0
137.20	109.0
140.90	375.0
143.00	450.0
145.00	109.0
146.00	124.0
149.10	52.0
155.00	80.0
157.00	98.0
171.10	99.0
172.20	306.0
173.10	274.0
174.10	24384.0
175.00	1678.0
176.00	22120.0
177.00	1395.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
36.00	733.0
37.10	3942.0
38.10	3433.0
39.10	1487.0
40.00	314.0
43.20	51.0
44.10	802.0
45.00	608.0
46.10	116.0
47.10	726.0
47.90	444.0
49.10	3273.0
50.10	15614.0
51.10	4552.0
52.00	117.0
52.90	129.0
54.80	243.0
56.10	1210.0
57.10	2005.0
57.90	52.0
60.10	600.0
61.10	3750.0
62.00	3848.0
63.00	2670.0
64.00	289.0
65.10	446.0
66.20	83.0
67.00	190.0
68.00	6966.0
69.00	7782.0
70.00	608.0
72.00	471.0
73.00	2732.0
74.00	13214.0
75.10	36384.0
76.10	3849.0
77.00	312.0
78.00	315.0
79.00	2722.0
80.00	656.0
81.00	2360.0
82.00	638.0
83.10	86.0
87.00	2441.0
88.00	2605.0
90.90	454.0
92.00	2046.0
93.10	3105.0
94.10	8027.0
95.10	67544.0
96.10	5085.0
97.00	167.0
104.10	433.0
104.80	114.0
105.90	377.0
110.00	121.0
111.10	93.0
114.80	55.0
116.00	269.0
117.10	467.0
117.90	360.0
119.00	345.0
128.00	282.0
128.90	279.0
129.90	365.0
130.90	86.0
134.90	74.0
137.10	84.0
140.30	98.0
141.00	909.0
142.30	121.0
143.10	796.0
145.10	168.0
146.00	110.0
147.80	148.0
155.00	138.0
157.00	90.0
159.10	136.0
170.00	81.0
171.10	163.0
172.20	445.0
173.10	572.0
174.00	43472.0
175.10	3410.0
176.10	40784.0
177.10	2946.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675

m/z	Abundance
36.10	435.0
37.10	3306.0
38.10	3050.0
39.20	1216.0
39.90	291.0
42.90	98.0
44.00	543.0
45.10	498.0
47.00	642.0
48.00	555.0
49.10	2599.0
50.10	12726.0
51.10	3873.0
52.00	153.0
52.90	78.0
54.90	205.0
56.10	1128.0
57.10	1662.0
57.90	58.0
60.00	606.0
61.10	3180.0
62.00	3440.0
63.10	2912.0
64.10	346.0
65.10	394.0
66.20	103.0
67.00	236.0
68.00	6582.0
69.00	7046.0
70.10	444.0
72.00	565.0
73.10	2749.0
74.10	11744.0
75.10	32536.0
76.10	2520.0
76.90	332.0
78.00	240.0
78.90	2425.0
80.00	703.0
81.00	2126.0
81.90	535.0
85.90	99.0
87.10	2280.0
88.00	2065.0
88.70	114.0
90.90	311.0
92.00	1623.0
93.00	2407.0
94.10	7185.0
95.10	62504.0
96.10	3392.0
97.00	98.0
104.00	297.0
104.80	59.0
106.00	383.0
109.90	161.0
114.80	74.0
115.80	146.0
117.00	421.0
118.00	210.0
119.00	390.0
125.10	53.0
127.80	326.0
128.80	70.0
129.90	307.0
134.90	83.0
136.90	175.0
141.00	760.0
142.00	170.0
143.00	796.0
145.20	127.0
147.90	143.0
155.00	181.0
157.00	95.0
159.10	110.0
170.00	78.0
172.10	435.0
173.20	584.0
174.10	44880.0
175.00	3297.0
176.10	45304.0
177.10	2977.0
178.00	128.0

Instrument :
MSVOA_X
ClientSampleId :
BFB675