
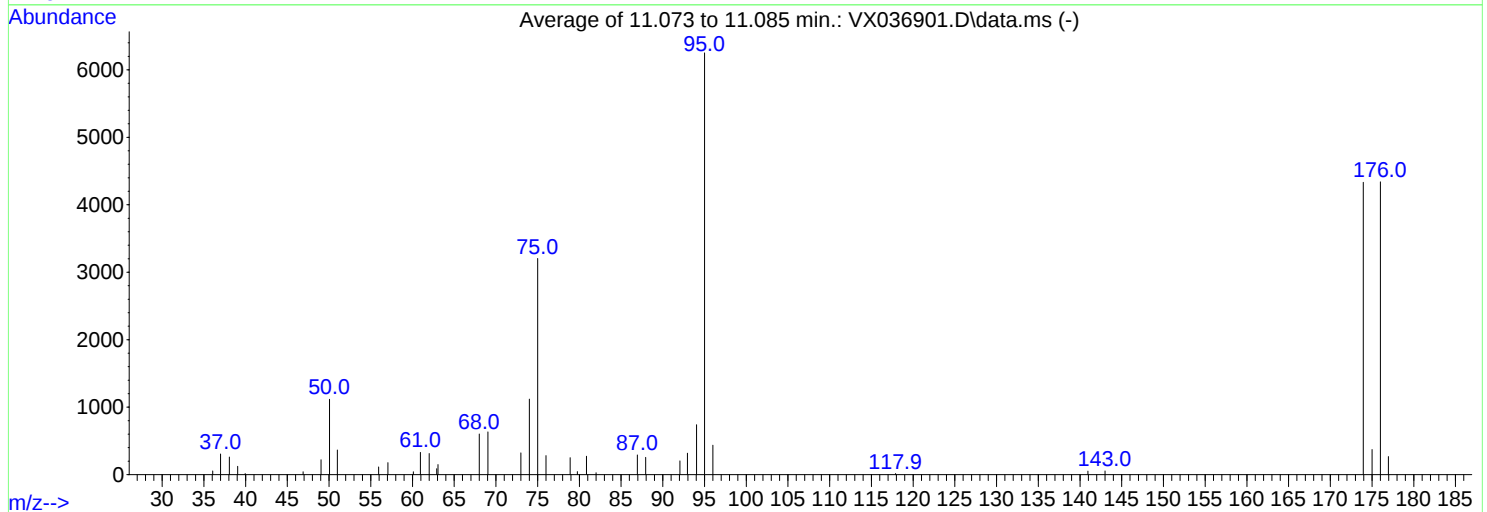


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081023\
Data File : VX036901.D
Acq On : 10 Aug 2023 08:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Title : SW846 8260
Last Update : Fri Jul 21 12:14:12 2023

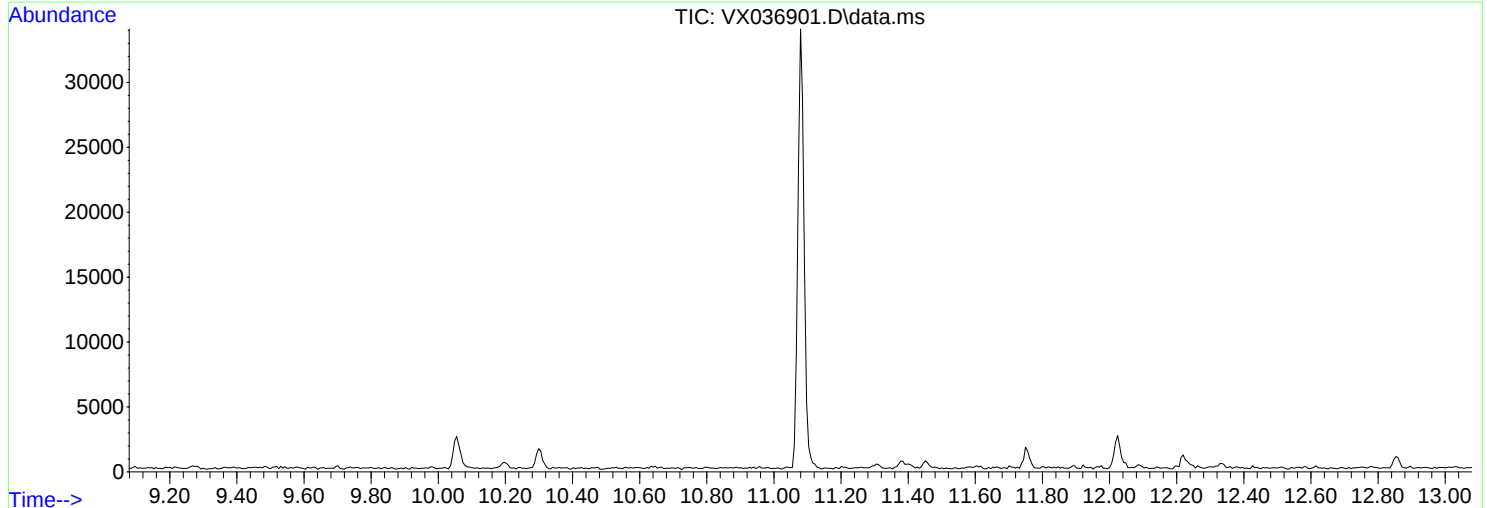

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	1116	PASS
75	95	30	60	51.3	3205	PASS
95	95	100	100	100.0	6251	PASS
96	95	5	9	7.0	437	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.3	4333	PASS
175	174	5	9	8.6	372	PASS
176	174	95	101	100.1	4339	PASS
177	176	5	9	6.2	267	PASS