

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX081119\
 Data File : VX011427.D
 Acq On : 11 Aug 2019 13:32
 Operator : JC/SP
 Sample : K4228-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 2S-F1-(0)

Quant Time: Aug 12 07:47:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	210326	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	306808	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	280170	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	125730	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	109180	51.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.10%	
35) Dibromofluoromethane	5.49	113	93351	46.60	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.20%	
50) Toluene-d8	8.71	98	363302	48.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.10%	
62) 4-Bromofluorobenzene	11.13	95	121700	45.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.16%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	391	0.214	ug/l #	88
5) Bromomethane	1.65	94	665	0.465	ug/l	92
6) Chloroethane	1.72	64	227	Below Cal		97
8) Diethyl Ether	2.18	74	555	0.436	ug/l	83
10) Methyl Iodide	2.51	142	534	0.219	ug/l #	73
11) Tert butyl alcohol	3.01	59	4342	10.302	ug/l #	78
13) Acrolein	2.32	56	28	Below Cal	#	1
16) Acetone	2.43	43	6032	5.983	ug/l	97
18) Methyl Acetate	2.78	43	846	0.367	ug/l #	65
20) Methylene Chloride	2.85	84	5956	2.698	ug/l	97
25) 2-Butanone	4.68	43	391	0.273	ug/l	97
31) Cyclohexane	5.65	56	3939	1.444	ug/l #	19
36) 1,1-Dichloropropene	5.66	75	13626	5.087	ug/l #	50
38) Carbon Tetrachloride	5.65	117	19702	7.311	ug/l #	13
43) Isopropyl Acetate	6.43	43	8197	1.908	ug/l	99
48) Methyl methacrylate	7.68	41	3627	1.794	ug/l #	10
49) 1,4-Dioxane	7.63	88	21	0.358	ug/l #	1
51) 4-Methyl-2-Pentanone	8.61	43	44198	15.942	ug/l #	47
53) t-1,3-Dichloropropene	9.04	75	104	2.871	ug/l #	43
54) cis-1,3-Dichloropropene	8.61	75	21884	7.322	ug/l #	65
57) 1,3-Dichloropropane	9.54	76	5325	1.550	ug/l #	42
59) 2-Hexanone	9.54	43	68022	31.677	ug/l #	49
76) 1,2,3-Trichloropropane	11.13	75	62598	27.339	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.13	75	62598	70.920	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX081119\
Data File : VX011427.D
Acq On : 11 Aug 2019 13:32
Operator : JC/SP
Sample : K4228-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
2S-F1-(0)

Quant Time: Aug 12 07:47:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

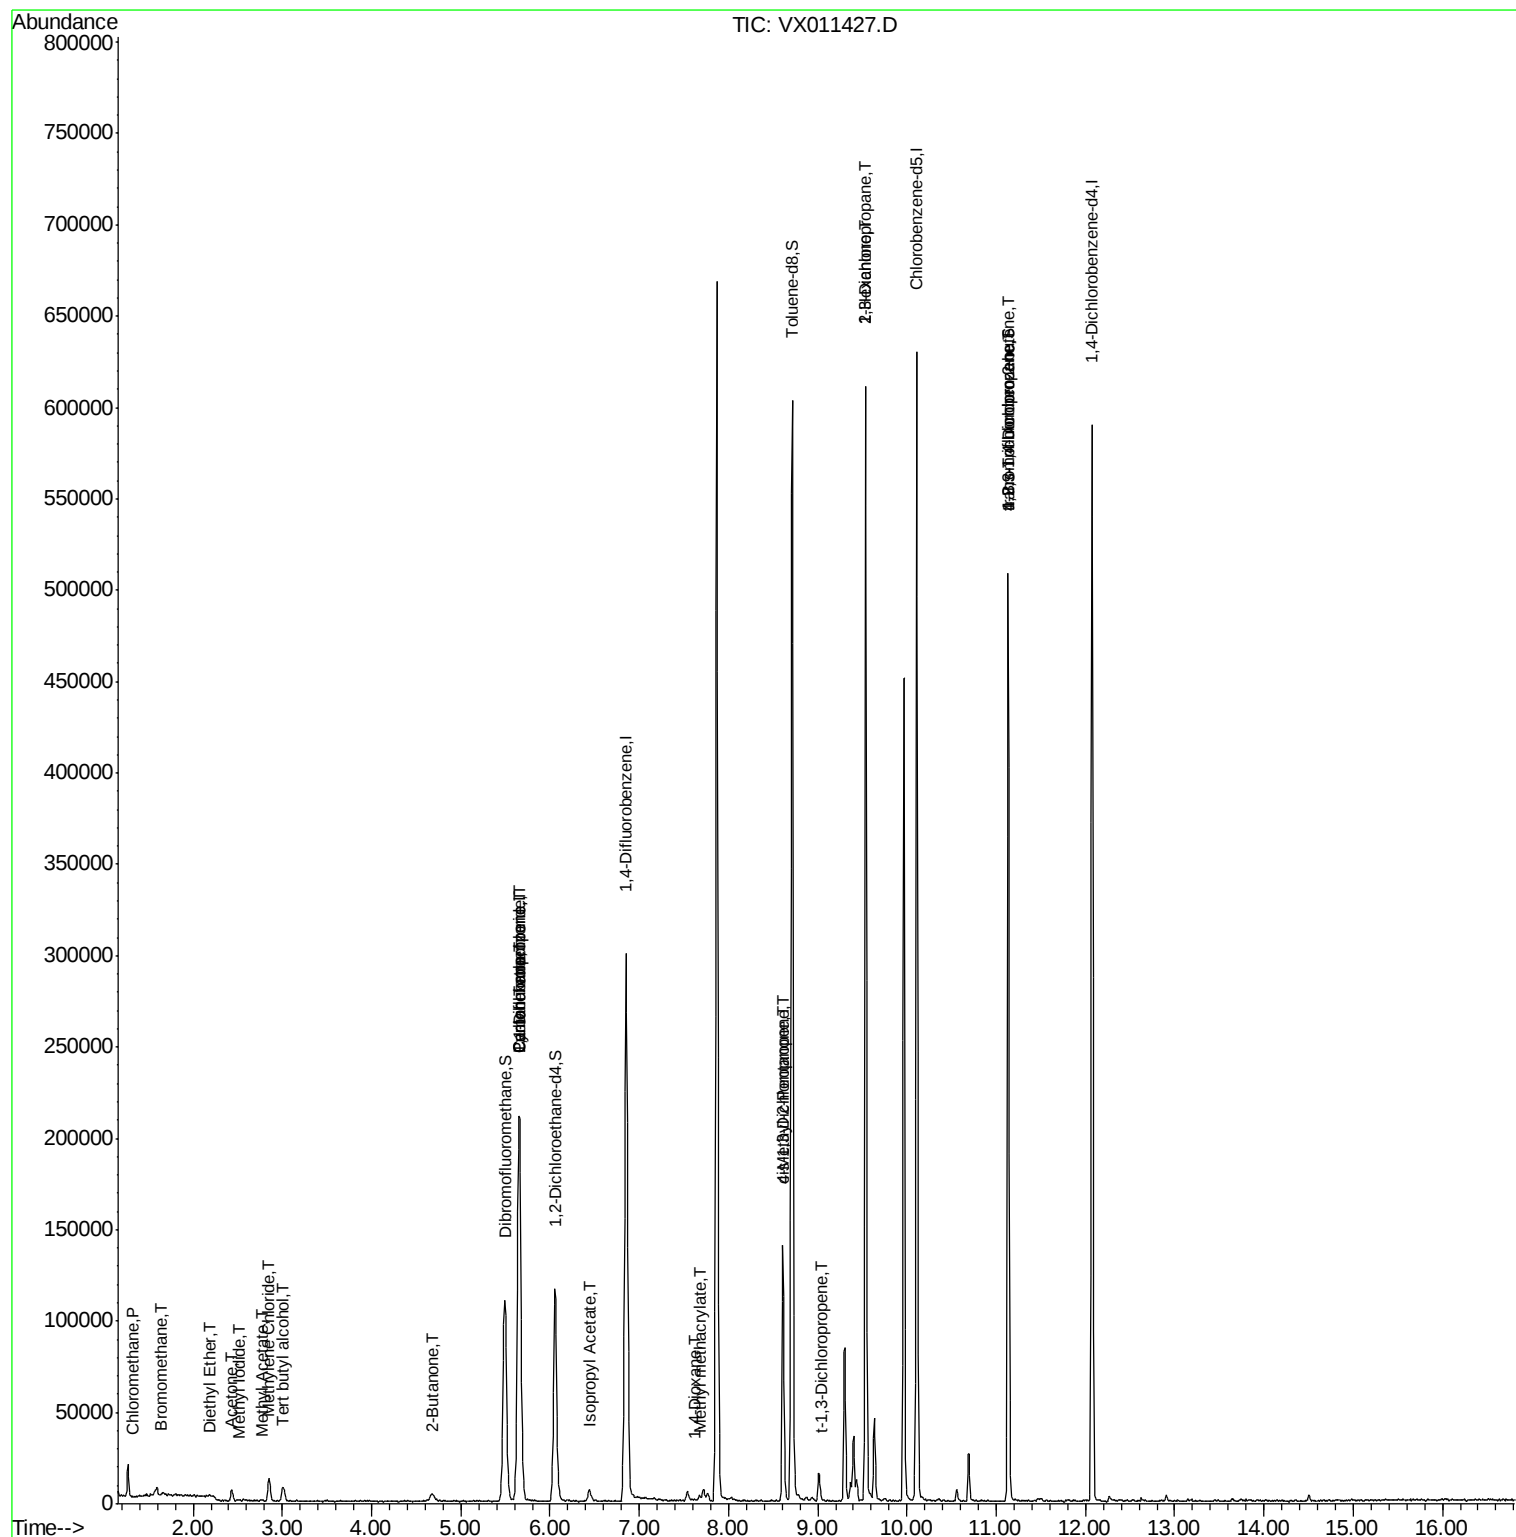



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.01 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampled :


2S-F1-(0)

Tgt Ion: 168 Resp: 210326

Ion Ratio Lower Upper




168 100

99 49.5 38.5 57.7

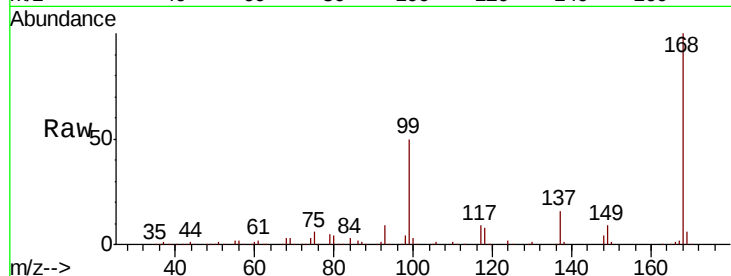

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

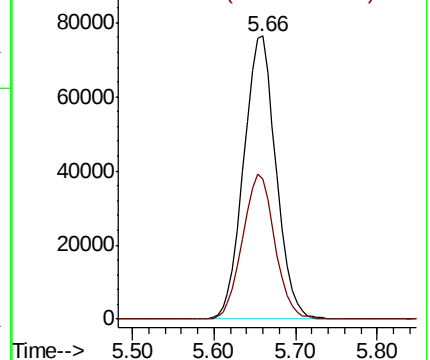

#3

Chloromethane

Concen: 0.214 ug/l

RT: 1.32 min Scan# 28

Delta R.T. 0.01 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 50 Resp: 391

Ion Ratio Lower Upper



50 100


52 26.3 26.4 39.6#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

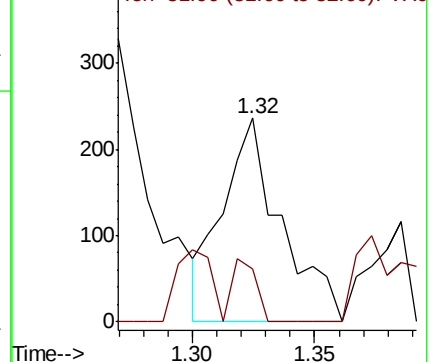

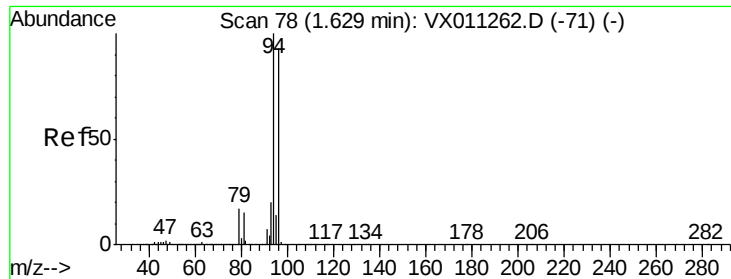

#5

Bromomethane

Concen: 0.465 ug/l

RT: 1.65 min Scan# 82

Delta R.T. 0.02 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampled :


2S-F1-(0)

Tgt Ion: 94 Resp: 665

Ion Ratio Lower Upper




94 100

96 85.6 74.6 112.0

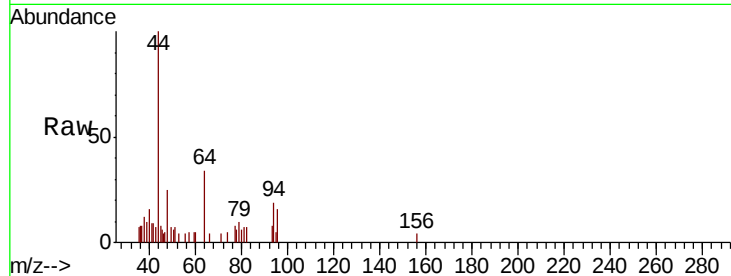

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

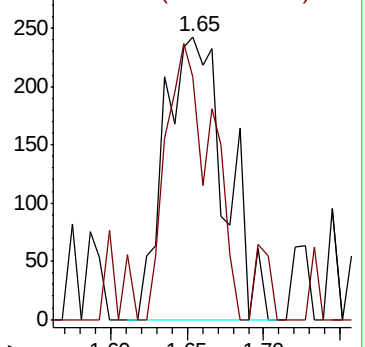

#6

Chloroethane

Concen: Below Cal

RT: 1.72 min Scan# 93

Delta R.T. 0.01 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 64 Resp: 227

Ion Ratio Lower Upper



64 100


66 29.7 25.1 37.7



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

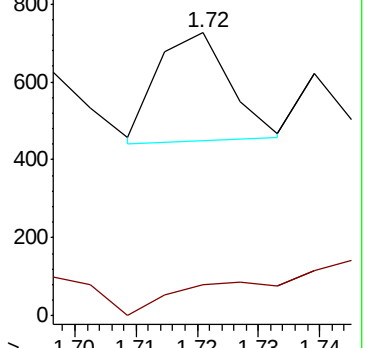

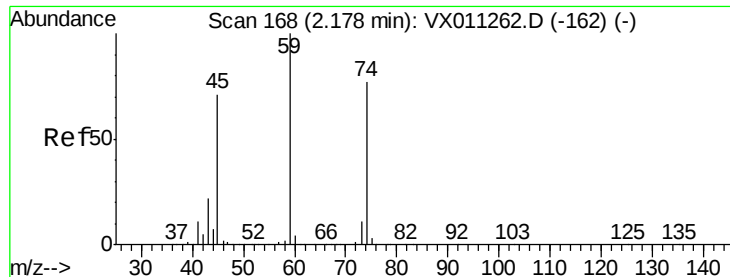

#8

Diethyl Ether

Concen: 0.436 ug/l

RT: 2.18 min Scan# 169

Delta R.T. 0.01 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :


2S-F1-(0)

Tgt Ion: 74 Resp: 555

Ion Ratio Lower Upper

74 100

45 76.4 46.1 138.3

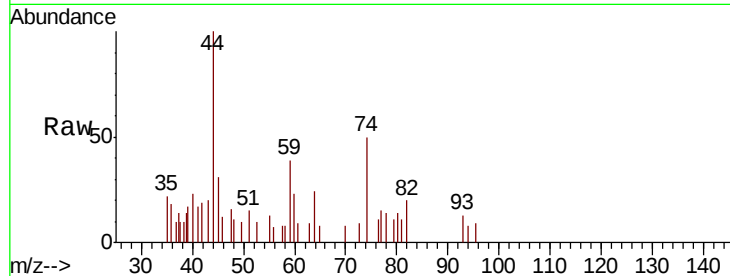

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

2.18

300

200

100



0

2.15

2.20

2.25

Time-->

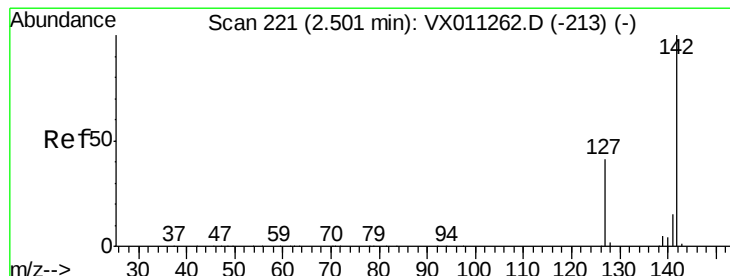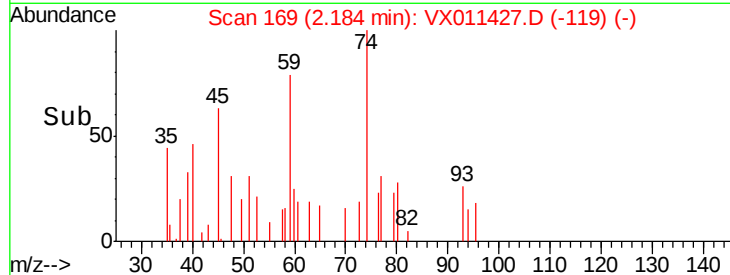

#10

Methyl Iodide

Concen: 0.219 ug/l

RT: 2.51 min Scan# 223

Delta R.T. 0.01 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32


Tgt Ion: 142 Resp: 534

Ion Ratio Lower Upper

142 100

127 59.6 33.8 50.8#

141 3.7 11.4 17.2#

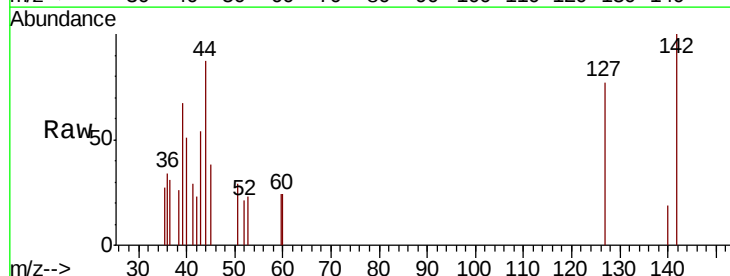

Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

300

200

100


0


2.45

2.50

2.55

Time-->

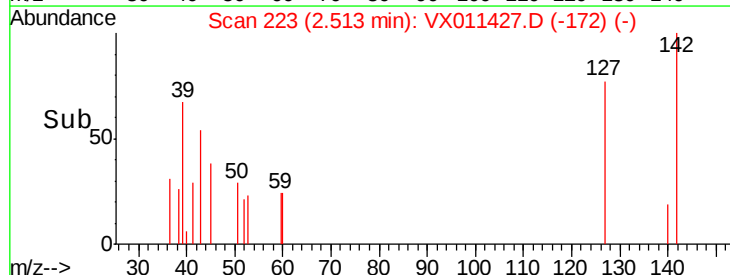

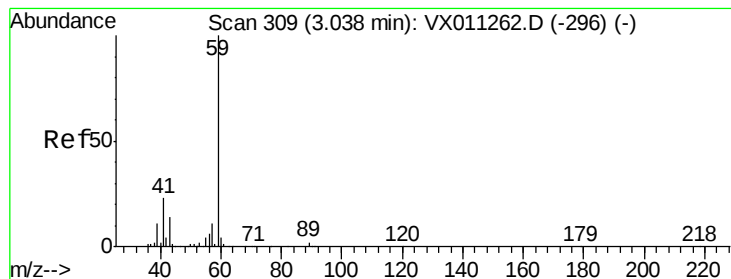

#11

Tert butyl alcohol

Concen: 10.302 ug/l

RT: 3.01 min Scan# 305

Delta R.T. -0.02 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :


2S-F1-(0)

Tgt Ion: 59 Resp: 4342

Ion Ratio Lower Upper




59 100

57 2.3 8.3 12.5#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

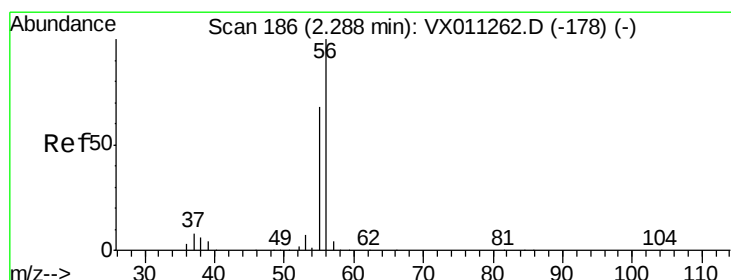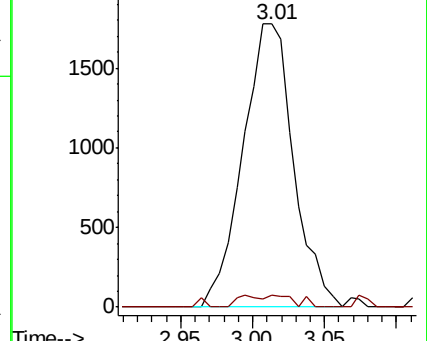

#13

Acrolein

Concen: Below Cal

RT: 2.32 min Scan# 192

Delta R.T. 0.04 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 56 Resp: 28

Ion Ratio Lower Upper



56 100


55 246.4 56.0 84.0#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

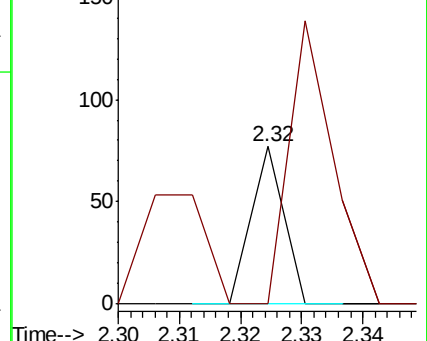

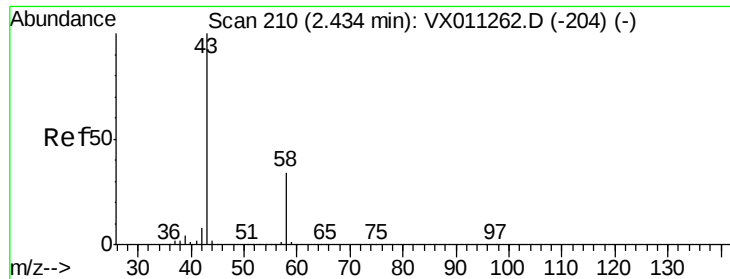

#16

Acetone

Concen: 5.983 ug/l

RT: 2.43 min Scan# 210

Delta R.T. 0.00 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :


2S-F1-(0)

Tgt Ion: 43 Resp: 6032

Ion Ratio Lower Upper




43 100

58 36.1 27.4 41.0

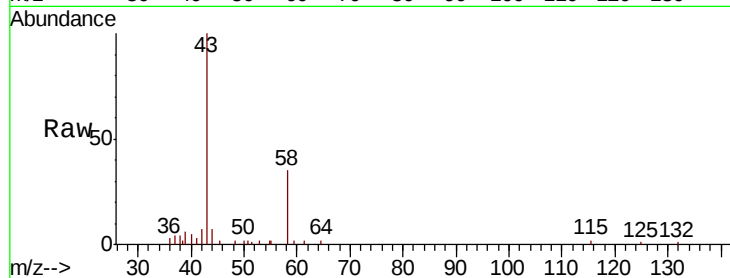

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

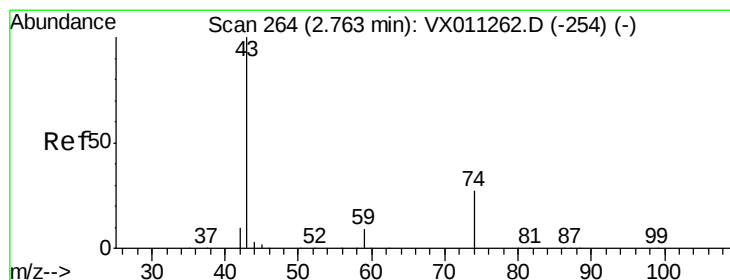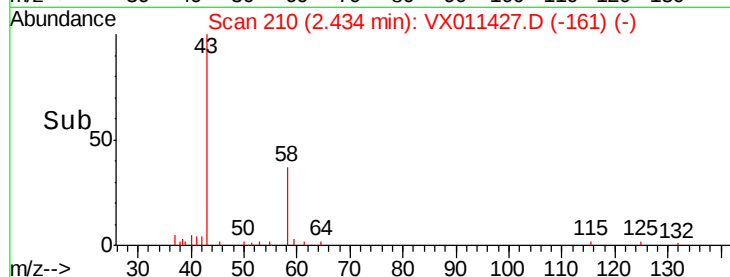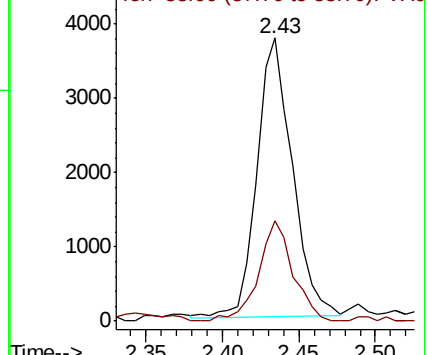

#18

Methyl Acetate

Concen: 0.367 ug/l

RT: 2.78 min Scan# 266

Delta R.T. 0.01 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 43 Resp: 846

Ion Ratio Lower Upper



43 100


74 44.1 21.0 31.6#

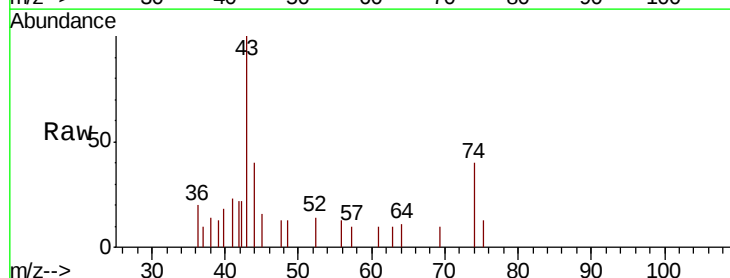

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0



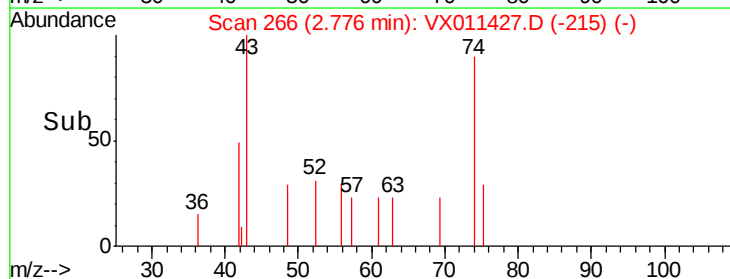
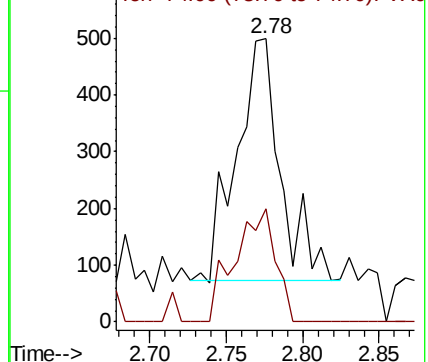




#20
Methylene Chloride
Concen: 2.698 ug/l
RT: 2.85 min Scan# 278
Delta R.T. 0.00 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32




Instrument :
MSVOA_X
ClientSampleId :
2S-F1-(0)


Tgt Ion:	84	Resp:	5956
Ion	Ratio	Lower	Upper
84	100		
49	112.5	89.3	133.9
51	36.5	28.3	42.5
86	62.6	54.5	81.7

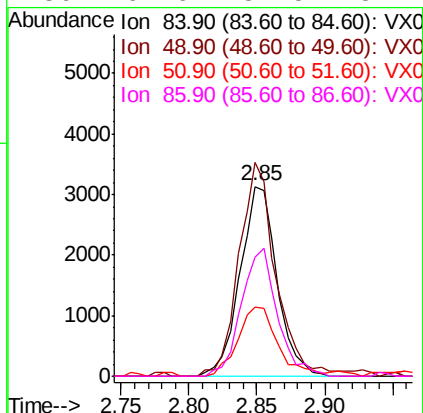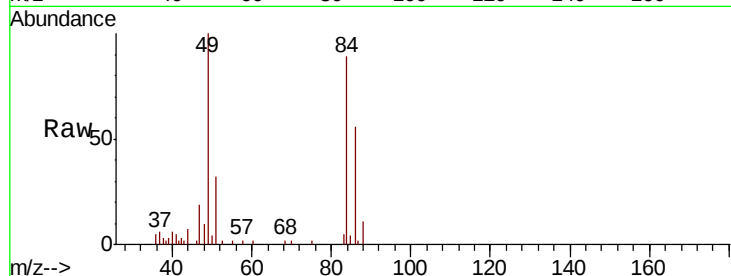

#25
2-Butanone
Concen: 0.273 ug/l
RT: 4.68 min Scan# 578
Delta R.T. 0.01 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32

Tgt Ion:	43	Resp:	391
Ion	Ratio	Lower	Upper
43	100		
72	30.5	23.2	34.8

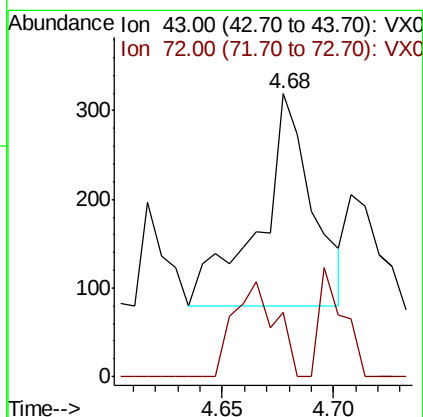

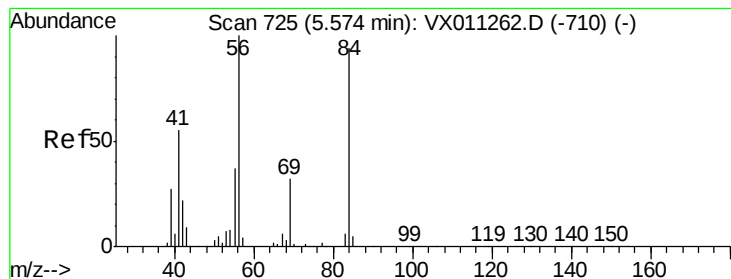

#31

Cyclohexane

Concen: 1.444 ug/l

RT: 5.65 min Scan# 738

Delta R.T. 0.08 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :

2S-F1-(0)


Tgt Ion: 56 Resp: 3939

Ion Ratio Lower Upper

56 100

69 147.1 25.5 38.3#




84 130.6 75.0 112.4#

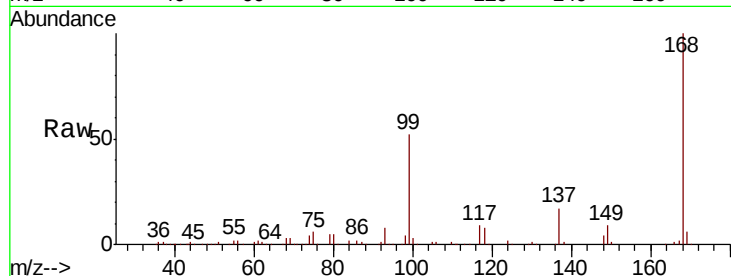

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

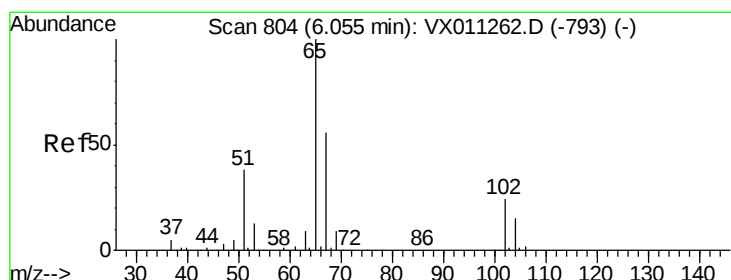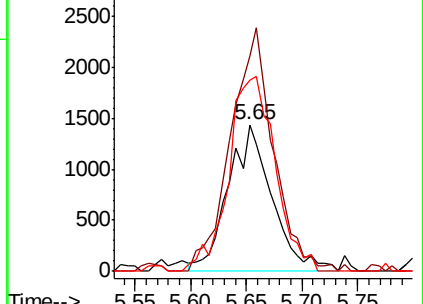

#33

1,2-Dichloroethane-d4

Concen: 51.546 ug/l

RT: 6.06 min Scan# 804

Delta R.T. 0.00 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 65 Resp: 109180

Ion Ratio Lower Upper



65 100


67 51.8 0.0 110.6



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

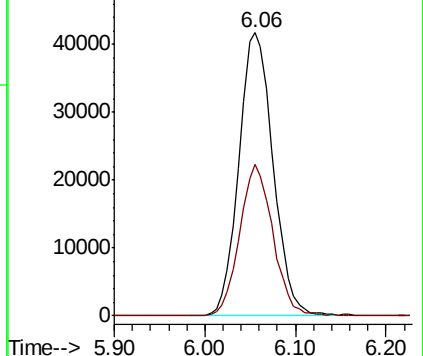

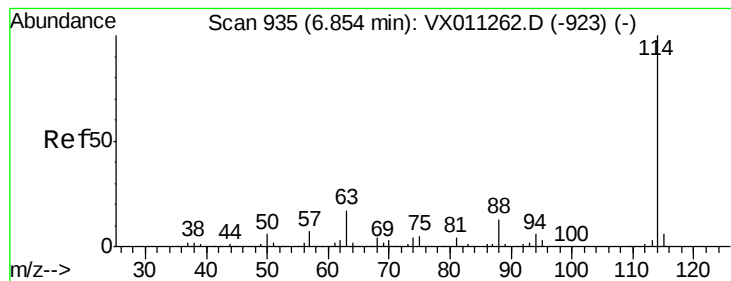

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. 0.00 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :

2S-F1-(0)


Tgt Ion:114 Resp: 306808

Ion Ratio Lower Upper

114 100

63 17.2 0.0 34.0




88 14.6 0.0 26.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

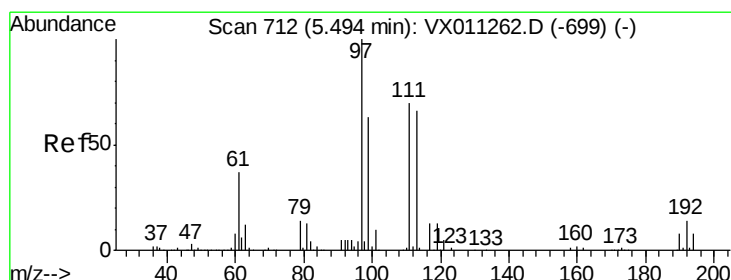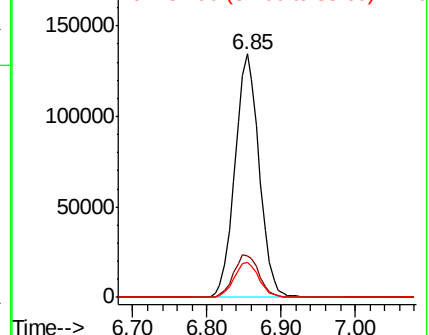

#35

Dibromofluoromethane

Concen: 46.604 ug/l

RT: 5.49 min Scan# 711

Delta R.T. -0.01 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32


Tgt Ion:113 Resp: 93351

Ion Ratio Lower Upper

113 100

111 102.7 81.9 122.9



192 21.5 17.8 26.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



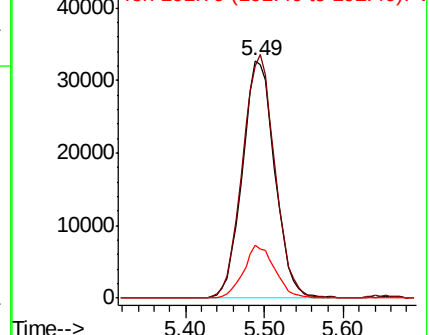





#36
 1,1-Dichloropropene
 Concen: 5.087 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.13 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32




Instrument :
 MSVOA_X
 ClientSampleId :
 2S-F1-(0)


Tgt Ion: 75 Resp: 13626
 Ion Ratio Lower Upper
 75 100
 110 11.7 20.0 59.9#
 77 0.0 24.8 37.2#

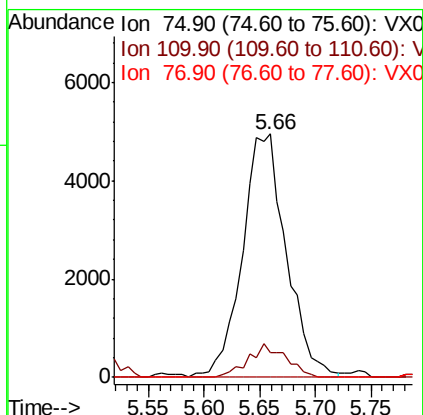

#38
 Carbon Tetrachloride
 Concen: 7.311 ug/l
 RT: 5.65 min Scan# 737
 Delta R.T. -0.13 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32

Tgt Ion: 117 Resp: 19702
 Ion Ratio Lower Upper
 117 100
 119 3.2 79.0 118.4#
 121 0.0 25.9 38.9#

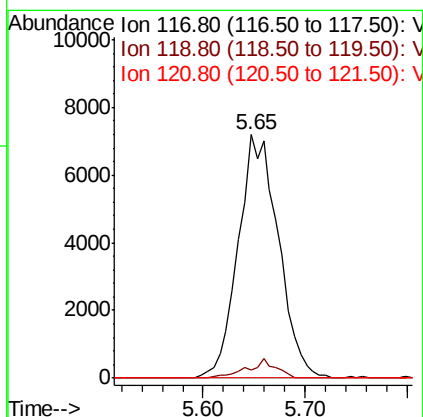

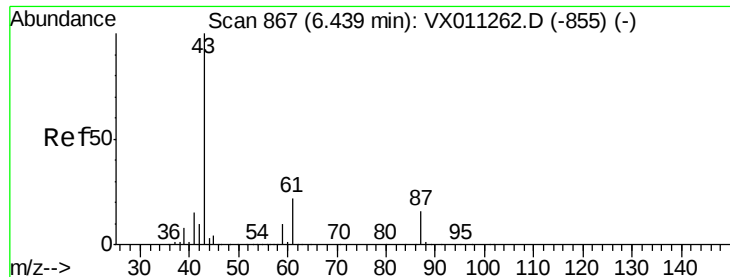

#43

Isopropyl Acetate

Concen: 1.908 ug/l

RT: 6.43 min Scan# 866

Delta R.T. -0.01 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :

2S-F1-(0)


Tgt Ion: 43 Resp: 8197

Ion Ratio Lower Upper

43 100

61 20.9 16.5 24.7




87 15.6 12.1 18.1

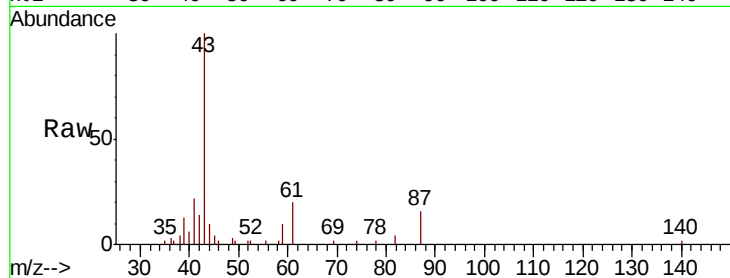

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

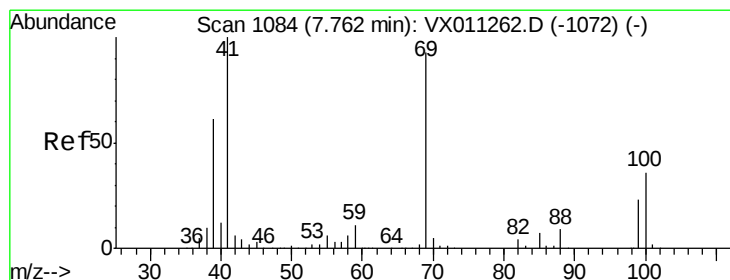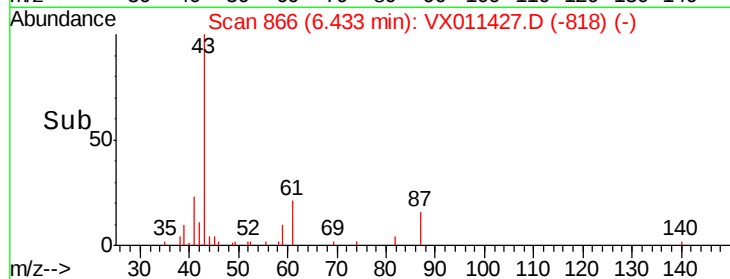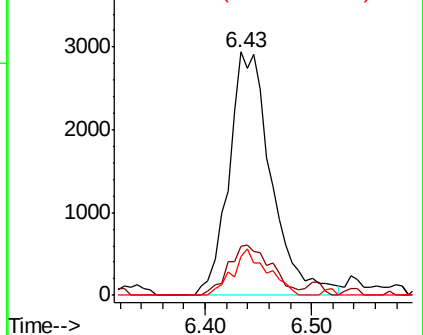

#48

Methyl methacrylate

Concen: 1.794 ug/l

RT: 7.68 min Scan# 1070

Delta R.T. -0.09 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32


Tgt Ion: 41 Resp: 3627

Ion Ratio Lower Upper

41 100

69 0.0 74.5 111.7#



39 0.0 48.6 72.8#

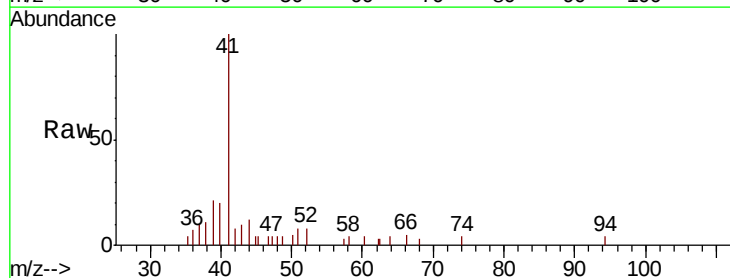


Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0



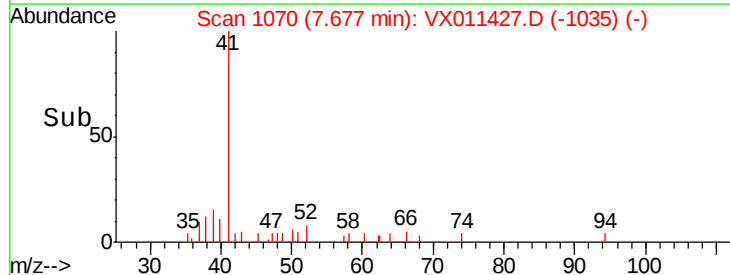
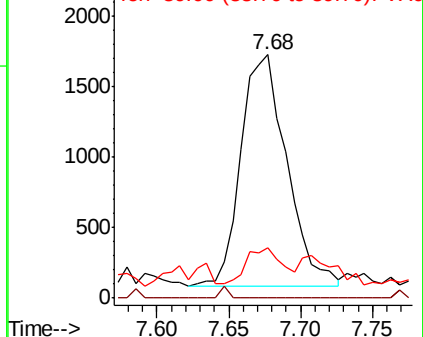


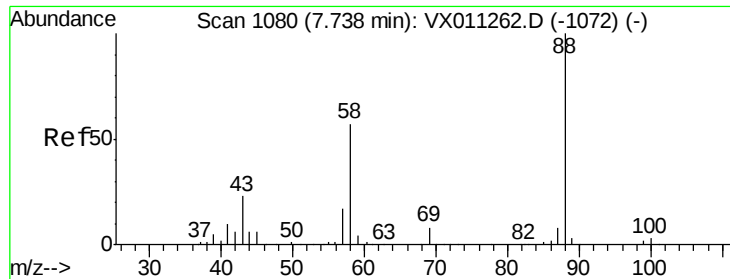

#49
1,4-Dioxane
Concen: 0.358 ug/l
RT: 7.63 min Scan# 1063
Delta R.T. -0.10 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32




Instrument :
MSVOA_X
ClientSampleId :
2S-F1-(0)


Tgt Ion: 88 Resp: 21
Ion Ratio Lower Upper
88 100
43 0.0 22.2 33.2#
58 823.8 47.8 71.8#

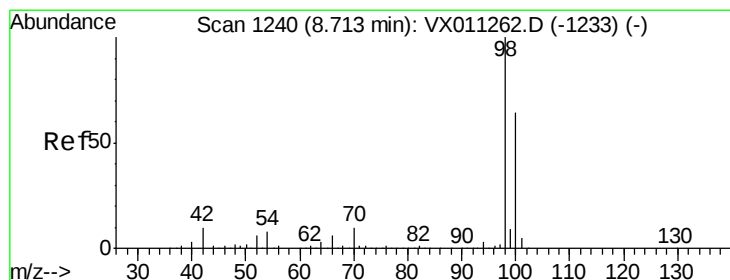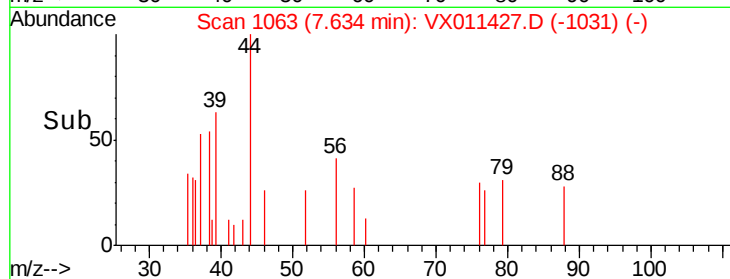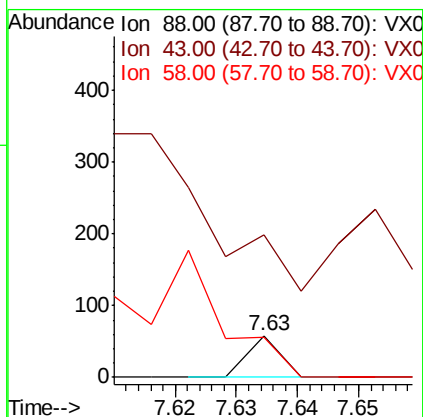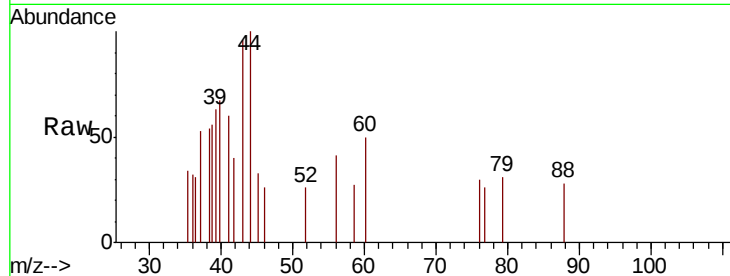

#50
Toluene-d8
Concen: 48.049 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32

Tgt Ion: 98 Resp: 363302
Ion Ratio Lower Upper
98 100
100 64.4 51.7 77.5

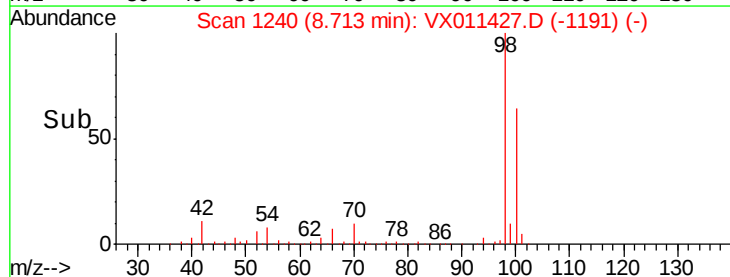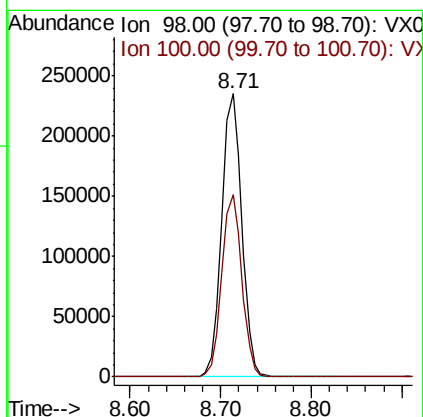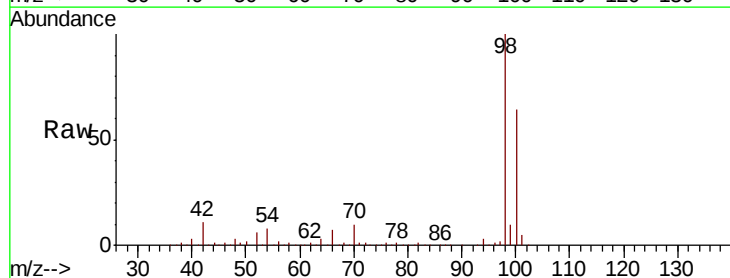

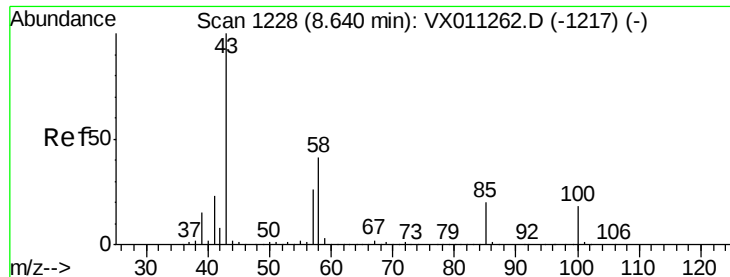

#51

4-Methyl-2-Pentanone

Concen: 15.942 ug/l

RT: 8.61 min Scan# 1223

Delta R.T. -0.03 min

Lab File: VX011427.D

Acq: 11 Aug 2019 13:32

Instrument :

MSVOA_X

ClientSampleId :


2S-F1-(0)

Tgt Ion: 43 Resp: 44198

Ion Ratio Lower Upper




43 100

58 7.8 32.3 48.5#

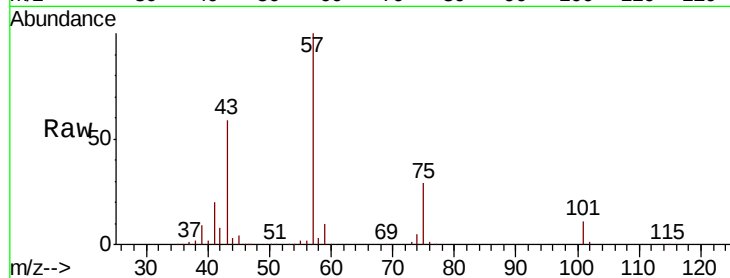

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

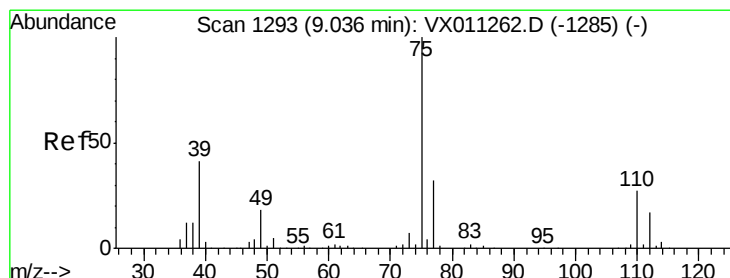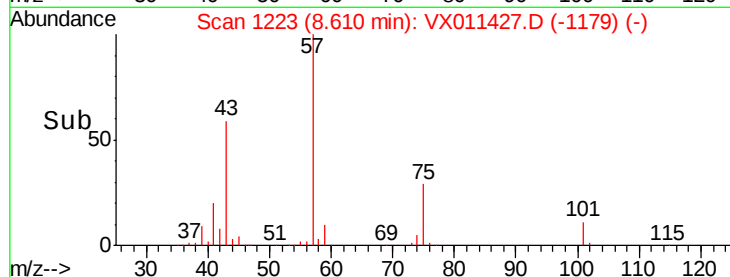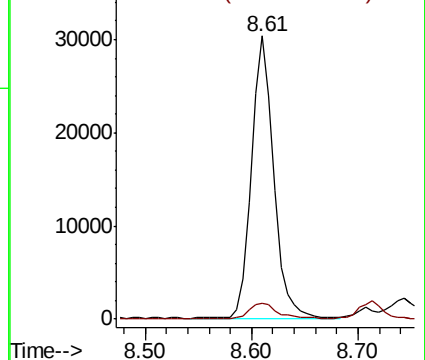

#53

t-1,3-Dichloropropene

Concen: 2.871 ug/l

RT: 9.04 min Scan# 1294

Delta R.T. 0.01 min

Lab File: VX011427.D


Acq: 11 Aug 2019 13:32

Tgt Ion: 75 Resp: 104

Ion Ratio Lower Upper



75 100


77 0.0 25.4 38.0#

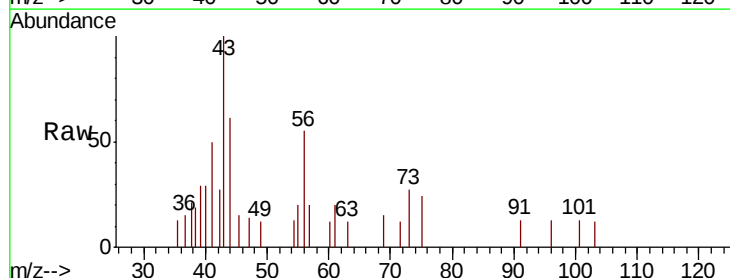

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

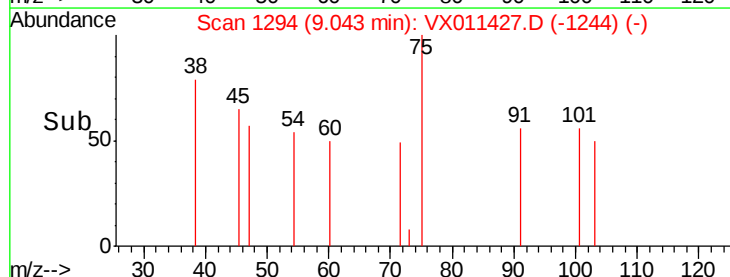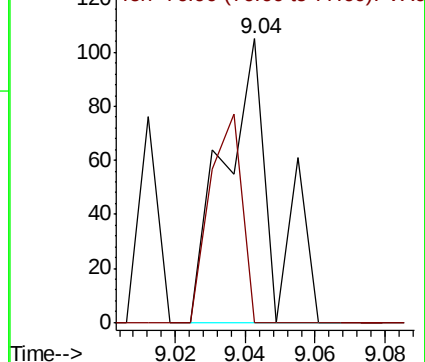

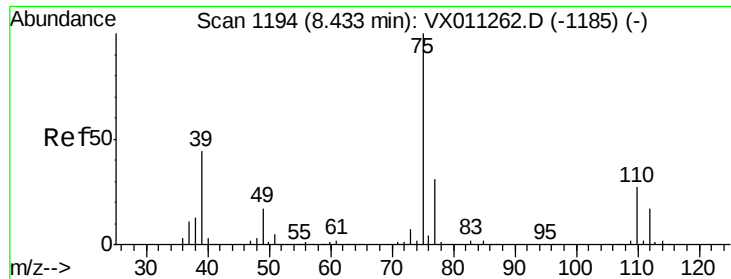


#54




cis-1,3-Dichloropropene
 Concen: 7.322 ug/l
 RT: 8.61 min Scan# 1223
 Delta R.T. 0.18 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32

Instrument :
 MSVOA_X
 ClientSampleId :
 2S-F1-(0)

Tgt Ion: 75 Resp: 21884
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.0 37.6#
 39 30.7 35.3 52.9#

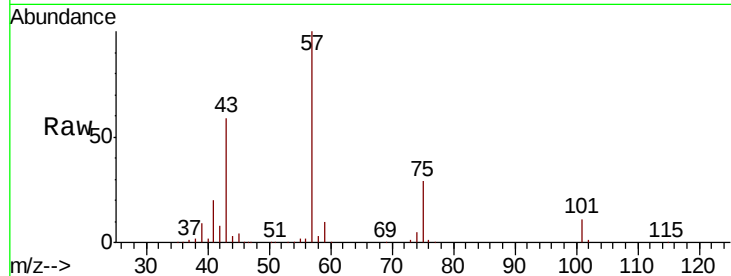


Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 76.90 (76.60 to 77.60): VX0
 Ion 39.00 (38.70 to 39.70): VX0

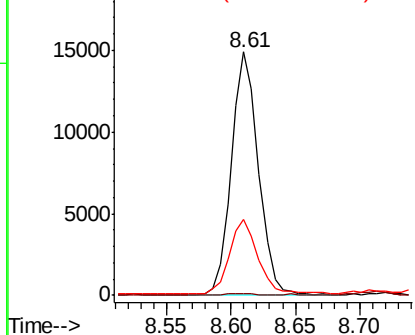



#57


1,3-Dichloropropane
 Concen: 1.550 ug/l
 RT: 9.54 min Scan# 1375
 Delta R.T. 0.17 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32

Tgt Ion: 76 Resp: 5325
 Ion Ratio Lower Upper
 76 100
 78 0.5 26.6 40.0#



Abundance Ion 75.90 (75.60 to 76.60): VX0
 Ion 77.90 (77.60 to 78.60): VX0



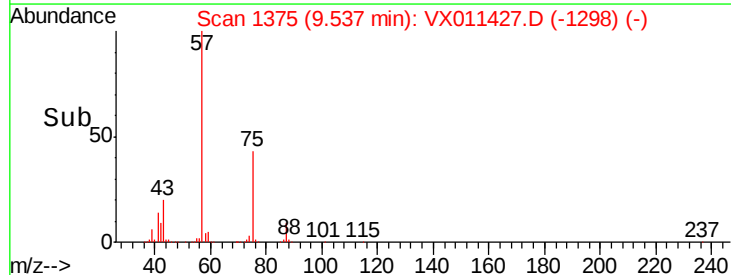
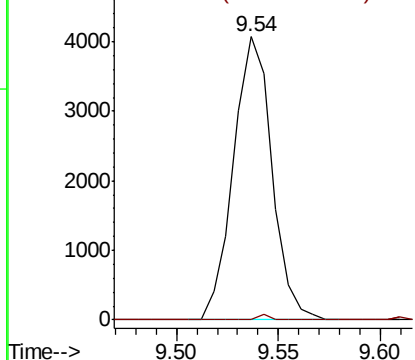


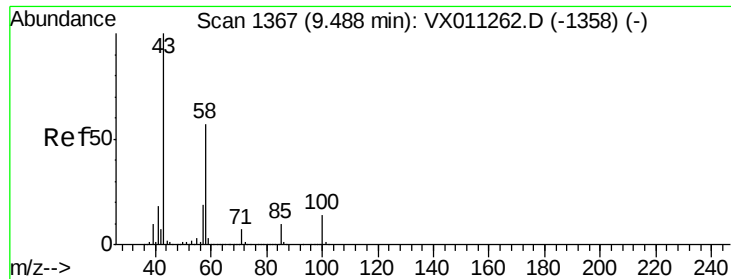

#59
2-Hexanone
Concen: 31.677 ug/l
RT: 9.54 min Scan# 1375
Delta R.T. 0.05 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32




Instrument :
MSVOA_X
ClientSampleId :
2S-F1-(0)


Tgt Ion: 43 Resp: 68022
Ion Ratio Lower Upper
43 100
58 19.1 28.2 84.6#

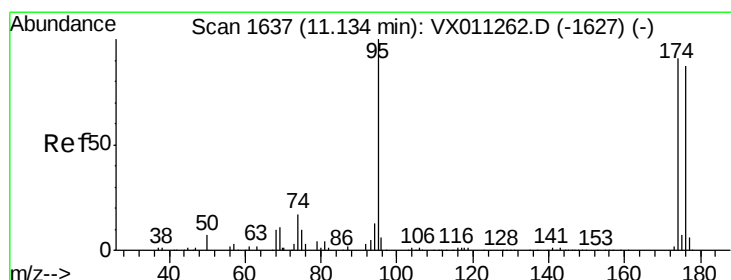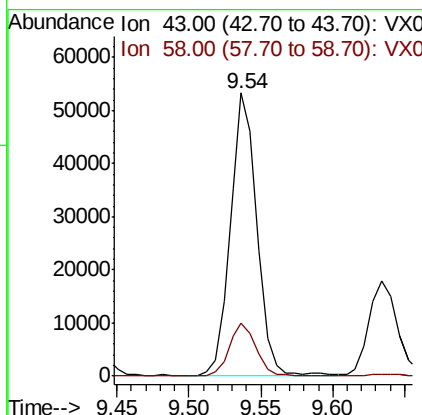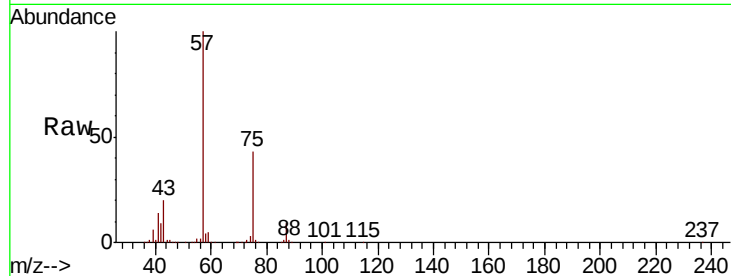

#62
4-Bromofluorobenzene
Concen: 45.082 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32

Tgt Ion: 95 Resp: 121700
Ion Ratio Lower Upper
95 100
174 90.9 0.0 191.2
176 88.8 0.0 184.8

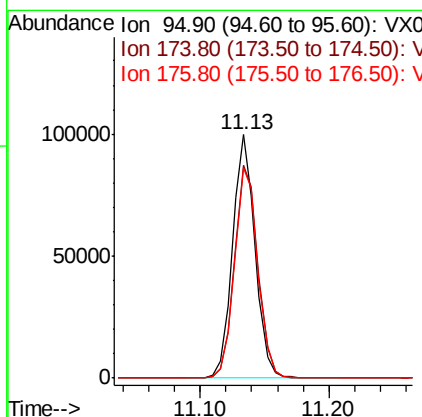


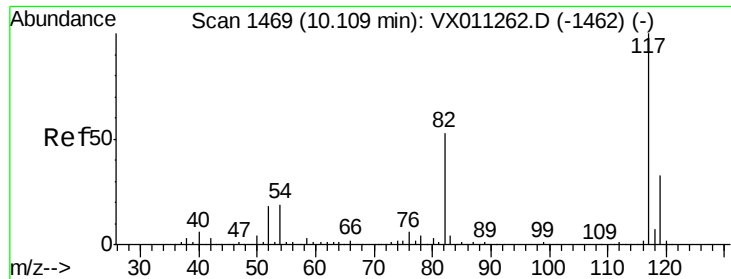




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32

Instrument :
MSVOA_X
ClientSampled :
2S-F1-(0)

Tgt Ion:117 Resp: 280170
Ion Ratio Lower Upper
117 100
82 52.0 42.2 63.2
119 32.1 26.6 39.8

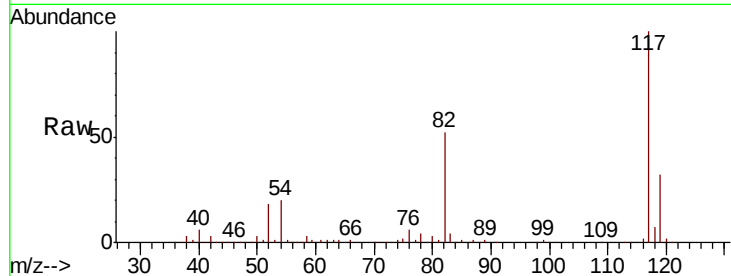


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V


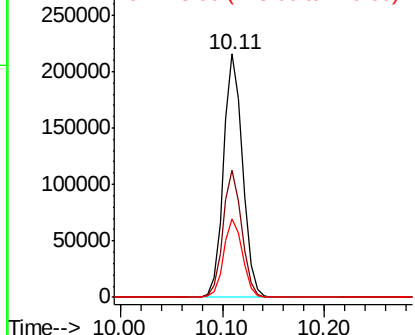



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1791
Delta R.T. -0.01 min
Lab File: VX011427.D
Acq: 11 Aug 2019 13:32

Tgt Ion:152 Resp: 125730
Ion Ratio Lower Upper
152 100
115 55.8 40.0 119.9
150 157.0 0.0 350.4



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V




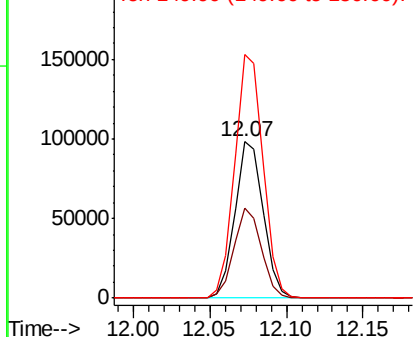


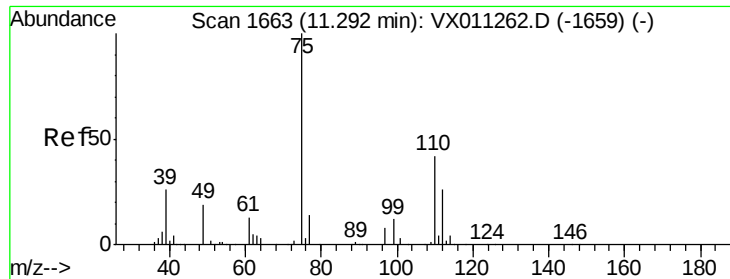

#76
 1,2,3-Trichloropropane
 Concen: 27.339 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32

Instrument :
 MSVOA_X
 ClientSampleId :
 2S-F1-(0)

Tgt Ion: 75 Resp: 62598
 Ion Ratio Lower Upper
 75 100
 77 1.2 21.1 63.4#

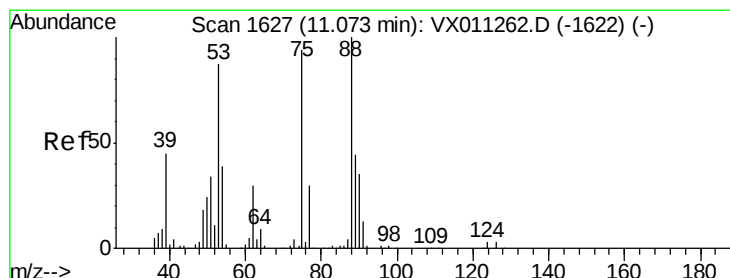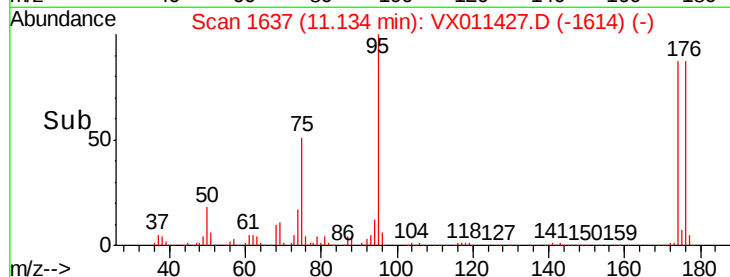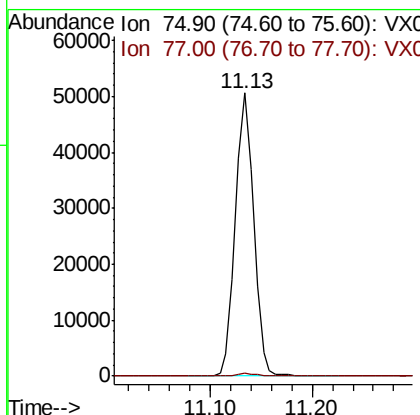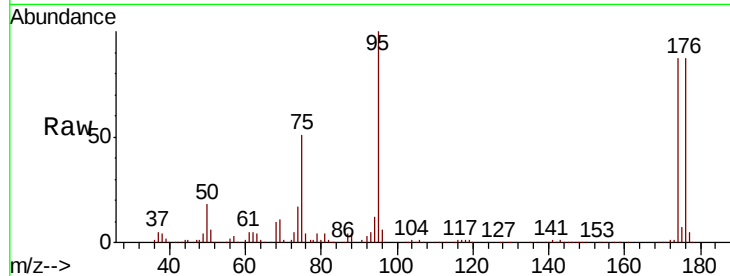

#81
 trans-1,4-Dichloro-2-butene
 Concen: 70.920 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX011427.D
 Acq: 11 Aug 2019 13:32

Tgt Ion: 75 Resp: 62598
 Ion Ratio Lower Upper
 75 100
 53 0.2 78.2 117.4#
 89 0.0 37.9 56.9#

