

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023652.D
 Acq On : 11 Aug 2021 16:29
 Operator : JC/MD
 Sample : M3364-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 12 01:28:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 11 12:02:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	324512	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	298984	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130235	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	77686	45.929	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.860%		
7) Chloroethane-d5	1.666	69	66925	48.164	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.320%		
11) 1,1-Dichloroethene-d2	2.306	63	131015	35.659	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.320%		
21) 2-Butanone-d5	4.465	46	158848	97.410	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.410%		
24) Chloroform-d	5.068	84	177837	46.432	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.860%		
26) 1,2-Dichloroethane-d4	5.964	65	124888	47.567	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.140%		
32) Benzene-d6	5.983	84	368474	48.923	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.840%		
36) 1,2-Dichloropropane-d6	7.318	67	115841	48.883	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.760%		
41) Toluene-d8	8.653	98	338830	46.712	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.420%		
43) trans-1,3-Dichloroprop...	9.025	79	180	0.161	ug/L	0.07
Spiked Amount 50.000	Range 60 - 125		Recovery =	0.320%#		
47) 2-Hexanone-d5	9.390	63	114824	100.783	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.780%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	156007	49.418	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.840%		
66) 1,2-Dichlorobenzene-d4	12.323	152	116553	50.999	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.000%		
Target Compounds						Qvalue
13) Acetone	2.392	43	6320	4.402	ug/L	87
39) cis-1,3-Dichloropropene	8.336	75	3746	1.194	ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023652.D
Acq On : 11 Aug 2021 16:29
Operator : JC/MD
Sample : M3364-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :

Quant Time: Aug 12 01:28:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 11 12:02:06 2021
Response via : Initial Calibration




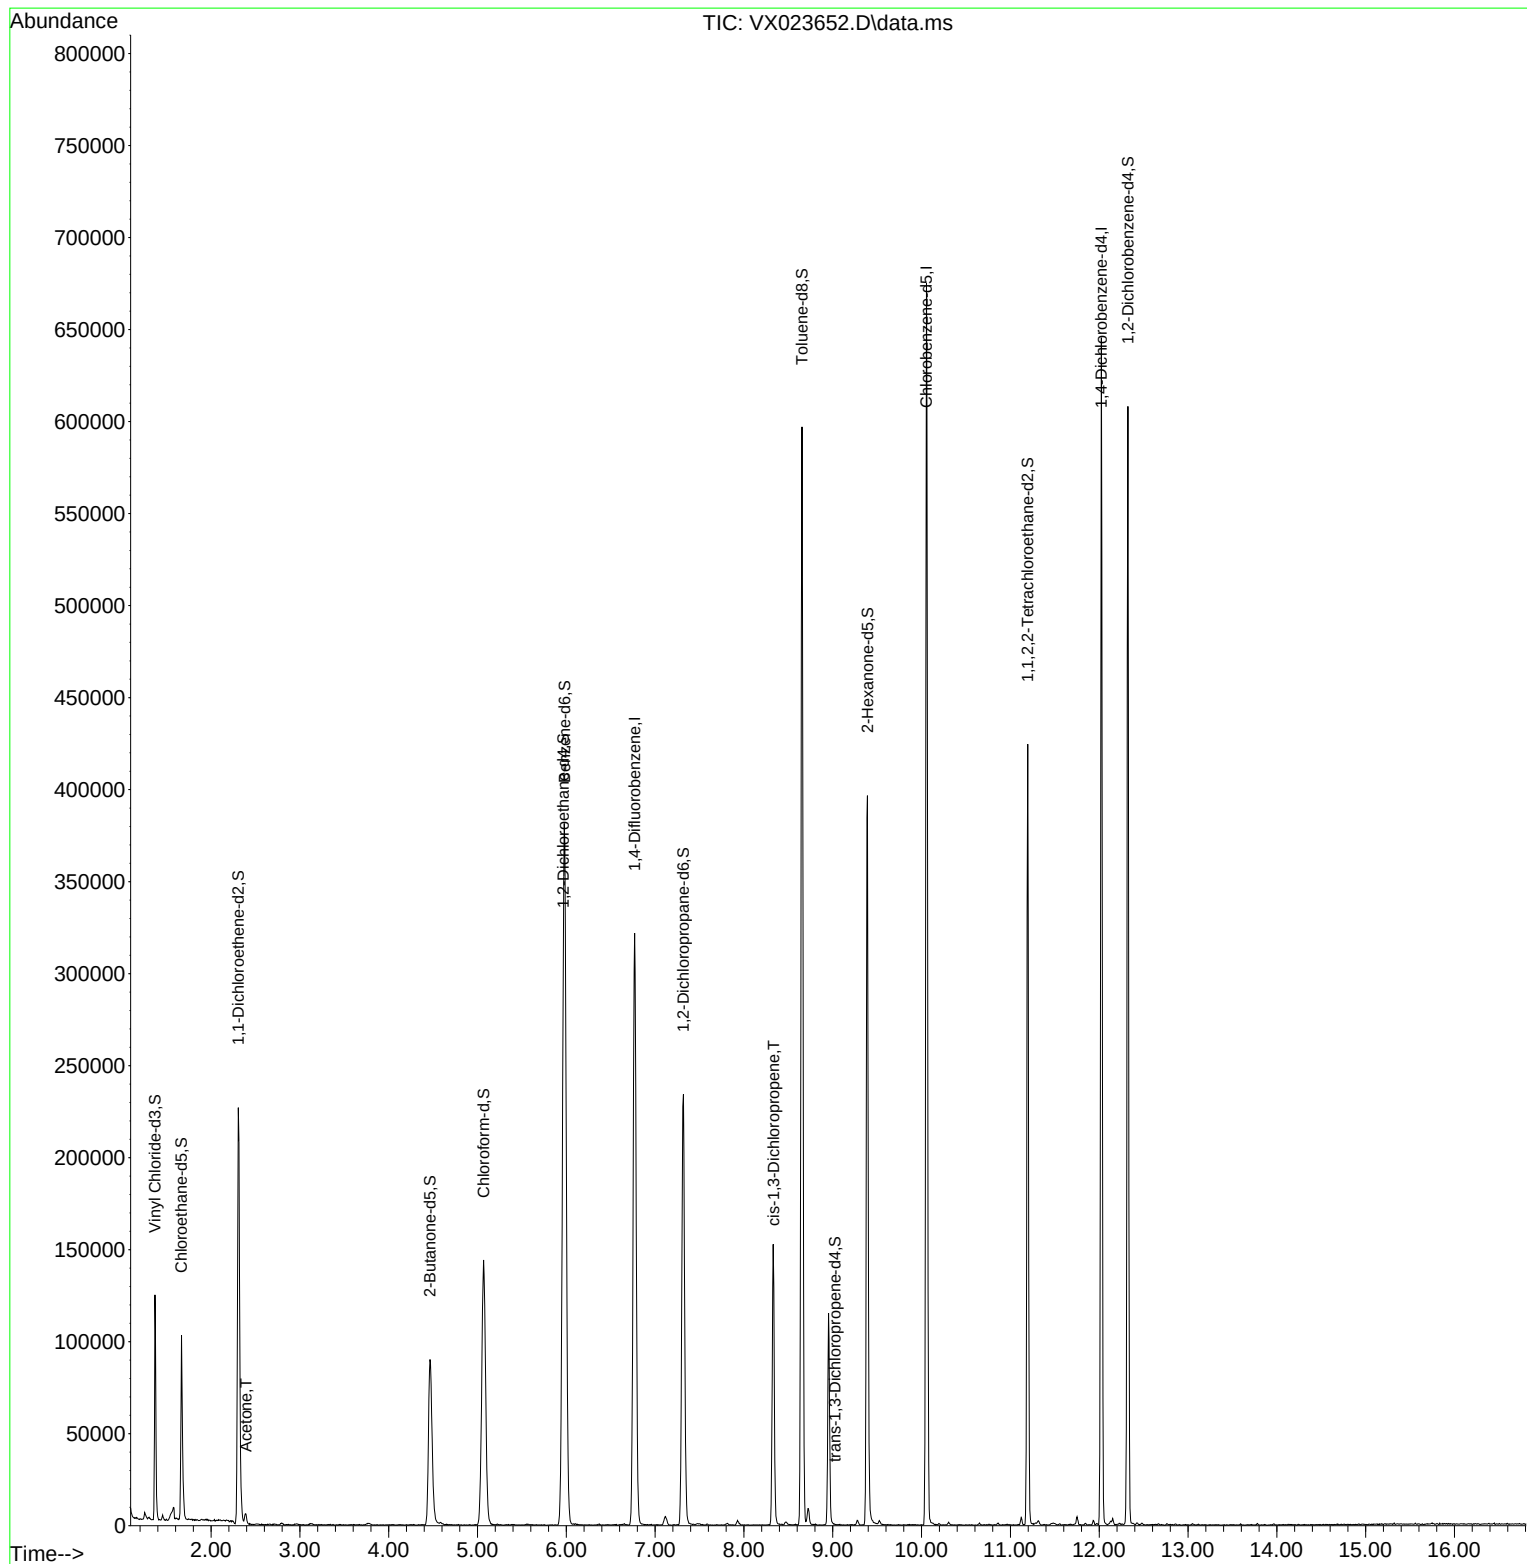


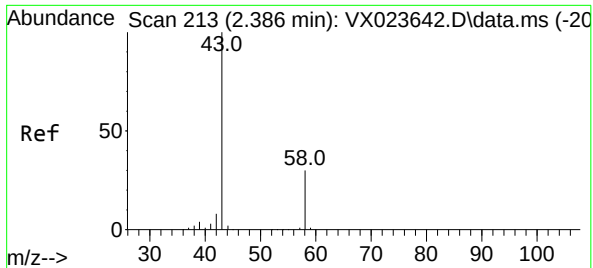

#13
Acetone
Concen: 4.402 ug/L
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX023652.D
Acq: 11 Aug 2021 16:29

Instrument :
MSVOA_X
ClientSampled :

Tgt Ion: 43 Resp: 6320
Ion Ratio Lower Upper
43 100
58 26.7 0.0 68.2

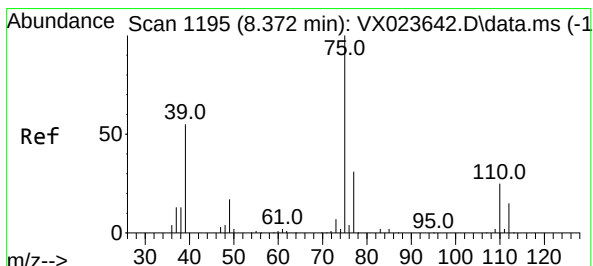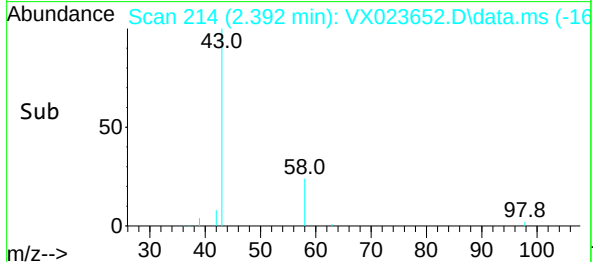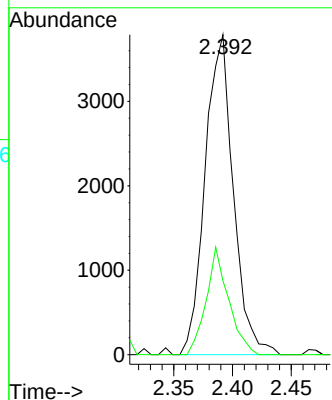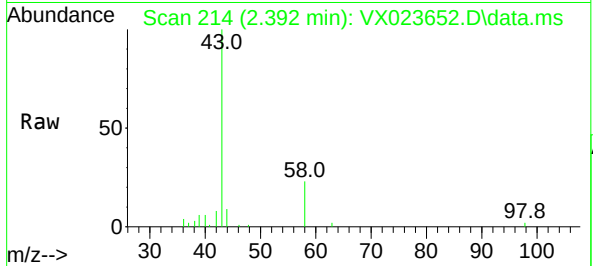

#39
cis-1,3-Dichloropropene
Concen: 1.194 ug/L
RT: 8.336 min Scan# 1189
Delta R.T. -0.037 min
Lab File: VX023652.D
Acq: 11 Aug 2021 16:29

Tgt Ion: 75 Resp: 3746
Ion Ratio Lower Upper
75 100
77 45.9 22.7 42.3#

