

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023657.D
 Acq On : 11 Aug 2021 18:27
 Operator : JC/MD
 Sample : M3364-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK90

Quant Time: Aug 12 01:29:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 11 12:02:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	309213	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	280698	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	122358	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	75064	46.574	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.140%
7) Chloroethane-d5	1.666	69	64655	48.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.660%
11) 1,1-Dichloroethene-d2	2.306	63	125495	35.846	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.700%
21) 2-Butanone-d5	4.465	46	156603	100.785	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.780%
24) Chloroform-d	5.068	84	170113	46.613	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.220%
26) 1,2-Dichloroethane-d4	5.970	65	120516	48.173	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.340%
32) Benzene-d6	5.983	84	353083	49.934	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.860%
36) 1,2-Dichloropropane-d6	7.318	67	109718	49.315	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.620%
41) Toluene-d8	8.653	98	326008	47.873	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.740%
43) trans-1,3-Dichloroprop...	8.952	79	46570	44.232	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.460%
47) 2-Hexanone-d5	9.390	63	112029	104.736	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.740%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	145994	49.259	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.520%
66) 1,2-Dichlorobenzene-d4	12.323	152	109550	51.021	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.040%
Target Compounds						
					Qvalue	
13) Acetone	2.386	43	6126	4.478	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023657.D
Acq On : 11 Aug 2021 18:27
Operator : JC/MD
Sample : M3364-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK90

Quant Time: Aug 12 01:29:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 11 12:02:06 2021
Response via : Initial Calibration

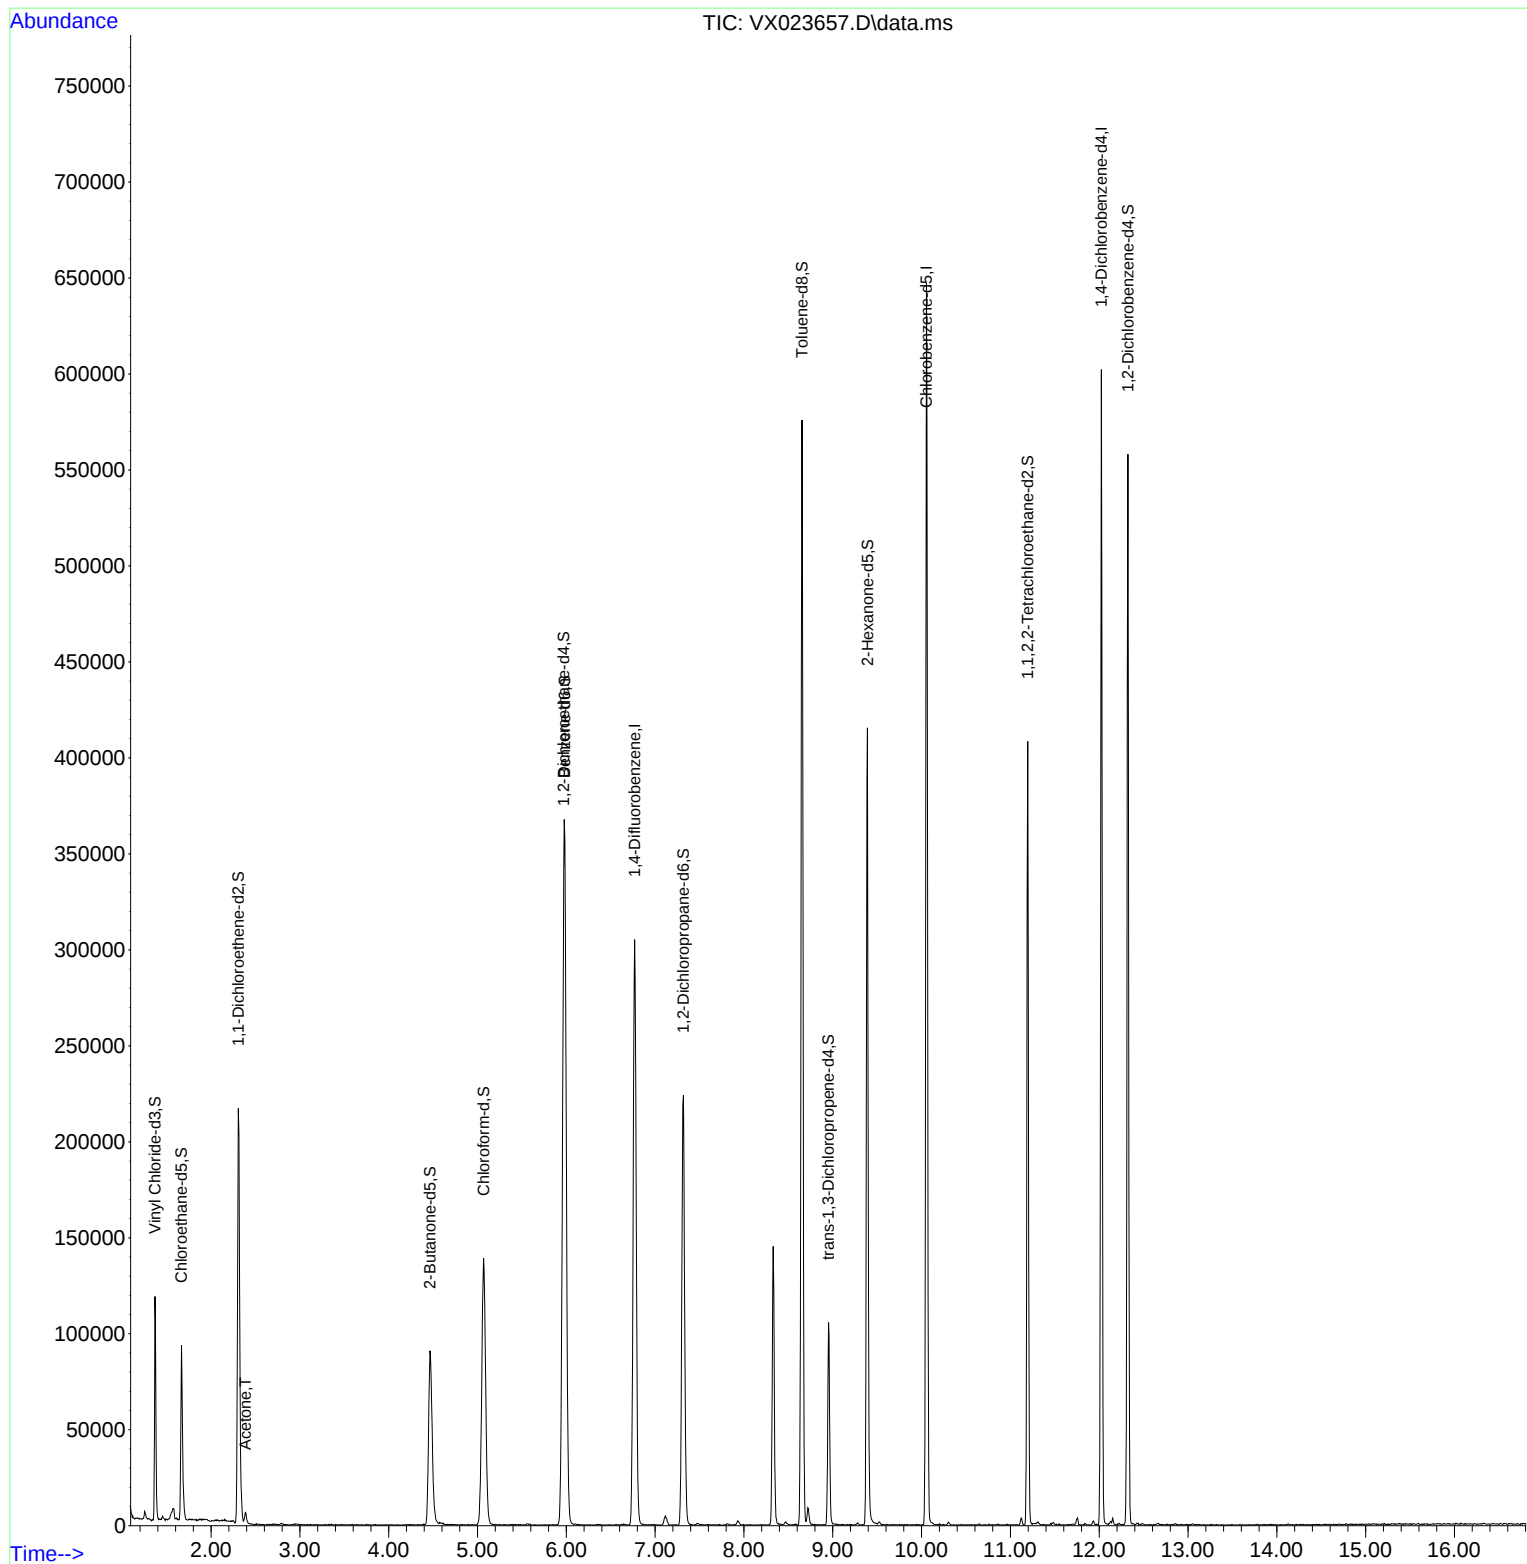

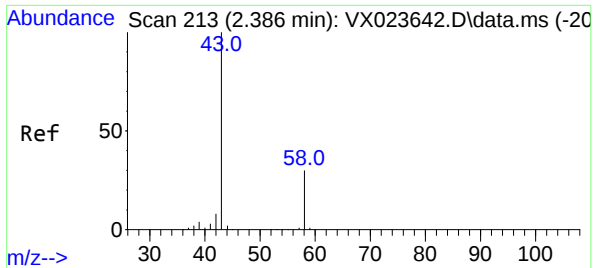

#13
 Acetone
 Concen: 4.478 ug/L
 RT: 2.386 min Scan# 213
 Delta R.T. -0.000 min
 Lab File: VX023657.D
 Acq: 11 Aug 2021 18:27

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK90

Tgt Ion:	43	Resp:	6126
Ion	Ratio	Lower	Upper
43	100		
58	29.0	0.0	68.2

