

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023658.D
 Acq On : 11 Aug 2021 18:50
 Operator : JC/MD
 Sample : M3364-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK92

Quant Time: Aug 12 01:29:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 11 12:02:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	293205	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	269880	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	118324	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	71143	46.551	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	93.100%	
7) Chloroethane-d5	1.666	69	62706	49.947	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	99.900%	
11) 1,1-Dichloroethene-d2	2.307	63	123565	37.222	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	74.440%	
21) 2-Butanone-d5	4.471	46	152586	103.561	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.560%	
24) Chloroform-d	5.068	84	166805	48.202	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.964	65	116575	49.142	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.280%	
32) Benzene-d6	5.983	84	345411	50.807	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.620%	
36) 1,2-Dichloropropane-d6	7.318	67	108613	50.775	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.560%	
41) Toluene-d8	8.653	98	317459	48.486	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.980%	
43) trans-1,3-Dichloroprop...	8.952	79	44665	44.123	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.240%	
47) 2-Hexanone-d5	9.391	63	107423	104.455	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	104.460%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	147147	51.638	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	103.280%	
66) 1,2-Dichlorobenzene-d4	12.323	152	110182	53.065	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.120%	
Target Compounds						
13) Acetone	2.392	43	4915	3.789	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023658.D
Acq On : 11 Aug 2021 18:50
Operator : JC/MD
Sample : M3364-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK92

Quant Time: Aug 12 01:29:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 11 12:02:06 2021
Response via : Initial Calibration

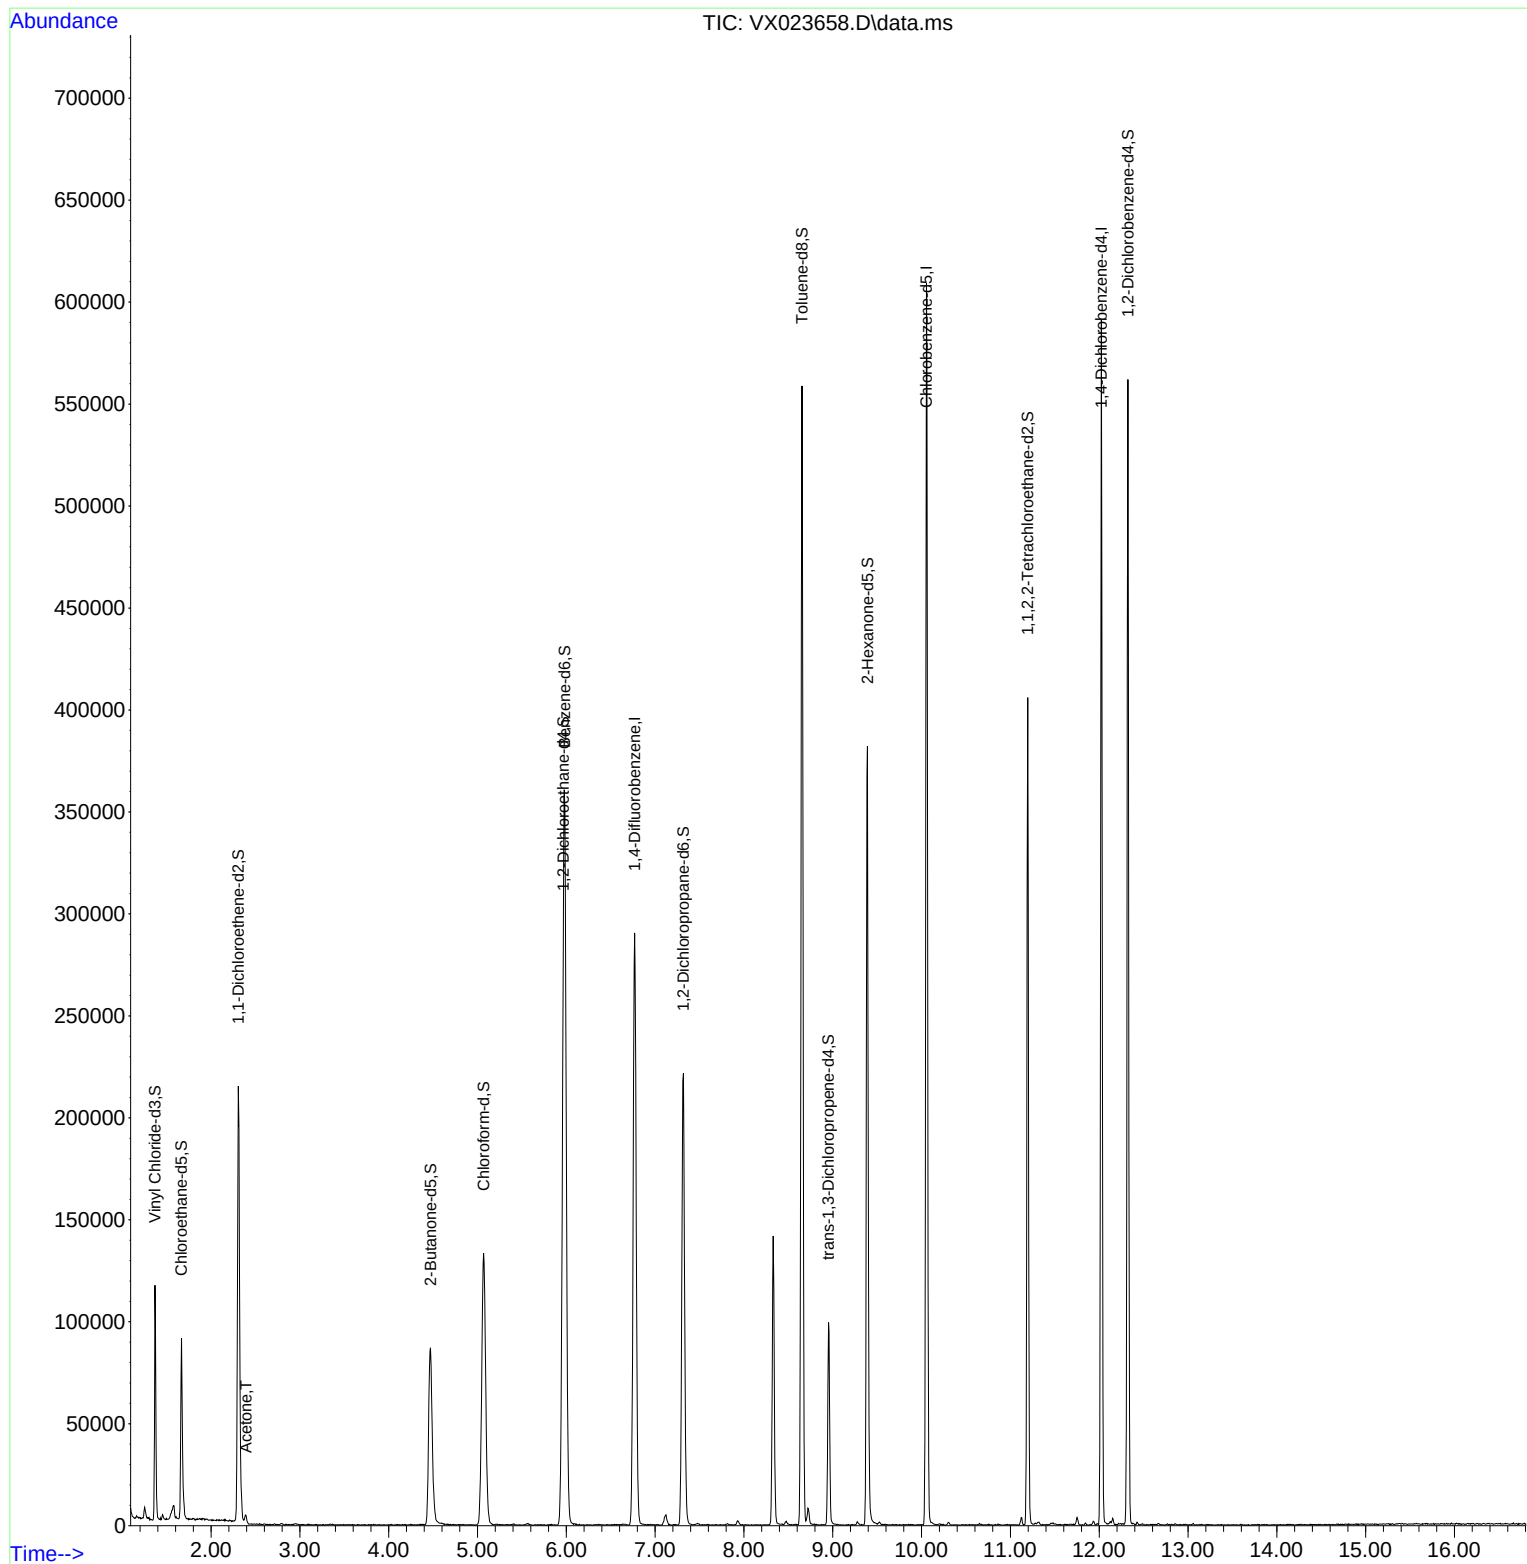

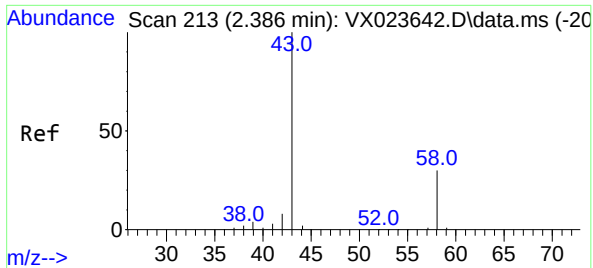

#13
Acetone
Concen: 3.789 ug/L
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX023658.D
Acq: 11 Aug 2021 18:50

Instrument :
MSVOA_X
ClientSampleId :
DBK92

Tgt Ion: 43 Resp: 4915
Ion Ratio Lower Upper
43 100
58 27.4 0.0 68.2

