

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023645.D
 Acq On : 11 Aug 2021 10:54
 Operator : JC/MD
 Sample : VIBLK600
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.173	11	14	18	rVB	4441	5097	0.40%	0.050%
2	1.295	32	34	40	rBV	2831	2767	0.22%	0.027%
3	1.368	43	46	54	rVB	143035	151894	11.91%	1.504%
4	1.666	91	95	104	rVB	111349	144945	11.37%	1.435%
5	2.307	194	200	211	rVB	254884	441080	34.59%	4.366%
6	2.514	230	234	246	rVB	7458	13895	1.09%	0.138%
7	2.636	252	254	257	rBV2	499	463	0.04%	0.005%
8	2.715	262	267	272	rBV4	1555	3069	0.24%	0.030%
9	2.794	275	280	290	rVB2	4778	9029	0.71%	0.089%
10	2.947	300	305	315	rVB4	1158	2947	0.23%	0.029%
11	3.050	321	322	324	rBV	386	320	0.03%	0.003%
12	3.105	324	331	342	rVB5	5931	16715	1.31%	0.165%
13	3.386	372	377	379	rBV3	238	393	0.03%	0.004%
14	3.556	403	405	407	rBV	284	327	0.03%	0.003%
15	3.623	410	416	422	rVB2	1235	2890	0.23%	0.029%
16	3.678	423	425	428	rVB	442	333	0.03%	0.003%
17	3.727	428	433	435	rBV2	523	682	0.05%	0.007%
18	3.837	449	451	454	rVB	444	288	0.02%	0.003%
19	3.934	464	467	470	rBV3	402	463	0.04%	0.005%
20	4.111	494	496	498	rBV2	440	263	0.02%	0.003%
21	4.471	545	555	569	rBV	108294	310322	24.33%	3.072%
22	4.757	600	602	605	rVB	358	334	0.03%	0.003%
23	4.812	609	611	613	rVB2	352	327	0.03%	0.003%
24	4.910	622	627	634	rVB7	1852	4488	0.35%	0.044%
25	5.068	641	653	670	rVV	160084	498619	39.10%	4.936%
26	5.385	698	705	706	rBV4	2530	3085	0.24%	0.031%
27	5.690	749	755	760	rVB4	1730	4286	0.34%	0.042%
28	5.818	774	776	778	rBV2	384	383	0.03%	0.004%
29	5.977	790	802	819	rBV2	432071	1275248	100.00%	12.624%
30	6.184	834	836	840	rVB4	349	378	0.03%	0.004%
31	6.476	883	884	887	rVB3	559	371	0.03%	0.004%
32	6.769	922	932	947	rBV	336800	789374	61.90%	7.814%
33	6.928	955	958	960	rVB3	347	340	0.03%	0.003%
34	7.123	982	990	1000	rVB5	9668	25197	1.98%	0.249%
35	7.318	1012	1022	1030	rBV	264229	577635	45.30%	5.718%
36	7.671	1078	1080	1083	rVB3	268	269	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023645.D
 Acq On : 11 Aug 2021 10:54
 Operator : JC/MD
 Sample : VIBLK600
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.824	1098	1105	1111	rVB5	2204	4767	0.37%	0.047%
38	7.934	1118	1123	1126	rBV2	2298	4153	0.33%	0.041%
39	8.025	1136	1138	1141	rBV4	246	278	0.02%	0.003%
40	8.110	1151	1152	1157	rVB	470	355	0.03%	0.004%
41	8.196	1164	1166	1169	rVV3	410	312	0.02%	0.003%
42	8.330	1181	1188	1202	rBV	176880	294852	23.12%	2.919%
43	8.470	1208	1211	1218	rVB3	1850	3028	0.24%	0.030%
44	8.580	1224	1229	1234	rBV2	4484	7672	0.60%	0.076%
45	8.653	1234	1241	1248	rVV	692763	1053038	82.58%	10.424%
46	8.726	1248	1253	1261	rVB	18110	30549	2.40%	0.302%
47	8.952	1284	1290	1301	rBV	128537	201018	15.76%	1.990%
48	9.159	1319	1324	1330	rVB5	3525	5627	0.44%	0.056%
49	9.281	1339	1344	1350	rVB2	10115	15162	1.19%	0.150%
50	9.391	1356	1362	1375	rBV	483104	696154	54.59%	6.892%
51	9.525	1381	1384	1388	rVB3	2141	2739	0.21%	0.027%
52	9.616	1395	1399	1403	rVB	1983	2789	0.22%	0.028%
53	9.933	1449	1451	1453	rVB2	372	265	0.02%	0.003%
54	10.012	1460	1464	1465	rBV3	255	383	0.03%	0.004%
55	10.055	1465	1471	1484	rVV	681088	960778	75.34%	9.511%
56	10.195	1490	1494	1499	rVB	12258	16727	1.31%	0.166%
57	10.305	1507	1512	1518	rBV2	14172	18662	1.46%	0.185%
58	10.366	1521	1522	1526	rVB2	391	338	0.03%	0.003%
59	10.403	1526	1528	1530	rBV2	282	262	0.02%	0.003%
60	10.439	1530	1534	1535	rBV	229	296	0.02%	0.003%
61	10.531	1546	1549	1551	rVB3	444	440	0.03%	0.004%
62	10.586	1556	1558	1560	rVV2	469	386	0.03%	0.004%
63	10.653	1563	1569	1578	rVV2	14884	28930	2.27%	0.286%
64	10.756	1584	1586	1589	rVV2	514	510	0.04%	0.005%
65	10.799	1590	1593	1598	rVB3	1595	2411	0.19%	0.024%
66	10.848	1598	1601	1602	rBV2	522	359	0.03%	0.004%
67	10.963	1615	1620	1628	rBV	13392	18506	1.45%	0.183%
68	11.085	1638	1640	1641	rBV	716	491	0.04%	0.005%
69	11.122	1642	1646	1652	rVB2	5269	6880	0.54%	0.068%
70	11.195	1652	1658	1664	rBV	461897	592781	46.48%	5.868%
71	11.451	1696	1700	1705	rBV	14855	20008	1.57%	0.198%
72	11.549	1714	1716	1719	rBV2	610	566	0.04%	0.006%
73	11.756	1745	1750	1757	rVB2	19797	25164	1.97%	0.249%
74	11.847	1761	1765	1767	rVB2	953	1269	0.10%	0.013%
75	11.933	1776	1779	1782	rBV4	2343	3322	0.26%	0.033%
76	11.969	1782	1785	1789	rVV	15281	19056	1.49%	0.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023645.D
 Acq On : 11 Aug 2021 10:54
 Operator : JC/MD
 Sample : VIBLK600
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1806	rVB	665192	840638	65.92%	8.322%
78	12.225	1824	1827	1830	rBV3	812	943	0.07%	0.009%
79	12.323	1836	1843	1851	rBV	669942	838239	65.73%	8.298%
80	12.384	1851	1853	1857	rVB2	756	774	0.06%	0.008%
81	12.433	1857	1861	1864	rVB3	1339	2123	0.17%	0.021%
82	12.482	1864	1869	1873	rBV4	1007	1545	0.12%	0.015%
83	12.622	1890	1892	1896	rVV5	455	460	0.04%	0.005%
84	12.664	1896	1899	1902	rVV3	826	1104	0.09%	0.011%
85	12.859	1928	1931	1934	rVB4	856	859	0.07%	0.009%
86	12.914	1937	1940	1942	rBV3	296	503	0.04%	0.005%
87	12.945	1942	1945	1949	rVB4	1169	1355	0.11%	0.013%
88	13.055	1959	1963	1966	rBV5	893	1320	0.10%	0.013%
89	13.116	1968	1973	1980	rVB	18404	21341	1.67%	0.211%
90	13.213	1985	1989	1994	rBV3	199	453	0.04%	0.004%
91	13.591	2046	2051	2058	rVB	16625	20957	1.64%	0.207%
92	13.780	2078	2082	2089	rVB	14864	18260	1.43%	0.181%
93	13.963	2107	2112	2117	rVB	13988	17402	1.36%	0.172%
94	14.048	2125	2126	2131	rVB2	385	455	0.04%	0.005%
95	14.097	2131	2134	2135	rBV2	338	387	0.03%	0.004%
96	14.128	2135	2139	2143	rVV3	750	1228	0.10%	0.012%
97	14.189	2147	2149	2152	rBV	327	327	0.03%	0.003%
98	14.603	2215	2217	2219	rBV3	331	416	0.03%	0.004%
99	14.743	2238	2240	2243	rVB	354	269	0.02%	0.003%
100	16.097	2460	2462	2464	rBV3	478	475	0.04%	0.005%


Sum of corrected areas: 10101632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023645.D
Acq On : 11 Aug 2021 10:54
Operator : JC/MD
Sample : VIBLK600
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
VIBLK600

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

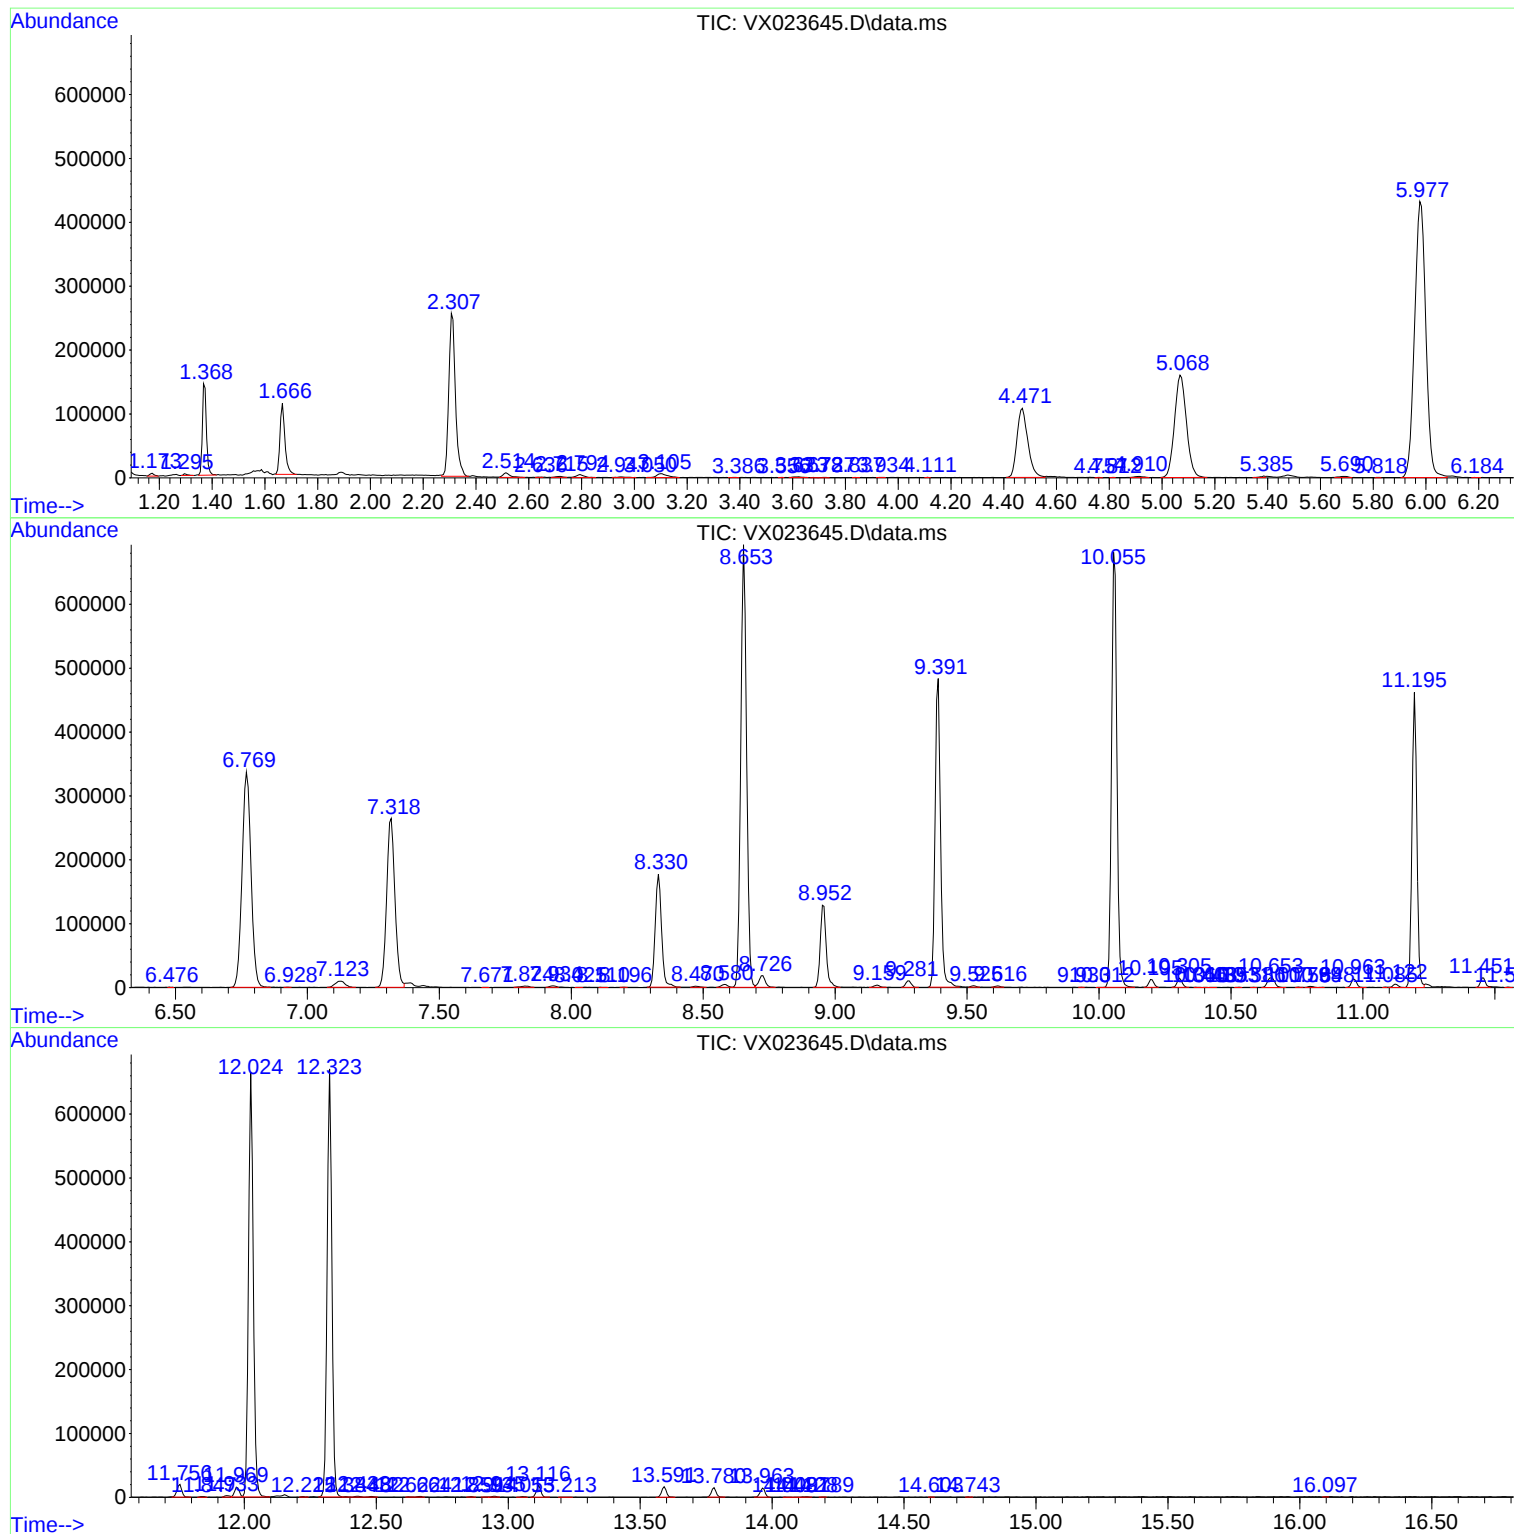

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023645.D
Acq On : 11 Aug 2021 10:54
Operator : JC/MD
Sample : VIBLK600
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK600

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023645.D
Acq On : 11 Aug 2021 10:54
Operator : JC/MD
Sample : VIBLK600
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK600

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
