

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023648.D
 Acq On : 11 Aug 2021 13:22
 Operator : JC/MD
 Sample : VX0811WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	139926	141701	11.41%	1.497%
2	1.666	90	95	105	rVB	110123	142609	11.48%	1.506%
3	2.306	194	200	211	rBV	258942	425986	34.29%	4.499%
4	2.514	229	234	237	rBV2	1480	2062	0.17%	0.022%
5	2.636	252	254	257	rVB3	373	408	0.03%	0.004%
6	3.282	358	360	363	rBV4	265	360	0.03%	0.004%
7	3.349	370	371	376	rVB2	275	271	0.02%	0.003%
8	3.434	383	385	386	rBV2	337	318	0.03%	0.003%
9	3.538	400	402	406	rBV3	360	390	0.03%	0.004%
10	3.581	406	409	411	rBV2	373	383	0.03%	0.004%
11	4.038	482	484	488	rBV2	429	337	0.03%	0.004%
12	4.160	501	504	506	rBV2	357	402	0.03%	0.004%
13	4.465	544	554	570	rBV	105698	300501	24.19%	3.174%
14	4.818	607	612	614	rVV2	355	510	0.04%	0.005%
15	4.867	617	620	621	rBV2	211	258	0.02%	0.003%
16	5.068	640	653	673	rBV	155918	489508	39.41%	5.170%
17	5.196	673	674	676	rVV	446	322	0.03%	0.003%
18	5.227	677	679	681	rVV2	684	398	0.03%	0.004%
19	5.501	723	724	726	rVB2	432	272	0.02%	0.003%
20	5.556	728	733	734	rBV2	1042	1319	0.11%	0.014%
21	5.617	741	743	745	rVB	437	346	0.03%	0.004%
22	5.635	745	746	748	rBV	537	402	0.03%	0.004%
23	5.678	748	753	754	rVV2	210	361	0.03%	0.004%
24	5.836	777	779	781	rBV2	277	357	0.03%	0.004%
25	5.976	788	802	821	rBV2	425265	1242236	100.00%	13.121%
26	6.348	858	863	865	rBV3	363	603	0.05%	0.006%
27	6.367	865	866	869	rVV2	422	253	0.02%	0.003%
28	6.769	922	932	945	rBV	328403	775314	62.41%	8.189%
29	7.019	970	973	979	rVB2	221	401	0.03%	0.004%
30	7.110	980	988	996	rBV4	6127	14092	1.13%	0.149%
31	7.312	1012	1021	1036	rBV	258165	566511	45.60%	5.984%
32	7.476	1045	1048	1054	rVB2	1110	2037	0.16%	0.022%
33	7.525	1054	1056	1059	rBV2	570	749	0.06%	0.008%
34	7.635	1071	1074	1075	rBV2	311	355	0.03%	0.004%
35	7.805	1099	1102	1105	rBV2	840	716	0.06%	0.008%
36	7.927	1118	1122	1130	rBV4	2583	4852	0.39%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023648.D
 Acq On : 11 Aug 2021 13:22
 Operator : JC/MD
 Sample : VX0811WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.171	1160	1162	1168	rVV2	290	450	0.04%	0.005%
38	8.330	1181	1188	1201	rBV	176737	282530	22.74%	2.984%
39	8.470	1206	1211	1215	rBV5	1856	3289	0.26%	0.035%
40	8.653	1234	1241	1249	rBV	666180	1023704	82.41%	10.813%
41	8.726	1249	1253	1258	rVB	9490	14509	1.17%	0.153%
42	8.799	1264	1265	1269	rVB2	354	314	0.03%	0.003%
43	8.836	1269	1271	1275	rVB2	307	340	0.03%	0.004%
44	8.952	1284	1290	1299	rBV	130493	186408	15.01%	1.969%
45	9.141	1317	1321	1323	rBV	398	632	0.05%	0.007%
46	9.250	1337	1339	1340	rBV	409	327	0.03%	0.003%
47	9.275	1340	1343	1349	rVB4	1294	1979	0.16%	0.021%
48	9.384	1356	1361	1372	rBV	457622	668642	53.83%	7.062%
49	10.055	1465	1471	1486	rVV	681446	921781	74.20%	9.736%
50	10.171	1488	1490	1491	rVV2	386	320	0.03%	0.003%
51	10.189	1491	1493	1499	rVB2	1048	1667	0.13%	0.018%
52	10.305	1508	1512	1517	rVB	2251	2697	0.22%	0.028%
53	10.378	1520	1524	1525	rBV2	270	260	0.02%	0.003%
54	10.549	1550	1552	1553	rBV2	302	252	0.02%	0.003%
55	10.652	1564	1569	1578	rVB4	1924	2952	0.24%	0.031%
56	10.762	1584	1587	1589	rVB3	447	499	0.04%	0.005%
57	10.969	1617	1621	1623	rBV3	954	1038	0.08%	0.011%
58	11.043	1632	1633	1635	rBV2	331	271	0.02%	0.003%
59	11.085	1638	1640	1642	rBV2	470	470	0.04%	0.005%
60	11.122	1642	1646	1651	rVB	4972	6509	0.52%	0.069%
61	11.195	1652	1658	1667	rBV	460345	572512	46.09%	6.047%
62	11.384	1685	1689	1692	rVB2	509	583	0.05%	0.006%
63	11.415	1692	1694	1697	rBV2	393	264	0.02%	0.003%
64	11.457	1697	1701	1702	rBV2	1106	1307	0.11%	0.014%
65	11.555	1713	1717	1722	rBV4	743	1048	0.08%	0.011%
66	11.628	1726	1729	1730	rVB2	415	408	0.03%	0.004%
67	11.640	1730	1731	1734	rBV3	488	510	0.04%	0.005%
68	11.677	1734	1737	1739	rVB3	450	431	0.03%	0.005%
69	11.750	1745	1749	1756	rVB2	5462	7314	0.59%	0.077%
70	11.841	1760	1764	1768	rVV4	966	1263	0.10%	0.013%
71	11.939	1775	1780	1783	rBV2	2248	3238	0.26%	0.034%
72	11.969	1783	1785	1789	rVB	1486	1449	0.12%	0.015%
73	12.024	1789	1794	1805	rBV	650528	807482	65.00%	8.529%
74	12.128	1808	1811	1812	rBV2	1684	1421	0.11%	0.015%
75	12.201	1821	1823	1824	rVB2	512	295	0.02%	0.003%
76	12.225	1824	1827	1830	rBV3	717	1074	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023648.D
 Acq On : 11 Aug 2021 13:22
 Operator : JC/MD
 Sample : VX0811WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK605

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.262	1831	1833	1834	rVV2	457	257	0.02%	0.003%
78	12.323	1837	1843	1850	rVB	652003	810802	65.27%	8.564%
79	12.427	1857	1860	1863	rVB3	1405	1534	0.12%	0.016%
80	12.475	1866	1868	1869	rBV	833	736	0.06%	0.008%
81	12.634	1890	1894	1895	rBV3	313	444	0.04%	0.005%
82	12.664	1895	1899	1905	rVB4	758	1392	0.11%	0.015%
83	12.768	1912	1916	1920	rBV3	604	848	0.07%	0.009%
84	12.805	1920	1922	1924	rBV2	253	291	0.02%	0.003%
85	12.969	1947	1949	1952	rBV3	347	344	0.03%	0.004%
86	13.054	1961	1963	1967	rVV4	880	982	0.08%	0.010%
87	13.115	1970	1973	1976	rVB2	1060	1268	0.10%	0.013%
88	13.164	1979	1981	1985	rBV3	226	274	0.02%	0.003%
89	13.597	2048	2052	2055	rVB2	1018	1448	0.12%	0.015%
90	13.780	2077	2082	2087	rBV3	1063	1351	0.11%	0.014%
91	13.963	2109	2112	2116	rBV3	814	925	0.07%	0.010%
92	14.127	2137	2139	2144	rBV3	896	1267	0.10%	0.013%
93	14.341	2172	2174	2176	rBV2	359	280	0.02%	0.003%
94	14.505	2200	2201	2204	rVB2	409	339	0.03%	0.004%
95	14.536	2204	2206	2208	rVB3	399	320	0.03%	0.003%
96	14.572	2208	2212	2213	rBV2	253	323	0.03%	0.003%
97	14.896	2260	2265	2266	rBV3	549	570	0.05%	0.006%
98	15.487	2361	2362	2364	rBV2	435	352	0.03%	0.004%
99	15.536	2368	2370	2372	rBV2	402	286	0.02%	0.003%
100	16.511	2528	2530	2533	rBV3	707	666	0.05%	0.007%


Sum of corrected areas: 9467638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023648.D
Acq On : 11 Aug 2021 13:22
Operator : JC/MD
Sample : VX0811WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

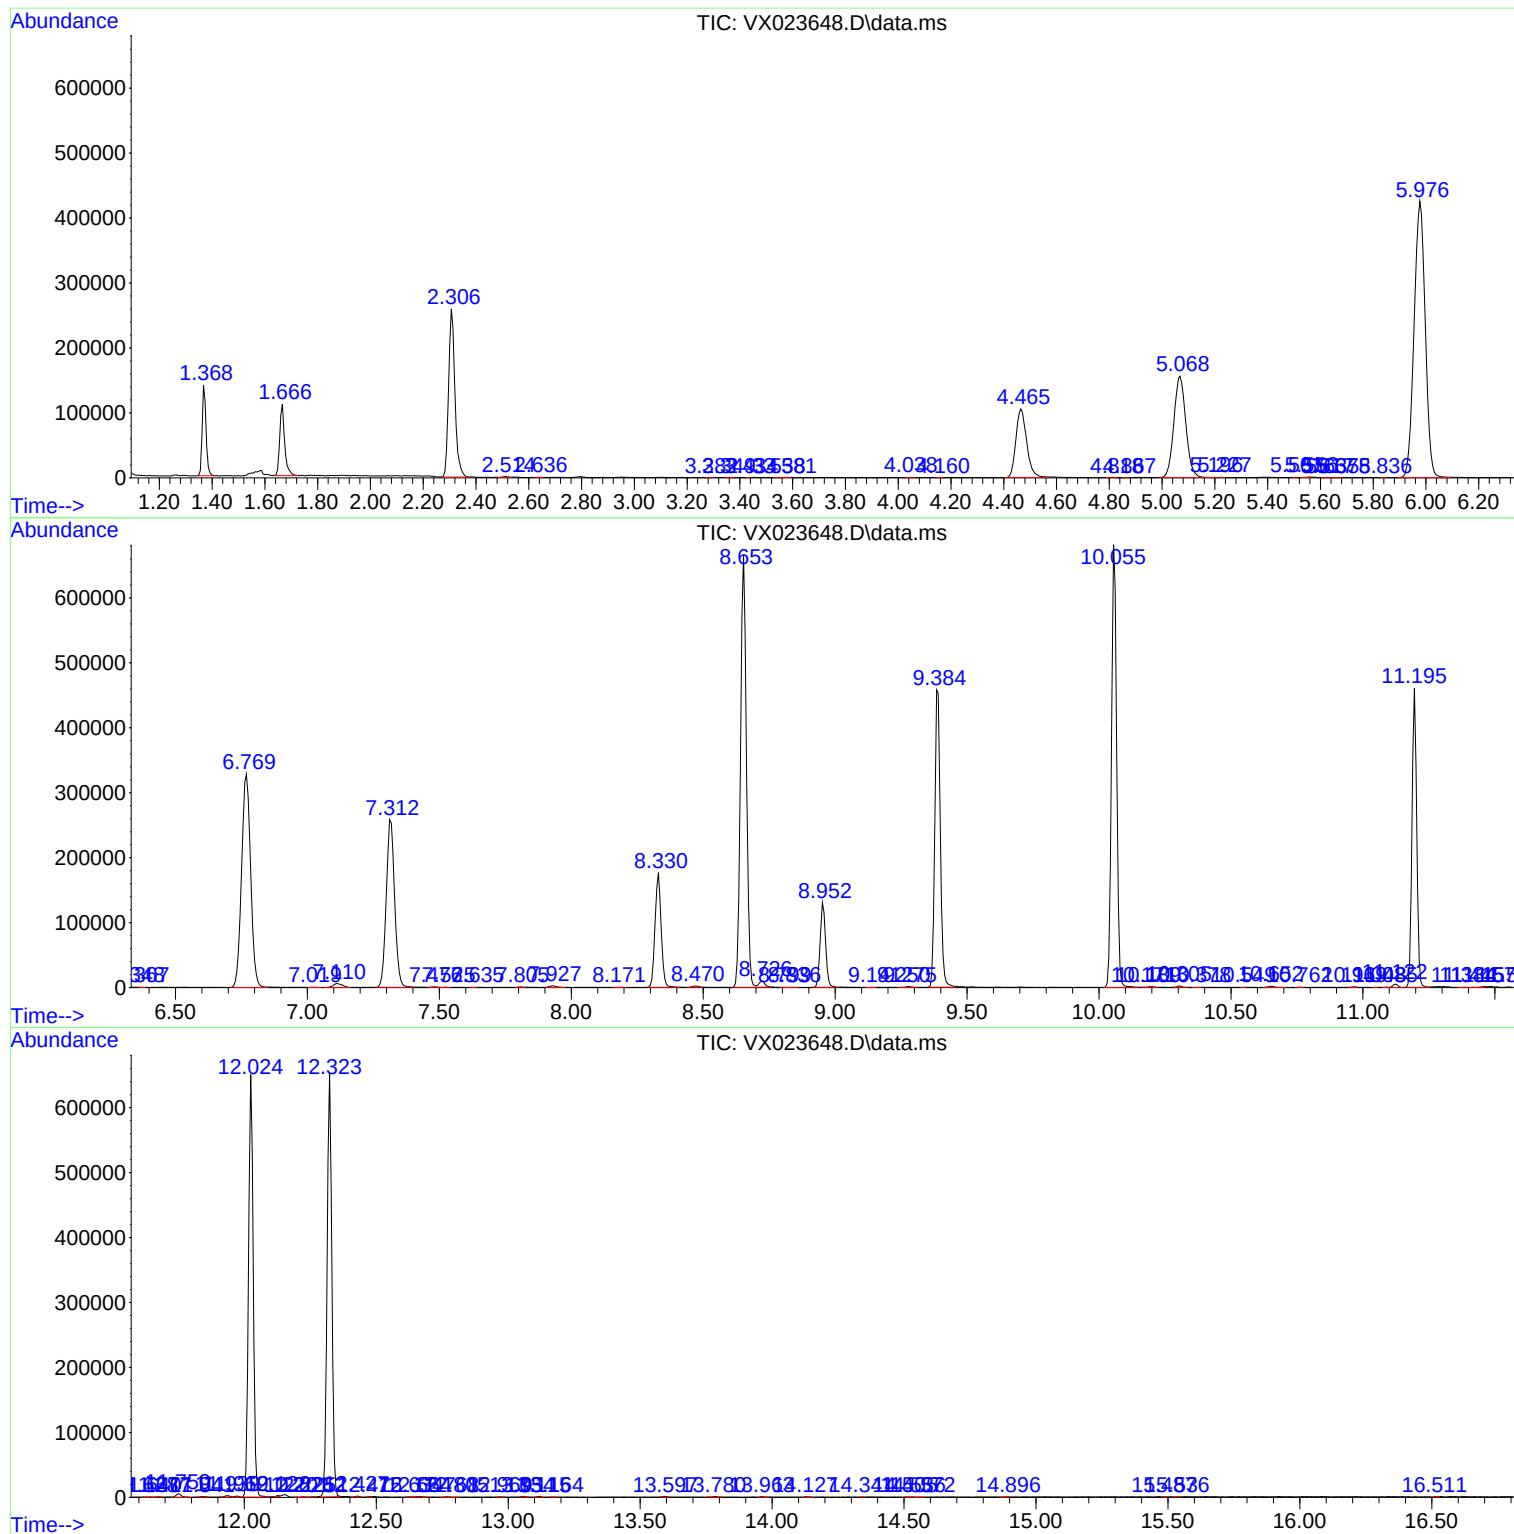

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023648.D
Acq On : 11 Aug 2021 13:22
Operator : JC/MD
Sample : VX0811WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023648.D
Acq On : 11 Aug 2021 13:22
Operator : JC/MD
Sample : VX0811WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
