

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023651.D
 Acq On : 11 Aug 2021 16:06
 Operator : JC/MD
 Sample : M3364-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

Signal : TIC: VX023651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	25	27	32	rVB3	4949	5519	0.45%	0.058%
2	1.368	43	46	56	rBV	107971	116010	9.55%	1.228%
3	1.660	90	94	106	rVB	94655	123226	10.15%	1.304%
4	2.306	194	200	210	rBV	206679	345629	28.46%	3.657%
5	2.459	223	225	227	rBV2	432	359	0.03%	0.004%
6	2.514	230	234	238	rBV3	1118	1763	0.15%	0.019%
7	2.550	238	240	247	rVB5	1203	1747	0.14%	0.018%
8	2.605	247	249	253	rBV3	309	380	0.03%	0.004%
9	2.709	263	266	273	rVB4	1107	1666	0.14%	0.018%
10	2.794	275	280	287	rVB6	2389	4847	0.40%	0.051%
11	2.873	289	293	294	rBV	413	377	0.03%	0.004%
12	2.892	294	296	298	rVB2	389	305	0.03%	0.003%
13	2.940	300	304	305	rBV2	860	1083	0.09%	0.011%
14	3.105	325	331	341	rBV6	1743	5684	0.47%	0.060%
15	3.959	467	471	472	rBV2	324	319	0.03%	0.003%
16	4.172	503	506	509	rBV3	231	335	0.03%	0.004%
17	4.343	529	534	535	rBV2	233	360	0.03%	0.004%
18	4.465	542	554	567	rBV	112074	316453	26.06%	3.349%
19	4.904	622	626	628	rBV3	649	883	0.07%	0.009%
20	5.062	640	652	672	rVV	150489	473686	39.00%	5.012%
21	5.477	716	720	721	rBV2	1116	1363	0.11%	0.014%
22	5.550	731	732	740	rVB3	566	936	0.08%	0.010%
23	5.666	747	751	752	rBV2	444	558	0.05%	0.006%
24	5.977	788	802	817	rBV2	413284	1214491	100.00%	12.852%
25	6.166	831	833	836	rBV2	398	470	0.04%	0.005%
26	6.208	836	840	841	rBV2	293	400	0.03%	0.004%
27	6.251	841	847	848	rBV4	960	1769	0.15%	0.019%
28	6.537	890	894	897	rBV4	248	391	0.03%	0.004%
29	6.568	897	899	901	rVB2	435	395	0.03%	0.004%
30	6.769	922	932	946	rVV	321333	767901	63.23%	8.126%
31	7.117	981	989	1000	rVB3	7584	18073	1.49%	0.191%
32	7.208	1003	1004	1007	rVB2	477	417	0.03%	0.004%
33	7.312	1012	1021	1033	rBV	258711	563405	46.39%	5.962%
34	7.586	1064	1066	1071	rVB	402	430	0.04%	0.005%
35	7.812	1096	1103	1109	rBV5	1244	3020	0.25%	0.032%
36	7.927	1117	1122	1129	rVV3	2906	5051	0.42%	0.053%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023651.D
 Acq On : 11 Aug 2021 16:06
 Operator : JC/MD
 Sample : M3364-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.232	1166	1172	1173	rBV2	339	442	0.04%	0.005%
38	8.330	1181	1188	1203	rVV	172170	279680	23.03%	2.960%
39	8.464	1206	1210	1218	rVB3	2094	3970	0.33%	0.042%
40	8.580	1224	1229	1234	rVB2	3250	4670	0.38%	0.049%
41	8.653	1234	1241	1248	rBV	628623	962938	79.29%	10.190%
42	8.720	1248	1252	1261	rVB	11962	20192	1.66%	0.214%
43	8.885	1277	1279	1282	rVB2	397	346	0.03%	0.004%
44	8.952	1284	1290	1301	rBV	129773	191957	15.81%	2.031%
45	9.153	1321	1323	1328	rVV3	2317	2928	0.24%	0.031%
46	9.214	1330	1333	1336	rVV2	391	453	0.04%	0.005%
47	9.281	1339	1344	1348	rVB6	3314	4859	0.40%	0.051%
48	9.391	1356	1362	1375	rBV	479749	710503	58.50%	7.518%
49	9.525	1380	1384	1390	rVB6	1556	2715	0.22%	0.029%
50	9.616	1395	1399	1404	rVB4	1007	1652	0.14%	0.017%
51	9.945	1450	1453	1454	rBV2	392	377	0.03%	0.004%
52	10.055	1465	1471	1481	rBV	714476	962297	79.23%	10.183%
53	10.201	1490	1495	1499	rBV	3802	5236	0.43%	0.055%
54	10.244	1499	1502	1507	rVB3	930	1273	0.10%	0.013%
55	10.305	1508	1512	1520	rVB2	4566	6464	0.53%	0.068%
56	10.653	1564	1569	1577	rVB2	6703	11870	0.98%	0.126%
57	10.762	1584	1587	1590	rVV4	508	660	0.05%	0.007%
58	10.799	1591	1593	1597	rVB3	919	962	0.08%	0.010%
59	10.963	1617	1620	1625	rBV	4511	5417	0.45%	0.057%
60	11.024	1628	1630	1633	rBV	270	305	0.03%	0.003%
61	11.091	1638	1641	1642	rBV	320	368	0.03%	0.004%
62	11.122	1642	1646	1650	rBB2	3181	3906	0.32%	0.041%
63	11.195	1652	1658	1665	rBV	477462	595105	49.00%	6.297%
64	11.372	1683	1687	1690	rBV4	688	1286	0.11%	0.014%
65	11.457	1697	1701	1704	rBV2	4513	5430	0.45%	0.057%
66	11.549	1713	1716	1720	rVB3	422	599	0.05%	0.006%
67	11.683	1734	1738	1740	rBV2	509	546	0.04%	0.006%
68	11.719	1741	1744	1746	rVV2	1067	1195	0.10%	0.013%
69	11.750	1746	1749	1754	rVV2	7007	9032	0.74%	0.096%
70	11.847	1756	1765	1770	rBV5	817	1607	0.13%	0.017%
71	11.896	1770	1773	1776	rBV4	484	672	0.06%	0.007%
72	11.939	1776	1780	1782	rBV3	1946	2441	0.20%	0.026%
73	11.975	1782	1786	1789	rVV2	3980	4690	0.39%	0.050%
74	12.024	1789	1794	1806	rVB	677878	820035	67.52%	8.677%
75	12.152	1812	1815	1820	rVB4	2368	3237	0.27%	0.034%
76	12.219	1822	1826	1836	rVV2	6213	9822	0.81%	0.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023651.D
 Acq On : 11 Aug 2021 16:06
 Operator : JC/MD
 Sample : M3364-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

77	12.323	1837	1843	1857	rVB	640635	797608	65.67%	8.440%
78	12.433	1857	1861	1865	rBV4	1158	1580	0.13%	0.017%
79	12.481	1866	1869	1878	rVB4	814	1262	0.10%	0.013%
80	12.664	1897	1899	1905	rVB	1427	1649	0.14%	0.017%
81	12.866	1929	1932	1935	rBV2	270	328	0.03%	0.003%
82	12.945	1943	1945	1948	rVB3	800	698	0.06%	0.007%
83	12.975	1948	1950	1953	rBV3	456	422	0.03%	0.004%
84	13.055	1960	1963	1966	rBV3	923	1027	0.08%	0.011%
85	13.115	1969	1973	1977	rVB2	2985	3303	0.27%	0.035%
86	13.414	2020	2022	2023	rBV	395	343	0.03%	0.004%
87	13.591	2047	2051	2055	rVV2	2699	2985	0.25%	0.032%
88	13.725	2070	2073	2076	rBV2	688	619	0.05%	0.007%
89	13.780	2078	2082	2087	rVB	5219	6095	0.50%	0.064%
90	13.963	2108	2112	2117	rVB3	4367	5172	0.43%	0.055%
91	13.999	2117	2118	2123	rVB2	380	465	0.04%	0.005%
92	14.134	2137	2140	2144	rVV2	774	898	0.07%	0.010%
93	14.969	2275	2277	2280	rBV2	364	534	0.04%	0.006%
94	15.066	2291	2293	2296	rBV2	345	306	0.03%	0.003%
95	15.103	2297	2299	2301	rBV	486	289	0.02%	0.003%
96	15.121	2301	2302	2306	rVV4	324	373	0.03%	0.004%
97	15.737	2401	2403	2407	rBV3	460	625	0.05%	0.007%
98	16.408	2510	2513	2516	rBV4	540	843	0.07%	0.009%
99	16.670	2554	2556	2559	rBV2	499	472	0.04%	0.005%
100	16.737	2566	2567	2570	rVB2	688	405	0.03%	0.004%




Sum of corrected areas: 9450139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023651.D
Acq On : 11 Aug 2021 16:06
Operator : JC/MD
Sample : M3364-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

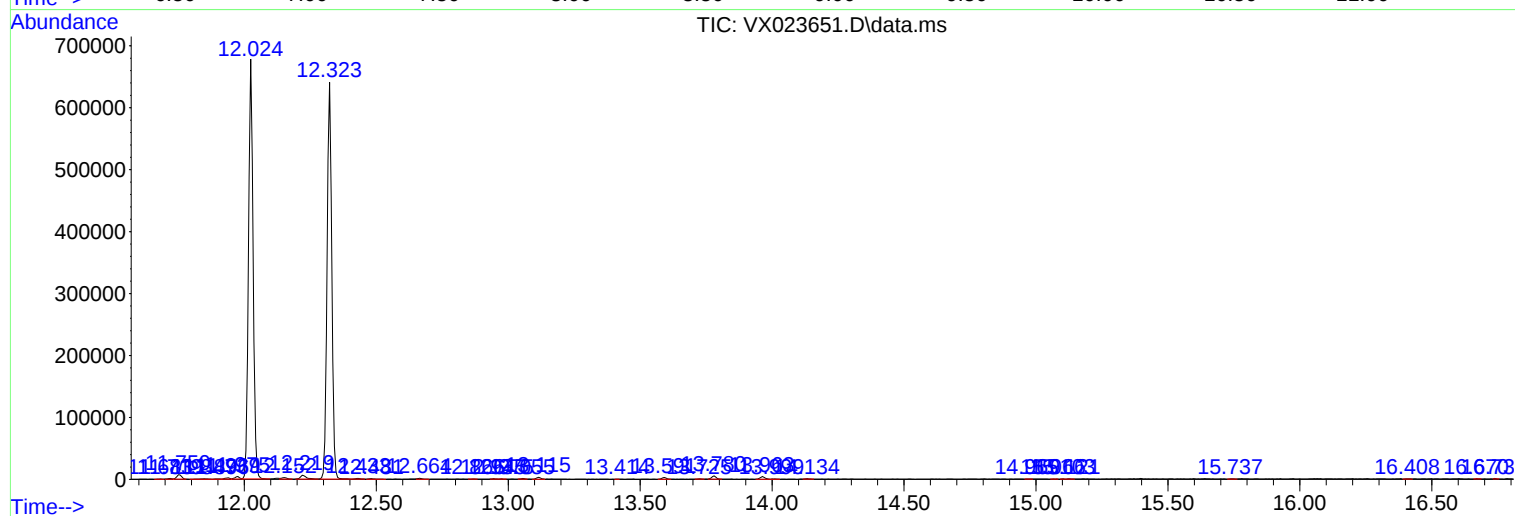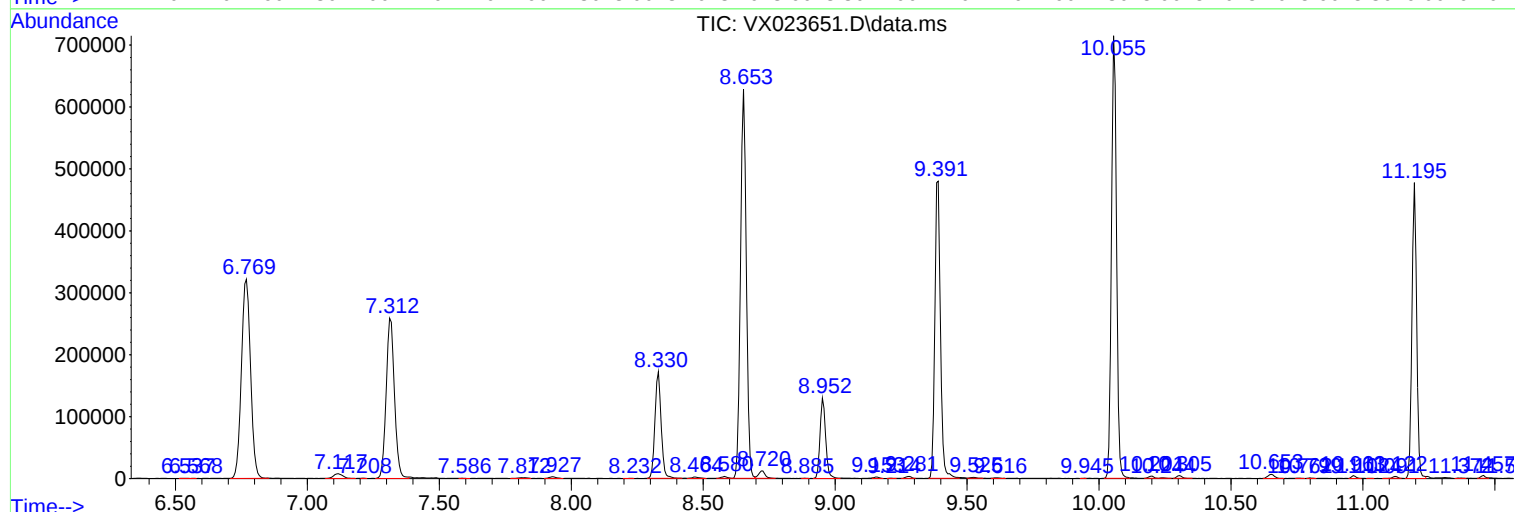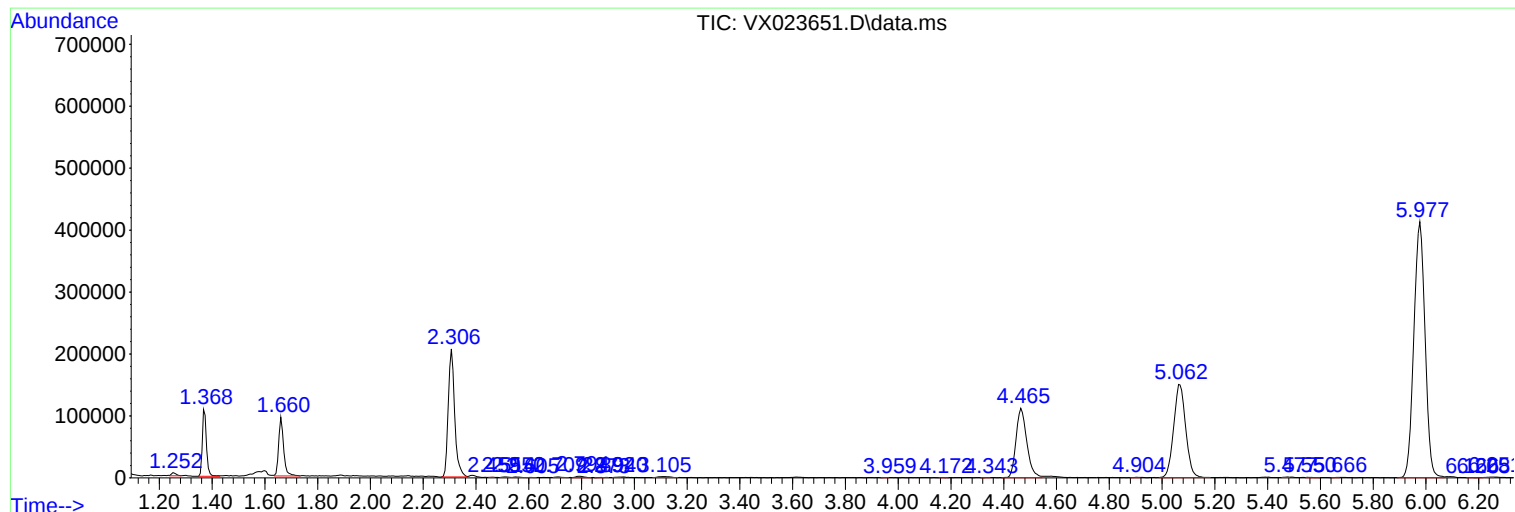

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023651.D
Acq On : 11 Aug 2021 16:06
Operator : JC/MD
Sample : M3364-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023651.D
Acq On : 11 Aug 2021 16:06
Operator : JC/MD
Sample : M3364-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
