

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023652.D
 Acq On : 11 Aug 2021 16:29
 Operator : JC/MD
 Sample : M3364-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	122363	125909	11.27%	1.440%
2	1.666	91	95	106	rVB	100151	126630	11.33%	1.449%
3	2.306	194	200	210	rBV	226217	372654	33.34%	4.263%
4	2.386	210	213	220	rVB2	5828	9828	0.88%	0.112%
5	2.697	263	264	265	rBV	527	261	0.02%	0.003%
6	2.715	265	267	268	rVV2	389	317	0.03%	0.004%
7	2.794	276	280	286	rVB4	1076	1984	0.18%	0.023%
8	2.843	286	288	291	rBV2	263	313	0.03%	0.004%
9	2.940	302	304	306	rBV2	504	487	0.04%	0.006%
10	3.081	324	327	329	rBV2	224	289	0.03%	0.003%
11	3.123	329	334	336	rBV5	783	1428	0.13%	0.016%
12	3.318	364	366	368	rBV2	282	269	0.02%	0.003%
13	3.373	373	375	379	rVB3	331	318	0.03%	0.004%
14	3.410	379	381	384	rBV2	198	249	0.02%	0.003%
15	3.446	384	387	392	rBV4	340	464	0.04%	0.005%
16	3.715	430	431	433	rBV2	302	285	0.03%	0.003%
17	3.763	435	439	440	rBV3	645	774	0.07%	0.009%
18	3.971	470	473	475	rBV2	230	254	0.02%	0.003%
19	4.044	482	485	486	rBV2	236	270	0.02%	0.003%
20	4.117	493	497	498	rBV3	311	427	0.04%	0.005%
21	4.276	522	523	528	rVB3	317	315	0.03%	0.004%
22	4.337	531	533	536	rBV	301	322	0.03%	0.004%
23	4.465	545	554	571	rBV	89849	258186	23.10%	2.954%
24	4.855	614	618	620	rBV	244	280	0.03%	0.003%
25	4.910	624	627	630	rVB	331	404	0.04%	0.005%
26	5.068	641	653	667	rBV	143897	436589	39.07%	4.994%
27	5.220	676	678	682	rVB3	490	477	0.04%	0.005%
28	5.324	690	695	698	rBV4	289	571	0.05%	0.007%
29	5.556	728	733	734	rBV	582	739	0.07%	0.008%
30	5.751	763	765	769	rVB2	318	336	0.03%	0.004%
31	5.976	789	802	817	rBV2	381199	1117576	100.00%	12.785%
32	6.098	821	822	825	rVB2	500	386	0.03%	0.004%
33	6.257	846	848	851	rBV	327	271	0.02%	0.003%
34	6.373	863	867	870	rVB2	678	934	0.08%	0.011%
35	6.403	870	872	876	rBV3	234	288	0.03%	0.003%
36	6.769	921	932	945	rBV	321648	764781	68.43%	8.749%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023652.D
 Acq On : 11 Aug 2021 16:29
 Operator : JC/MD
 Sample : M3364-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.019	970	973	974	rVB2	332	317	0.03%	0.004%
38	7.031	974	975	978	rBV2	257	308	0.03%	0.004%
39	7.116	982	989	997	rVB4	4662	10340	0.93%	0.118%
40	7.208	1003	1004	1008	rBV2	228	297	0.03%	0.003%
41	7.318	1013	1022	1033	rBV	234028	512799	45.88%	5.866%
42	7.476	1044	1048	1050	rBV4	644	1079	0.10%	0.012%
43	7.586	1063	1066	1070	rVB2	644	804	0.07%	0.009%
44	7.696	1081	1084	1087	rBV2	344	401	0.04%	0.005%
45	7.811	1097	1103	1108	rBV4	935	1878	0.17%	0.021%
46	7.927	1117	1122	1130	rBV5	2556	4509	0.40%	0.052%
47	8.330	1181	1188	1199	rBV	152555	248504	22.24%	2.843%
48	8.470	1207	1211	1219	rBV6	1475	2842	0.25%	0.033%
49	8.653	1234	1241	1248	rBV	596781	916152	81.98%	10.481%
50	8.726	1248	1253	1259	rVB	8664	15078	1.35%	0.172%
51	8.805	1265	1266	1270	rVB2	563	455	0.04%	0.005%
52	8.952	1284	1290	1300	rVV	115017	164528	14.72%	1.882%
53	9.195	1328	1330	1333	rVV2	229	246	0.02%	0.003%
54	9.275	1339	1343	1348	rVB5	2561	3771	0.34%	0.043%
55	9.390	1356	1362	1380	rBV	396092	580238	51.92%	6.638%
56	9.525	1381	1384	1388	rVB2	2024	2522	0.23%	0.029%
57	10.055	1465	1471	1488	rVV	674704	918248	82.16%	10.504%
58	10.195	1492	1494	1500	rVB2	856	945	0.08%	0.011%
59	10.305	1508	1512	1517	rVV3	1517	1970	0.18%	0.023%
60	10.427	1530	1532	1533	rBV	323	263	0.02%	0.003%
61	10.494	1541	1543	1545	rBV	262	245	0.02%	0.003%
62	10.537	1547	1550	1552	rBV2	205	269	0.02%	0.003%
63	10.652	1564	1569	1572	rBV3	1232	1577	0.14%	0.018%
64	10.756	1584	1586	1589	rBV2	406	497	0.04%	0.006%
65	10.866	1600	1604	1607	rVB3	1075	1439	0.13%	0.016%
66	10.963	1618	1620	1624	rVB2	456	450	0.04%	0.005%
67	11.085	1638	1640	1642	rBV2	283	252	0.02%	0.003%
68	11.122	1642	1646	1650	rVB2	4029	4734	0.42%	0.054%
69	11.195	1652	1658	1667	rBV	424212	540665	48.38%	6.185%
70	11.286	1669	1673	1674	rBV2	764	1001	0.09%	0.011%
71	11.463	1698	1702	1703	rBV2	721	927	0.08%	0.011%
72	11.750	1741	1749	1753	rBV2	4409	6164	0.55%	0.071%
73	11.817	1758	1760	1762	rBV2	239	256	0.02%	0.003%
74	11.847	1762	1765	1768	rBV3	866	1057	0.09%	0.012%
75	11.933	1776	1779	1782	rBV2	2460	2850	0.26%	0.033%
76	11.975	1783	1786	1789	rVB3	665	655	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023652.D
 Acq On : 11 Aug 2021 16:29
 Operator : JC/MD
 Sample : M3364-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1805	rVB	645096	802283	71.79%	9.178%
78	12.128	1805	1811	1813	rBV3	1915	3296	0.29%	0.038%
79	12.231	1825	1828	1831	rVB2	620	615	0.06%	0.007%
80	12.323	1835	1843	1851	rBV	607628	744137	66.58%	8.513%
81	12.420	1857	1859	1864	rVB3	1148	1800	0.16%	0.021%
82	12.457	1864	1865	1866	rBV	365	261	0.02%	0.003%
83	12.481	1866	1869	1872	rVB2	908	1177	0.11%	0.013%
84	12.670	1897	1900	1903	rVB4	609	682	0.06%	0.008%
85	12.762	1910	1915	1920	rBV3	837	1378	0.12%	0.016%
86	12.859	1928	1931	1934	rVB4	539	709	0.06%	0.008%
87	13.048	1958	1962	1967	rVB4	817	1249	0.11%	0.014%
88	13.115	1970	1973	1977	rBV3	497	593	0.05%	0.007%
89	13.591	2049	2051	2055	rVB2	696	686	0.06%	0.008%
90	13.780	2079	2082	2088	rVV3	883	1146	0.10%	0.013%
91	13.829	2088	2090	2094	rVV3	216	342	0.03%	0.004%
92	13.859	2094	2095	2100	rVB2	388	416	0.04%	0.005%
93	13.932	2105	2107	2110	rVB2	248	244	0.02%	0.003%
94	13.969	2110	2113	2117	rBV2	671	877	0.08%	0.010%
95	14.243	2155	2158	2163	rVB2	390	551	0.05%	0.006%
96	14.554	2207	2209	2210	rBV	307	268	0.02%	0.003%
97	14.883	2262	2263	2266	rBV2	240	239	0.02%	0.003%
98	15.322	2333	2335	2337	rVB2	719	458	0.04%	0.005%
99	15.834	2418	2419	2420	rBV	667	297	0.03%	0.003%
100	16.596	2542	2544	2546	rBV2	485	387	0.03%	0.004%




Sum of corrected areas: 8741488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023652.D
Acq On : 11 Aug 2021 16:29
Operator : JC/MD
Sample : M3364-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

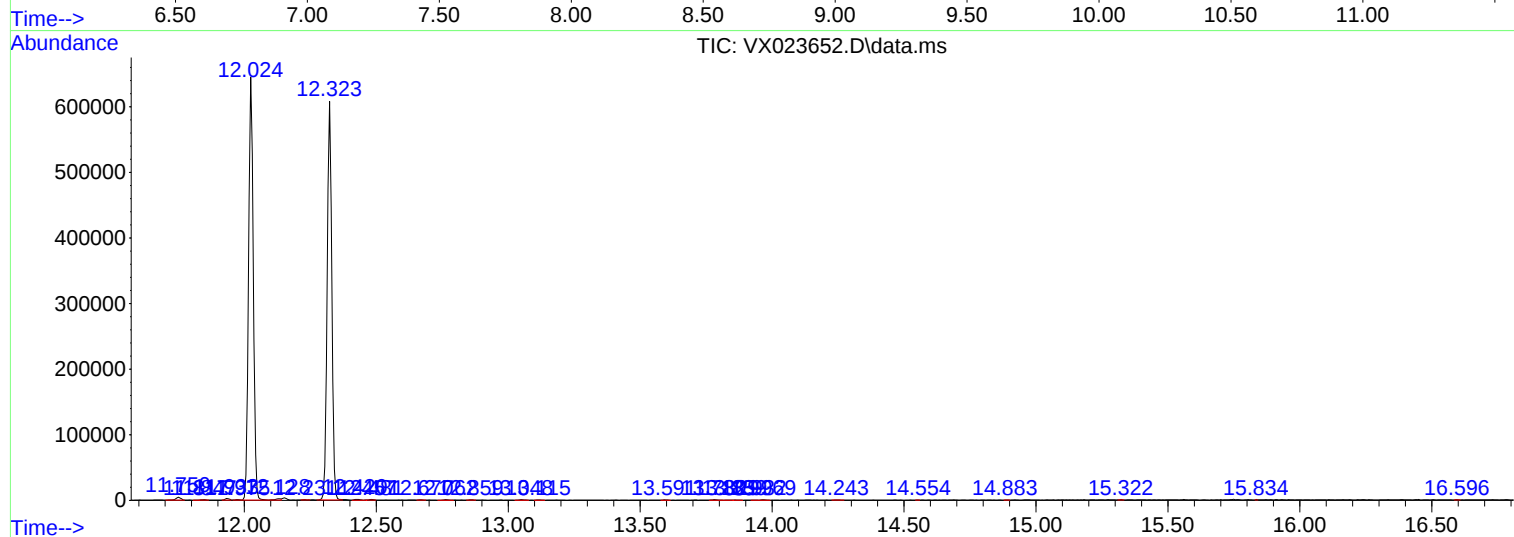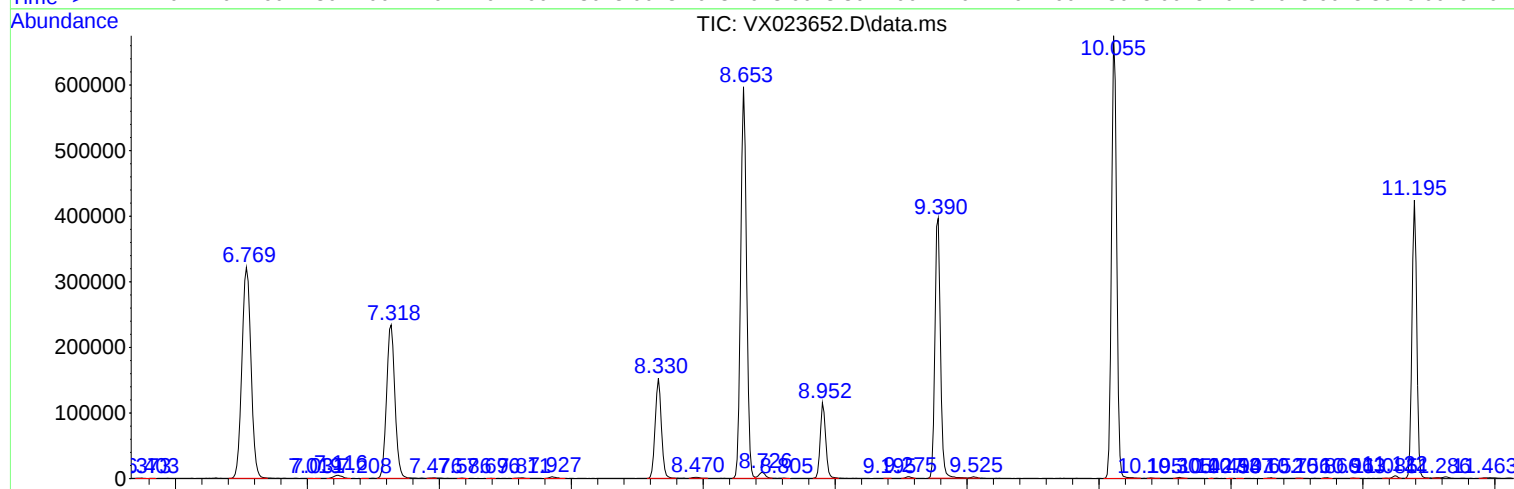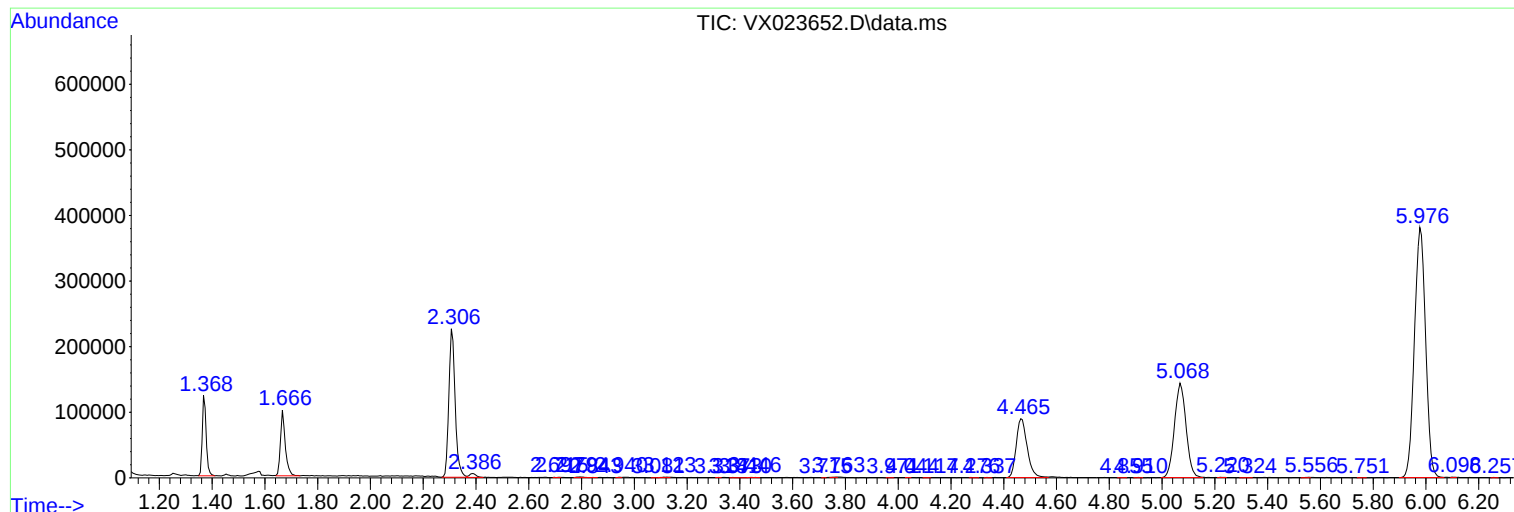

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023652.D
Acq On : 11 Aug 2021 16:29
Operator : JC/MD
Sample : M3364-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023652.D
Acq On : 11 Aug 2021 16:29
Operator : JC/MD
Sample : M3364-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
