

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023654.D
 Acq On : 11 Aug 2021 17:16
 Operator : JC/MD
 Sample : M3364-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	122275	123617	11.30%	1.367%
2	1.666	91	95	105	rVB	93791	122999	11.24%	1.360%
3	2.306	194	200	209	rBV	220244	365230	33.38%	4.039%
4	2.392	210	214	221	rVB	5595	9628	0.88%	0.106%
5	2.587	243	246	249	rVB3	276	382	0.03%	0.004%
6	2.630	249	253	256	rBV2	292	459	0.04%	0.005%
7	2.800	274	281	284	rBV4	1025	1773	0.16%	0.020%
8	2.959	303	307	309	rBV3	642	839	0.08%	0.009%
9	3.123	326	334	346	rVB	5512	12164	1.11%	0.135%
10	3.361	370	373	374	rVB2	584	456	0.04%	0.005%
11	3.611	410	414	422	rVB2	1206	2640	0.24%	0.029%
12	3.770	436	440	443	rBV4	599	1063	0.10%	0.012%
13	4.202	508	511	514	rBV3	356	603	0.06%	0.007%
14	4.465	542	554	570	rBV	90313	258844	23.66%	2.862%
15	4.678	587	589	592	rBV3	358	412	0.04%	0.005%
16	5.068	640	653	669	rBV	139463	433194	39.60%	4.790%
17	5.227	678	679	682	rVV3	453	381	0.03%	0.004%
18	5.397	699	707	714	rBV6	833	2321	0.21%	0.026%
19	5.556	727	733	736	rBV3	1278	2547	0.23%	0.028%
20	5.977	790	802	818	rBV2	372644	1094022	100.00%	12.098%
21	6.647	908	912	921	rVB4	597	1413	0.13%	0.016%
22	6.769	921	932	951	rBV	316921	751146	68.66%	8.306%
23	7.110	983	988	996	rVB4	4883	11514	1.05%	0.127%
24	7.232	1004	1008	1012	rBV2	295	421	0.04%	0.005%
25	7.318	1012	1022	1037	rBV	229074	505153	46.17%	5.586%
26	7.470	1045	1047	1053	rVB3	965	1638	0.15%	0.018%
27	7.580	1063	1065	1071	rVB3	424	682	0.06%	0.008%
28	7.635	1071	1074	1079	rBV3	327	381	0.03%	0.004%
29	7.684	1079	1082	1084	rBV2	384	433	0.04%	0.005%
30	7.812	1097	1103	1106	rBV4	794	1218	0.11%	0.013%
31	7.933	1117	1123	1129	rBV4	2110	4271	0.39%	0.047%
32	8.025	1134	1138	1141	rBV2	262	520	0.05%	0.006%
33	8.153	1156	1159	1162	rBV3	295	394	0.04%	0.004%
34	8.330	1181	1188	1198	rBV	148846	238539	21.80%	2.638%
35	8.470	1206	1211	1218	rVB3	1824	3559	0.33%	0.039%
36	8.519	1218	1219	1226	rBV2	408	530	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023654.D
 Acq On : 11 Aug 2021 17:16
 Operator : JC/MD
 Sample : M3364-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.580	1226	1229	1230	rBV2	346	433	0.04%	0.005%
38	8.653	1234	1241	1249	rVV	603887	901908	82.44%	9.973%
39	8.720	1249	1252	1260	rVV	10558	16207	1.48%	0.179%
40	8.781	1260	1262	1266	rVB3	544	685	0.06%	0.008%
41	8.952	1284	1290	1300	rVV	108601	159483	14.58%	1.764%
42	9.037	1302	1304	1306	rVV2	502	463	0.04%	0.005%
43	9.275	1337	1343	1349	rVB3	2470	3646	0.33%	0.040%
44	9.391	1356	1362	1380	rVV	405272	579902	53.01%	6.413%
45	9.525	1380	1384	1390	rVV4	2165	3725	0.34%	0.041%
46	10.055	1465	1471	1479	rBV	660829	903366	82.57%	9.989%
47	10.195	1491	1494	1498	rVB2	1574	2066	0.19%	0.023%
48	10.305	1508	1512	1516	rBV3	2544	3363	0.31%	0.037%
49	10.646	1565	1568	1573	rBV4	903	1640	0.15%	0.018%
50	10.860	1600	1603	1607	rVB4	1107	1341	0.12%	0.015%
51	10.970	1616	1621	1625	rVB2	1897	2421	0.22%	0.027%
52	11.122	1642	1646	1651	rVB	3665	4934	0.45%	0.055%
53	11.195	1653	1658	1667	rBV	425223	529984	48.44%	5.861%
54	11.274	1670	1671	1673	rBV2	781	602	0.06%	0.007%
55	11.311	1674	1677	1683	rVB4	3094	4488	0.41%	0.050%
56	11.402	1687	1692	1695	rBV3	1014	1268	0.12%	0.014%
57	11.451	1697	1700	1701	rBV3	868	772	0.07%	0.009%
58	11.549	1714	1716	1720	rVB2	388	447	0.04%	0.005%
59	11.616	1723	1727	1732	rVB3	1729	2062	0.19%	0.023%
60	11.756	1744	1750	1754	rVB2	4577	6744	0.62%	0.075%
61	11.841	1762	1764	1768	rVB3	711	962	0.09%	0.011%
62	11.933	1775	1779	1783	rBV3	2495	3385	0.31%	0.037%
63	11.969	1783	1785	1789	rBV3	475	727	0.07%	0.008%
64	12.024	1789	1794	1803	rBV	660732	794765	72.65%	8.789%
65	12.122	1808	1810	1812	rVV2	1246	1523	0.14%	0.017%
66	12.152	1813	1815	1821	rVB2	3073	3471	0.32%	0.038%
67	12.244	1825	1830	1836	rBV	64042	79861	7.30%	0.883%
68	12.323	1836	1843	1850	rBV	604899	742162	67.84%	8.207%
69	12.427	1858	1860	1863	rVB2	1370	1374	0.13%	0.015%
70	12.481	1867	1869	1874	rVB3	1048	1397	0.13%	0.015%
71	12.609	1887	1890	1893	rVV5	820	1169	0.11%	0.013%
72	12.646	1893	1896	1901	rVV4	2861	3801	0.35%	0.042%
73	12.701	1901	1905	1911	rVB2	7362	9187	0.84%	0.102%
74	12.762	1912	1915	1916	rBV2	587	655	0.06%	0.007%
75	12.853	1926	1930	1933	rBV3	700	916	0.08%	0.010%
76	12.926	1940	1942	1945	rVB3	637	664	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023654.D
 Acq On : 11 Aug 2021 17:16
 Operator : JC/MD
 Sample : M3364-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.975	1946	1950	1957	rVV4	990	1754	0.16%	0.019%
78	13.055	1959	1963	1967	rVB2	997	1404	0.13%	0.016%
79	13.170	1979	1982	1986	rVV	7016	7726	0.71%	0.085%
80	13.298	1998	2003	2007	rBV	13892	17618	1.61%	0.195%
81	13.426	2021	2024	2026	rBV3	674	707	0.06%	0.008%
82	13.542	2041	2043	2046	rBV2	433	414	0.04%	0.005%
83	13.603	2048	2053	2054	rBV2	324	488	0.04%	0.005%
84	13.780	2079	2082	2086	rVB2	2025	2624	0.24%	0.029%
85	13.865	2094	2096	2100	rVB3	450	707	0.06%	0.008%
86	13.963	2110	2112	2115	rVB2	471	434	0.04%	0.005%
87	14.134	2137	2140	2144	rBV3	445	569	0.05%	0.006%
88	14.329	2168	2172	2173	rBV	338	406	0.04%	0.004%
89	14.603	2212	2217	2219	rBV	6031	7746	0.71%	0.086%
90	14.640	2219	2223	2230	rVB	71063	85377	7.80%	0.944%
91	14.731	2233	2238	2241	rBV5	1997	3045	0.28%	0.034%
92	14.780	2241	2246	2252	rVV	114185	146646	13.40%	1.622%
93	15.481	2356	2361	2364	rBV4	1271	1886	0.17%	0.021%
94	15.615	2380	2383	2387	rBV3	2662	3584	0.33%	0.040%
95	15.792	2411	2412	2414	rBV2	506	515	0.05%	0.006%
96	15.993	2443	2445	2448	rBV2	631	893	0.08%	0.010%
97	16.078	2457	2459	2460	rBV2	546	432	0.04%	0.005%
98	16.170	2472	2474	2475	rBV2	608	513	0.05%	0.006%
99	16.328	2495	2500	2507	rBV	13183	23590	2.16%	0.261%
100	16.401	2511	2512	2518	rBV3	564	739	0.07%	0.008%


Sum of corrected areas: 9043172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023654.D
Acq On : 11 Aug 2021 17:16
Operator : JC/MD
Sample : M3364-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

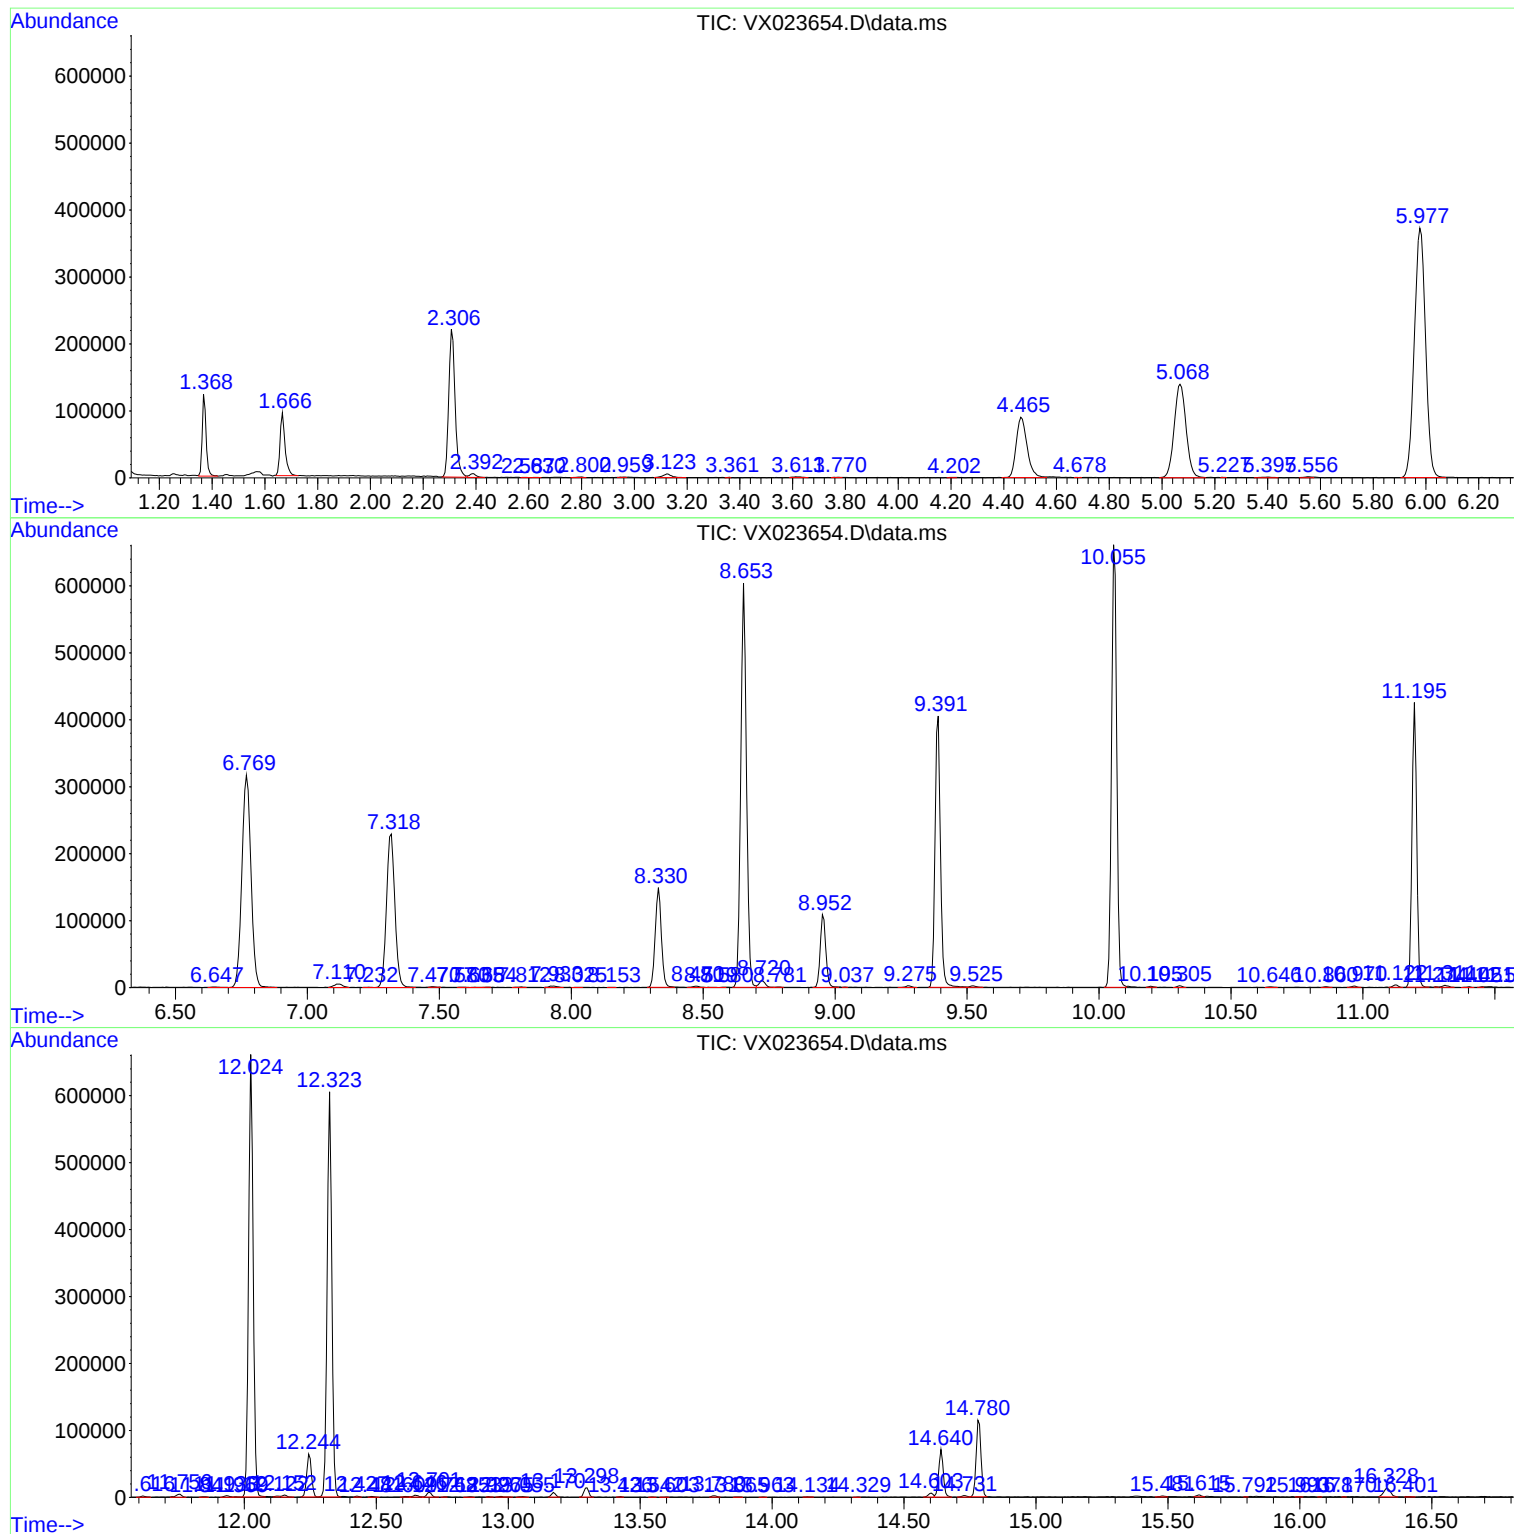

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023654.D
Acq On : 11 Aug 2021 17:16
Operator : JC/MD
Sample : M3364-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK84










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.244	5.02 ug/L	79861	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	95
2	Indane			118	C9H10	000496-11-7	76
3	Indane			118	C9H10	000496-11-7	70
4	Benzene, cyclopropyl-			118	C9H10	000873-49-4	62
5	Benzene, 1-ethenyl-4-methyl-			118	C9H10	000622-97-9	62

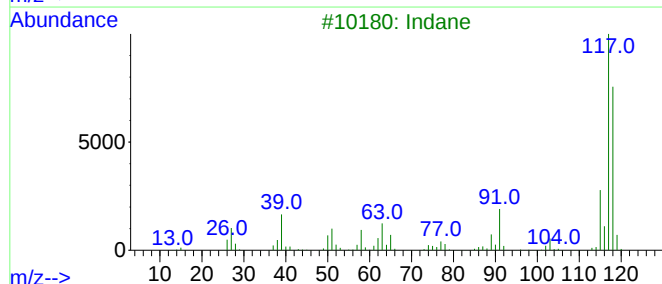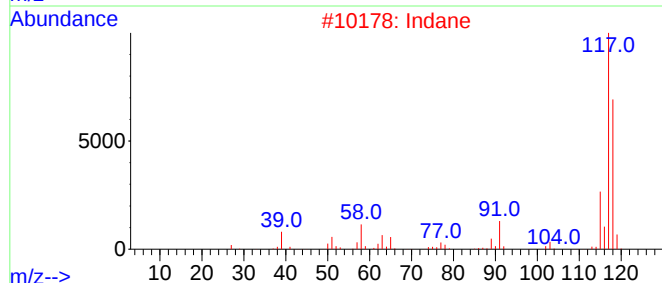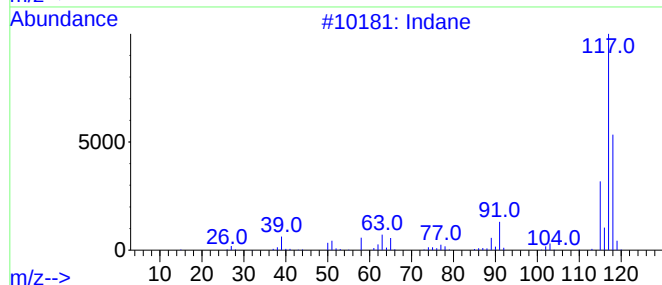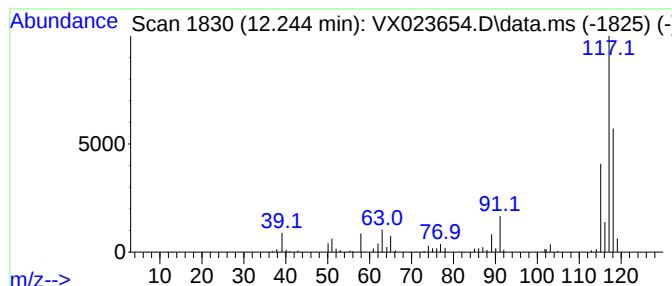

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023654.D
Acq On : 11 Aug 2021 17:16
Operator : JC/MD
Sample : M3364-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.244	5.0	ug/L	79861	3	12.024	794765	50.0