

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023656.D
 Acq On : 11 Aug 2021 18:03
 Operator : JC/MD
 Sample : M3364-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	121322	122153	11.10%	1.424%
2	1.666	91	95	103	rBV	92737	124551	11.31%	1.452%
3	2.307	194	200	210	rBV	220280	368094	33.44%	4.291%
4	2.386	210	213	221	rVB	6154	10005	0.91%	0.117%
5	2.514	230	234	236	rBV3	683	1092	0.10%	0.013%
6	2.788	277	279	285	rVB4	837	1264	0.11%	0.015%
7	2.953	303	306	307	rBV2	708	623	0.06%	0.007%
8	3.123	327	334	342	rVB	4021	9573	0.87%	0.112%
9	3.441	384	386	388	rBV	292	352	0.03%	0.004%
10	3.495	392	395	399	rBV2	265	335	0.03%	0.004%
11	3.617	409	415	418	rBV4	1054	2169	0.20%	0.025%
12	3.770	436	440	445	rBV4	402	688	0.06%	0.008%
13	4.172	504	506	509	rVB2	375	270	0.02%	0.003%
14	4.221	512	514	516	rBV2	338	319	0.03%	0.004%
15	4.373	537	539	542	rBV2	402	416	0.04%	0.005%
16	4.465	544	554	570	rBV	93144	262270	23.82%	3.058%
17	5.068	641	653	669	rBV	142386	427730	38.85%	4.987%
18	5.245	680	682	686	rVB2	254	306	0.03%	0.004%
19	5.391	703	706	712	rVB5	588	1134	0.10%	0.013%
20	5.562	727	734	742	rVB3	1164	3097	0.28%	0.036%
21	5.629	742	745	747	rBV2	298	378	0.03%	0.004%
22	5.818	774	776	778	rBV	416	331	0.03%	0.004%
23	5.977	789	802	820	rBV2	375770	1100893	100.00%	12.835%
24	6.288	851	853	856	rBV	291	298	0.03%	0.003%
25	6.342	859	862	863	rBV2	372	374	0.03%	0.004%
26	6.769	922	932	947	rBV	313762	738467	67.08%	8.610%
27	7.117	982	989	996	rBV6	5275	12320	1.12%	0.144%
28	7.318	1012	1022	1040	rVV	227730	501235	45.53%	5.844%
29	7.482	1045	1049	1056	rVB4	1005	2040	0.19%	0.024%
30	7.586	1063	1066	1067	rBV2	614	732	0.07%	0.009%
31	7.671	1079	1080	1084	rBV2	371	364	0.03%	0.004%
32	7.799	1099	1101	1102	rBV	613	340	0.03%	0.004%
33	7.934	1118	1123	1127	rBV4	2051	3929	0.36%	0.046%
34	8.269	1174	1178	1181	rBV2	221	290	0.03%	0.003%
35	8.330	1181	1188	1200	rBV	145948	236085	21.44%	2.752%
36	8.476	1206	1212	1219	rVB3	1627	3379	0.31%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023656.D
 Acq On : 11 Aug 2021 18:03
 Operator : JC/MD
 Sample : M3364-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.586	1224	1230	1234	rBV5	569	1105	0.10%	0.013%
38	8.653	1234	1241	1248	rBV	584155	893824	81.19%	10.421%
39	8.726	1248	1253	1265	rVB	10114	17574	1.60%	0.205%
40	8.836	1270	1271	1277	rVB2	335	334	0.03%	0.004%
41	8.952	1284	1290	1303	rBV	106499	160712	14.60%	1.874%
42	9.068	1305	1309	1311	rBV3	397	501	0.05%	0.006%
43	9.281	1338	1344	1348	rBV4	1768	2560	0.23%	0.030%
44	9.391	1356	1362	1375	rBV	416520	588754	53.48%	6.864%
45	9.525	1381	1384	1388	rVB2	2736	3797	0.34%	0.044%
46	9.647	1401	1404	1407	rBV3	309	403	0.04%	0.005%
47	10.055	1465	1471	1487	rVV	650480	875432	79.52%	10.206%
48	10.195	1491	1494	1500	rVV3	1080	1556	0.14%	0.018%
49	10.305	1508	1512	1517	rVB4	1694	2378	0.22%	0.028%
50	10.427	1528	1532	1535	rBV3	194	379	0.03%	0.004%
51	10.470	1535	1539	1542	rVB3	433	461	0.04%	0.005%
52	10.543	1548	1551	1554	rBV2	236	293	0.03%	0.003%
53	10.647	1565	1568	1574	rBV3	872	1124	0.10%	0.013%
54	10.720	1576	1580	1581	rBV2	335	351	0.03%	0.004%
55	10.860	1599	1603	1608	rVB2	2191	2763	0.25%	0.032%
56	10.964	1617	1620	1623	rVB3	815	901	0.08%	0.011%
57	11.085	1638	1640	1642	rVB	451	283	0.03%	0.003%
58	11.122	1642	1646	1650	rBV	4046	5206	0.47%	0.061%
59	11.195	1652	1658	1666	rBV	408227	507648	46.11%	5.918%
60	11.372	1684	1687	1688	rBV2	347	335	0.03%	0.004%
61	11.451	1698	1700	1701	rBV2	749	562	0.05%	0.007%
62	11.482	1703	1705	1709	rVB3	1069	1204	0.11%	0.014%
63	11.555	1715	1717	1722	rVB3	598	611	0.06%	0.007%
64	11.610	1722	1726	1728	rBV3	577	822	0.07%	0.010%
65	11.689	1736	1739	1741	rBV3	586	637	0.06%	0.007%
66	11.720	1741	1744	1745	rVV	595	573	0.05%	0.007%
67	11.750	1746	1749	1756	rVB3	3955	5514	0.50%	0.064%
68	11.841	1762	1764	1767	rVB2	851	847	0.08%	0.010%
69	11.933	1776	1779	1783	rVV3	2587	3164	0.29%	0.037%
70	11.982	1783	1787	1788	rVV2	517	678	0.06%	0.008%
71	12.024	1789	1794	1804	rVV	618663	750259	68.15%	8.747%
72	12.128	1807	1811	1813	rVV3	1808	2730	0.25%	0.032%
73	12.152	1813	1815	1819	rVB2	2929	3083	0.28%	0.036%
74	12.244	1824	1830	1835	rVB	12247	16873	1.53%	0.197%
75	12.323	1836	1843	1851	rVV	567782	707768	64.29%	8.252%
76	12.433	1857	1861	1865	rVB4	1254	1831	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023656.D
 Acq On : 11 Aug 2021 18:03
 Operator : JC/MD
 Sample : M3364-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.482	1865	1869	1873	rBV4	894	1568	0.14%	0.018%
78	12.701	1902	1905	1910	rVB2	2475	3126	0.28%	0.036%
79	12.768	1911	1916	1920	rBV2	580	1071	0.10%	0.012%
80	12.853	1928	1930	1936	rVB5	1101	1632	0.15%	0.019%
81	12.902	1936	1938	1942	rVB3	442	534	0.05%	0.006%
82	13.055	1959	1963	1967	rVB4	985	1343	0.12%	0.016%
83	13.134	1974	1976	1979	rVB3	318	321	0.03%	0.004%
84	13.170	1979	1982	1986	rBV2	1392	1764	0.16%	0.021%
85	13.244	1992	1994	1996	rBV	281	278	0.03%	0.003%
86	13.292	1999	2002	2007	rVV	4219	4880	0.44%	0.057%
87	13.427	2019	2024	2027	rBV3	234	404	0.04%	0.005%
88	13.780	2079	2082	2086	rVB2	1462	1837	0.17%	0.021%
89	13.920	2102	2105	2108	rBV2	360	442	0.04%	0.005%
90	14.128	2137	2139	2142	rVB2	358	285	0.03%	0.003%
91	14.353	2175	2176	2180	rVB2	322	356	0.03%	0.004%
92	14.390	2180	2182	2183	rBV2	284	303	0.03%	0.004%
93	14.463	2193	2194	2197	rBV	332	277	0.03%	0.003%
94	14.597	2213	2216	2219	rVV2	1988	2462	0.22%	0.029%
95	14.640	2219	2223	2227	rVB	8152	9977	0.91%	0.116%
96	14.780	2242	2246	2253	rVB	27305	36008	3.27%	0.420%
97	15.066	2291	2293	2295	rVB3	388	362	0.03%	0.004%
98	15.255	2321	2324	2326	rBV3	434	479	0.04%	0.006%
99	15.304	2331	2332	2334	rBV2	443	325	0.03%	0.004%
100	16.328	2496	2500	2510	rVB4	1927	3586	0.33%	0.042%




Sum of corrected areas: 8577346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023656.D
Acq On : 11 Aug 2021 18:03
Operator : JC/MD
Sample : M3364-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

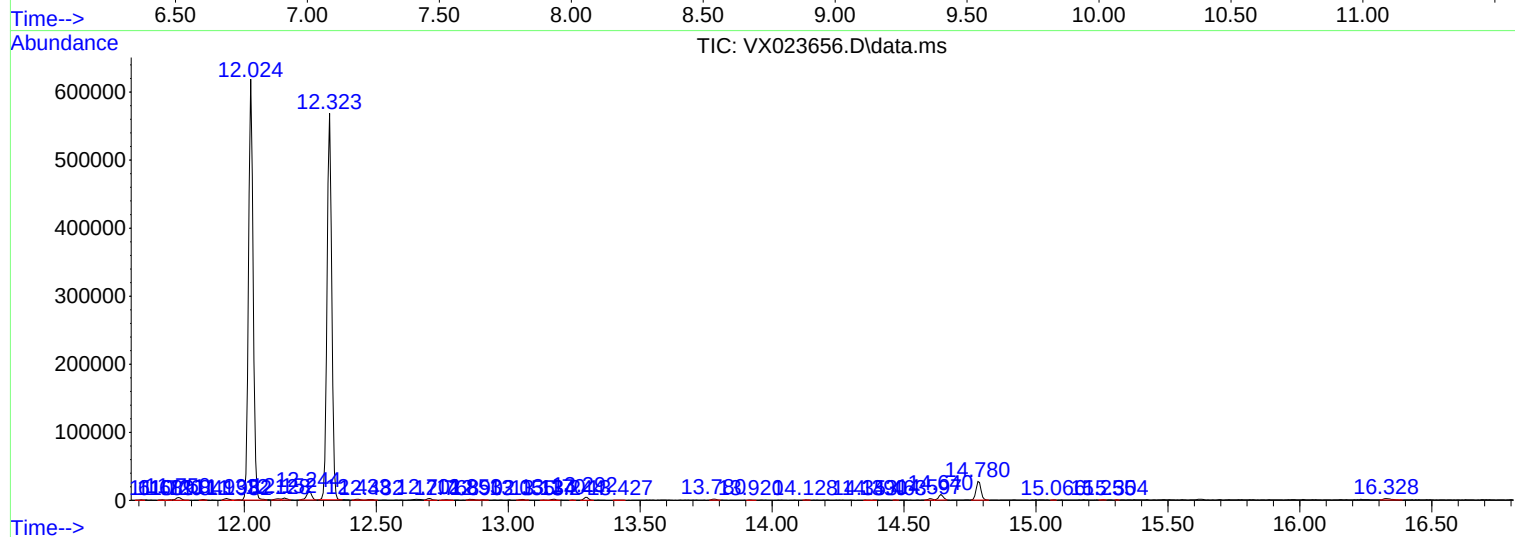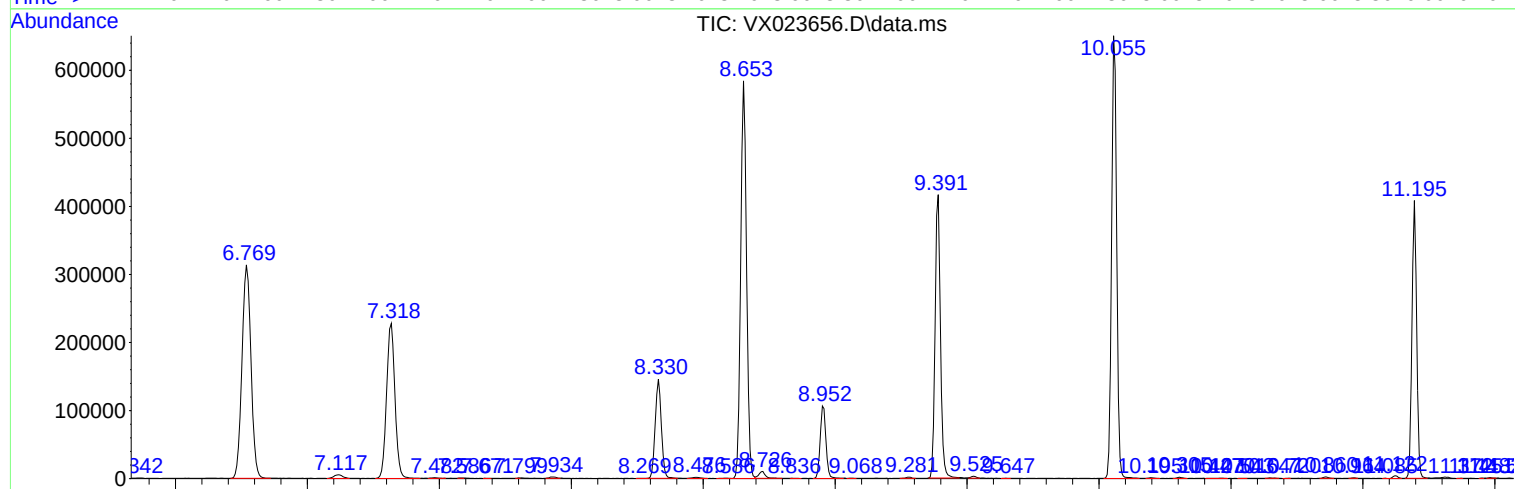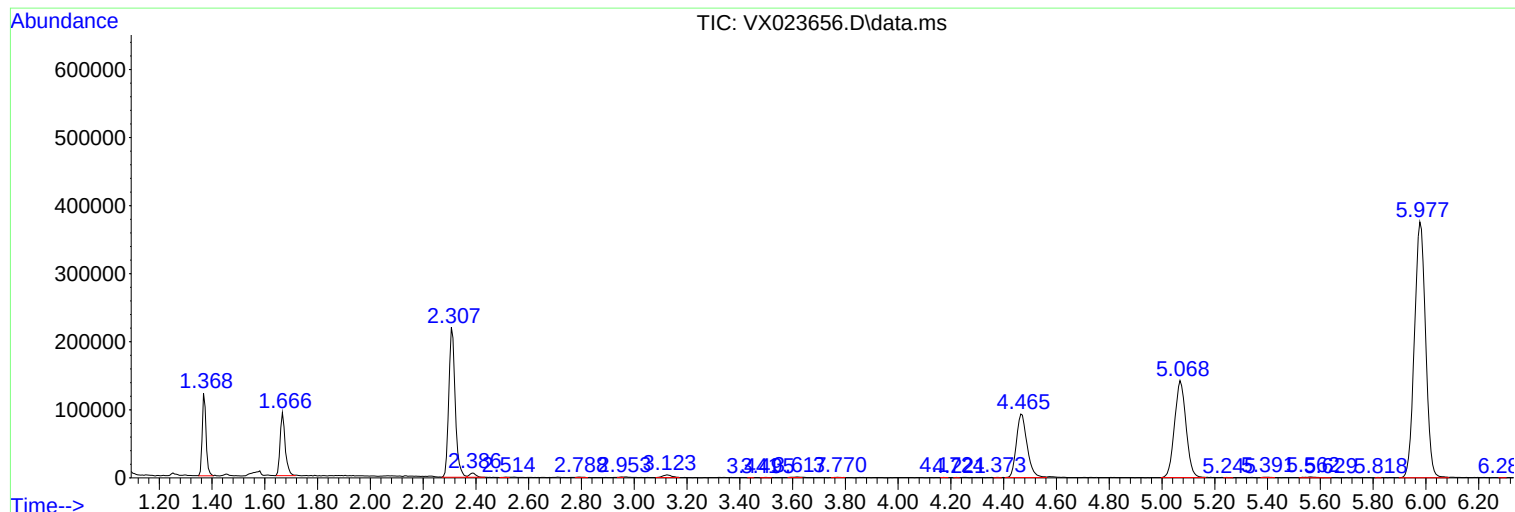

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023656.D
Acq On : 11 Aug 2021 18:03
Operator : JC/MD
Sample : M3364-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023656.D
Acq On : 11 Aug 2021 18:03
Operator : JC/MD
Sample : M3364-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
