

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023657.D
 Acq On : 11 Aug 2021 18:27
 Operator : JC/MD
 Sample : M3364-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	25	27	32	rVB4	3858	4547	0.42%	0.055%
2	1.368	43	46	52	rBV	116253	120359	11.16%	1.443%
3	1.666	91	95	107	rVB	91204	123894	11.49%	1.486%
4	2.306	194	200	209	rBV	215977	355823	33.00%	4.267%
5	2.386	210	213	220	rVB	5904	8962	0.83%	0.107%
6	2.508	230	233	234	rBV	552	435	0.04%	0.005%
7	2.630	251	253	255	rBV3	325	301	0.03%	0.004%
8	2.697	262	264	265	rBV	521	374	0.03%	0.004%
9	2.788	276	279	281	rBV3	771	917	0.09%	0.011%
10	2.843	286	288	290	rBV2	314	337	0.03%	0.004%
11	2.934	301	303	305	rBV2	475	373	0.03%	0.004%
12	3.325	365	367	370	rBV3	304	311	0.03%	0.004%
13	3.593	405	411	414	rBV3	323	561	0.05%	0.007%
14	3.898	458	461	464	rVB	369	314	0.03%	0.004%
15	4.391	538	542	543	rBV	526	508	0.05%	0.006%
16	4.465	546	554	571	rVV	90253	252664	23.43%	3.030%
17	4.818	608	612	615	rBV2	303	465	0.04%	0.006%
18	4.940	629	632	634	rBV2	334	411	0.04%	0.005%
19	5.068	638	653	668	rBV	139083	420696	39.02%	5.045%
20	5.196	671	674	675	rBV	384	331	0.03%	0.004%
21	5.349	695	699	700	rVB	263	294	0.03%	0.004%
22	5.385	700	705	706	rBV3	416	635	0.06%	0.008%
23	5.434	712	713	716	rBV3	276	309	0.03%	0.004%
24	5.464	716	718	720	rVV	364	296	0.03%	0.004%
25	5.556	728	733	734	rBV2	663	863	0.08%	0.010%
26	5.891	786	788	790	rBV2	301	328	0.03%	0.004%
27	5.976	790	802	820	rVV2	367443	1078259	100.00%	12.929%
28	6.141	827	829	832	rVB2	322	299	0.03%	0.004%
29	6.172	832	834	838	rVB3	310	375	0.03%	0.004%
30	6.257	845	848	851	rVB2	280	312	0.03%	0.004%
31	6.348	861	863	866	rBV4	353	418	0.04%	0.005%
32	6.629	905	909	911	rBV2	385	564	0.05%	0.007%
33	6.647	911	912	918	rVB3	626	839	0.08%	0.010%
34	6.769	922	932	946	rBV	305013	729379	67.64%	8.746%
35	6.946	959	961	964	rBV3	264	316	0.03%	0.004%
36	7.117	982	989	997	rBV5	4826	10912	1.01%	0.131%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023657.D
 Acq On : 11 Aug 2021 18:27
 Operator : JC/MD
 Sample : M3364-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.318	1012	1022	1035	rBV	223975	489923	45.44%	5.875%
38	7.470	1045	1047	1048	rBV	536	356	0.03%	0.004%
39	7.653	1072	1077	1081	rBV2	241	574	0.05%	0.007%
40	7.805	1100	1102	1110	rVB3	629	1140	0.11%	0.014%
41	7.933	1115	1123	1129	rVB4	2136	4219	0.39%	0.051%
42	8.068	1142	1145	1149	rVB2	379	527	0.05%	0.006%
43	8.330	1179	1188	1197	rBV	145076	231893	21.51%	2.781%
44	8.470	1207	1211	1221	rVB5	1658	3411	0.32%	0.041%
45	8.580	1226	1229	1231	rBV2	567	612	0.06%	0.007%
46	8.653	1234	1241	1248	rBV	575716	879372	81.55%	10.545%
47	8.720	1248	1252	1258	rVB	8580	13847	1.28%	0.166%
48	8.891	1276	1280	1284	rBV2	250	529	0.05%	0.006%
49	8.952	1284	1290	1298	rBV	105439	155187	14.39%	1.861%
50	9.116	1315	1317	1318	rBV	405	327	0.03%	0.004%
51	9.165	1321	1325	1327	rVV2	332	394	0.04%	0.005%
52	9.281	1341	1344	1347	rVB3	1093	1290	0.12%	0.015%
53	9.391	1356	1362	1376	rBV	414948	574727	53.30%	6.892%
54	9.610	1397	1398	1403	rVB2	338	402	0.04%	0.005%
55	10.055	1465	1471	1488	rBV	646726	866827	80.39%	10.394%
56	10.201	1494	1495	1500	rVB2	691	605	0.06%	0.007%
57	10.305	1506	1512	1517	rVB4	1493	2167	0.20%	0.026%
58	10.445	1533	1535	1537	rBV	429	317	0.03%	0.004%
59	10.646	1565	1568	1575	rVB3	636	1022	0.09%	0.012%
60	10.756	1583	1586	1590	rBV3	508	628	0.06%	0.008%
61	10.835	1596	1599	1600	rBV2	270	290	0.03%	0.003%
62	10.860	1600	1603	1608	rVB4	477	798	0.07%	0.010%
63	10.963	1618	1620	1624	rBV2	494	451	0.04%	0.005%
64	11.122	1641	1646	1650	rVB3	3698	4835	0.45%	0.058%
65	11.195	1653	1658	1666	rVV	407976	510547	47.35%	6.122%
66	11.457	1697	1701	1702	rBV2	868	864	0.08%	0.010%
67	11.482	1702	1705	1709	rVB3	1040	1371	0.13%	0.016%
68	11.549	1714	1716	1720	rVB3	674	674	0.06%	0.008%
69	11.756	1745	1750	1753	rVB2	3621	4783	0.44%	0.057%
70	11.841	1760	1764	1768	rBV4	835	1096	0.10%	0.013%
71	11.933	1775	1779	1784	rBV4	2169	3156	0.29%	0.038%
72	12.024	1788	1794	1803	rVV	601828	746509	69.23%	8.951%
73	12.128	1807	1811	1813	rBV3	1697	2344	0.22%	0.028%
74	12.152	1813	1815	1822	rVB3	3449	3663	0.34%	0.044%
75	12.225	1822	1827	1831	rBV3	754	1048	0.10%	0.013%
76	12.262	1831	1833	1836	rBV2	302	310	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023657.D
 Acq On : 11 Aug 2021 18:27
 Operator : JC/MD
 Sample : M3364-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1851	rBV	557589	696996	64.64%	8.358%
78	12.427	1857	1860	1861	rBV2	856	957	0.09%	0.011%
79	12.488	1866	1870	1874	rVB4	724	1221	0.11%	0.015%
80	12.762	1914	1915	1918	rBV2	356	288	0.03%	0.003%
81	12.853	1928	1930	1933	rBV2	564	585	0.05%	0.007%
82	12.914	1938	1940	1947	rVB4	354	581	0.05%	0.007%
83	12.981	1947	1951	1952	rBV2	255	365	0.03%	0.004%
84	13.054	1959	1963	1966	rBV4	546	811	0.08%	0.010%
85	13.585	2048	2050	2054	rVV2	311	308	0.03%	0.004%
86	13.774	2078	2081	2087	rBV3	396	681	0.06%	0.008%
87	13.871	2094	2097	2098	rVB	354	337	0.03%	0.004%
88	13.914	2102	2104	2106	rBV3	256	304	0.03%	0.004%
89	14.396	2181	2183	2186	rBV2	365	457	0.04%	0.005%
90	14.524	2200	2204	2207	rBV2	481	852	0.08%	0.010%
91	14.640	2220	2223	2225	rBV3	483	517	0.05%	0.006%
92	14.780	2244	2246	2249	rBV3	520	421	0.04%	0.005%
93	15.182	2311	2312	2316	rBV2	411	557	0.05%	0.007%
94	15.438	2352	2354	2355	rBV	364	289	0.03%	0.003%
95	16.017	2447	2449	2450	rBV	519	294	0.03%	0.004%
96	16.072	2457	2458	2464	rVB2	651	605	0.06%	0.007%
97	16.225	2481	2483	2488	rBV4	511	764	0.07%	0.009%
98	16.261	2488	2489	2492	rBV2	307	324	0.03%	0.004%
99	16.615	2545	2547	2549	rBV2	567	533	0.05%	0.006%
100	16.749	2568	2569	2572	rBV3	434	473	0.04%	0.006%


Sum of corrected areas: 8339536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023657.D
Acq On : 11 Aug 2021 18:27
Operator : JC/MD
Sample : M3364-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
DBK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

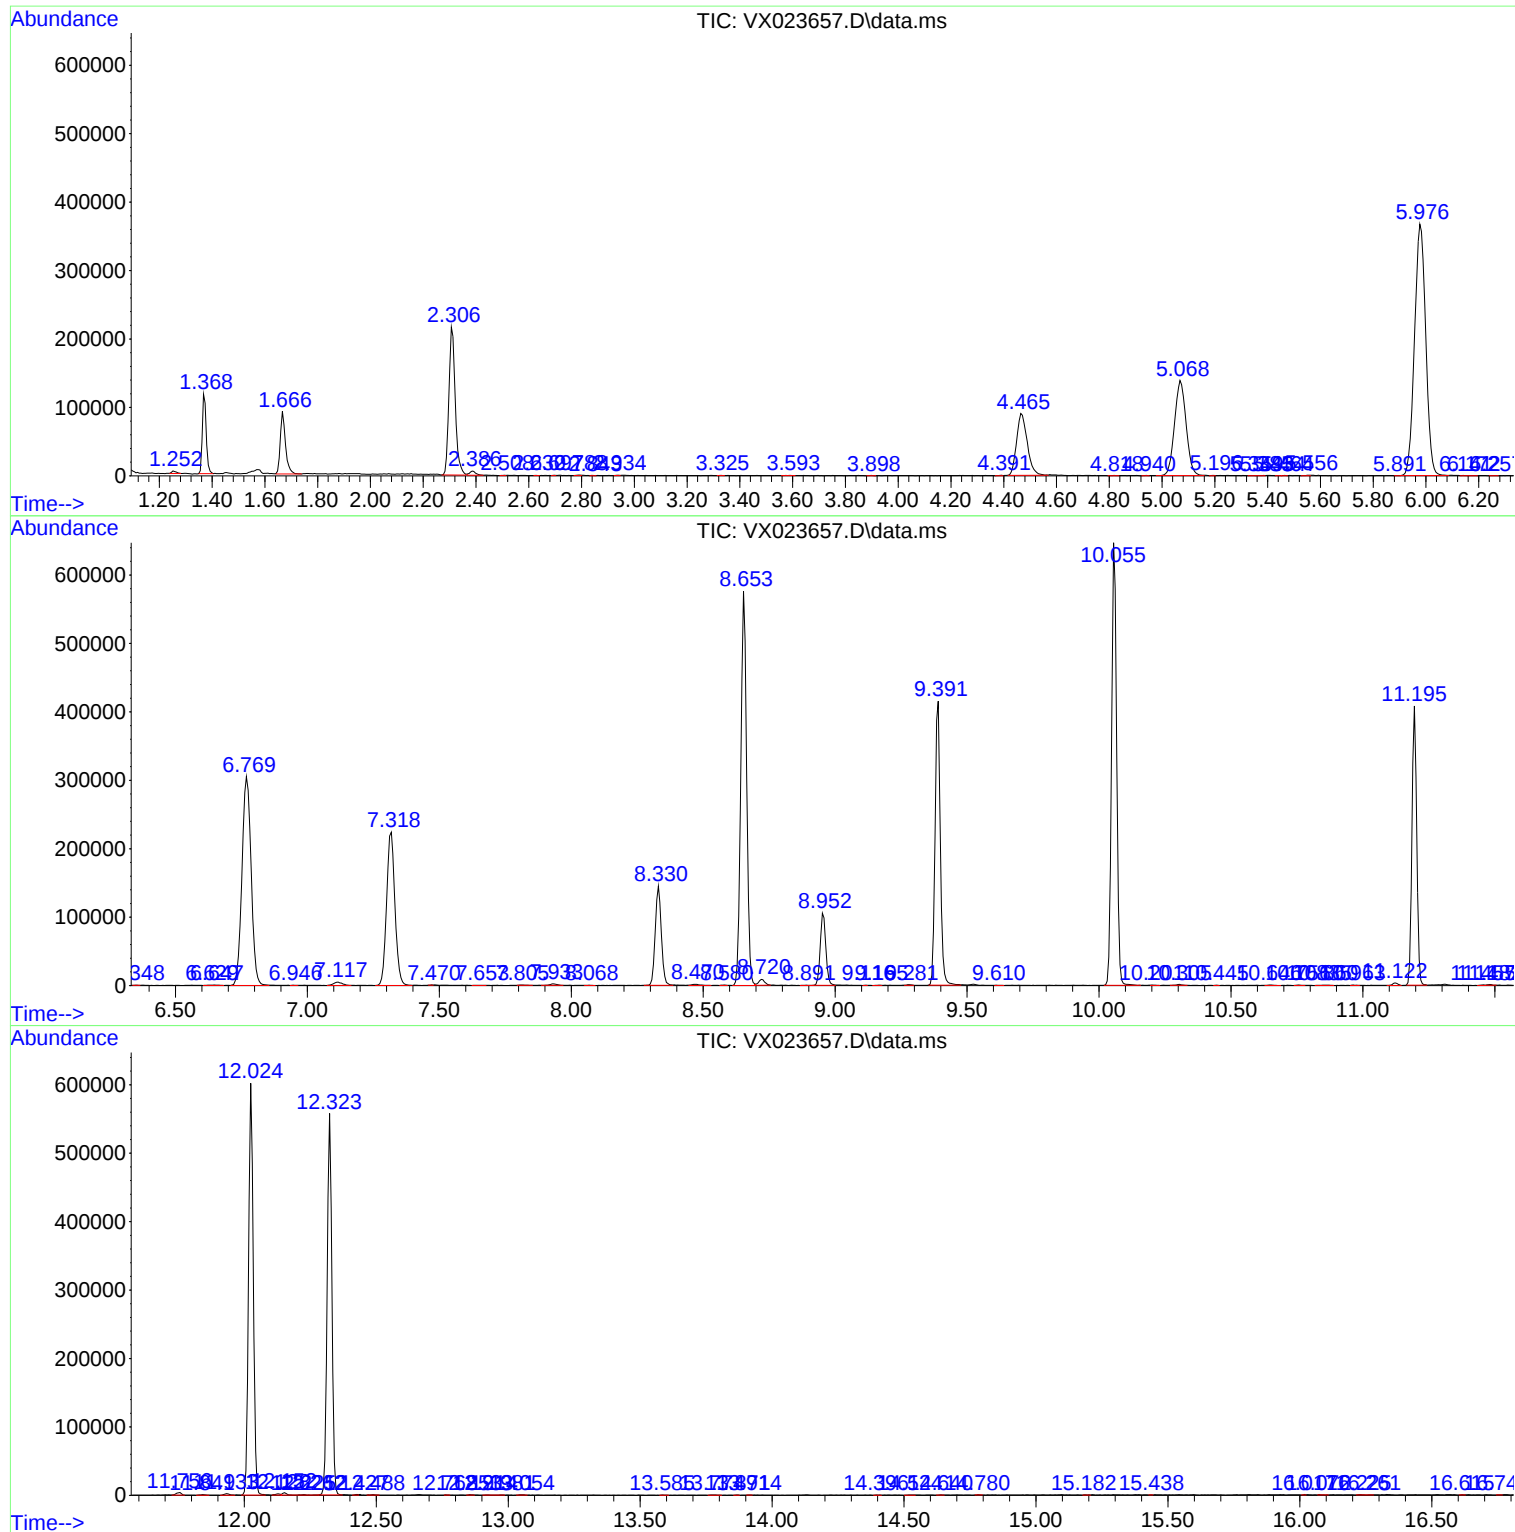

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023657.D
Acq On : 11 Aug 2021 18:27
Operator : JC/MD
Sample : M3364-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023657.D
Acq On : 11 Aug 2021 18:27
Operator : JC/MD
Sample : M3364-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
