

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023658.D
 Acq On : 11 Aug 2021 18:50
 Operator : JC/MD
 Sample : M3364-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

Signal : TIC: VX023658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rVB2	5306	6509	0.62%	0.080%
2	1.368	43	46	55	rVB	114854	115438	10.98%	1.422%
3	1.666	91	95	106	rVB	88733	118019	11.23%	1.454%
4	2.307	194	200	210	rBV	212829	343049	32.63%	4.226%
5	2.544	237	239	242	rVB	463	355	0.03%	0.004%
6	2.715	264	267	269	rVB3	496	561	0.05%	0.007%
7	2.788	275	279	282	rBV3	645	1037	0.10%	0.013%
8	2.843	286	288	290	rBV	412	294	0.03%	0.004%
9	2.910	296	299	301	rVB2	315	328	0.03%	0.004%
10	2.953	301	306	308	rBV2	668	1223	0.12%	0.015%
11	3.172	340	342	346	rVB3	266	353	0.03%	0.004%
12	3.288	358	361	364	rBV2	245	323	0.03%	0.004%
13	3.526	397	400	402	rBV2	271	324	0.03%	0.004%
14	3.739	432	435	437	rVB2	292	323	0.03%	0.004%
15	3.892	457	460	463	rBV2	351	405	0.04%	0.005%
16	4.081	487	491	492	rBV2	268	337	0.03%	0.004%
17	4.245	516	518	522	rVB2	517	685	0.07%	0.008%
18	4.349	533	535	537	rVB2	399	373	0.04%	0.005%
19	4.471	543	555	574	rBV	86808	250219	23.80%	3.082%
20	4.666	586	587	590	rVB2	543	352	0.03%	0.004%
21	4.837	613	615	620	rBV2	319	484	0.05%	0.006%
22	5.068	640	653	671	rVV2	133289	410533	39.05%	5.057%
23	5.245	680	682	685	rVB3	288	306	0.03%	0.004%
24	5.556	730	733	734	rBV2	532	523	0.05%	0.006%
25	5.714	757	759	762	rVV2	340	351	0.03%	0.004%
26	5.800	770	773	775	rBV	282	359	0.03%	0.004%
27	5.977	789	802	819	rVV2	360532	1051381	100.00%	12.951%
28	6.092	819	821	825	rVV3	679	976	0.09%	0.012%
29	6.635	908	910	913	rBV2	453	608	0.06%	0.007%
30	6.769	920	932	947	rBV	290390	695074	66.11%	8.562%
31	6.946	957	961	964	rBV3	341	620	0.06%	0.008%
32	7.123	982	990	998	rVV4	5070	11218	1.07%	0.138%
33	7.318	1011	1022	1039	rBV	221438	479578	45.61%	5.908%
34	7.592	1063	1067	1070	rBV3	372	520	0.05%	0.006%
35	7.678	1080	1081	1086	rVB	217	297	0.03%	0.004%
36	7.818	1099	1104	1108	rBV3	709	1418	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023658.D
 Acq On : 11 Aug 2021 18:50
 Operator : JC/MD
 Sample : M3364-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.927	1118	1122	1129	rVV2	2060	3680	0.35%	0.045%
38	8.019	1134	1137	1141	rBV3	245	297	0.03%	0.004%
39	8.135	1153	1156	1159	rBV2	224	296	0.03%	0.004%
40	8.330	1181	1188	1200	rBV	141573	225899	21.49%	2.783%
41	8.476	1208	1212	1215	rBV2	1482	1946	0.19%	0.024%
42	8.580	1223	1229	1230	rBV4	329	453	0.04%	0.006%
43	8.653	1234	1241	1248	rBV	558493	857077	81.52%	10.558%
44	8.720	1248	1252	1258	rVB	7693	12672	1.21%	0.156%
45	8.952	1283	1290	1301	rBV	99274	148732	14.15%	1.832%
46	9.177	1324	1327	1330	rBV2	369	449	0.04%	0.006%
47	9.275	1338	1343	1350	rBV3	1680	2571	0.24%	0.032%
48	9.324	1350	1351	1355	rBV2	324	313	0.03%	0.004%
49	9.391	1356	1362	1380	rVV	381688	557948	53.07%	6.873%
50	9.677	1406	1409	1411	rVB	383	399	0.04%	0.005%
51	9.714	1411	1415	1417	rBV2	305	405	0.04%	0.005%
52	9.823	1431	1433	1436	rBV	263	339	0.03%	0.004%
53	10.055	1466	1471	1487	rVB	608663	829328	78.88%	10.216%
54	10.305	1506	1512	1517	rVB4	1322	2049	0.19%	0.025%
55	10.451	1534	1536	1541	rBV	284	565	0.05%	0.007%
56	10.653	1564	1569	1572	rBV5	716	975	0.09%	0.012%
57	10.756	1585	1586	1590	rVB2	445	311	0.03%	0.004%
58	10.860	1599	1603	1605	rBV2	482	529	0.05%	0.007%
59	11.122	1642	1646	1650	rBV	3704	4805	0.46%	0.059%
60	11.195	1652	1658	1669	rVV	405607	509166	48.43%	6.272%
61	11.281	1669	1672	1674	rVV3	663	706	0.07%	0.009%
62	11.317	1674	1678	1683	rVB4	1397	2822	0.27%	0.035%
63	11.457	1698	1701	1703	rBV3	706	789	0.08%	0.010%
64	11.610	1725	1726	1733	rVB3	329	552	0.05%	0.007%
65	11.677	1733	1737	1740	rBV3	410	718	0.07%	0.009%
66	11.713	1741	1743	1744	rVB2	516	310	0.03%	0.004%
67	11.750	1744	1749	1754	rBV2	3655	5126	0.49%	0.063%
68	11.848	1761	1765	1767	rBV3	1060	1176	0.11%	0.014%
69	11.933	1775	1779	1783	rVB4	1817	2393	0.23%	0.029%
70	11.976	1783	1786	1789	rBV3	647	705	0.07%	0.009%
71	12.024	1789	1794	1805	rBV	590755	727072	69.15%	8.956%
72	12.152	1812	1815	1819	rVB3	3236	4069	0.39%	0.050%
73	12.219	1824	1826	1827	rBV2	742	549	0.05%	0.007%
74	12.268	1832	1834	1836	rBB3	434	312	0.03%	0.004%
75	12.323	1836	1843	1851	rBV	561409	702098	66.78%	8.649%
76	12.427	1858	1860	1864	rVB3	1203	1215	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023658.D
 Acq On : 11 Aug 2021 18:50
 Operator : JC/MD
 Sample : M3364-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.664	1897	1899	1905	rVB3	651	912	0.09%	0.011%
78	12.768	1912	1916	1918	rVB3	560	553	0.05%	0.007%
79	12.853	1928	1930	1936	rVB3	669	844	0.08%	0.010%
80	12.914	1938	1940	1941	rBV2	353	312	0.03%	0.004%
81	12.951	1944	1946	1948	rBV2	365	354	0.03%	0.004%
82	13.061	1961	1964	1967	rVB2	783	841	0.08%	0.010%
83	13.152	1977	1979	1983	rVB2	326	390	0.04%	0.005%
84	13.378	2012	2016	2020	rBV	307	436	0.04%	0.005%
85	13.591	2049	2051	2057	rVB2	382	612	0.06%	0.008%
86	13.731	2070	2074	2075	rBV2	298	349	0.03%	0.004%
87	13.756	2075	2078	2081	rBV3	254	402	0.04%	0.005%
88	14.115	2134	2137	2138	rBV2	382	342	0.03%	0.004%
89	14.182	2146	2148	2151	rVB2	366	365	0.03%	0.004%
90	14.225	2151	2155	2157	rBV2	246	298	0.03%	0.004%
91	14.591	2210	2215	2216	rBV2	299	320	0.03%	0.004%
92	14.768	2242	2244	2246	rBV2	352	345	0.03%	0.004%
93	15.158	2305	2308	2310	rBV2	517	722	0.07%	0.009%
94	15.792	2409	2412	2414	rBV	372	402	0.04%	0.005%
95	15.969	2439	2441	2443	rBV3	604	439	0.04%	0.005%
96	16.024	2448	2450	2452	rBV	601	610	0.06%	0.008%
97	16.060	2454	2456	2458	rVB	437	332	0.03%	0.004%
98	16.152	2468	2471	2473	rBV2	479	597	0.06%	0.007%
99	16.664	2554	2555	2558	rVB3	585	329	0.03%	0.004%
100	16.725	2564	2565	2567	rBV	631	428	0.04%	0.005%


Sum of corrected areas: 8118103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023658.D
Acq On : 11 Aug 2021 18:50
Operator : JC/MD
Sample : M3364-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

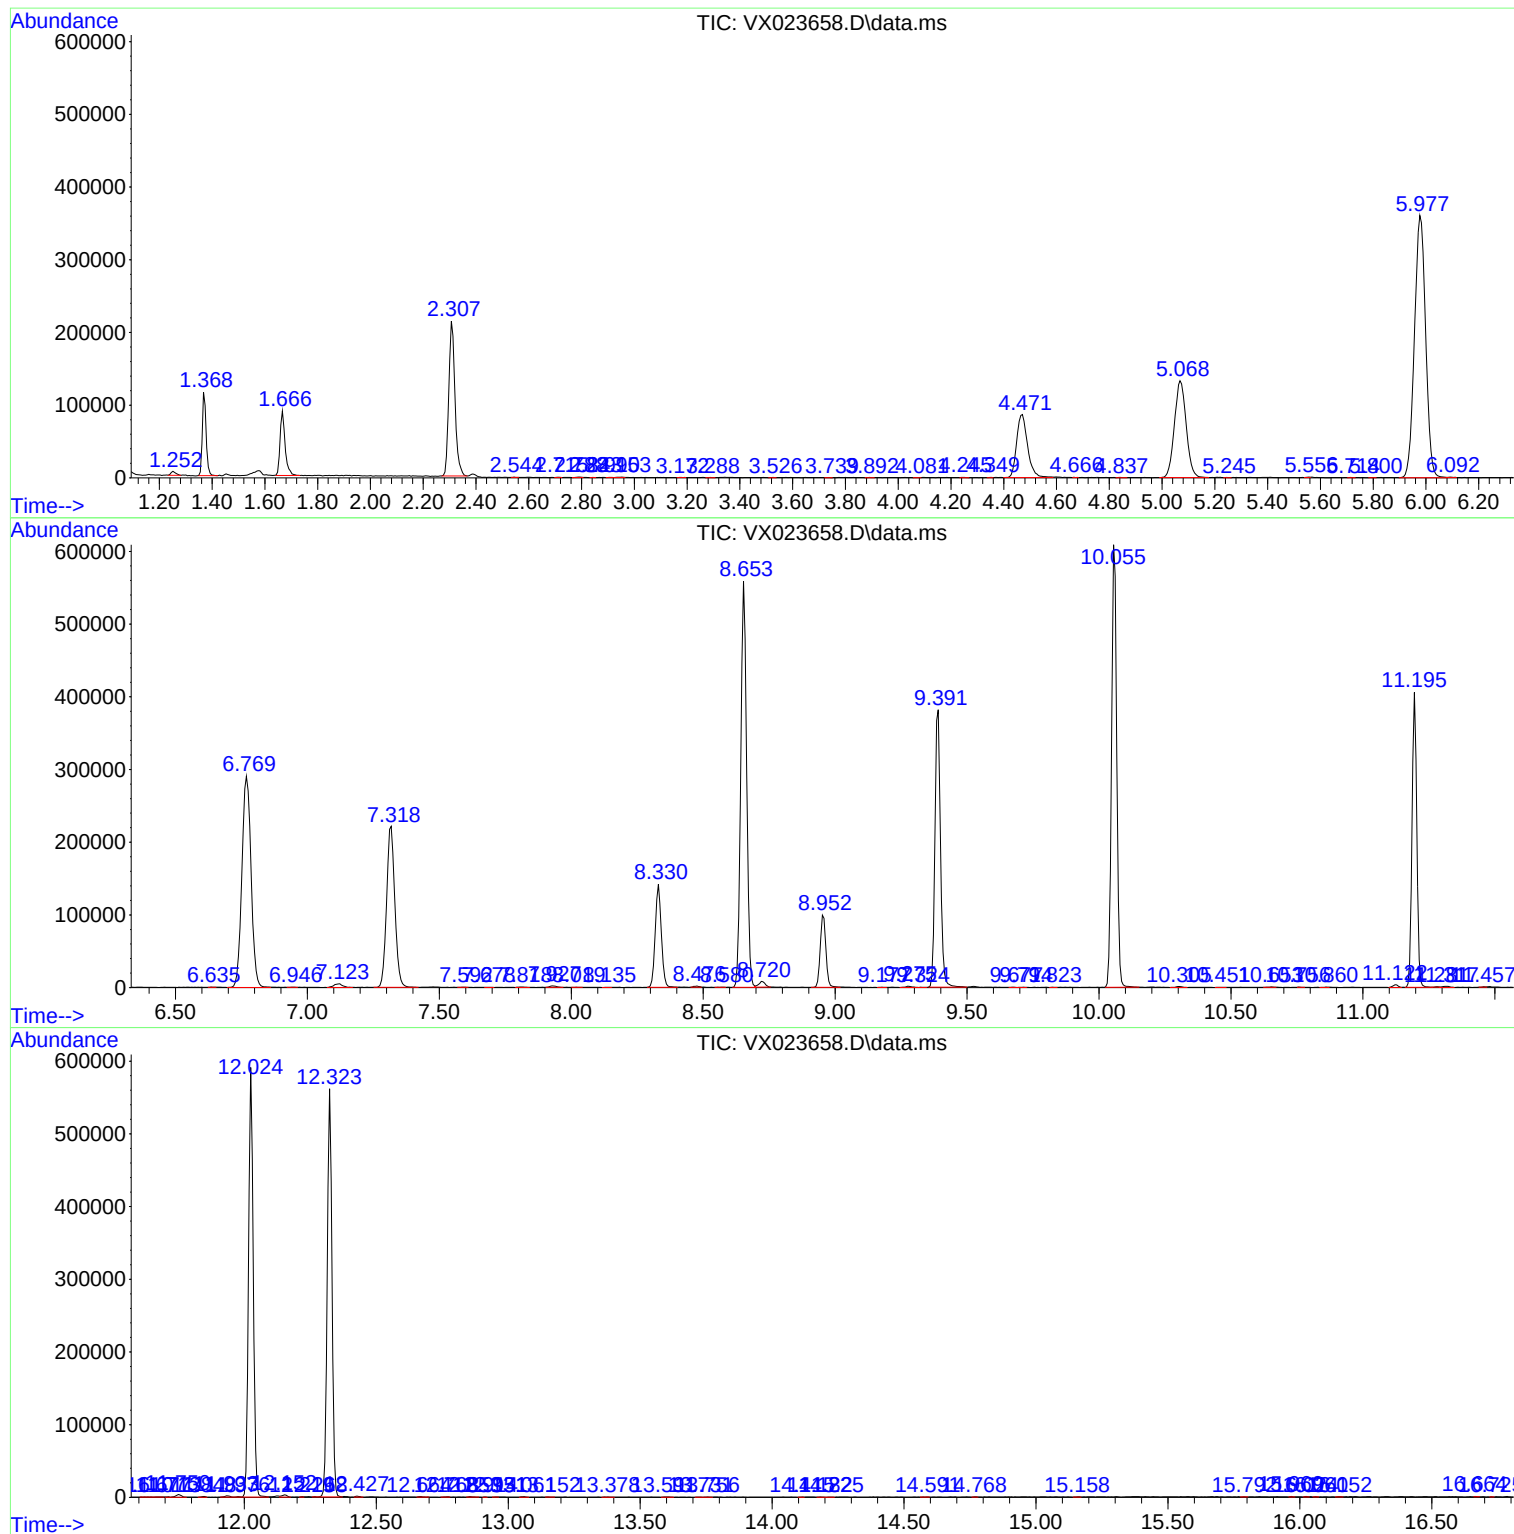

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023658.D
Acq On : 11 Aug 2021 18:50
Operator : JC/MD
Sample : M3364-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023658.D
Acq On : 11 Aug 2021 18:50
Operator : JC/MD
Sample : M3364-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
