

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023659.D
 Acq On : 11 Aug 2021 19:14
 Operator : JC/MD
 Sample : VIBLK601
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	53	rVB	117818	119861	10.88%	1.395%
2	1.666	90	95	105	rBV	93029	125635	11.41%	1.462%
3	2.306	194	200	211	rVB	220315	363516	33.01%	4.231%
4	2.794	274	280	286	rBV5	2093	4035	0.37%	0.047%
5	2.946	301	305	306	rBV	814	964	0.09%	0.011%
6	3.154	336	339	342	rBV2	385	577	0.05%	0.007%
7	3.203	345	347	351	rVB2	303	310	0.03%	0.004%
8	3.263	356	357	362	rVV2	316	397	0.04%	0.005%
9	3.349	370	371	374	rBV2	293	335	0.03%	0.004%
10	3.696	426	428	431	rVB	394	284	0.03%	0.003%
11	3.928	463	466	471	rBV2	232	266	0.02%	0.003%
12	4.032	479	483	484	rBV	307	304	0.03%	0.004%
13	4.361	534	537	539	rBV2	344	397	0.04%	0.005%
14	4.464	545	554	573	rBV	99342	279332	25.36%	3.251%
15	4.782	605	606	611	rVV2	314	349	0.03%	0.004%
16	4.885	620	623	627	rVB2	198	350	0.03%	0.004%
17	4.916	627	628	630	rBV2	309	275	0.02%	0.003%
18	5.068	640	653	671	rVV2	138353	432197	39.24%	5.031%
19	5.556	727	733	738	rBV5	1308	2916	0.26%	0.034%
20	5.665	750	751	755	rBV2	263	350	0.03%	0.004%
21	5.976	789	802	819	rVV2	377440	1101287	100.00%	12.819%
22	6.165	828	833	837	rVB4	384	747	0.07%	0.009%
23	6.415	872	874	877	rVB2	360	379	0.03%	0.004%
24	6.489	884	886	888	rVB	425	273	0.02%	0.003%
25	6.769	922	932	943	rBV	309341	739921	67.19%	8.613%
26	7.110	982	988	997	rVB4	6242	13968	1.27%	0.163%
27	7.318	1013	1022	1037	rVV	227095	500702	45.47%	5.828%
28	7.531	1054	1057	1059	rBV	274	285	0.03%	0.003%
29	7.811	1100	1103	1105	rBV	527	481	0.04%	0.006%
30	7.927	1116	1122	1130	rVV2	2676	4283	0.39%	0.050%
31	8.330	1181	1188	1198	rBV	150117	237316	21.55%	2.762%
32	8.476	1207	1212	1218	rBV4	1753	2823	0.26%	0.033%
33	8.580	1226	1229	1233	rVB2	550	782	0.07%	0.009%
34	8.653	1234	1241	1249	rBV	581899	899539	81.68%	10.471%
35	8.720	1249	1252	1259	rVB	8219	13257	1.20%	0.154%
36	8.866	1275	1276	1281	rBV2	341	326	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023659.D
 Acq On : 11 Aug 2021 19:14
 Operator : JC/MD
 Sample : VIBLK601
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.951	1285	1290	1300	rBV	109294	158950	14.43%	1.850%
38	9.153	1322	1323	1326	rBV	286	342	0.03%	0.004%
39	9.208	1330	1332	1337	rBV3	267	317	0.03%	0.004%
40	9.275	1341	1343	1347	rVB4	928	1202	0.11%	0.014%
41	9.390	1356	1362	1375	rBV	430216	627204	56.95%	7.301%
42	9.701	1410	1413	1419	rVB2	595	1073	0.10%	0.012%
43	9.750	1419	1421	1425	rBV2	263	370	0.03%	0.004%
44	9.982	1455	1459	1463	rBV2	374	436	0.04%	0.005%
45	10.055	1465	1471	1484	rVV	652015	891462	80.95%	10.377%
46	10.195	1491	1494	1498	rBV3	1034	1422	0.13%	0.017%
47	10.305	1508	1512	1519	rBV5	1559	2321	0.21%	0.027%
48	10.470	1532	1539	1542	rVB3	259	540	0.05%	0.006%
49	10.537	1547	1550	1552	rBV	350	290	0.03%	0.003%
50	10.585	1555	1558	1562	rVB2	202	294	0.03%	0.003%
51	10.646	1562	1568	1573	rBV5	1128	2158	0.20%	0.025%
52	10.756	1584	1586	1593	rVB2	242	365	0.03%	0.004%
53	10.854	1599	1602	1604	rBV2	310	352	0.03%	0.004%
54	10.963	1615	1620	1624	rVB3	696	928	0.08%	0.011%
55	11.122	1641	1646	1652	rVB2	3421	4358	0.40%	0.051%
56	11.195	1652	1658	1664	rBV	436713	532948	48.39%	6.204%
57	11.286	1670	1673	1674	rBV2	850	806	0.07%	0.009%
58	11.457	1697	1701	1703	rBV3	795	937	0.09%	0.011%
59	11.482	1703	1705	1708	rVV2	630	609	0.06%	0.007%
60	11.549	1713	1716	1718	rBV2	542	542	0.05%	0.006%
61	11.616	1725	1727	1730	rBV2	324	409	0.04%	0.005%
62	11.683	1736	1738	1741	rVB	261	274	0.02%	0.003%
63	11.713	1741	1743	1745	rBV3	296	346	0.03%	0.004%
64	11.750	1745	1749	1756	rVB3	3691	5138	0.47%	0.060%
65	11.835	1761	1763	1768	rVB4	741	912	0.08%	0.011%
66	11.933	1776	1779	1783	rBV3	1641	2154	0.20%	0.025%
67	11.969	1783	1785	1789	rVB3	692	635	0.06%	0.007%
68	12.024	1789	1794	1807	rVB	615243	759813	68.99%	8.844%
69	12.128	1807	1811	1812	rBV2	1379	1904	0.17%	0.022%
70	12.323	1836	1843	1851	rBV	587843	726182	65.94%	8.453%
71	12.426	1859	1860	1864	rVB3	1061	840	0.08%	0.010%
72	12.634	1892	1894	1896	rBV2	301	308	0.03%	0.004%
73	12.768	1913	1916	1920	rVV2	663	796	0.07%	0.009%
74	12.823	1923	1925	1928	rVB2	382	315	0.03%	0.004%
75	12.859	1928	1931	1933	rBV2	368	424	0.04%	0.005%
76	12.902	1935	1938	1942	rBV2	259	281	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023659.D
 Acq On : 11 Aug 2021 19:14
 Operator : JC/MD
 Sample : VIBLK601
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	13.012	1954	1956	1959	rBV2	256	265	0.02%	0.003%
78	13.036	1959	1960	1961	rVV	429	304	0.03%	0.004%
79	13.054	1961	1963	1967	rVV2	793	875	0.08%	0.010%
80	13.115	1969	1973	1977	rVV4	544	624	0.06%	0.007%
81	13.731	2070	2074	2077	rVV2	255	411	0.04%	0.005%
82	13.780	2077	2082	2087	rVB3	584	1201	0.11%	0.014%
83	13.920	2103	2105	2108	rBV2	369	396	0.04%	0.005%
84	14.018	2118	2121	2123	rBV3	358	353	0.03%	0.004%
85	14.042	2123	2125	2129	rVV3	300	269	0.02%	0.003%
86	14.133	2138	2140	2142	rVB2	762	621	0.06%	0.007%
87	14.225	2152	2155	2158	rBV3	322	357	0.03%	0.004%
88	14.298	2165	2167	2170	rBV2	415	439	0.04%	0.005%
89	14.420	2183	2187	2189	rBV3	312	298	0.03%	0.003%
90	14.542	2206	2207	2209	rBV	382	320	0.03%	0.004%
91	14.609	2215	2218	2219	rBV2	283	359	0.03%	0.004%
92	14.737	2235	2239	2242	rBV3	532	694	0.06%	0.008%
93	14.804	2247	2250	2253	rVV3	555	623	0.06%	0.007%
94	14.853	2256	2258	2261	rBV3	251	292	0.03%	0.003%
95	14.963	2274	2276	2278	rBV2	421	366	0.03%	0.004%
96	15.017	2284	2285	2287	rBV2	514	429	0.04%	0.005%
97	15.249	2321	2323	2326	rVV3	495	429	0.04%	0.005%
98	15.322	2333	2335	2338	rBV2	358	450	0.04%	0.005%
99	15.426	2351	2352	2357	rBV4	299	405	0.04%	0.005%
100	16.517	2529	2531	2533	rBV	379	309	0.03%	0.004%


Sum of corrected areas: 8591065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023659.D
Acq On : 11 Aug 2021 19:14
Operator : JC/MD
Sample : VIBLK601
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

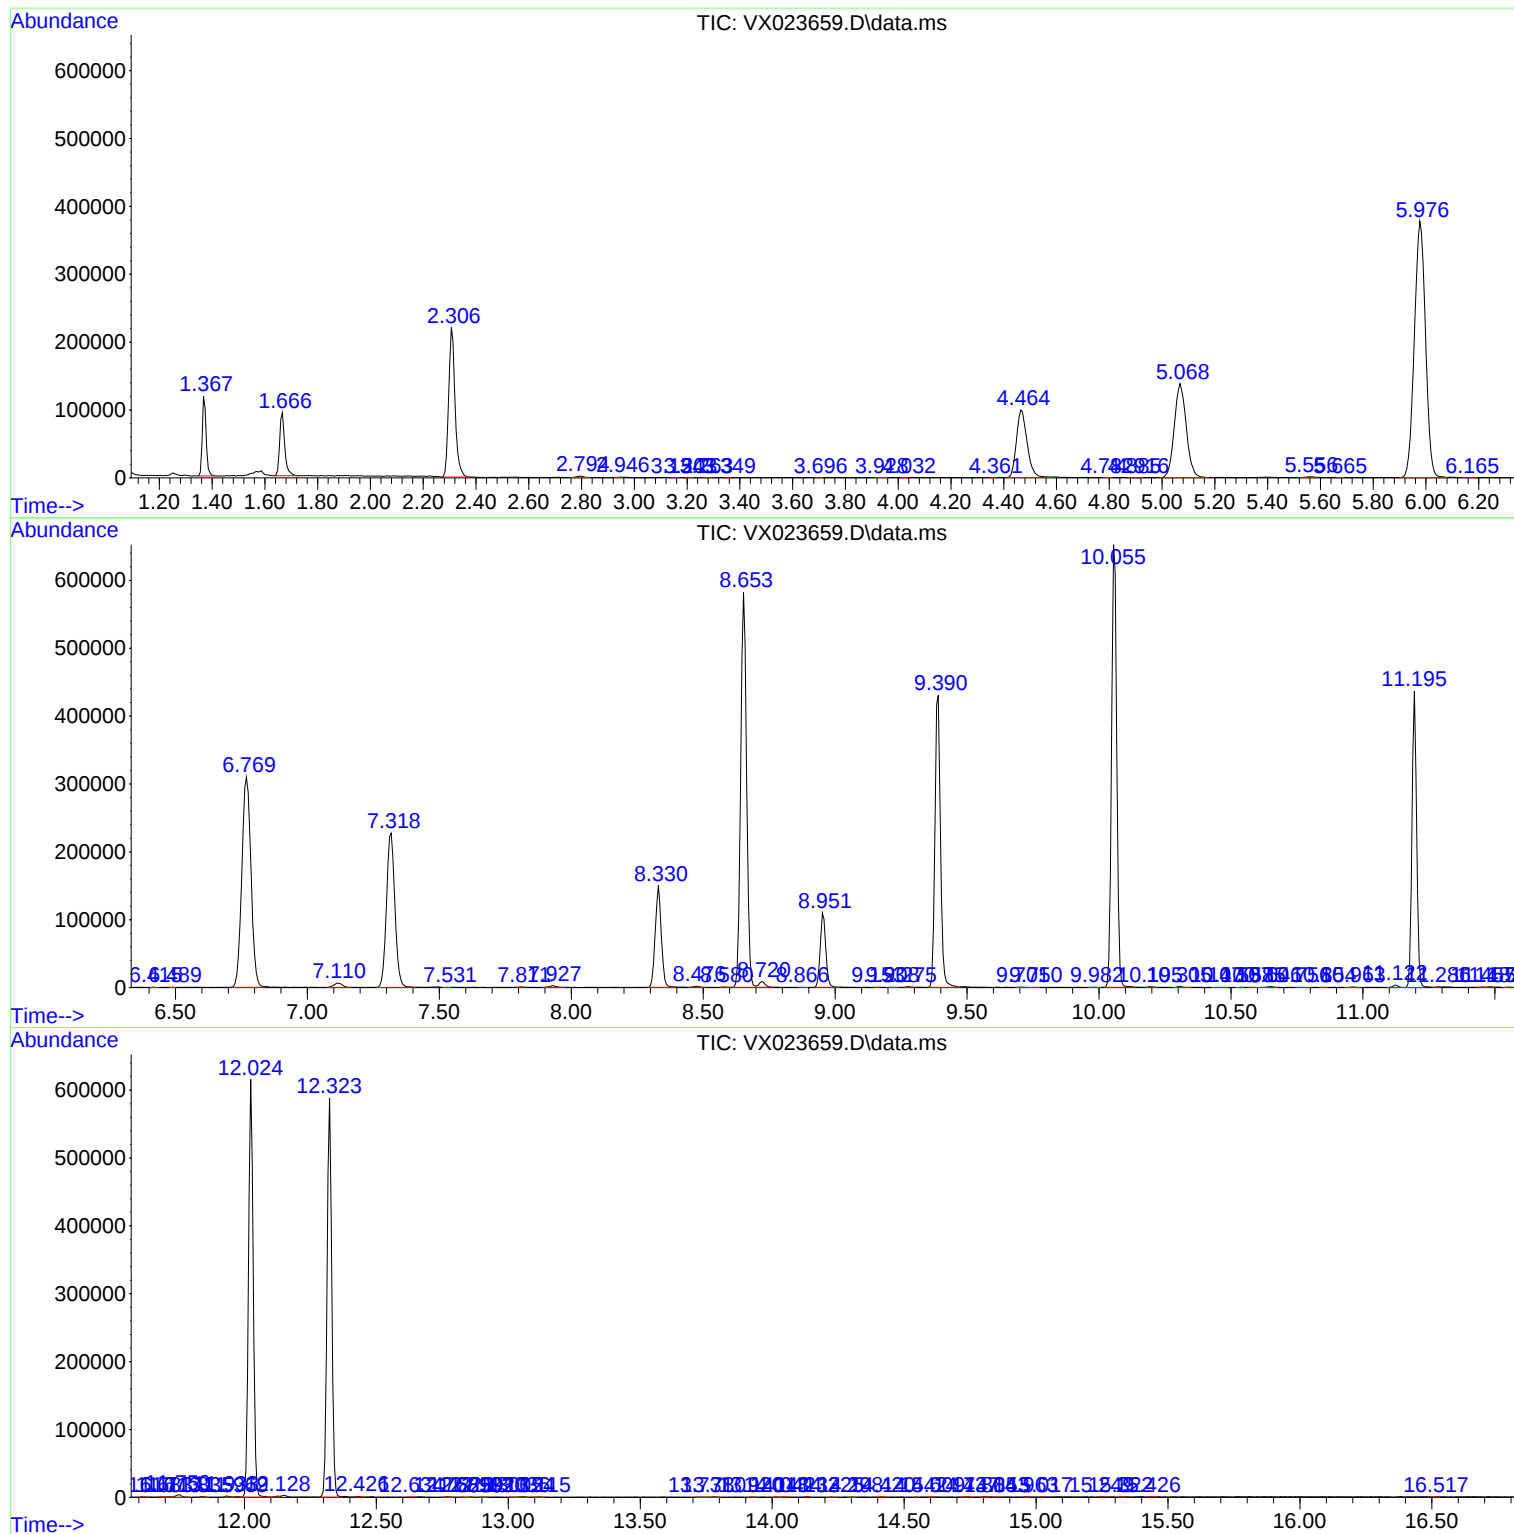

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023659.D
Acq On : 11 Aug 2021 19:14
Operator : JC/MD
Sample : VIBLK601
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
Data File : VX023659.D
Acq On : 11 Aug 2021 19:14
Operator : JC/MD
Sample : VIBLK601
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
