
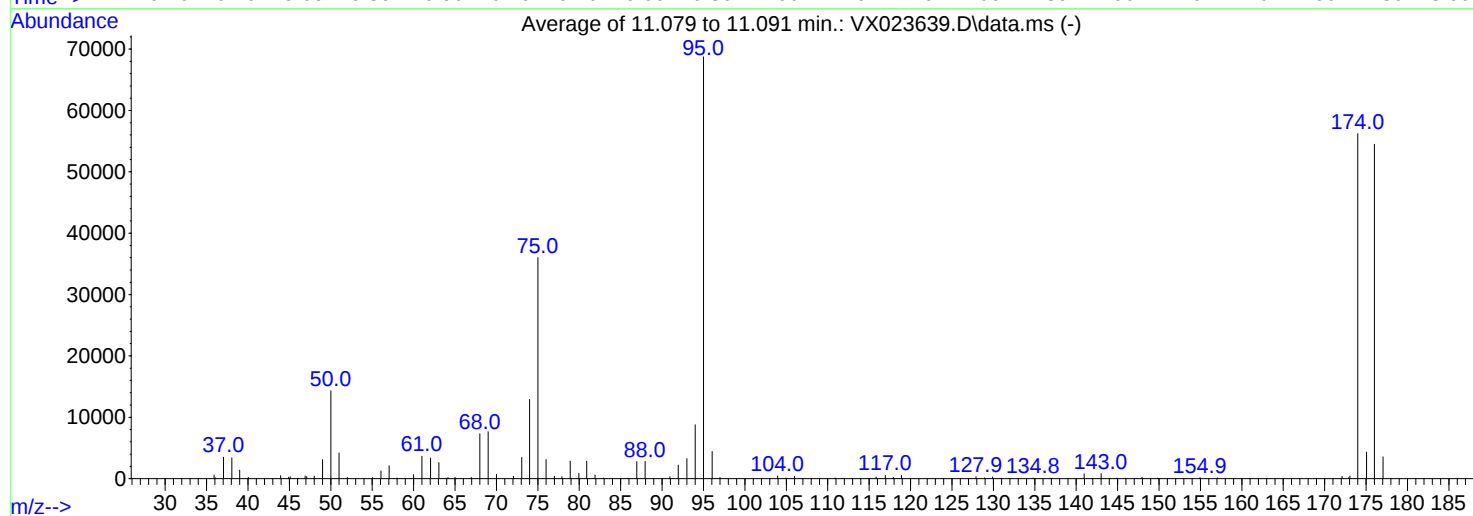


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081121\
 Data File : VX023639.D
 Acq On : 11 Aug 2021 08:21
 Operator : JC/MD
 Sample : BFB602
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB602

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM081121WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 13 01:00:38 2021

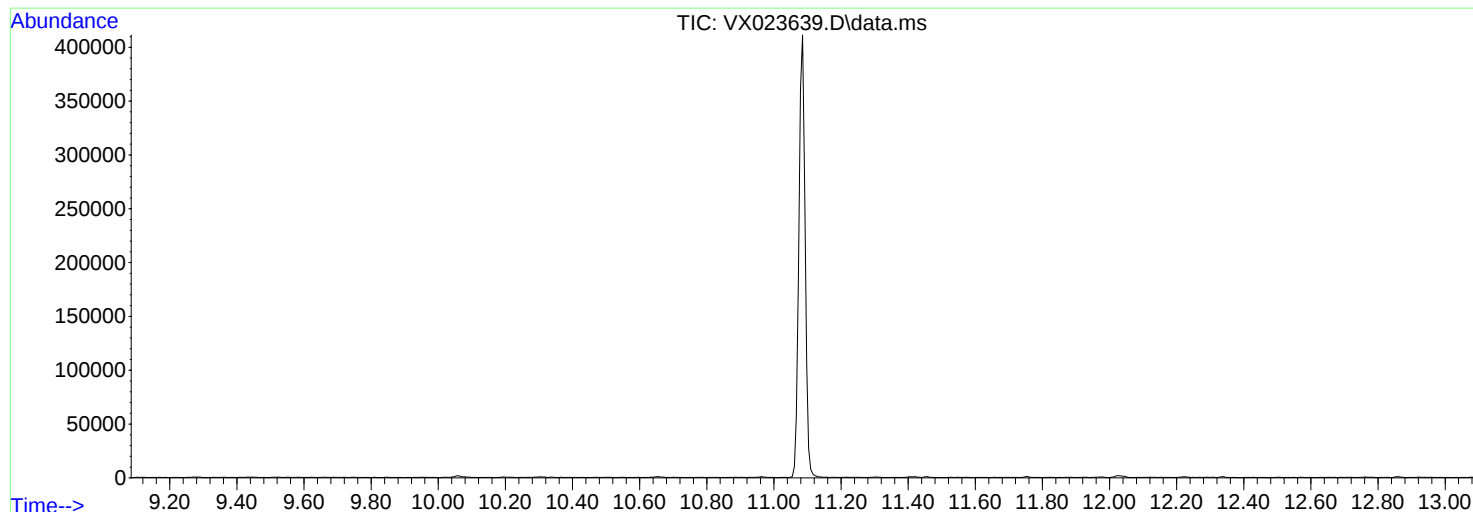

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	14314	PASS
75	95	30	80	52.4	36029	PASS
95	95	100	100	100.0	68741	PASS
96	95	5	9	6.5	4446	PASS
173	174	0.00	2	0.7	421	PASS
174	95	50	120	81.8	56208	PASS
175	174	5	9	7.7	4332	PASS
176	174	95	101	96.9	54491	PASS
177	176	5	9	6.5	3547	PASS

m/z	Abundance
35.90	953.0
37.00	3723.0
38.10	3973.0
39.00	1667.0
40.00	304.0
44.00	883.0
45.10	666.0
47.10	1062.0
47.90	404.0
49.00	3502.0
50.00	16872.0
51.00	5063.0
52.00	236.0
55.10	165.0
56.10	1413.0
57.10	2381.0
58.00	94.0
60.00	743.0
61.00	4091.0
62.10	3705.0
63.00	3083.0
64.10	274.0
65.00	340.0
66.90	303.0
68.00	8567.0
69.00	8542.0
70.00	762.0
72.10	395.0
73.00	3997.0
74.00	16042.0
75.00	42480.0
76.00	3789.0
77.00	511.0
77.80	411.0
78.90	3254.0
80.00	970.0
80.90	3340.0
81.90	880.0
82.90	155.0
85.80	106.0
86.90	3373.0
87.90	3077.0
90.90	382.0
91.90	2581.0
93.00	3806.0
94.00	10304.0
95.00	82128.0
96.10	5294.0
97.00	170.0
103.10	50.0
103.90	590.0
104.90	135.0
106.00	416.0
106.90	52.0
110.90	99.0
111.70	87.0
112.90	89.0
114.90	59.0
115.90	342.0
116.80	475.0
118.00	312.0
118.90	482.0
127.90	397.0
128.90	186.0
129.90	344.0
131.00	134.0
134.80	135.0
137.10	211.0
140.00	76.0
141.00	975.0
141.80	69.0
143.00	914.0
144.10	77.0
144.90	104.0
145.90	110.0
148.00	271.0
149.80	122.0
154.90	240.0
157.00	123.0
159.00	181.0
160.90	80.0
171.00	73.0
172.10	569.0
173.10	697.0
174.00	66792.0
175.10	5547.0
176.00	64440.0
177.00	4068.0
178.00	59.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
36.10	396.0
37.00	2470.0
38.00	1891.0
39.00	1068.0
40.10	211.0
44.00	610.0
45.10	315.0
46.90	646.0
48.00	342.0
49.10	2141.0
50.00	9421.0
51.00	2949.0
52.00	123.0
55.00	134.0
56.00	868.0
57.00	1701.0
58.10	70.0
60.00	527.0
61.00	2790.0
62.00	2643.0
63.10	1769.0
63.90	251.0
64.90	141.0
65.20	148.0
66.90	128.0
68.00	4788.0
69.00	6325.0
69.90	430.0
72.00	335.0
73.00	2273.0
74.00	8843.0
75.00	26456.0
76.10	2084.0
76.90	283.0
78.00	136.0
78.90	1967.0
79.90	684.0
80.90	2057.0
81.90	359.0
83.00	73.0
87.00	2145.0
88.00	2161.0
90.90	201.0
92.00	1819.0
93.00	2402.0
94.00	6596.0
95.10	50968.0
96.00	3117.0
96.90	116.0
103.90	393.0
105.90	236.0
110.80	63.0
114.90	57.0
115.90	287.0
117.00	447.0
117.90	286.0
118.90	531.0
127.90	245.0
128.90	89.0
130.00	185.0
131.00	95.0
134.80	95.0
136.80	140.0
140.90	636.0
142.00	84.0
143.00	591.0
145.00	88.0
145.80	66.0
148.00	185.0
154.90	177.0
157.00	161.0
160.90	54.0
172.00	280.0
173.00	567.0
174.00	48848.0
175.00	3680.0
176.00	49776.0
177.10	3030.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
39.00	100.0
39.90	165.0
44.00	240.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602

m/z	Abundance
35.90	843.0
37.10	4277.0
38.00	4280.0
39.00	1745.0
39.80	125.0
40.20	140.0
42.90	53.0
43.90	696.0
44.90	728.0
46.10	59.0
46.90	701.0
48.10	517.0
49.00	3650.0
50.00	16648.0
51.00	4526.0
52.00	261.0
55.00	214.0
56.00	1445.0
57.10	2290.0
58.00	181.0
60.00	722.0
61.00	4072.0
62.00	3779.0
63.10	3011.0
64.20	315.0
65.00	177.0
67.00	196.0
68.00	8566.0
69.00	8046.0
70.00	844.0
72.00	418.0
73.10	4074.0
74.00	13865.0
75.00	39152.0
76.00	3417.0
77.10	422.0
78.00	379.0
78.90	3305.0
79.90	901.0
80.90	3148.0
81.90	592.0
83.00	83.0
85.80	76.0
86.90	2815.0
88.00	3216.0
91.00	378.0
92.00	2278.0
93.00	3551.0
94.00	9510.0
95.00	73128.0
96.00	4927.0
97.10	255.0
103.00	50.0
104.00	339.0
105.00	177.0
106.00	518.0
106.90	93.0
110.90	137.0
111.80	109.0
113.00	100.0
115.80	259.0
117.00	667.0
117.80	285.0
118.90	529.0
123.90	70.0
127.90	308.0
129.00	112.0
129.90	319.0
130.80	88.0
134.80	99.0
136.90	119.0
140.10	60.0
140.90	760.0
143.00	901.0
144.10	55.0
144.80	113.0
145.90	110.0
147.90	145.0
149.90	103.0
155.00	129.0
157.10	116.0
159.00	97.0
172.10	369.0
172.90	503.0
174.00	52984.0
175.00	3768.0
176.00	49256.0
177.00	3542.0
178.00	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB602