

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030568.D
 Acq On : 11 Aug 2022 13:09
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK668

Quant Time: Aug 12 04:18:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 12 04:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	283110	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	255449	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	115865	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85102	46.809	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.620%
7) Chloroethane-d5	1.666	69	68532	53.471	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.940%
11) 1,1-Dichloroethene-d2	2.307	63	135836	39.498	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.000%
21) 2-Butanone-d5	4.471	46	206679	122.691	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	122.690%
24) Chloroform-d	5.068	84	197749	52.838	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.680%
26) 1,2-Dichloroethane-d4	5.964	65	142783	56.187	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.380%
32) Benzene-d6	5.983	84	376918	51.511	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.020%
36) 1,2-Dichloropropane-d6	7.312	67	127447	53.684	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.360%
41) Toluene-d8	8.653	98	342263	49.623	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.240%
43) trans-1,3-Dichloroprop...	8.952	79	58318	49.379	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.760%
47) 2-Hexanone-d5	9.385	63	136839	113.081	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.080%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	172767	55.397	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	120188	53.480	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.960%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.307	101	1441	0.838	ug/L	Qvalue # 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030568.D
Acq On : 11 Aug 2022 13:09
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK668

Quant Time: Aug 12 04:18:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 04:17:17 2022
Response via : Initial Calibration

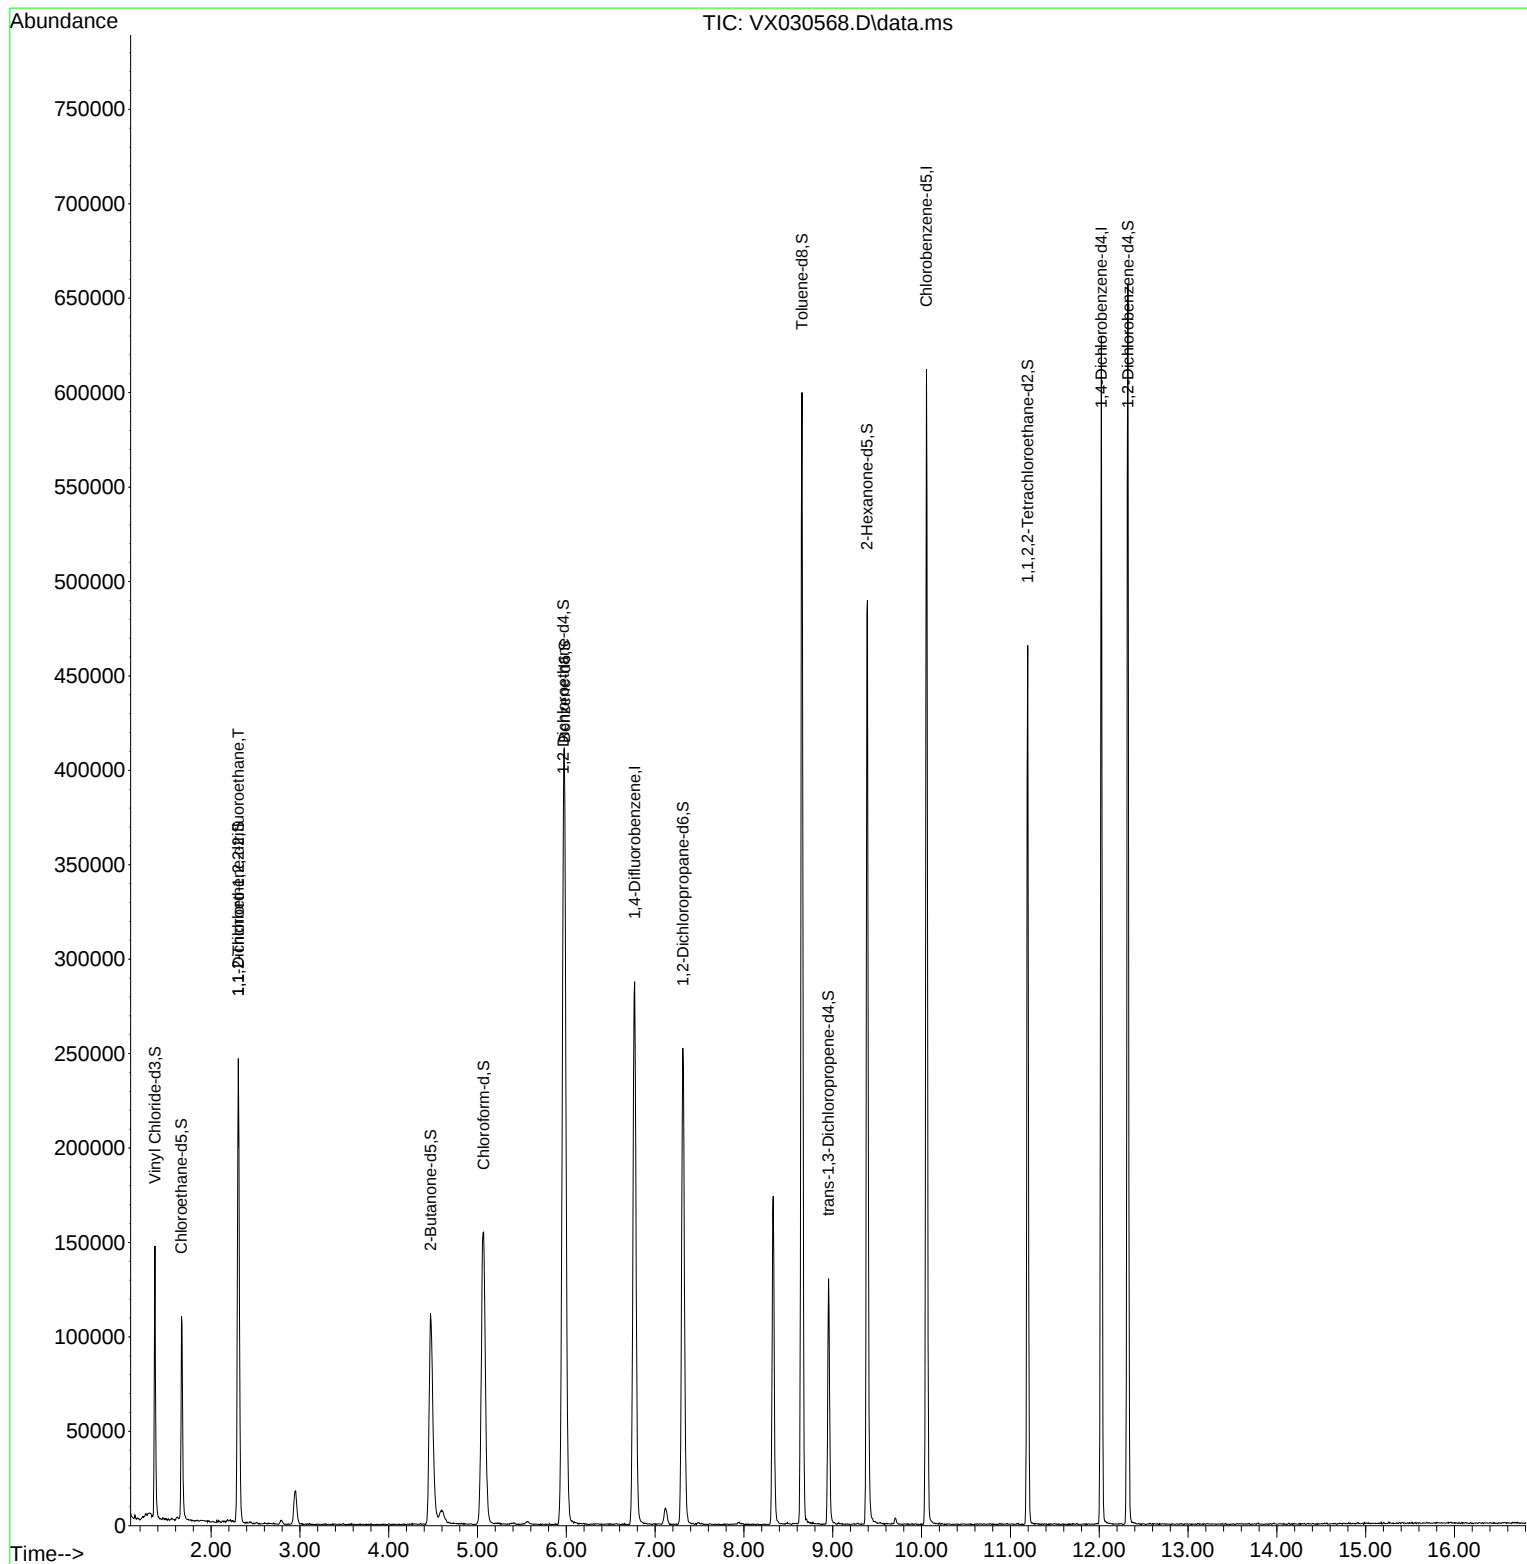

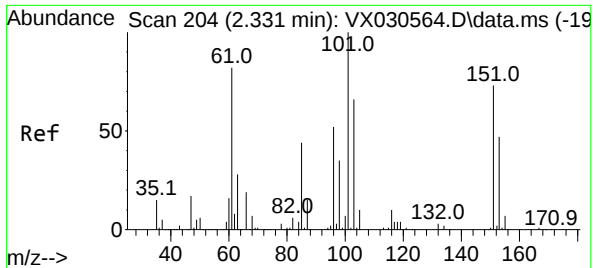

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.838 ug/L
 RT: 2.307 min Scan# 20
 Delta R.T. -0.024 min
 Lab File: VX030568.D
 Acq: 11 Aug 2022 13:09

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK668

Tgt Ion:101 Resp: 1441
 Ion Ratio Lower Upper
 101 100
 85 5.2 35.3 52.9#
 151 0.0 58.3 87.5#

