

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030574.D
 Acq On : 11 Aug 2022 15:30
 Operator : JC/MD
 Sample : VIBLK671
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK671

Quant Time: Aug 12 04:19:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 12 04:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	253869	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	228169	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	104492	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	79584	48.815	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	97.640%	
7) Chloroethane-d5	1.666	69	65627	57.103	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	114.200%	
11) 1,1-Dichloroethene-d2	2.306	63	125635	40.739	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.480%	
21) 2-Butanone-d5	4.477	46	194142	128.523	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	128.520%	
24) Chloroform-d	5.062	84	192521	57.366	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	114.740%	
26) 1,2-Dichloroethane-d4	5.964	65	137979	60.550	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	121.100%	
32) Benzene-d6	5.982	84	362075	55.399	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	110.800%	
36) 1,2-Dichloropropane-d6	7.318	67	122663	57.846	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	115.700%	
41) Toluene-d8	8.653	98	325591	52.849	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.700%	
43) trans-1,3-Dichloroprop...	8.951	79	54845	51.990	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	103.980%	
47) 2-Hexanone-d5	9.390	63	127761	118.203	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	118.200%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	165534	59.424	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	118.840%	
66) 1,2-Dichlorobenzene-d4	12.323	152	117736	58.091	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	116.180%	
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	4.495	96	1965	1.061	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030574.D
Acq On : 11 Aug 2022 15:30
Operator : JC/MD
Sample : VIBLK671
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK671

Quant Time: Aug 12 04:19:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 04:17:17 2022
Response via : Initial Calibration

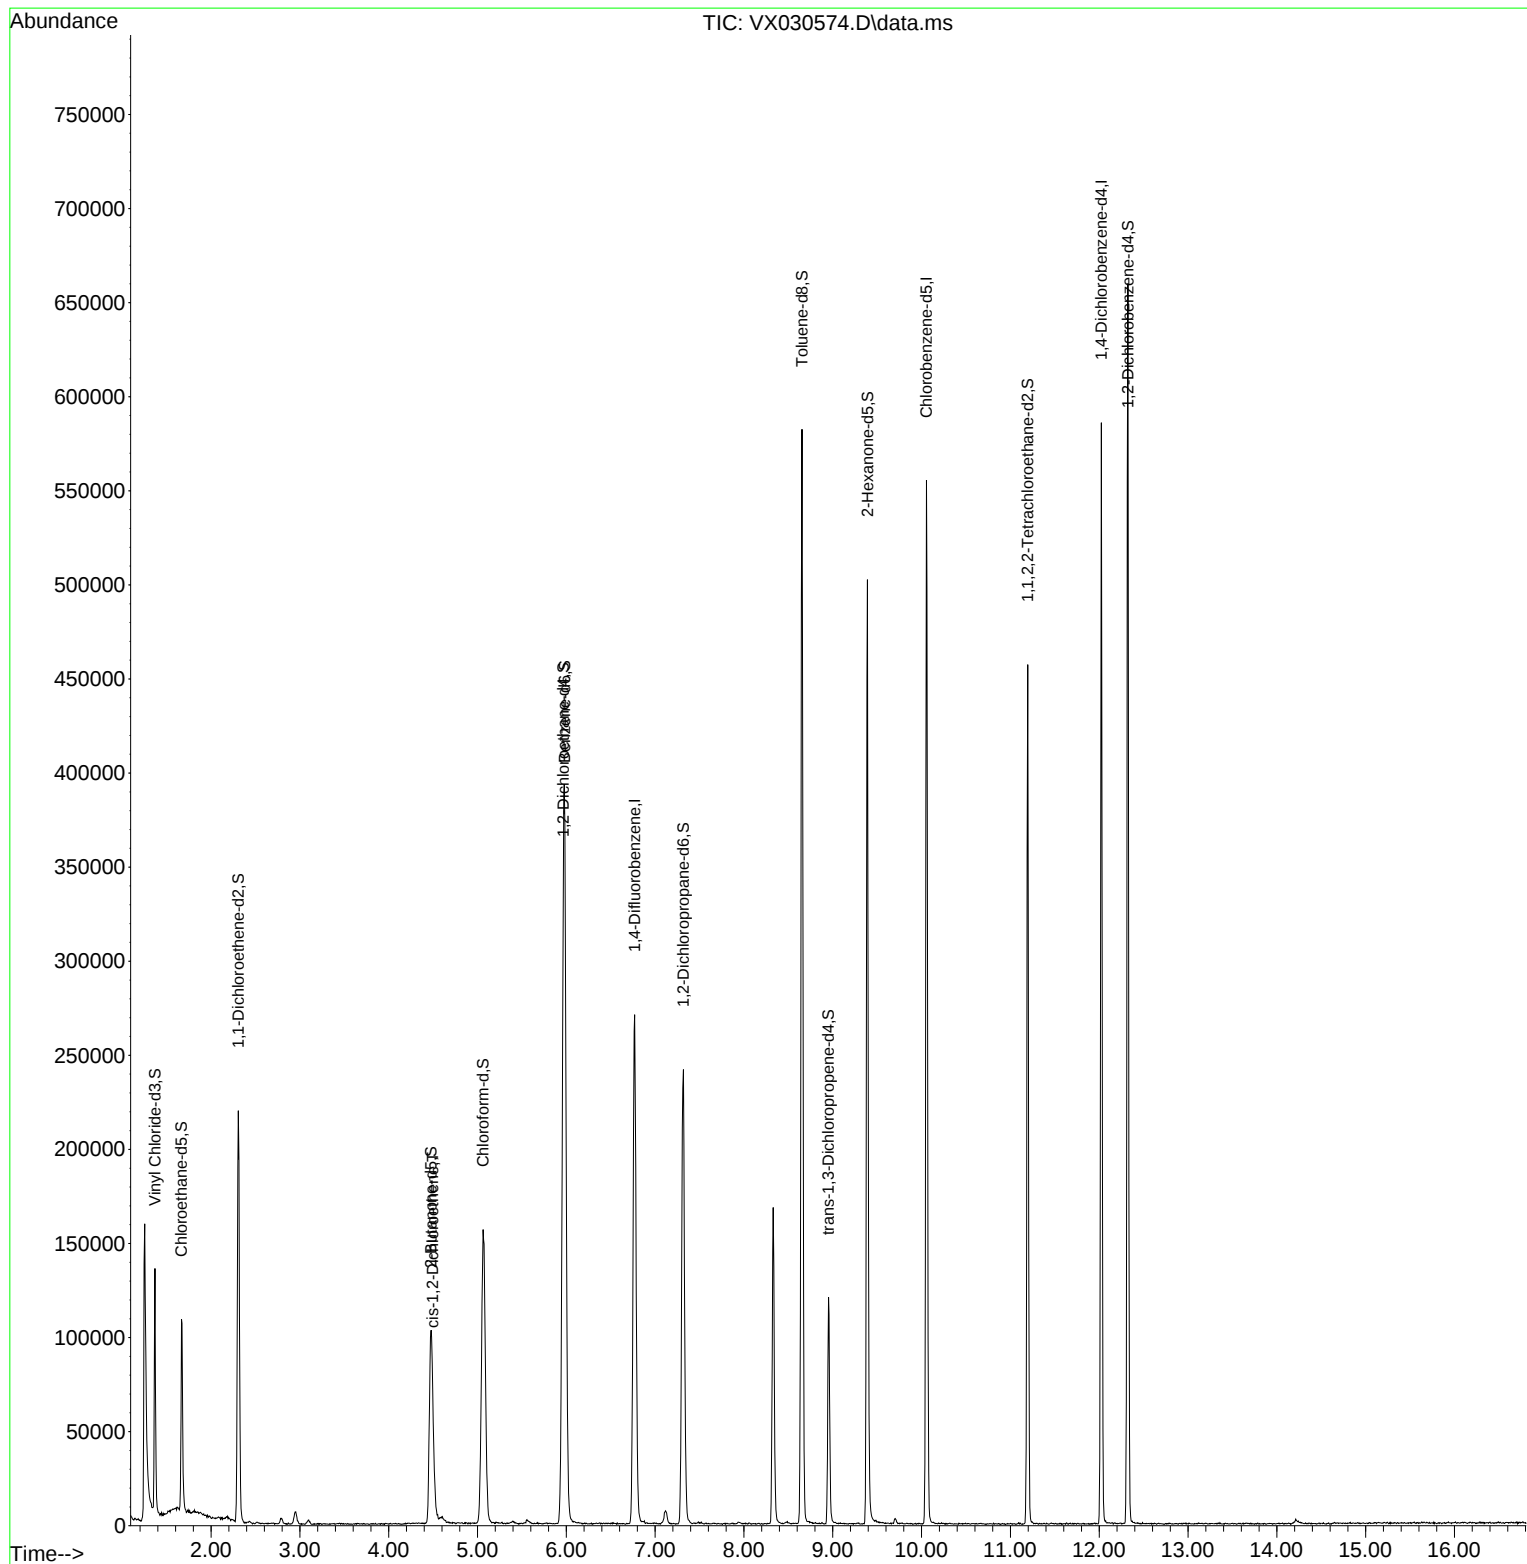

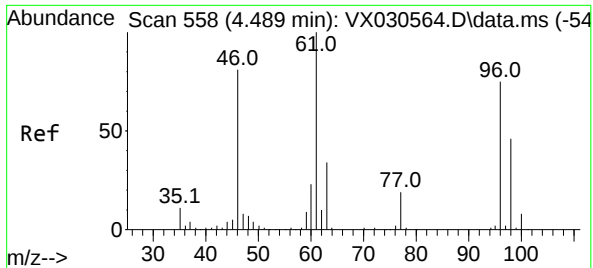

#20
 cis-1,2-Dichloroethene
 Concen: 1.061 ug/L
 RT: 4.495 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VX030574.D
 Acq: 11 Aug 2022 15:30

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK671

Tgt Ion: 96 Resp: 1965

Ion	Ratio	Lower	Upper
96	100		
61	101.8	94.0	174.6
68	0.0	0.0	0.0

