

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030567.D
 Acq On : 11 Aug 2022 12:46
 Operator : JC/MD
 Sample : N4114-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	202980	224017	18.65%	2.341%
2	1.666	91	95	104	rVB	107321	139168	11.58%	1.454%
3	2.306	194	200	210	rVB	248655	373168	31.06%	3.899%
4	2.495	229	231	232	rBV2	777	628	0.05%	0.007%
5	2.788	275	279	285	rVB5	1758	2829	0.24%	0.030%
6	2.947	300	305	306	rBV3	1163	1690	0.14%	0.018%
7	3.093	323	329	339	rVB2	7710	15411	1.28%	0.161%
8	3.160	339	340	343	rBV2	312	368	0.03%	0.004%
9	3.306	362	364	369	rBV2	551	744	0.06%	0.008%
10	3.349	369	371	372	rBV	662	397	0.03%	0.004%
11	3.489	392	394	397	rVV	352	360	0.03%	0.004%
12	3.526	397	400	402	rVB	379	399	0.03%	0.004%
13	3.709	428	430	432	rVV3	392	373	0.03%	0.004%
14	4.044	483	485	487	rBV2	440	398	0.03%	0.004%
15	4.324	528	531	533	rVB2	659	693	0.06%	0.007%
16	4.391	539	542	546	rBV3	602	892	0.07%	0.009%
17	4.489	546	558	572	rBV2	272142	848878	70.66%	8.870%
18	4.800	607	609	613	rVB3	481	597	0.05%	0.006%
19	4.843	613	616	619	rVB3	628	908	0.08%	0.009%
20	4.879	619	622	624	rBV2	495	542	0.05%	0.006%
21	5.068	641	653	665	rBV2	158204	493672	41.09%	5.158%
22	5.391	702	706	713	rVB4	983	1972	0.16%	0.021%
23	5.538	728	730	732	rBV3	582	469	0.04%	0.005%
24	5.855	781	782	784	rBV2	487	437	0.04%	0.005%
25	5.970	787	801	819	rBV3	406057	1201320	100.00%	12.552%
26	6.251	844	847	850	rVV4	630	953	0.08%	0.010%
27	6.306	852	856	858	rBV2	512	651	0.05%	0.007%
28	6.635	908	910	912	rVB2	446	357	0.03%	0.004%
29	6.653	912	913	915	rBV	376	368	0.03%	0.004%
30	6.763	921	931	945	rBV	274411	652523	54.32%	6.818%
31	6.915	954	956	958	rVB3	539	491	0.04%	0.005%
32	7.110	981	988	996	rVB4	8717	19756	1.64%	0.206%
33	7.312	1010	1021	1035	rBV	252334	555502	46.24%	5.804%
34	7.470	1045	1047	1050	rBV4	882	1212	0.10%	0.013%
35	7.781	1096	1098	1101	rBV3	315	360	0.03%	0.004%
36	7.885	1114	1115	1119	rBV2	576	667	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030567.D
 Acq On : 11 Aug 2022 12:46
 Operator : JC/MD
 Sample : N4114-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.940	1119	1124	1126	rBV4	1682	2087	0.17%	0.022%
38	8.086	1145	1148	1151	rBV	421	591	0.05%	0.006%
39	8.153	1158	1159	1162	rBV2	366	358	0.03%	0.004%
40	8.183	1162	1164	1169	rVB	410	457	0.04%	0.005%

41	8.263	1174	1177	1180	rBV2	450	738	0.06%	0.008%
42	8.330	1180	1188	1198	rBV	171969	289821	24.13%	3.028%
43	8.482	1211	1213	1216	rBV2	812	895	0.07%	0.009%
44	8.653	1232	1241	1250	rBV	596906	932132	77.59%	9.740%
45	8.952	1284	1290	1303	rBV	130488	193849	16.14%	2.026%

46	9.116	1315	1317	1319	rVB3	688	436	0.04%	0.005%
47	9.232	1334	1336	1338	rBV	545	564	0.05%	0.006%
48	9.275	1341	1343	1346	rVB	491	364	0.03%	0.004%
49	9.311	1346	1349	1352	rVB3	775	1144	0.10%	0.012%
50	9.342	1352	1354	1355	rBV	418	372	0.03%	0.004%

51	9.391	1355	1362	1376	rBV	474831	692964	57.68%	7.241%
52	9.695	1410	1412	1415	rBV2	453	473	0.04%	0.005%
53	9.897	1443	1445	1449	rBV2	310	408	0.03%	0.004%
54	9.994	1459	1461	1463	rBV2	482	453	0.04%	0.005%
55	10.055	1465	1471	1482	rBV	571295	774276	64.45%	8.090%

56	10.165	1487	1489	1490	rBV	698	414	0.03%	0.004%
57	10.305	1510	1512	1514	rBV2	393	368	0.03%	0.004%
58	10.384	1521	1525	1527	rBV3	370	516	0.04%	0.005%
59	10.561	1552	1554	1556	rBV	490	375	0.03%	0.004%
60	10.579	1556	1557	1561	rVB2	442	470	0.04%	0.005%

61	10.610	1561	1562	1564	rBV	760	395	0.03%	0.004%
62	10.713	1577	1579	1580	rBV2	570	498	0.04%	0.005%
63	10.945	1616	1617	1619	rVV	480	340	0.03%	0.004%
64	10.994	1622	1625	1627	rVV3	362	351	0.03%	0.004%
65	11.055	1633	1635	1637	rBV2	268	357	0.03%	0.004%

66	11.195	1652	1658	1671	rVV	465323	573568	47.74%	5.993%
67	11.634	1725	1730	1731	rBV2	535	897	0.07%	0.009%
68	11.762	1748	1751	1753	rVV3	507	442	0.04%	0.005%
69	11.805	1755	1758	1759	rBV2	439	350	0.03%	0.004%
70	11.829	1759	1762	1765	rVB3	396	505	0.04%	0.005%

71	11.908	1772	1775	1776	rBV2	415	415	0.03%	0.004%
72	12.024	1789	1794	1803	rVB	591290	720094	59.94%	7.524%
73	12.323	1837	1843	1855	rBV	639528	819760	68.24%	8.566%
74	12.500	1870	1872	1873	rBV2	503	469	0.04%	0.005%
75	12.707	1903	1906	1908	rBV	437	358	0.03%	0.004%

76	12.945	1942	1945	1947	rVV2	379	500	0.04%	0.005%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030567.D
 Acq On : 11 Aug 2022 12:46
 Operator : JC/MD
 Sample : N4114-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.012	1954	1956	1958	rBV	433	460	0.04%	0.005%
78	13.073	1963	1966	1968	rVB	454	484	0.04%	0.005%
79	13.097	1968	1970	1972	rBV	518	479	0.04%	0.005%
80	13.122	1972	1974	1977	rVV	443	404	0.03%	0.004%
81	13.201	1984	1987	1990	rBV2	474	620	0.05%	0.006%
82	13.268	1996	1998	2000	rVB	468	345	0.03%	0.004%
83	13.542	2041	2043	2045	rVB	633	339	0.03%	0.004%
84	13.597	2049	2052	2055	rVV3	627	746	0.06%	0.008%
85	13.652	2058	2061	2062	rBV	589	563	0.05%	0.006%
86	13.731	2072	2074	2078	rBV	433	473	0.04%	0.005%
87	13.780	2078	2082	2084	rVV2	692	825	0.07%	0.009%
88	13.859	2093	2095	2098	rVB	493	441	0.04%	0.005%
89	13.884	2098	2099	2102	rBV2	415	504	0.04%	0.005%
90	14.085	2130	2132	2136	rBV3	500	722	0.06%	0.008%
91	14.268	2161	2162	2164	rBV	608	352	0.03%	0.004%
92	14.402	2182	2184	2187	rVB2	521	573	0.05%	0.006%
93	14.475	2194	2196	2200	rBV2	462	634	0.05%	0.007%
94	14.512	2200	2202	2205	rVB2	485	575	0.05%	0.006%
95	14.560	2208	2210	2211	rBV	630	397	0.03%	0.004%
96	14.737	2238	2239	2243	rVB4	711	545	0.05%	0.006%
97	14.768	2243	2244	2248	rBV2	523	561	0.05%	0.006%
98	14.816	2250	2252	2253	rVB	662	346	0.03%	0.004%
99	14.938	2269	2272	2274	rBV2	1003	1151	0.10%	0.012%
100	15.389	2344	2346	2349	rVB4	926	889	0.07%	0.009%




Sum of corrected areas: 9570422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030567.D
Acq On : 11 Aug 2022 12:46
Operator : JC/MD
Sample : N4114-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

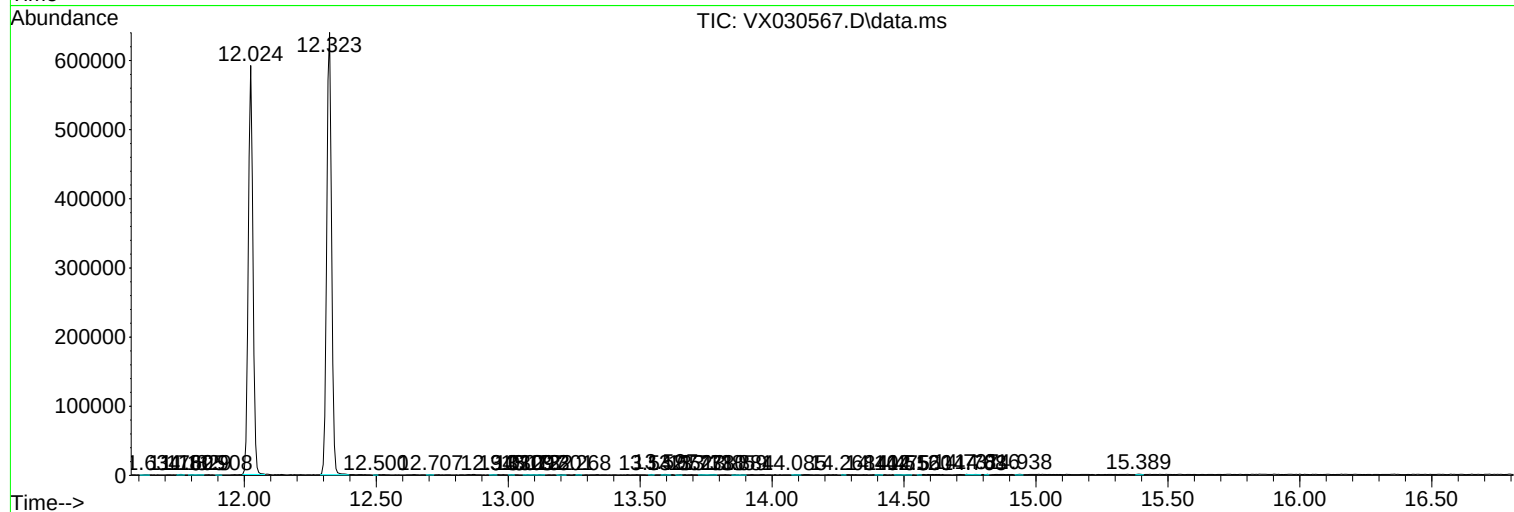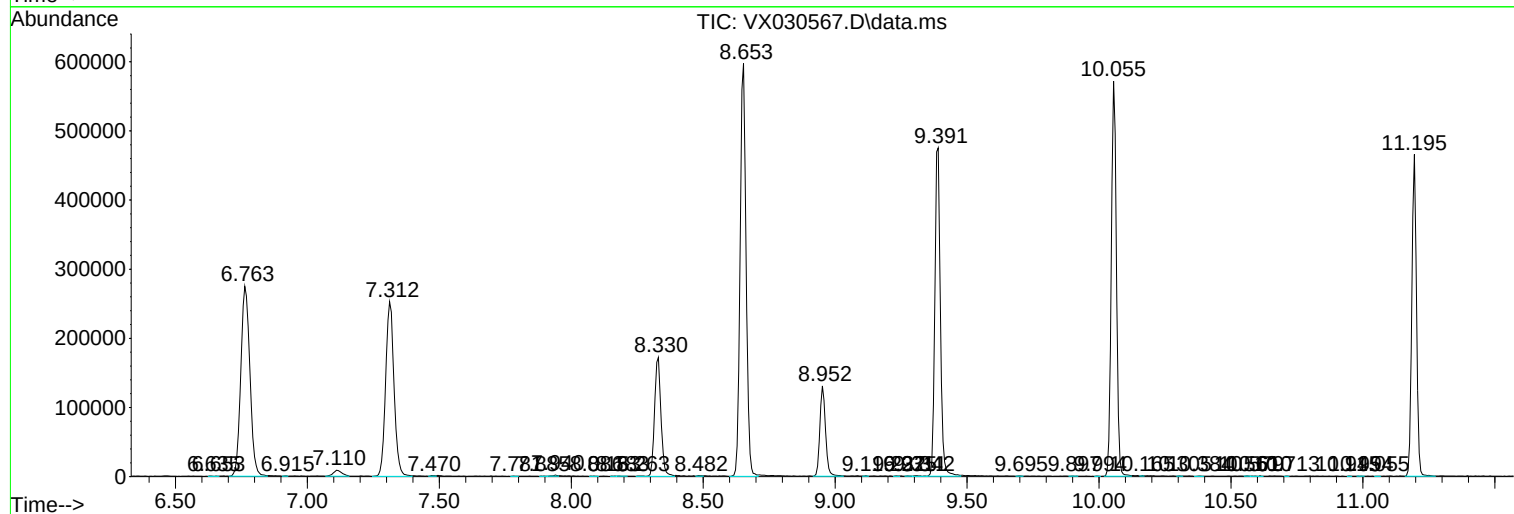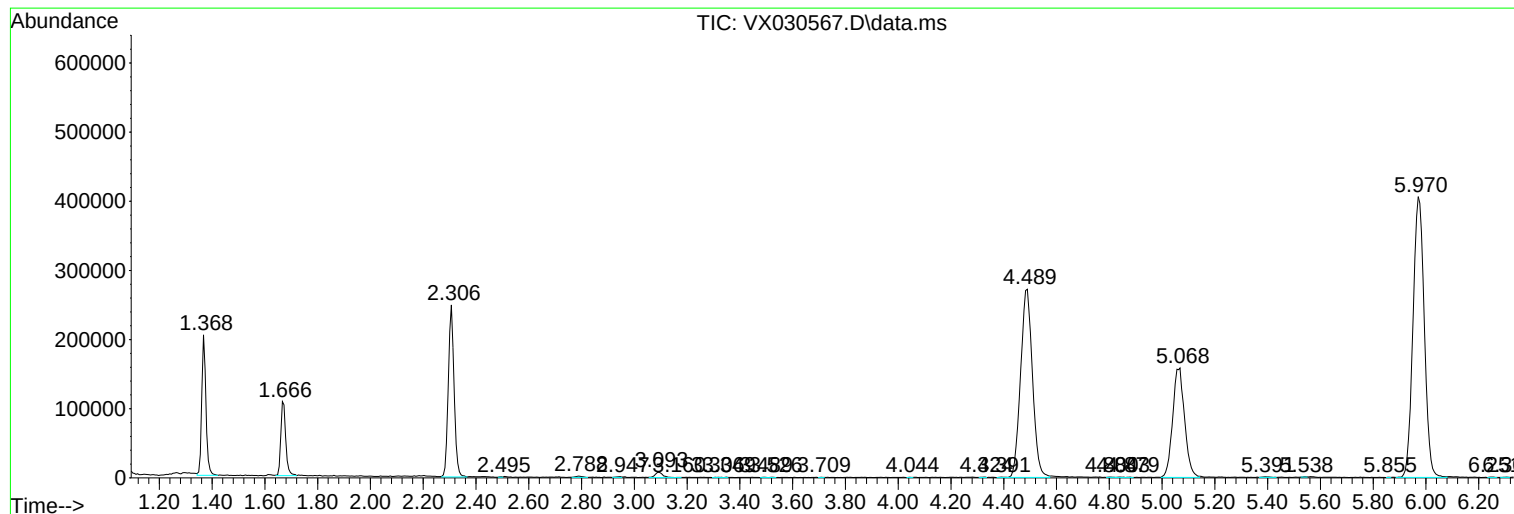

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030567.D
Acq On : 11 Aug 2022 12:46
Operator : JC/MD
Sample : N4114-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030567.D
Acq On : 11 Aug 2022 12:46
Operator : JC/MD
Sample : N4114-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc