

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030568.D
 Acq On : 11 Aug 2022 13:09
 Operator : JC/MD
 Sample : VIBLK668
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	144568	144230	11.91%	1.569%
2	1.666	91	95	106	rVB	107573	136050	11.23%	1.480%
3	2.063	159	160	161	rBV	975	453	0.04%	0.005%
4	2.307	194	200	212	rVB	246031	372001	30.71%	4.047%
5	2.483	227	229	230	rBV	494	310	0.03%	0.003%
6	2.544	237	239	240	rVB2	558	348	0.03%	0.004%
7	2.599	247	248	253	rVB4	694	828	0.07%	0.009%
8	2.642	253	255	256	rBV2	561	377	0.03%	0.004%
9	2.794	275	280	286	rVB4	2174	4314	0.36%	0.047%
10	2.947	297	305	313	rVV	17583	41269	3.41%	0.449%
11	3.105	329	331	334	rVV2	606	487	0.04%	0.005%
12	3.264	355	357	359	rVB2	473	378	0.03%	0.004%
13	3.447	385	387	388	rBV	486	392	0.03%	0.004%
14	3.544	400	403	405	rBV2	453	463	0.04%	0.005%
15	3.562	405	406	408	rVV	500	432	0.04%	0.005%
16	3.605	411	413	415	rVB	456	361	0.03%	0.004%
17	3.794	442	444	449	rVB2	417	438	0.04%	0.005%
18	3.867	454	456	458	rVB2	378	280	0.02%	0.003%
19	3.971	472	473	476	rBV2	314	354	0.03%	0.004%
20	4.001	476	478	482	rVB3	592	732	0.06%	0.008%
21	4.044	482	485	487	rBV2	363	443	0.04%	0.005%
22	4.471	546	555	569	rBV	111782	332636	27.46%	3.619%
23	4.794	607	608	610	rBV2	503	391	0.03%	0.004%
24	4.861	617	619	620	rBV2	406	348	0.03%	0.004%
25	5.068	639	653	671	rBV2	154781	495882	40.94%	5.394%
26	5.379	701	704	705	rBV3	619	725	0.06%	0.008%
27	5.513	724	726	728	rBV4	536	519	0.04%	0.006%
28	5.556	728	733	734	rBV3	1294	1745	0.14%	0.019%
29	5.727	759	761	766	rBV2	427	744	0.06%	0.008%
30	5.812	773	775	778	rVB3	576	454	0.04%	0.005%
31	5.977	790	802	819	rBV2	410449	1211169	100.00%	13.175%
32	6.092	819	821	823	rBV2	688	522	0.04%	0.006%
33	6.275	847	851	852	rBV	363	467	0.04%	0.005%
34	6.629	908	909	911	rBV2	470	318	0.03%	0.003%
35	6.653	911	913	914	rVB	728	376	0.03%	0.004%
36	6.672	914	916	920	rBV	318	282	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030568.D
 Acq On : 11 Aug 2022 13:09
 Operator : JC/MD
 Sample : VIBLK668
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	922	932	949	rBV	287437	702584	58.01%	7.643%
38	6.983	965	967	970	rBV2	594	749	0.06%	0.008%
39	7.031	972	975	976	rBV	470	530	0.04%	0.006%
40	7.117	981	989	997	rVV5	8767	21895	1.81%	0.238%
41	7.172	997	998	1001	rVB	465	320	0.03%	0.003%
42	7.312	1011	1021	1038	rBV	252545	560188	46.25%	6.094%
43	7.482	1046	1049	1053	rBV4	1049	1763	0.15%	0.019%
44	7.610	1068	1070	1074	rBV3	395	537	0.04%	0.006%
45	7.775	1095	1097	1100	rBV	559	541	0.04%	0.006%
46	7.946	1120	1125	1127	rBV5	1070	1585	0.13%	0.017%
47	8.025	1137	1138	1140	rBV2	411	345	0.03%	0.004%
48	8.159	1157	1160	1161	rBV2	377	423	0.03%	0.005%
49	8.226	1166	1171	1172	rBV	478	638	0.05%	0.007%
50	8.330	1181	1188	1200	rBV	173698	291544	24.07%	3.172%
51	8.549	1222	1224	1227	rBV	704	964	0.08%	0.010%
52	8.653	1234	1241	1248	rBV	598823	928828	76.69%	10.104%
53	8.769	1258	1260	1261	rBV	679	350	0.03%	0.004%
54	8.952	1285	1290	1299	rBV	129901	193453	15.97%	2.104%
55	9.068	1306	1309	1310	rBV2	851	690	0.06%	0.008%
56	9.391	1356	1362	1374	rBV	488939	720226	59.47%	7.835%
57	9.665	1405	1407	1410	rBV	565	502	0.04%	0.005%
58	9.702	1410	1413	1420	rVB3	3279	5059	0.42%	0.055%
59	9.805	1428	1430	1434	rBV	302	306	0.03%	0.003%
60	9.933	1448	1451	1453	rBV3	379	477	0.04%	0.005%
61	10.055	1465	1471	1485	rBV	611617	829003	68.45%	9.018%
62	10.201	1493	1495	1498	rVB3	764	586	0.05%	0.006%
63	10.262	1504	1505	1507	rBV	557	333	0.03%	0.004%
64	10.287	1507	1509	1511	rBV2	515	428	0.04%	0.005%
65	10.384	1523	1525	1528	rBV	302	293	0.02%	0.003%
66	10.634	1564	1566	1568	rBV	382	357	0.03%	0.004%
67	10.695	1574	1576	1577	rBV	390	288	0.02%	0.003%
68	10.878	1603	1606	1607	rBV	592	529	0.04%	0.006%
69	11.128	1645	1647	1650	rVB2	345	358	0.03%	0.004%
70	11.195	1652	1658	1666	rVV	465352	580582	47.94%	6.316%
71	11.543	1713	1715	1716	rBV	493	421	0.03%	0.005%
72	11.579	1719	1721	1724	rVB2	446	509	0.04%	0.006%
73	11.622	1726	1728	1731	rVB2	446	489	0.04%	0.005%
74	11.659	1731	1734	1735	rBV2	609	541	0.04%	0.006%
75	11.878	1768	1770	1773	rBV	282	290	0.02%	0.003%
76	11.976	1784	1786	1789	rBV2	385	321	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030568.D
 Acq On : 11 Aug 2022 13:09
 Operator : JC/MD
 Sample : VIBLK668
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1801	rVV	628508	751280	62.03%	8.173%
78	12.323	1837	1843	1851	rBV	656832	826660	68.25%	8.993%
79	12.445	1861	1863	1866	rVB3	651	595	0.05%	0.006%
80	12.603	1887	1889	1890	rVB	651	410	0.03%	0.004%
81	12.622	1890	1892	1895	rBV2	576	844	0.07%	0.009%
82	12.762	1913	1915	1917	rBV	368	338	0.03%	0.004%
83	13.122	1970	1974	1975	rBV2	592	638	0.05%	0.007%
84	13.219	1986	1990	1991	rBV3	456	570	0.05%	0.006%
85	13.555	2043	2045	2047	rVV2	416	331	0.03%	0.004%
86	13.792	2080	2084	2085	rBV3	726	899	0.07%	0.010%
87	13.926	2104	2106	2109	rVB2	515	532	0.04%	0.006%
88	13.969	2109	2113	2120	rBV4	818	1542	0.13%	0.017%
89	14.140	2138	2141	2143	rBV2	719	725	0.06%	0.008%
90	14.170	2143	2146	2147	rBV	492	396	0.03%	0.004%
91	14.256	2158	2160	2161	rVB	622	369	0.03%	0.004%
92	14.469	2194	2195	2197	rBV	496	441	0.04%	0.005%
93	14.688	2229	2231	2233	rBV2	515	624	0.05%	0.007%
94	14.810	2249	2251	2253	rVB2	635	360	0.03%	0.004%
95	14.987	2278	2280	2281	rBV	1032	769	0.06%	0.008%
96	15.176	2310	2311	2312	rVB	902	330	0.03%	0.004%
97	15.207	2312	2316	2317	rBV2	831	862	0.07%	0.009%
98	15.262	2323	2325	2326	rBV2	731	337	0.03%	0.004%
99	15.377	2342	2344	2347	rVB3	616	585	0.05%	0.006%
100	16.658	2552	2554	2557	rBV3	724	826	0.07%	0.009%




Sum of corrected areas: 9192606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030568.D
Acq On : 11 Aug 2022 13:09
Operator : JC/MD
Sample : VIBLK668
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

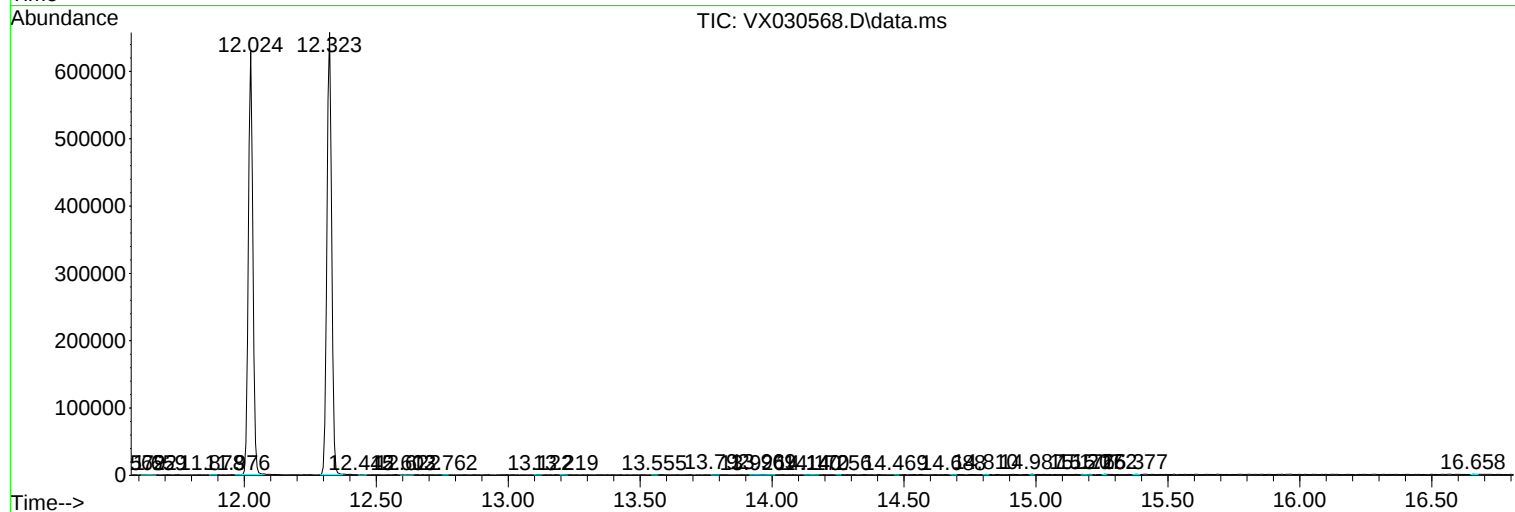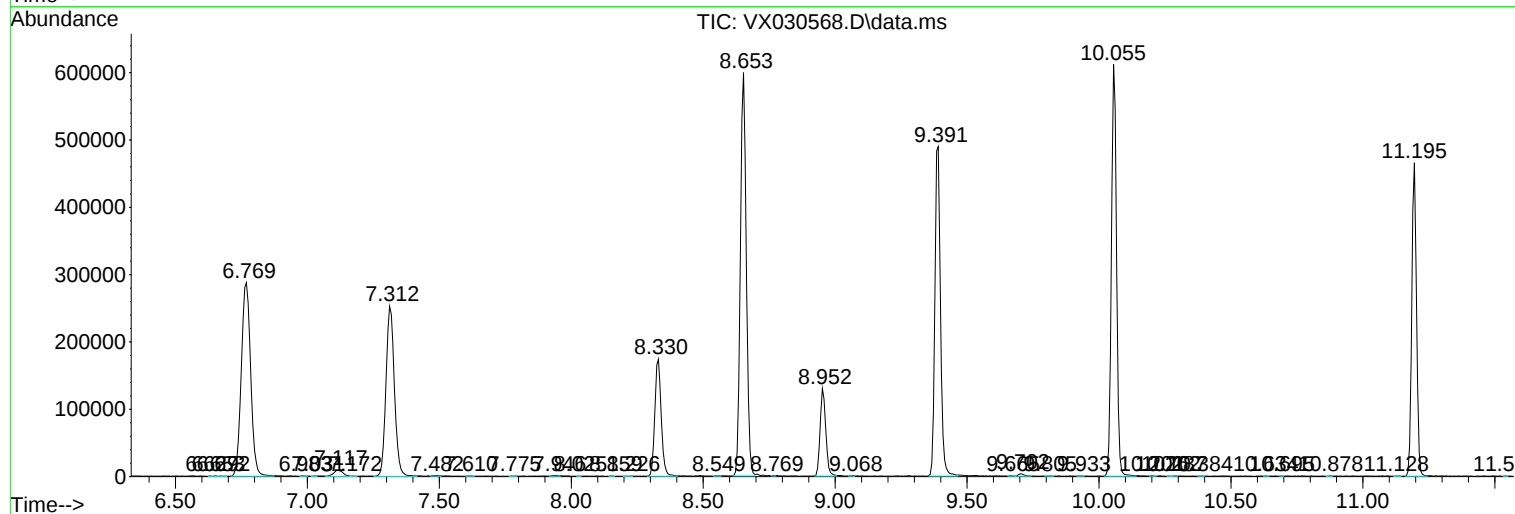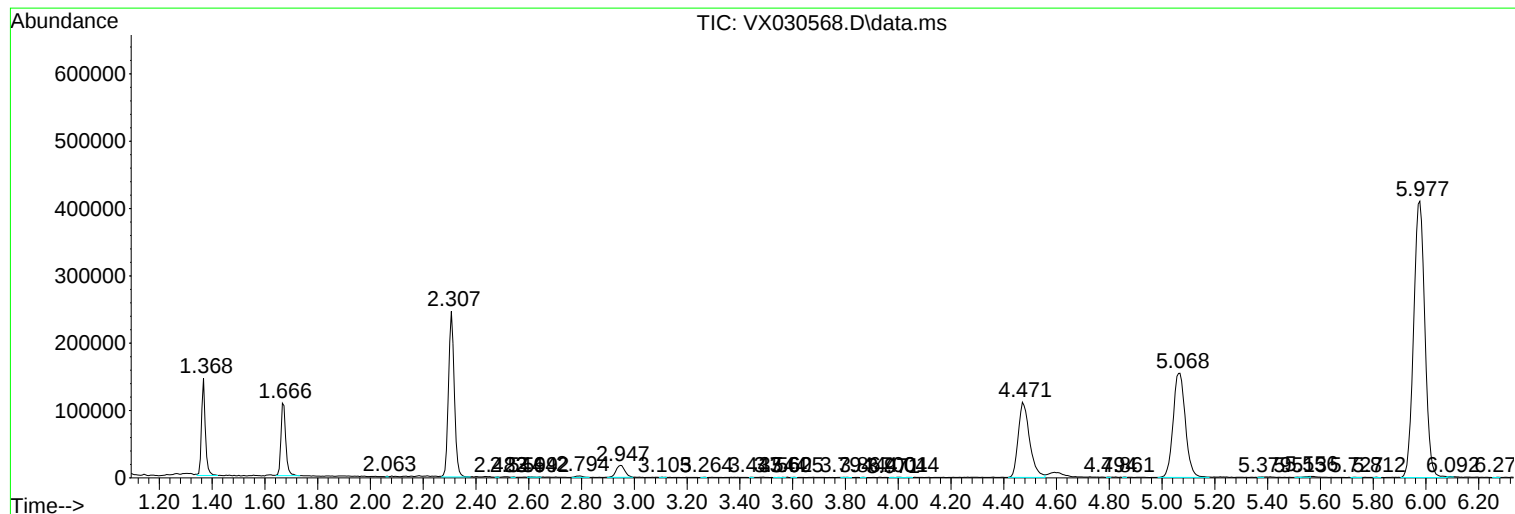

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030568.D
Acq On : 11 Aug 2022 13:09
Operator : JC/MD
Sample : VIBLK668
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
Data File : VX030568.D
Acq On : 11 Aug 2022 13:09
Operator : JC/MD
Sample : VIBLK668
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc