
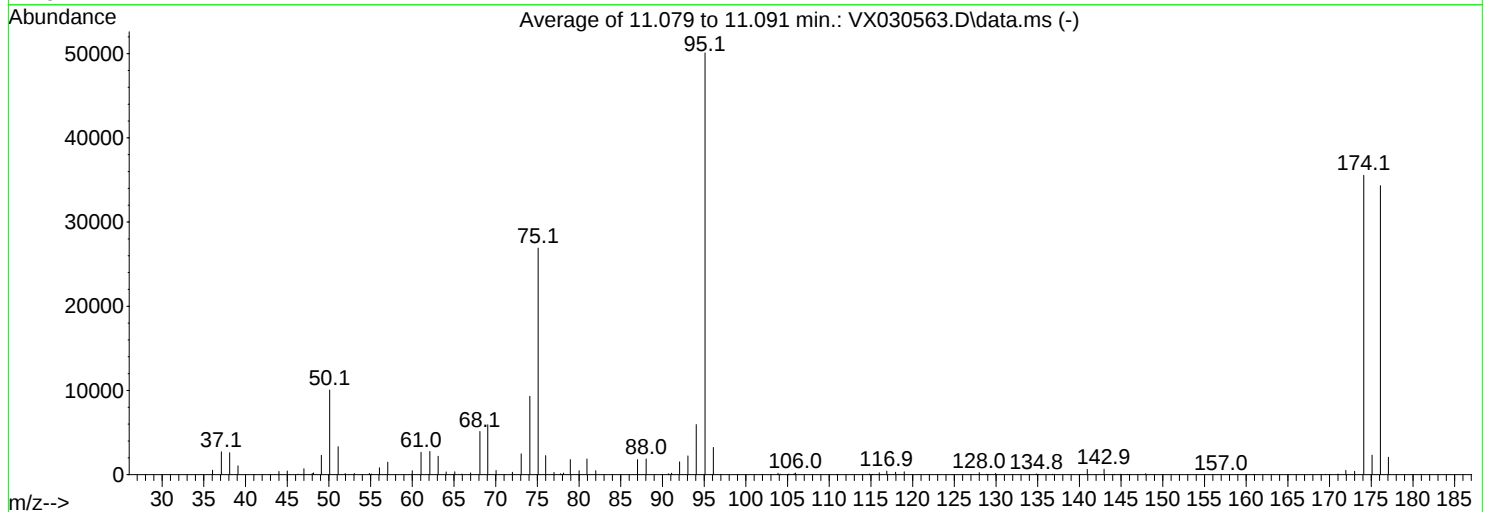


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081122\
 Data File : VX030563.D
 Acq On : 11 Aug 2022 08:48
 Operator : JC/MD
 Sample : BFB676
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB676

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 12 04:17:17 2022

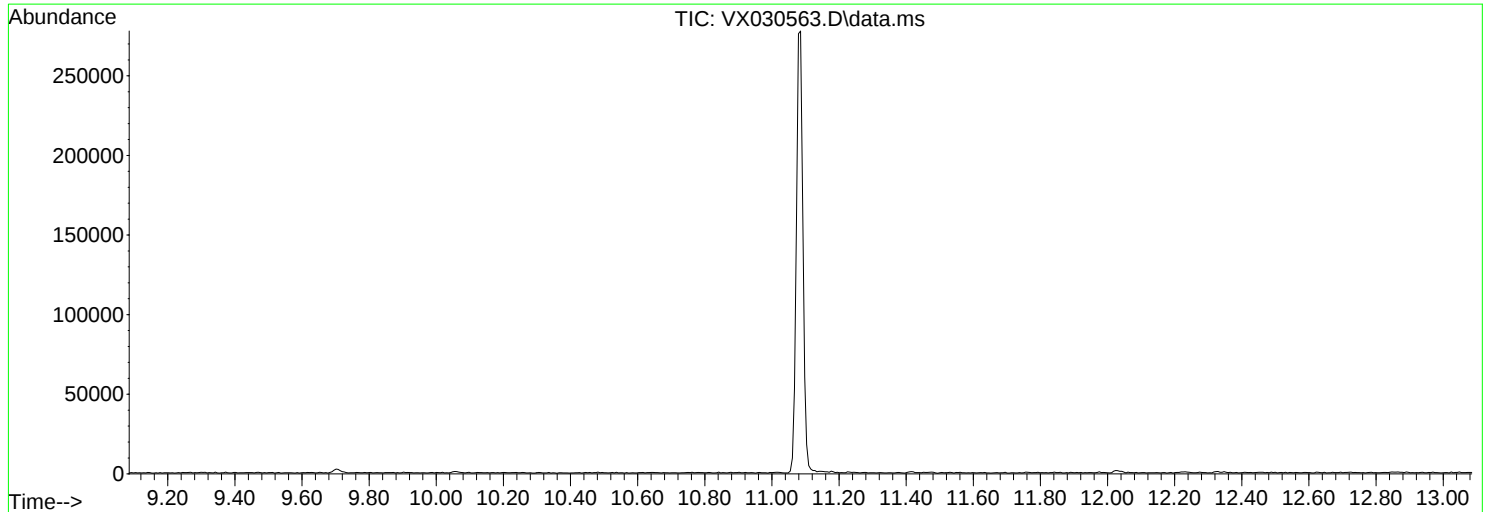

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10047	PASS
75	95	30	80	53.7	26904	PASS
95	95	100	100	100.0	50096	PASS
96	95	5	9	6.5	3239	PASS
173	174	0.00	2	1.1	394	PASS
174	95	50	120	71.0	35565	PASS
175	174	5	9	6.5	2329	PASS
176	174	95	101	96.5	34317	PASS
177	176	5	9	6.0	2068	PASS

Scan 1633 (11.043 min): VX030563.D\data.ms
BFB676

m/z	Abundance
39.00	58.0
40.00	357.0
44.00	230.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.10	747.0
37.10	3646.0
38.10	3503.0
39.20	1378.0
39.90	379.0
44.00	676.0
45.10	525.0
46.30	57.0
47.10	915.0
48.00	417.0
49.10	3198.0
50.10	12231.0
51.10	4288.0
52.00	111.0
53.10	85.0
55.10	256.0
56.10	1141.0
57.10	1703.0
60.00	615.0
61.00	3043.0
62.10	3412.0
63.10	2646.0
64.10	304.0
65.10	381.0
66.00	58.0
67.10	201.0
68.10	6238.0
69.10	7152.0
70.10	540.0
72.00	292.0
73.00	3151.0
74.10	10781.0
75.10	32704.0
76.00	2760.0
77.00	338.0
78.10	420.0
79.00	2142.0
80.00	695.0
80.90	2398.0
81.90	539.0
87.00	1971.0
88.00	2378.0
90.70	165.0
91.10	392.0
92.00	2061.0
93.10	2843.0
94.10	6844.0
95.10	58152.0
96.10	3976.0
97.00	51.0
103.80	340.0
105.10	105.0
105.80	337.0
114.90	55.0
116.10	277.0
116.90	553.0
117.90	379.0
119.10	321.0
128.00	239.0
129.10	89.0
130.00	108.0
134.80	146.0
135.10	148.0
136.80	156.0
141.00	743.0
142.90	567.0
144.90	80.0
145.80	72.0
147.90	137.0
155.00	64.0
157.00	94.0
169.50	92.0
171.00	108.0
172.00	492.0
173.00	272.0
174.10	36464.0
175.10	2347.0
176.10	34344.0
177.00	2378.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.00	613.0
37.10	2737.0
38.10	2959.0
39.10	1166.0
40.00	491.0
44.10	683.0
45.00	512.0
46.30	79.0
47.00	600.0
48.20	430.0
49.10	2308.0
50.10	11993.0
51.10	3477.0
51.90	169.0
53.00	171.0
54.80	332.0
56.00	871.0
57.00	1943.0
60.00	475.0
61.10	3153.0
62.10	3335.0
63.10	2379.0
64.10	384.0
65.10	357.0
66.00	93.0
66.90	264.0
68.10	5697.0
69.00	6514.0
70.00	640.0
71.00	62.0
72.00	365.0
73.10	2625.0
74.10	11268.0
75.10	30856.0
76.00	2569.0
77.10	296.0
77.80	174.0
78.90	1963.0
80.00	421.0
81.00	2050.0
82.00	568.0
87.00	1941.0
88.10	2224.0
90.80	158.0
92.10	1412.0
93.10	2016.0
94.00	7056.0
95.10	58552.0
96.10	3688.0
97.00	89.0
104.10	233.0
105.20	56.0
106.00	269.0
114.80	86.0
115.90	208.0
116.90	444.0
117.90	274.0
119.00	402.0
128.00	327.0
128.80	107.0
129.90	225.0
134.90	93.0
137.00	152.0
140.10	54.0
140.90	566.0
143.00	923.0
144.20	55.0
144.90	106.0
145.80	68.0
148.00	224.0
160.90	85.0
171.00	124.0
172.00	602.0
173.00	624.0
174.10	40648.0
175.10	2982.0
176.10	40984.0
177.10	2059.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676

m/z	Abundance
36.10	258.0
37.10	1766.0
38.10	1343.0
39.10	767.0
40.10	287.0
41.10	62.0
43.00	63.0
44.00	489.0
44.90	301.0
46.30	57.0
46.90	576.0
48.10	227.0
49.10	1407.0
50.10	5918.0
51.10	2218.0
51.90	99.0
53.00	131.0
54.90	123.0
56.10	445.0
57.00	826.0
60.10	317.0
61.00	1780.0
62.00	1498.0
63.10	1560.0
63.90	281.0
65.10	291.0
65.90	69.0
67.00	148.0
68.00	3458.0
69.10	4118.0
70.10	284.0
72.00	191.0
73.00	1622.0
74.10	5901.0
75.10	17152.0
76.00	1464.0
76.90	140.0
77.80	188.0
78.20	164.0
78.90	1286.0
80.10	310.0
81.00	1153.0
82.10	335.0
87.00	1441.0
88.10	1004.0
91.10	103.0
92.10	1081.0
93.00	1800.0
94.00	3961.0
95.10	33584.0
96.00	2052.0
103.90	165.0
105.20	86.0
105.90	282.0
110.90	56.0
114.80	77.0
115.20	114.0
116.00	196.0
117.00	284.0
118.00	229.0
118.90	316.0
128.00	171.0
128.90	83.0
130.00	133.0
134.90	72.0
141.00	560.0
142.90	450.0
144.20	61.0
145.10	52.0
171.90	433.0
173.10	285.0
174.10	29584.0
175.10	1657.0
176.10	27624.0
177.10	1767.0

Instrument :
MSVOA_X
ClientSampleId :
BFB676