

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081219\
 Data File : VX011520.D
 Acq On : 13 Aug 2019 06:17
 Operator : JC/SP
 Sample : K4279-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0669

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	16	19	22	rBV	9741	12622	1.45%	0.166%
2	1.398	36	40	45	rBV	15457	15982	1.83%	0.210%
3	1.782	97	103	110	rBV	77602	111416	12.76%	1.466%
4	1.995	133	138	148	rVB	32396	47598	5.45%	0.626%
5	2.391	193	203	208	rBV2	17137	36257	4.15%	0.477%
6	2.843	270	277	280	rBV	18983	43278	4.96%	0.570%
7	2.885	280	284	286	rVV2	19815	36096	4.13%	0.475%
8	2.928	286	291	301	rVB	54812	117419	13.44%	1.545%
9	3.166	320	330	342	rBV2	43526	102051	11.68%	1.343%
10	4.397	521	532	546	rVB2	59139	172513	19.75%	2.271%
11	5.495	699	712	719	rBV	107243	307696	35.23%	4.050%
12	5.574	719	725	731	rVV3	52225	160649	18.39%	2.114%
13	5.653	731	738	763	rVB	199999	583921	66.86%	7.686%
14	5.946	775	786	795	rBV10	5883	20898	2.39%	0.275%
15	6.062	795	805	811	rVV	109195	294592	33.73%	3.877%
16	6.135	811	817	830	rVV	218473	574982	65.83%	7.568%
17	6.263	830	838	846	rVV6	6295	24007	2.75%	0.316%
18	6.348	846	852	862	rVV5	7154	22238	2.55%	0.293%
19	6.452	862	869	878	rVB6	6432	17130	1.96%	0.225%
20	6.854	925	935	949	rBV	275955	657031	75.23%	8.648%
21	7.458	1025	1034	1045	rVB3	29661	71924	8.24%	0.947%
22	8.031	1122	1128	1138	rVB6	4370	14575	1.67%	0.192%
23	8.183	1144	1153	1156	rBV4	4623	9952	1.14%	0.131%
24	8.665	1225	1232	1233	rBV3	6557	9136	1.05%	0.120%
25	8.713	1233	1240	1250	rVB	568153	873389	100.00%	11.496%
26	8.835	1255	1260	1265	rVV6	6010	11698	1.34%	0.154%
27	9.037	1288	1293	1301	rVB3	11438	19842	2.27%	0.261%
28	9.677	1393	1398	1403	rBV	7128	9690	1.11%	0.128%
29	10.110	1463	1469	1477	rBV	569748	746433	85.46%	9.825%
30	10.250	1486	1492	1499	rVV	108872	143800	16.46%	1.893%
31	10.353	1501	1509	1515	rVB9	7039	16846	1.93%	0.222%
32	10.640	1549	1556	1563	rBV7	4927	15165	1.74%	0.200%
33	10.835	1578	1588	1593	rBV7	6042	11418	1.31%	0.150%
34	11.018	1612	1618	1628	rVB	75619	101758	11.65%	1.339%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081219\
 Data File : VX011520.D
 Acq On : 13 Aug 2019 06:17
 Operator : JC/SP
 Sample : K4279-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0669

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

35	11.134	1631	1637	1643	rBV	467829	574341	65.76%	7.560%
36	11.274	1652	1660	1664	rBV10	5553	13981	1.60%	0.184%
37	11.359	1668	1674	1680	rVV	81742	107825	12.35%	1.419%
38	11.664	1717	1724	1734	rBV	10816	22413	2.57%	0.295%
39	11.920	1756	1766	1767	rBV8	4390	8794	1.01%	0.116%
40	11.945	1767	1770	1776	rVB	13404	18801	2.15%	0.247%
41	12.073	1786	1791	1797	rBV	518574	670762	76.80%	8.829%
42	12.140	1797	1802	1807	rVV	160503	194855	22.31%	2.565%
43	12.231	1811	1817	1821	rVB	6701	8793	1.01%	0.116%
44	12.298	1821	1828	1835	rBV	69762	92926	10.64%	1.223%
45	12.365	1835	1839	1847	rVB4	13132	23175	2.65%	0.305%
46	12.457	1850	1854	1859	rBV2	13587	18832	2.16%	0.248%
47	12.518	1859	1864	1869	rBV	25937	34819	3.99%	0.458%
48	12.664	1880	1888	1891	rBV2	17347	24266	2.78%	0.319%
49	12.701	1891	1894	1899	rVV3	12708	19359	2.22%	0.255%
50	12.755	1899	1903	1910	rVB3	20091	36836	4.22%	0.485%
51	12.902	1922	1927	1932	rVB2	18183	26597	3.05%	0.350%
52	12.975	1932	1939	1943	rVV	16760	25193	2.88%	0.332%
53	13.341	1995	1999	2004	rVB2	44238	62636	7.17%	0.824%
54	13.475	2014	2021	2032	rVB	24196	36140	4.14%	0.476%
55	13.639	2044	2048	2051	rBV6	7108	10894	1.25%	0.143%
56	13.719	2058	2061	2066	rVB4	9293	13408	1.54%	0.176%
57	13.835	2072	2080	2086	rBV	40231	65803	7.53%	0.866%
58	13.981	2097	2104	2108	rBV3	9381	14392	1.65%	0.189%
59	14.273	2147	2152	2159	rVB6	5141	11211	1.28%	0.148%
60	14.536	2191	2195	2200	rBV2	10561	14716	1.68%	0.194%
61	14.694	2214	2221	2224	rBV2	8140	12753	1.46%	0.168%
62	14.834	2238	2244	2249	rBV2	12771	19043	2.18%	0.251%


Sum of corrected areas: 7597566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081219\
Data File : VX011520.D
Acq On : 13 Aug 2019 06:17
Operator : JC/SP
Sample : K4279-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0669

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

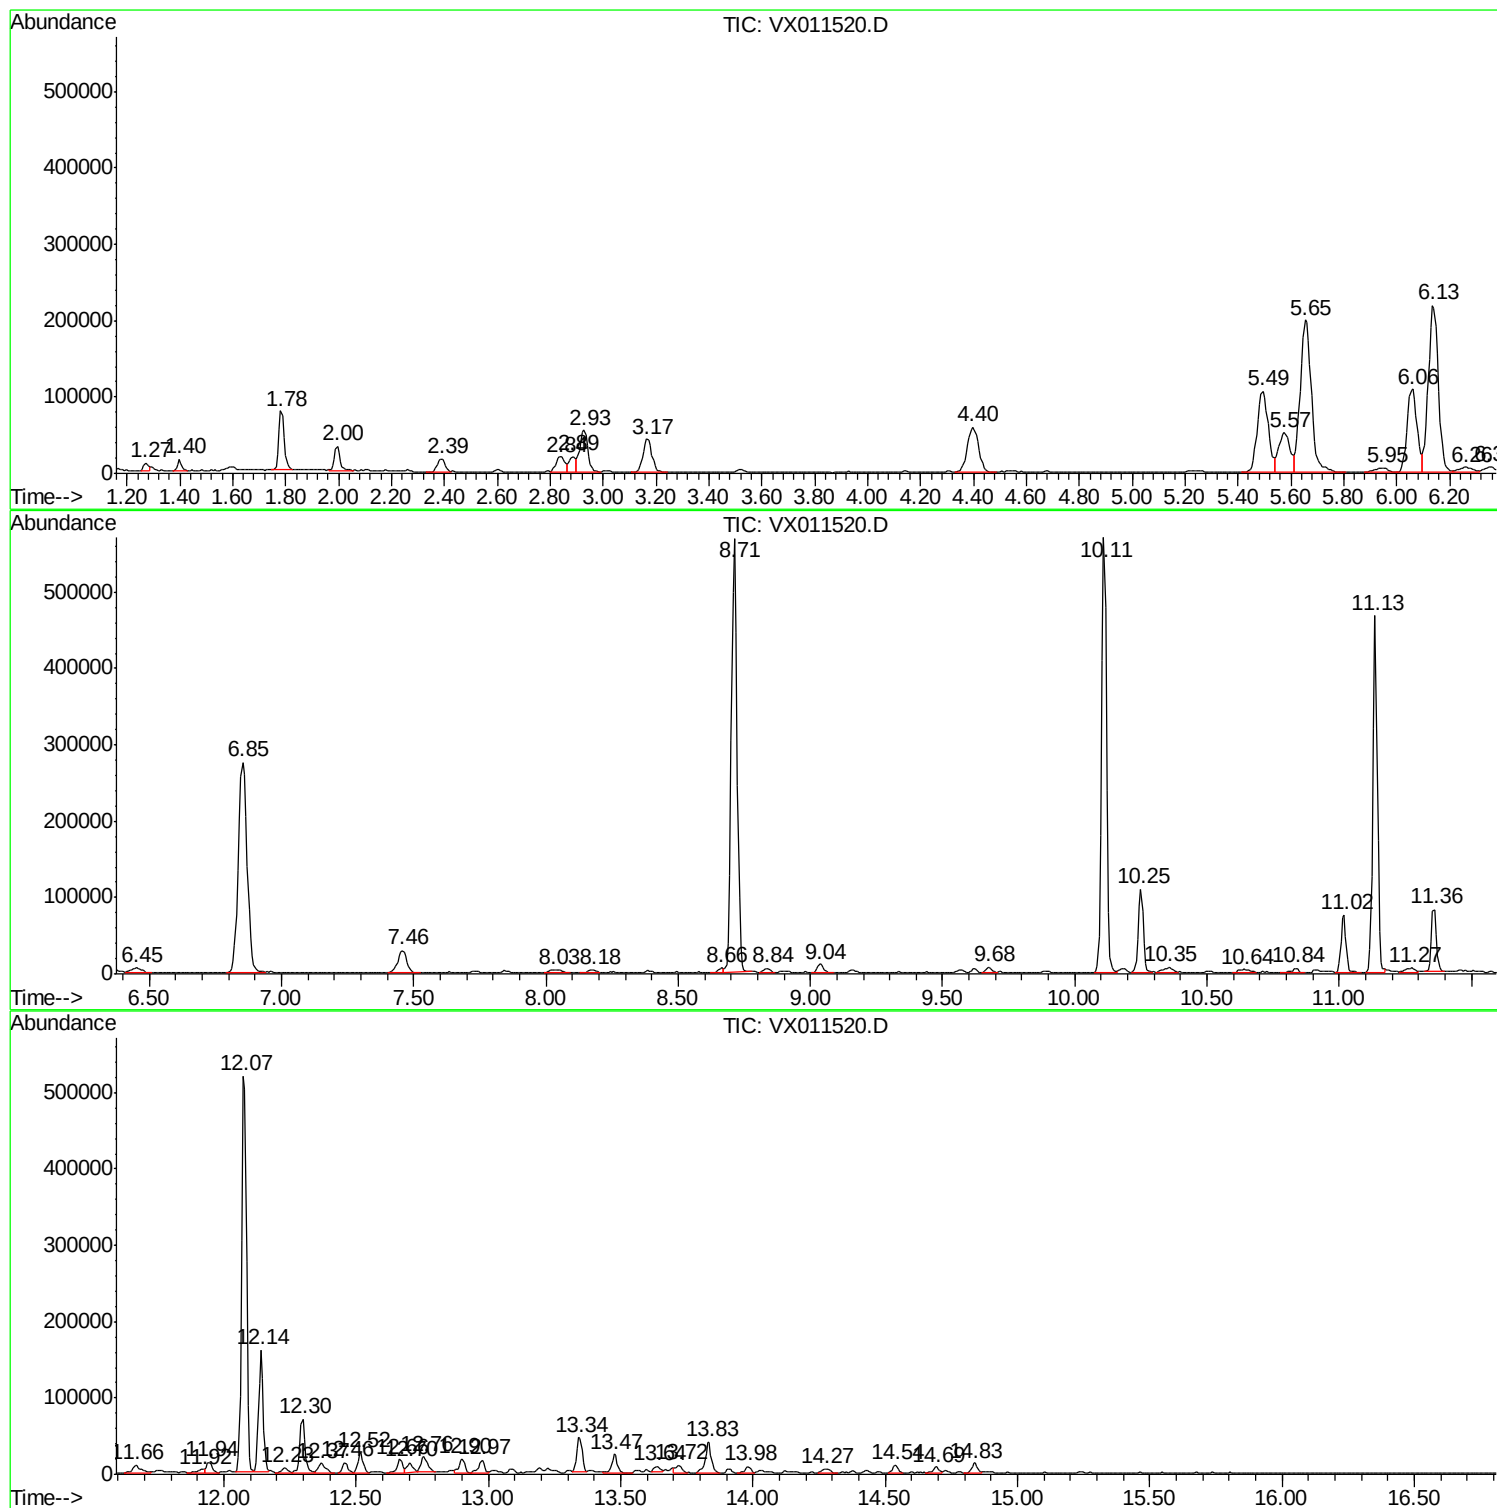

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081219\
Data File : VX011520.D
Acq On : 13 Aug 2019 06:17
Operator : JC/SP
Sample : K4279-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0669

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081219\
Data File : VX011520.D
Acq On : 13 Aug 2019 06:17
Operator : JC/SP
Sample : K4279-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0669

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc