


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081219\  
Data File : VX011471.D  
Acq On : 12 Aug 2019 09:03  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Title : SW846 8260  
Last Update : Fri Aug 02 01:55:00 2019

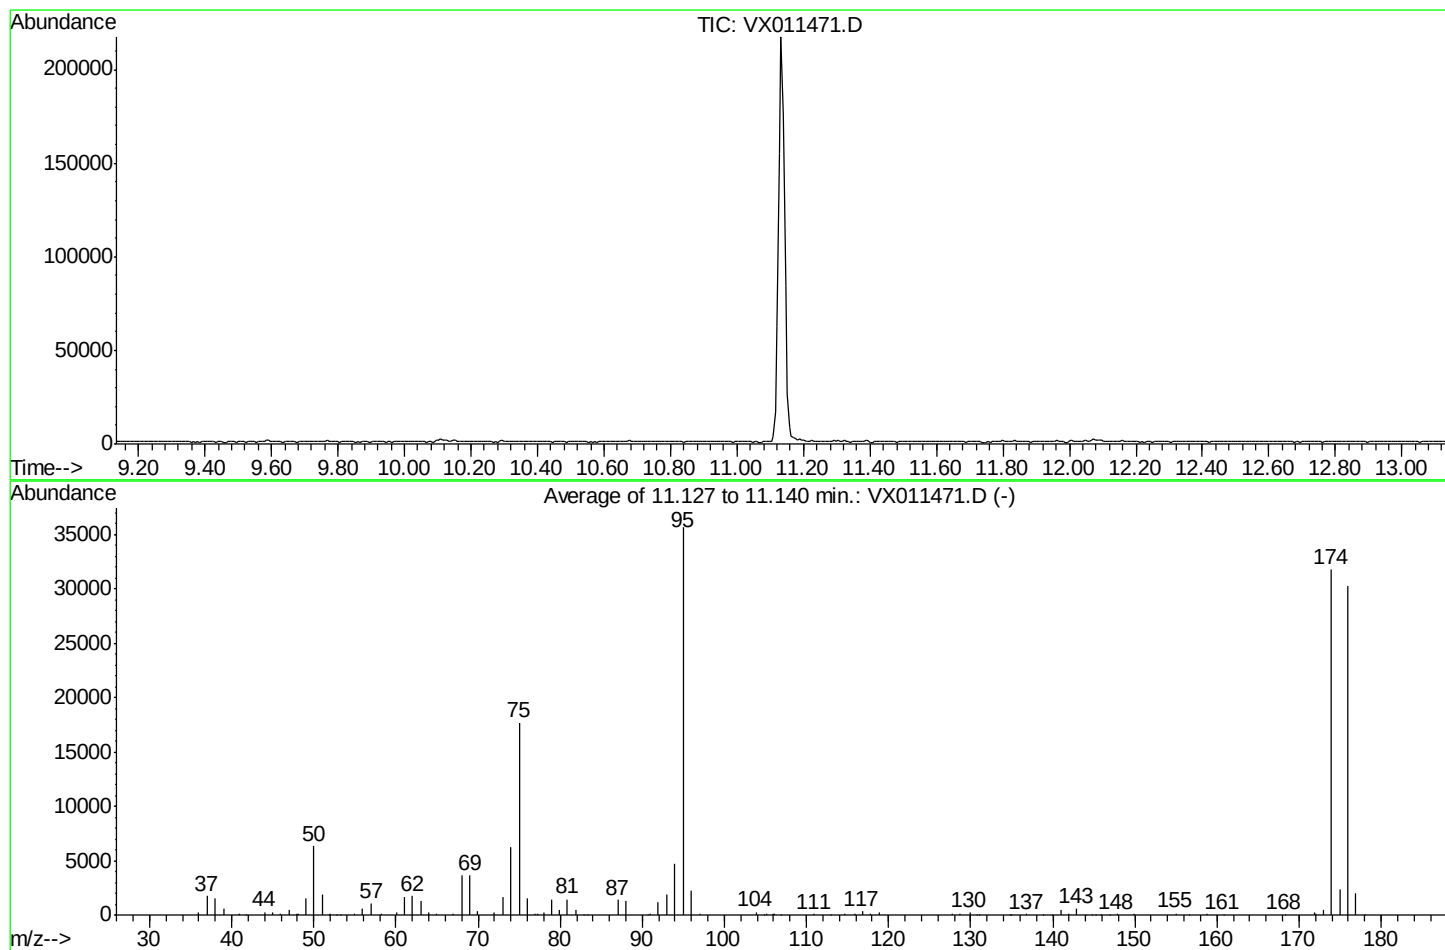

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.8      | 6333    | PASS             |
| 75          | 95           | 30           | 60           | 49.7      | 17713   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 35642   | PASS             |
| 96          | 95           | 5            | 9            | 6.4       | 2269    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.6       | 515     | PASS             |
| 174         | 95           | 50           | 100          | 89.0      | 31730   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 2372    | PASS             |
| 176         | 174          | 95           | 101          | 95.2      | 30194   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 2028    | PASS             |