


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081219\
 Data File : VX011498.D
 Acq On : 12 Aug 2019 20:56
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260
 Last Update : Fri Aug 02 01:55:00 2019

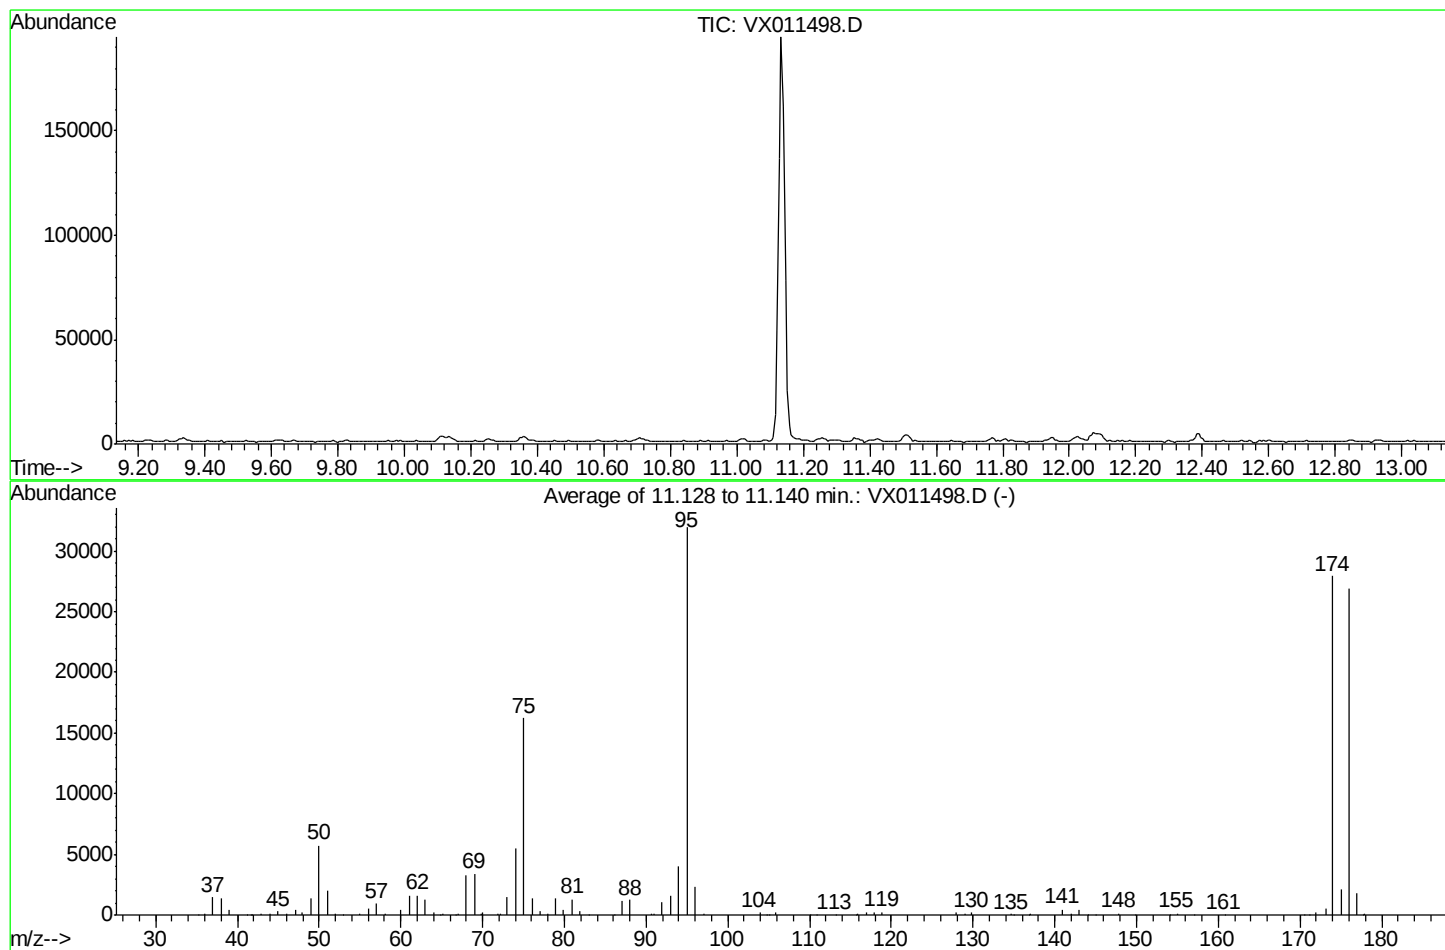

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	5704	PASS
75	95	30	60	50.8	16238	PASS
95	95	100	100	100.0	31957	PASS
96	95	5	9	7.2	2303	PASS
173	174	0.00	2	1.7	481	PASS
174	95	50	100	87.3	27914	PASS
175	174	5	9	7.5	2106	PASS
176	174	95	101	96.5	26936	PASS
177	176	5	9	6.7	1801	PASS