


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081220\
 Data File : VX017855.D
 Acq On : 12 Aug 2020 09:54
 Operator : JC/SP
 Sample : BFB67
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB67

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 14 07:39:24 2020

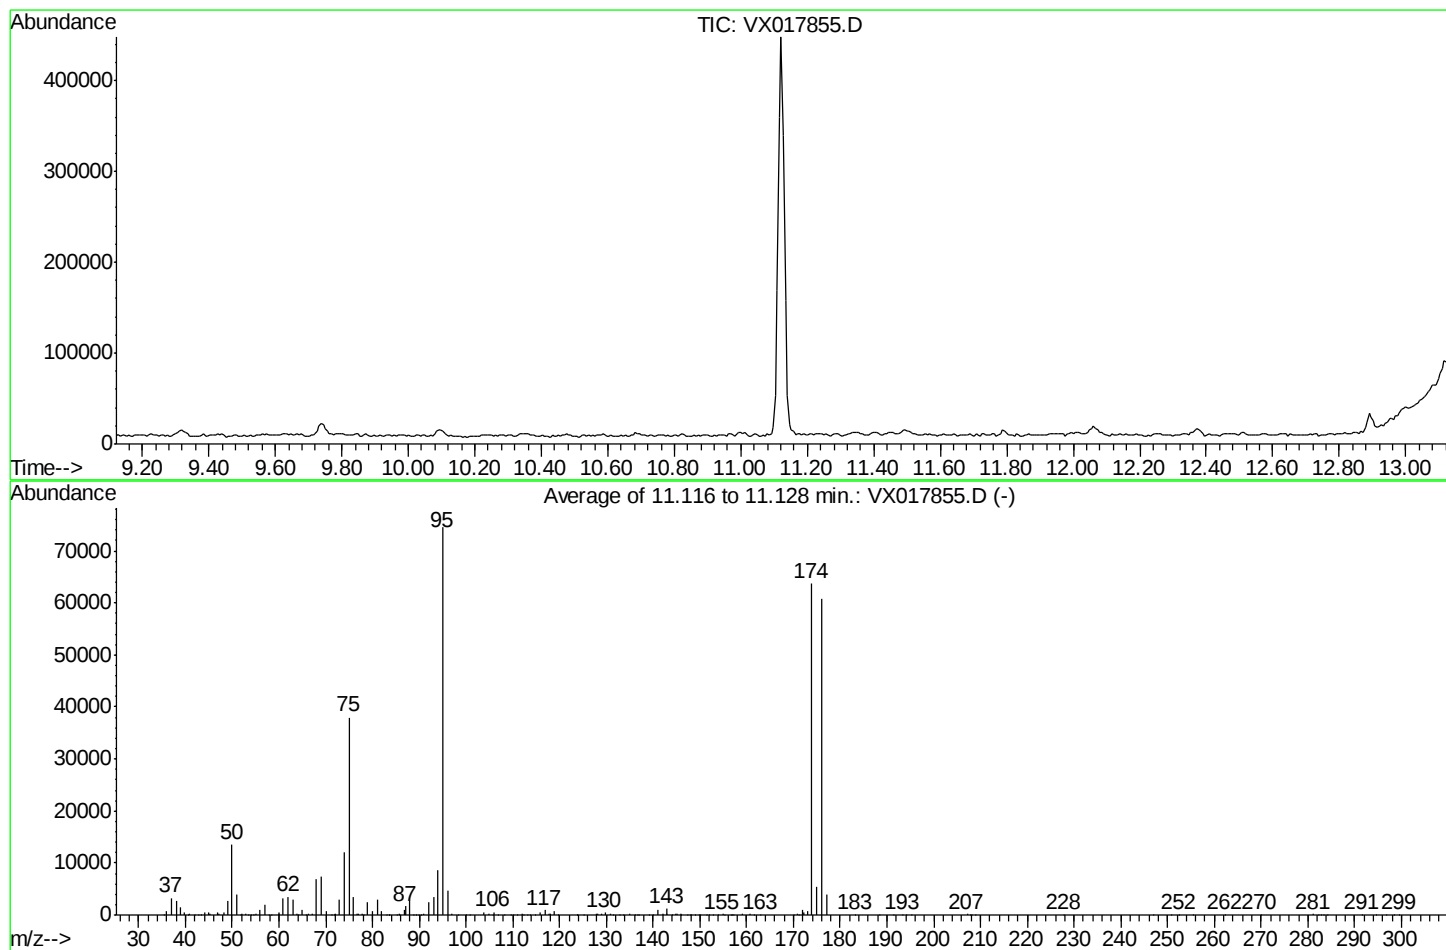

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	13527	PASS
75	95	30	80	50.9	37973	PASS
95	95	100	100	100.0	74533	PASS
96	95	5	9	6.4	4733	PASS
173	174	0.00	2	1.1	716	PASS
174	95	50	120	85.5	63722	PASS
175	174	5	9	8.3	5320	PASS
176	174	95	101	95.4	60792	PASS
177	176	5	9	6.7	4059	PASS

m/z	Abundance
35.30	143.0
36.10	749.0
37.00	3907.0
38.00	3253.0
39.00	1805.0
39.90	316.0
41.30	401.0
42.00	224.0
42.70	191.0
43.20	144.0
44.00	1569.0
45.00	979.0
45.70	152.0
46.90	583.0
48.20	402.0
49.00	2603.0
50.00	14680.0
51.00	4566.0
51.80	371.0
53.00	205.0
54.00	128.0
55.10	292.0
55.90	1247.0
56.90	2123.0
57.90	90.0
58.30	233.0
59.00	140.0
60.00	992.0
61.00	3711.0
62.00	3815.0
63.10	3402.0
64.00	608.0
65.00	953.0
65.70	82.0
66.30	154.0
66.90	418.0
68.00	7340.0
69.00	8222.0
70.10	798.0
71.10	92.0
71.90	428.0
73.00	3061.0
74.10	13207.0
75.00	37592.0
76.00	3782.0
77.00	441.0
77.80	518.0
79.00	2666.0
80.00	720.0
81.00	3119.0
81.90	927.0
83.40	78.0
85.70	152.0
86.90	2818.0
88.00	2542.0
89.20	115.0
91.00	363.0
92.00	2291.0
93.00	3961.0
94.00	8118.0
95.00	72040.0
96.00	4159.0
97.00	418.0
100.00	57.0
103.90	510.0
105.10	132.0
105.70	321.0
106.10	476.0
106.80	157.0
109.50	64.0
110.90	150.0
112.10	256.0
113.20	91.0
114.70	250.0
115.90	342.0
116.80	876.0
117.80	507.0
119.00	849.0
119.80	78.0
123.60	106.0
127.90	277.0
128.90	193.0
129.80	555.0
130.80	105.0
131.30	116.0
132.90	103.0
133.50	172.0
134.90	162.0
136.70	221.0
139.10	124.0
140.90	1269.0
142.00	210.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

142.80	1114.0
144.90	497.0
145.80	150.0
147.30	258.0
147.90	140.0
149.70	66.0
151.90	135.0
152.80	125.0
155.20	228.0
156.90	98.0
158.90	114.0
160.70	123.0
161.70	66.0
165.90	115.0
169.90	138.0
170.80	217.0
171.90	1159.0
173.00	948.0
173.90	50640.0
174.90	4273.0
176.00	49752.0
177.00	3330.0
183.20	105.0
188.30	63.0
191.30	121.0
193.10	55.0
207.00	472.0
207.80	69.0
208.90	95.0
250.70	52.0
252.50	187.0
262.30	53.0
281.30	211.0
282.20	84.0
284.10	80.0
298.30	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

m/z	Abundance
35.90	700.0
36.10	706.0
37.00	4170.0
38.00	3522.0
39.00	1652.0
39.80	422.0
40.60	229.0
41.20	238.0
42.30	111.0
44.10	1314.0
45.20	791.0
46.30	306.0
46.90	932.0
47.80	385.0
48.20	518.0
49.10	2857.0
50.00	15774.0
51.00	4639.0
52.00	359.0
52.90	169.0
53.30	95.0
54.00	66.0
54.50	145.0
55.00	254.0
55.90	1048.0
57.00	2372.0
57.90	166.0
58.50	79.0
59.80	836.0
60.90	3932.0
62.00	4359.0
63.00	3572.0
63.90	488.0
65.10	978.0
66.20	267.0
67.00	374.0
68.00	7803.0
69.10	8742.0
70.00	757.0
71.10	117.0
72.10	663.0
73.00	3966.0
74.00	14253.0
75.00	45856.0
76.00	3960.0
77.10	478.0
77.80	408.0
78.90	2844.0
79.90	896.0
80.90	3500.0
81.90	803.0
82.90	95.0
85.30	67.0
85.90	366.0
87.10	2870.0
87.90	3436.0
88.80	168.0
89.30	123.0
91.00	680.0
92.00	3078.0
93.00	4553.0
94.10	10021.0
95.00	87688.0
96.00	6500.0
97.00	278.0
98.40	103.0
100.80	101.0
103.10	84.0
103.90	481.0
105.10	150.0
105.90	450.0
106.90	76.0
108.10	97.0
109.50	114.0
110.90	82.0
111.90	182.0
113.20	124.0
113.70	75.0
114.60	98.0
115.90	635.0
116.90	1041.0
118.10	356.0
118.80	793.0
119.70	143.0
123.70	113.0
125.00	167.0
127.70	302.0
128.20	269.0
128.90	134.0
129.60	332.0
130.20	196.0
130.80	121.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

131.40	157.0
132.80	122.0
134.80	339.0
137.10	149.0
139.10	81.0
139.90	98.0
140.90	792.0
142.00	118.0
143.00	1959.0
145.10	632.0
146.00	484.0
146.80	106.0
147.30	136.0
147.90	199.0
149.10	119.0
151.40	72.0
151.90	62.0
153.90	188.0
154.90	317.0
156.60	195.0
157.10	124.0
159.00	157.0
160.80	167.0
161.60	64.0
163.00	54.0
169.90	130.0
170.70	244.0
171.20	273.0
172.10	1442.0
173.10	1202.0
174.00	73656.0
175.00	6285.0
175.90	71352.0
177.00	4662.0
193.00	152.0
207.10	405.0
208.80	59.0
247.00	50.0
269.10	141.0
280.80	167.0
282.20	120.0
283.40	63.0
284.10	61.0
294.50	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

m/z	Abundance
35.10	54.0
36.00	595.0
37.00	2091.0
37.90	2009.0
39.00	1363.0
39.90	478.0
40.90	409.0
41.90	135.0
42.80	238.0
43.30	212.0
44.00	1319.0
44.90	659.0
45.70	171.0
47.10	812.0
48.10	309.0
49.00	2569.0
50.00	10674.0
51.00	2995.0
52.00	265.0
52.50	191.0
53.00	183.0
55.10	399.0
56.00	761.0
56.90	1682.0
58.50	108.0
60.10	862.0
61.00	2349.0
62.00	2522.0
62.90	2090.0
64.20	260.0
65.10	702.0
65.80	110.0
67.10	204.0
68.10	5263.0
69.00	5575.0
70.00	583.0
72.00	225.0
72.90	2683.0
74.00	9196.0
75.00	30472.0
76.00	2718.0
76.80	429.0
77.50	170.0
78.00	426.0
78.90	2232.0
80.00	710.0
80.90	2245.0
82.00	494.0
82.90	141.0
83.60	110.0
85.20	117.0
85.80	178.0
87.00	2271.0
88.00	1868.0
89.70	74.0
90.50	312.0
91.90	1809.0
93.10	2125.0
94.00	7459.0
95.00	63872.0
96.00	3542.0
97.00	155.0
98.30	112.0
100.90	112.0
103.00	126.0
103.90	485.0
104.90	289.0
105.90	714.0
108.20	178.0
109.60	121.0
110.20	73.0
110.70	129.0
111.90	50.0
112.20	50.0
113.20	139.0
115.10	60.0
115.70	276.0
116.80	761.0
118.10	311.0
118.80	663.0
123.90	167.0
125.10	86.0
128.00	230.0
129.00	181.0
129.80	312.0
130.80	191.0
132.80	104.0
134.80	244.0
136.20	67.0
136.90	195.0
139.10	124.0
140.90	720.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

142.00	179.0
142.90	1452.0
144.00	135.0
144.90	617.0
145.80	208.0
146.80	130.0
148.10	178.0
149.00	117.0
150.10	115.0
154.00	61.0
154.90	262.0
156.60	74.0
157.10	211.0
159.10	174.0
160.70	181.0
169.90	54.0
170.70	241.0
171.80	1468.0
174.00	66872.0
175.10	5404.0
176.00	61272.0
177.00	4186.0
192.50	155.0
193.40	144.0
194.20	56.0
195.20	95.0
207.20	326.0
208.00	118.0
227.80	65.0
255.50	58.0
269.90	61.0
281.20	254.0
282.90	175.0
291.60	63.0
296.70	61.0
299.60	120.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

m/z	Abundance
36.10	160.0
36.80	68.0
37.50	76.0
38.10	153.0
38.80	71.0
39.30	88.0
40.10	477.0
41.10	239.0
42.40	118.0
42.80	111.0
44.00	1015.0
45.50	170.0
46.10	104.0
46.70	56.0
47.30	94.0
47.90	178.0
48.60	128.0
49.60	131.0
50.10	182.0
50.60	137.0
52.30	66.0
53.80	60.0
54.80	174.0
55.60	101.0
56.80	124.0
58.60	76.0
59.10	62.0
60.20	131.0
62.50	188.0
63.70	95.0
64.70	57.0
66.70	70.0
67.80	97.0
71.20	50.0
71.80	60.0
72.80	225.0
74.00	77.0
75.90	117.0
77.50	121.0
78.20	55.0
80.40	65.0
81.70	77.0
86.10	120.0
90.30	60.0
96.60	72.0
103.10	76.0
104.90	52.0
108.20	77.0
111.50	78.0
115.10	69.0
118.10	62.0
120.80	51.0
130.40	67.0
133.10	102.0
141.00	51.0
146.90	137.0
165.70	151.0
168.90	58.0
177.80	82.0
181.30	84.0
181.80	108.0
192.40	150.0
193.10	75.0
207.10	269.0
231.80	51.0
267.90	121.0
269.20	107.0
281.00	331.0
287.40	68.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67