

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023674.D
 Acq On : 12 Aug 2021 15:01
 Operator : JC/MD
 Sample : M3364-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBKA1

Quant Time: Aug 13 01:03:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 13 01:00:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	316981	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	287096	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	123380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	65320	39.535	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.080%
7) Chloroethane-d5	1.666	69	58970	43.448	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.900%
11) 1,1-Dichloroethene-d2	2.306	63	113615	31.658	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.320%
21) 2-Butanone-d5	4.465	46	150090	94.226	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.230%
24) Chloroform-d	5.068	84	162054	43.316	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.640%
26) 1,2-Dichloroethane-d4	5.964	65	113868	44.401	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.800%
32) Benzene-d6	5.983	84	331258	45.803	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	7.318	67	106584	46.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	8.653	98	304562	43.727	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.460%
43) trans-1,3-Dichloroprop...	8.952	79	44113	40.965	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.920%
47) 2-Hexanone-d5	9.390	63	106396	97.253	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.250%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	141429	46.655	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.320%
66) 1,2-Dichlorobenzene-d4	12.323	152	104820	48.414	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.820%
Target Compounds						Qvalue
13) Acetone	2.386	43	6262	4.465	ug/L	90
61) 1,2,3-Trichloropropane	12.024	75	15164	6.110	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023674.D
Acq On : 12 Aug 2021 15:01
Operator : JC/MD
Sample : M3364-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBKA1


Quant Time: Aug 13 01:03:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 13 01:00:38 2021
Response via : Initial Calibration

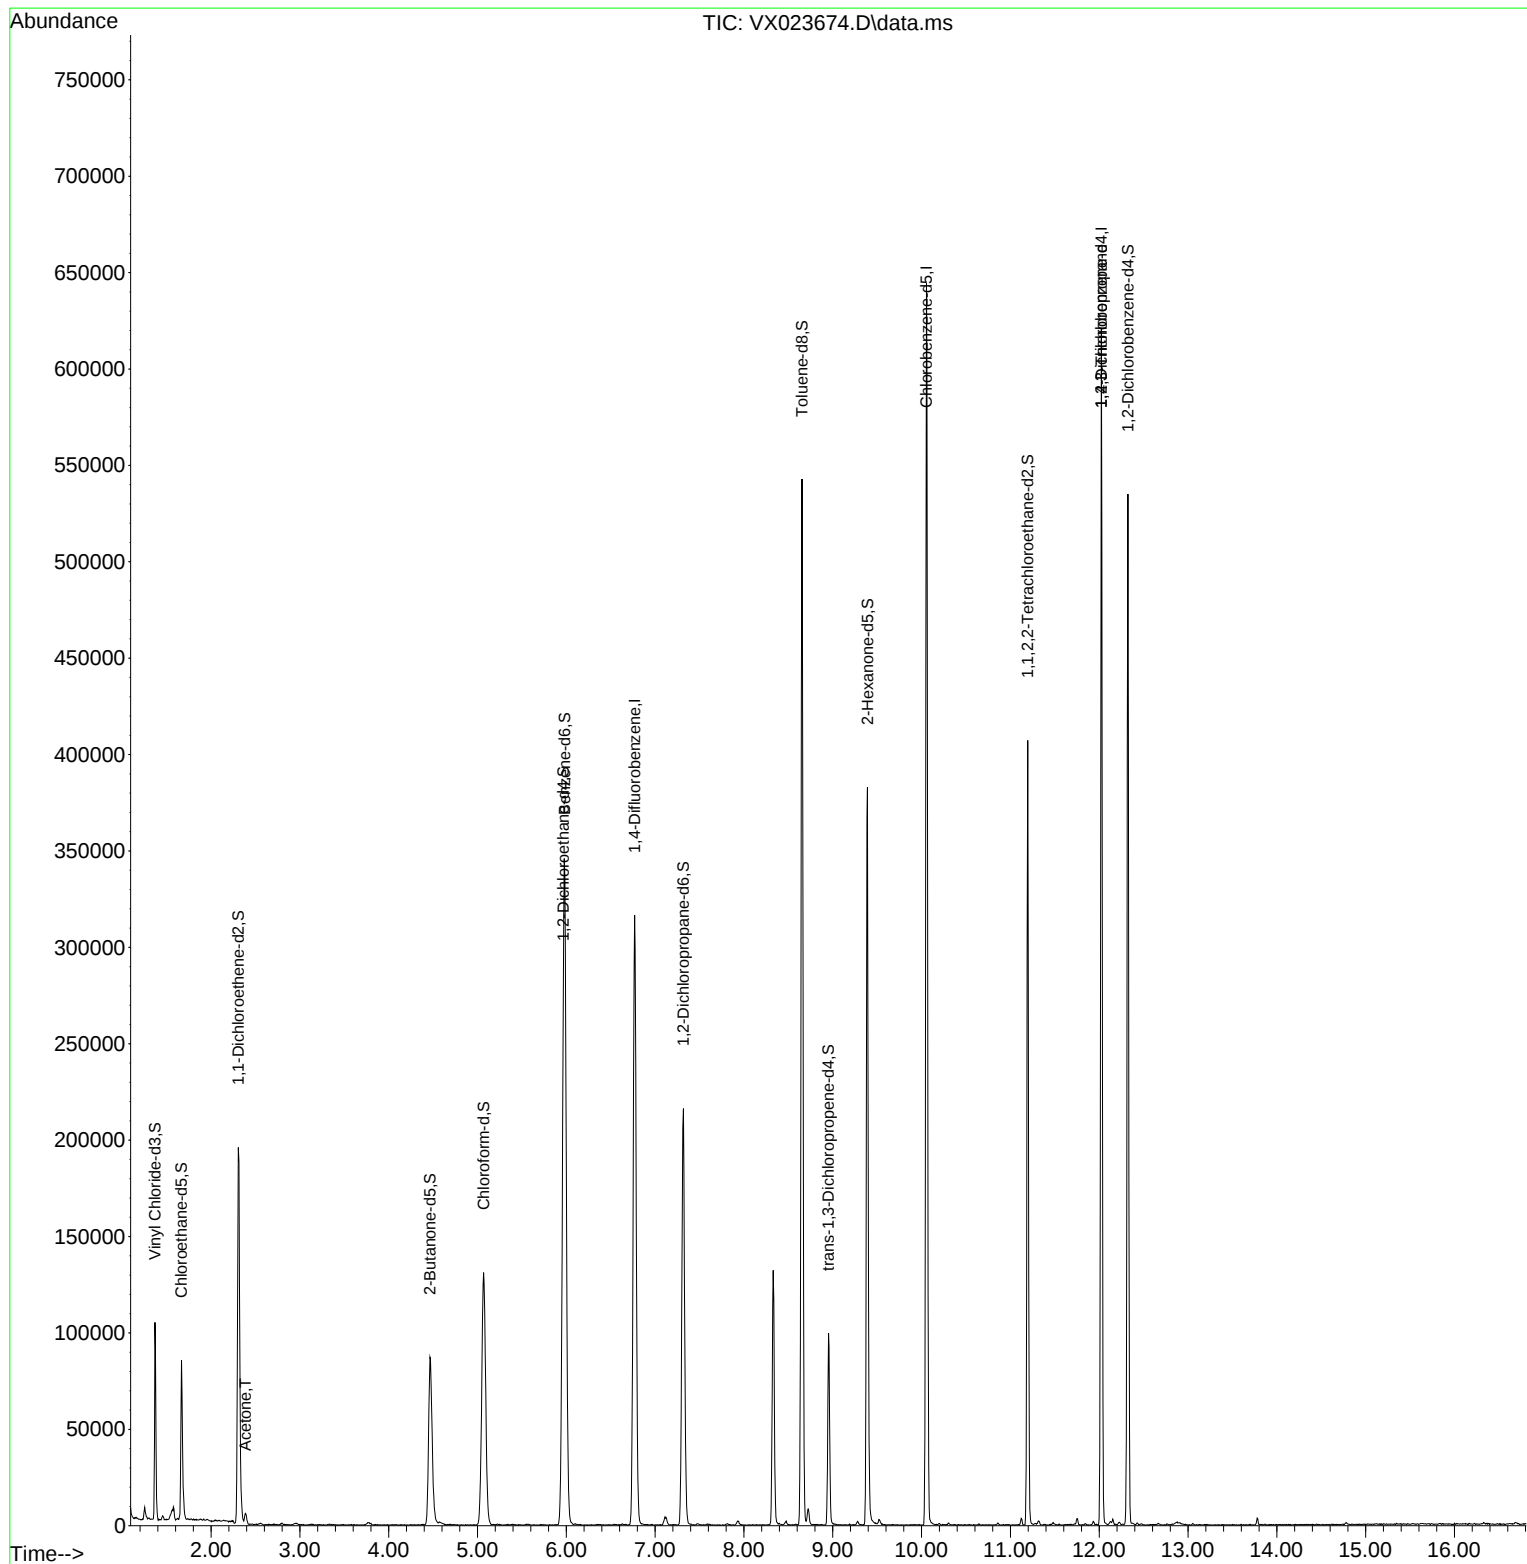



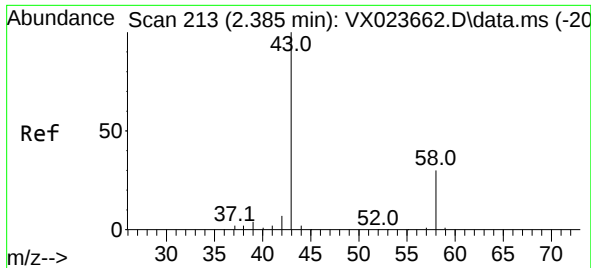


#13
Acetone
Concen: 4.465 ug/L
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX023674.D
Acq: 12 Aug 2021 15:01


Instrument :
MSVOA_X
ClientSampleId :
DBKA1

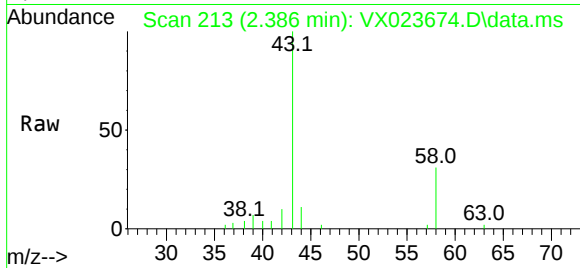

Tgt Ion: 43 Resp: 6262
Ion Ratio Lower Upper
43 100
58 28.6 0.0 68.2

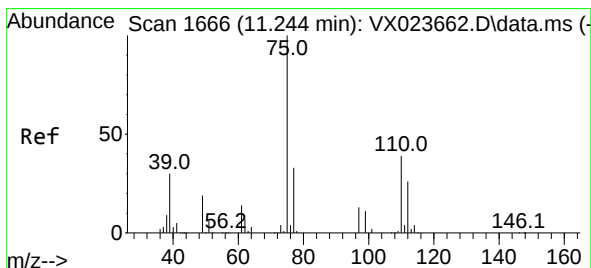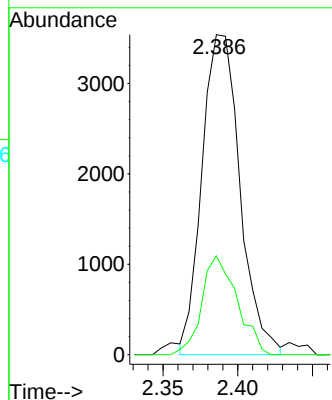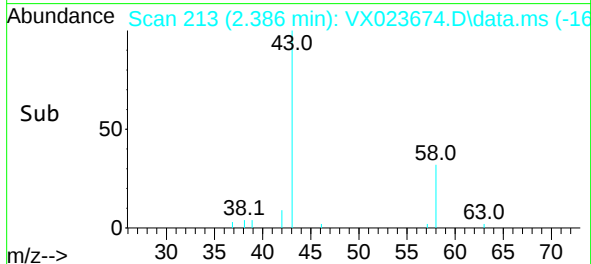

#61
1,2,3-Trichloropropane
Concen: 6.110 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.781 min
Lab File: VX023674.D
Acq: 12 Aug 2021 15:01

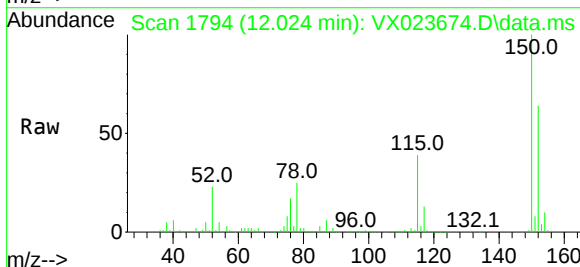

Tgt Ion: 75 Resp: 15164
Ion Ratio Lower Upper
75 100
77 35.9 26.2 39.2
110 3.1 31.8 47.8#

