

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023670.D
 Acq On : 12 Aug 2021 13:27
 Operator : JC/MD
 Sample : M3364-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK96

Quant Time: Aug 13 01:02:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 13 01:00:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	317219	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	290818	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	124412	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	65808	39.801	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.600%
7) Chloroethane-d5	1.666	69	60178	44.304	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.600%
11) 1,1-Dichloroethene-d2	2.306	63	115662	32.204	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.400%
21) 2-Butanone-d5	4.465	46	153710	96.426	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.430%
24) Chloroform-d	5.068	84	164130	43.838	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.680%
26) 1,2-Dichloroethane-d4	5.964	65	115550	45.023	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.040%
32) Benzene-d6	5.983	84	332993	45.454	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.900%
36) 1,2-Dichloropropane-d6	7.318	67	105581	45.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.600%
41) Toluene-d8	8.653	98	309408	43.854	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.700%
43) trans-1,3-Dichloroprop...	8.952	79	44085	40.415	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.820%
47) 2-Hexanone-d5	9.391	63	110213	99.452	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.450%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	144893	47.186	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.380%
66) 1,2-Dichlorobenzene-d4	12.323	152	106286	48.684	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.360%
Target Compounds						
					Qvalue	
13) Acetone	2.386	43	4071	2.901	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023670.D
Acq On : 12 Aug 2021 13:27
Operator : JC/MD
Sample : M3364-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK96

Quant Time: Aug 13 01:02:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 13 01:00:38 2021
Response via : Initial Calibration

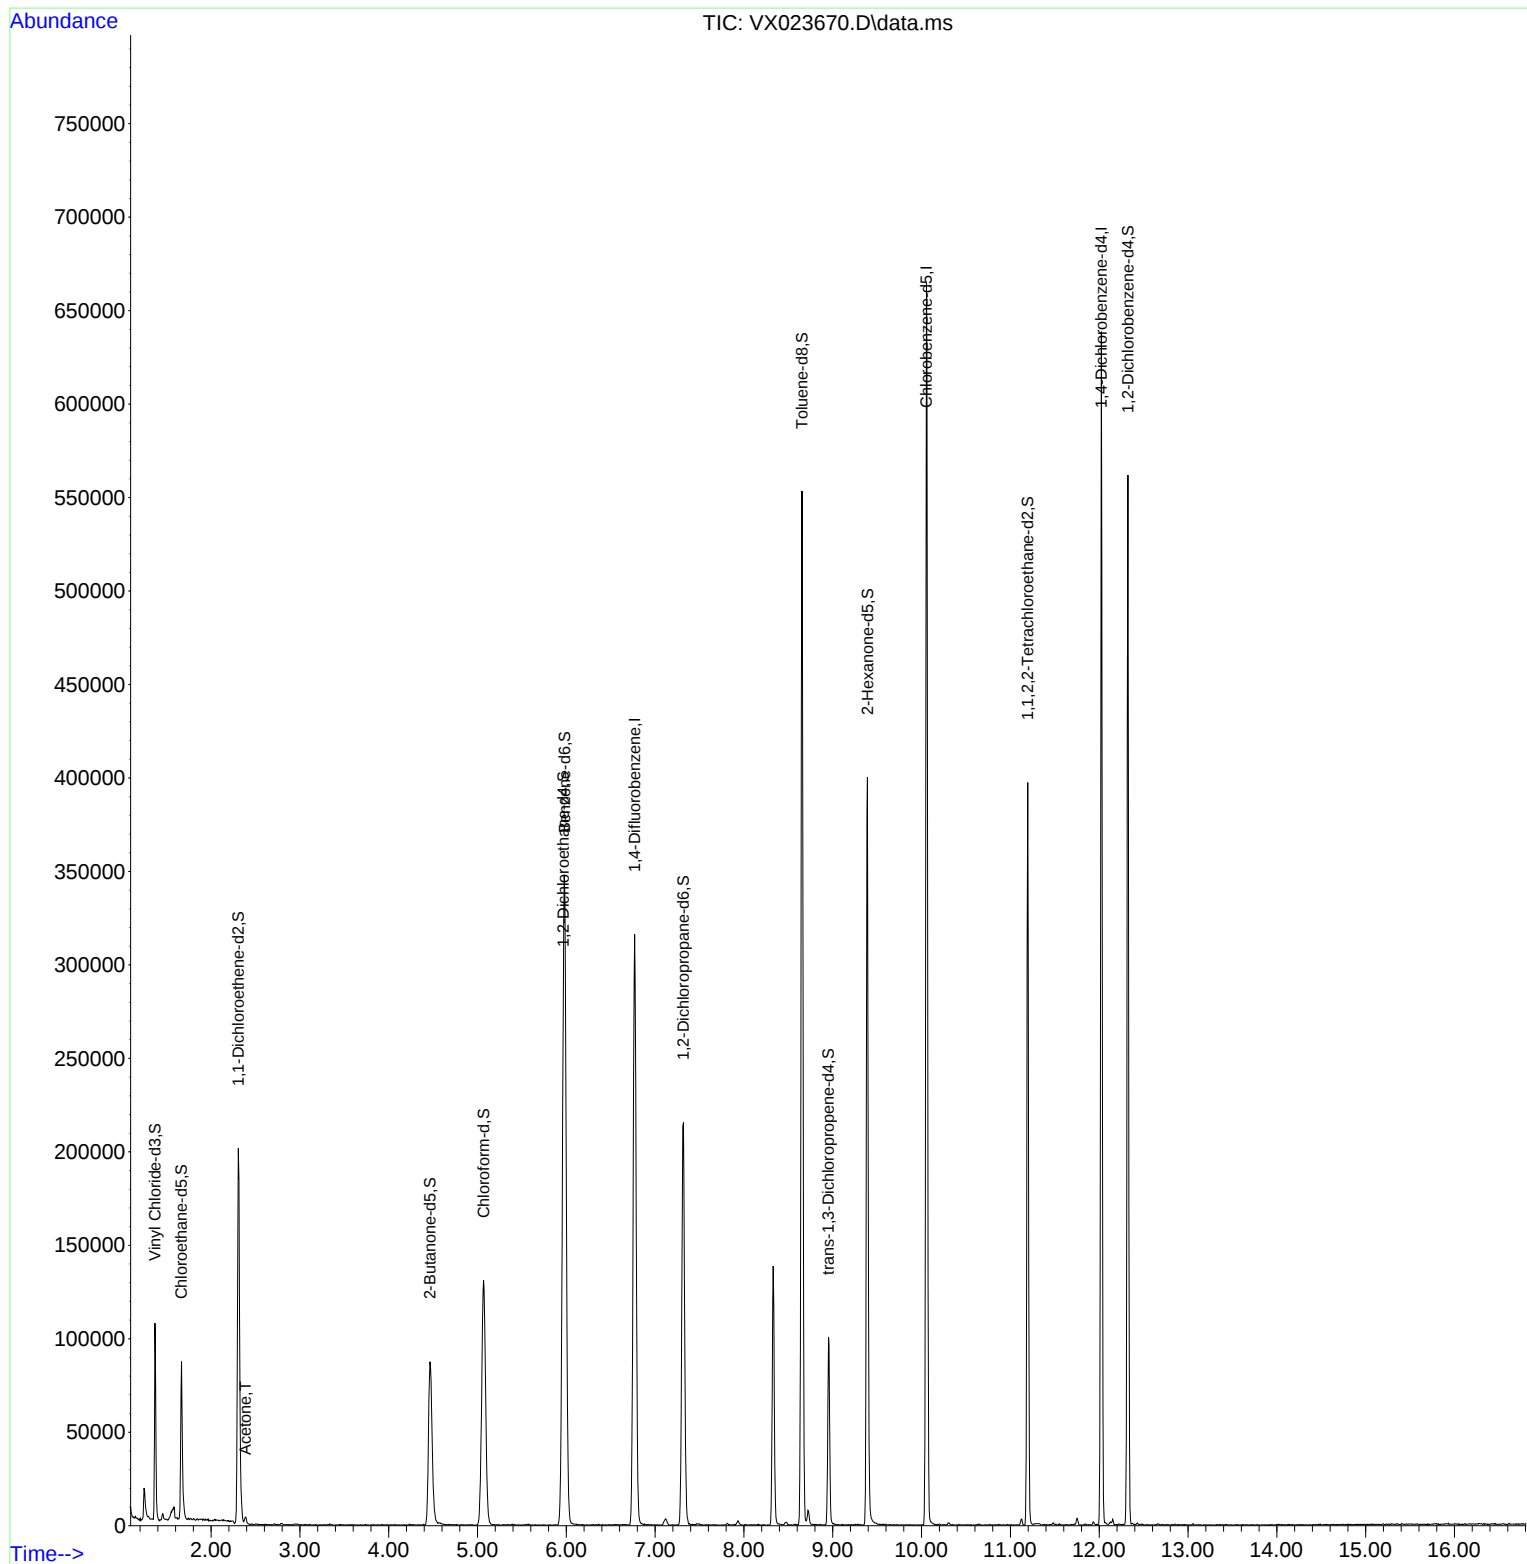

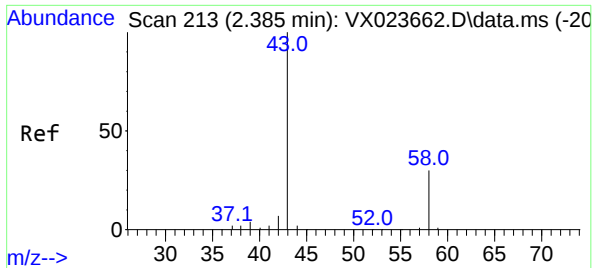

#13
Acetone
Concen: 2.901 ug/L
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX023670.D
Acq: 12 Aug 2021 13:27

Instrument :
MSVOA_X
ClientSampleId :
DBK96

Tgt Ion: 43 Resp: 4071
Ion Ratio Lower Upper
43 100
58 31.6 0.0 68.2

