

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023664.D
 Acq On : 12 Aug 2021 10:51
 Operator : JC/MD
 Sample : VX0812WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK607

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

Signal : TIC: VX023664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	108619	109250	10.69%	1.344%
2	1.666	90	95	105	rVB	81931	111310	10.89%	1.369%
3	2.307	194	200	210	rBV	196861	326303	31.92%	4.014%
4	2.508	230	233	237	rBV3	1127	2052	0.20%	0.025%
5	2.715	262	267	270	rBV4	793	1427	0.14%	0.018%
6	2.788	275	279	286	rVB4	3204	5533	0.54%	0.068%
7	3.111	325	332	334	rBV5	1814	3839	0.38%	0.047%
8	3.349	369	371	374	rVB2	408	361	0.04%	0.004%
9	3.666	421	423	426	rVB	402	260	0.03%	0.003%
10	3.867	452	456	461	rVB3	305	563	0.06%	0.007%
11	3.916	461	464	466	rBV2	299	436	0.04%	0.005%
12	4.337	530	533	535	rBV2	223	278	0.03%	0.003%
13	4.465	544	554	568	rBV	95409	269488	26.36%	3.315%
14	4.879	619	622	623	rBV	327	300	0.03%	0.004%
15	4.898	623	625	628	rBV2	618	735	0.07%	0.009%
16	4.952	633	634	637	rBV2	299	250	0.02%	0.003%
17	5.062	640	652	671	rBV2	128053	408558	39.96%	5.026%
18	5.227	675	679	683	rBV3	320	738	0.07%	0.009%
19	5.373	702	703	704	rBV	511	266	0.03%	0.003%
20	5.471	715	719	726	rVB4	951	2261	0.22%	0.028%
21	5.666	749	751	754	rBV3	387	533	0.05%	0.007%
22	5.977	789	802	817	rBV2	344136	1022367	100.00%	12.576%
23	6.190	835	837	839	rBV2	410	411	0.04%	0.005%
24	6.306	853	856	857	rBV	258	220	0.02%	0.003%
25	6.361	862	865	867	rBV3	377	541	0.05%	0.007%
26	6.538	891	894	896	rVV	374	363	0.04%	0.004%
27	6.605	900	905	907	rBV2	315	493	0.05%	0.006%
28	6.769	921	932	946	rBV	277247	665548	65.10%	8.187%
29	7.117	980	989	1000	rVB4	6952	15963	1.56%	0.196%
30	7.312	1012	1021	1032	rBV	213237	471966	46.16%	5.806%
31	7.604	1067	1069	1072	rVV	280	247	0.02%	0.003%
32	7.793	1098	1100	1101	rBV2	503	388	0.04%	0.005%
33	7.928	1116	1122	1130	rVV2	2312	4358	0.43%	0.054%
34	8.013	1134	1136	1138	rVB2	237	234	0.02%	0.003%
35	8.135	1154	1156	1159	rVB	325	311	0.03%	0.004%
36	8.165	1159	1161	1166	rVB2	289	320	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023664.D
 Acq On : 12 Aug 2021 10:51
 Operator : JC/MD
 Sample : VX0812WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK607

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.214	1166	1169	1171	rBV	238	286	0.03%	0.004%
38	8.330	1181	1188	1201	rBV	137064	229397	22.44%	2.822%
39	8.470	1206	1211	1218	rVB4	1841	3290	0.32%	0.040%
40	8.525	1218	1220	1223	rBV	419	413	0.04%	0.005%
41	8.580	1225	1229	1233	rVV4	3027	4616	0.45%	0.057%
42	8.653	1234	1241	1248	rVV	536367	816230	79.84%	10.041%
43	8.720	1248	1252	1260	rVB	10923	17500	1.71%	0.215%
44	8.952	1284	1290	1301	rBV	103921	154013	15.06%	1.895%
45	9.153	1319	1323	1329	rVB4	2169	3118	0.30%	0.038%
46	9.238	1335	1337	1340	rBV2	235	264	0.03%	0.003%
47	9.275	1340	1343	1351	rVB5	2580	3802	0.37%	0.047%
48	9.385	1356	1361	1374	rBV	403582	588500	57.56%	7.239%
49	9.525	1382	1384	1389	rVB3	1332	1676	0.16%	0.021%
50	9.610	1394	1398	1403	rBV4	1134	1709	0.17%	0.021%
51	9.702	1410	1413	1415	rBV	458	553	0.05%	0.007%
52	10.055	1465	1471	1487	rVV	611080	819519	80.16%	10.081%
53	10.165	1487	1489	1490	rVV	413	253	0.02%	0.003%
54	10.195	1490	1494	1501	rVB	3674	5654	0.55%	0.070%
55	10.305	1507	1512	1517	rBV2	4231	6076	0.59%	0.075%
56	10.360	1520	1521	1524	rBV3	260	281	0.03%	0.003%
57	10.476	1537	1540	1543	rBV2	245	305	0.03%	0.004%
58	10.653	1564	1569	1575	rVB3	4933	9143	0.89%	0.112%
59	10.756	1584	1586	1590	rVV3	396	454	0.04%	0.006%
60	10.799	1590	1593	1596	rVB2	721	781	0.08%	0.010%
61	10.964	1616	1620	1625	rVB2	3699	4740	0.46%	0.058%
62	11.073	1635	1638	1639	rBV2	203	248	0.02%	0.003%
63	11.122	1642	1646	1652	rVB2	4074	4999	0.49%	0.061%
64	11.195	1652	1658	1664	rBV	422066	526784	51.53%	6.480%
65	11.384	1686	1689	1693	rBV	706	707	0.07%	0.009%
66	11.451	1697	1700	1708	rBV	3971	6509	0.64%	0.080%
67	11.549	1714	1716	1720	rVB2	351	299	0.03%	0.004%
68	11.622	1725	1728	1729	rBV	385	406	0.04%	0.005%
69	11.677	1734	1737	1738	rVV3	389	401	0.04%	0.005%
70	11.750	1745	1749	1754	rVB2	6209	8179	0.80%	0.101%
71	11.848	1762	1765	1767	rVB3	584	685	0.07%	0.008%
72	11.933	1774	1779	1782	rBV2	1750	2197	0.21%	0.027%
73	11.976	1782	1786	1789	rVB2	2709	3385	0.33%	0.042%
74	12.024	1789	1794	1806	rVB	604508	739322	72.31%	9.095%
75	12.128	1808	1811	1812	rBV3	894	975	0.10%	0.012%
76	12.323	1835	1843	1850	rBV	569954	710390	69.48%	8.739%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023664.D
 Acq On : 12 Aug 2021 10:51
 Operator : JC/MD
 Sample : VX0812WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK607

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.408	1855	1857	1858	rBV2	457	385	0.04%	0.005%
78	12.427	1858	1860	1865	rVB3	985	1270	0.12%	0.016%
79	12.475	1866	1868	1869	rBV2	455	239	0.02%	0.003%
80	12.664	1897	1899	1902	rVB3	723	812	0.08%	0.010%
81	12.695	1902	1904	1907	rBV2	270	323	0.03%	0.004%
82	12.768	1912	1916	1919	rVV2	729	999	0.10%	0.012%
83	12.823	1923	1925	1927	rVB2	429	373	0.04%	0.005%
84	12.860	1927	1931	1936	rBV4	615	876	0.09%	0.011%
85	12.908	1938	1939	1941	rBV	353	336	0.03%	0.004%
86	12.951	1942	1946	1950	rVB3	928	1155	0.11%	0.014%
87	13.049	1959	1962	1969	rBV4	823	1137	0.11%	0.014%
88	13.116	1969	1973	1979	rVV2	2497	3017	0.30%	0.037%
89	13.305	2003	2004	2007	rVB2	272	260	0.03%	0.003%
90	13.427	2021	2024	2027	rBV2	334	348	0.03%	0.004%
91	13.591	2047	2051	2055	rBV2	2090	2345	0.23%	0.029%
92	13.780	2078	2082	2087	rVB	2605	3215	0.31%	0.040%
93	13.963	2107	2112	2116	rBV2	2303	2762	0.27%	0.034%
94	14.128	2137	2139	2144	rVB2	694	803	0.08%	0.010%
95	14.841	2254	2256	2257	rBV2	362	245	0.02%	0.003%
96	14.871	2260	2261	2263	rBV2	457	380	0.04%	0.005%
97	15.548	2371	2372	2373	rBV	719	319	0.03%	0.004%
98	15.615	2381	2383	2385	rBV2	471	366	0.04%	0.005%
99	16.347	2502	2503	2504	rBV	479	233	0.02%	0.003%
100	16.664	2553	2555	2557	rBV3	453	492	0.05%	0.006%




Sum of corrected areas: 8129220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023664.D
Acq On : 12 Aug 2021 10:51
Operator : JC/MD
Sample : VX0812WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK607

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

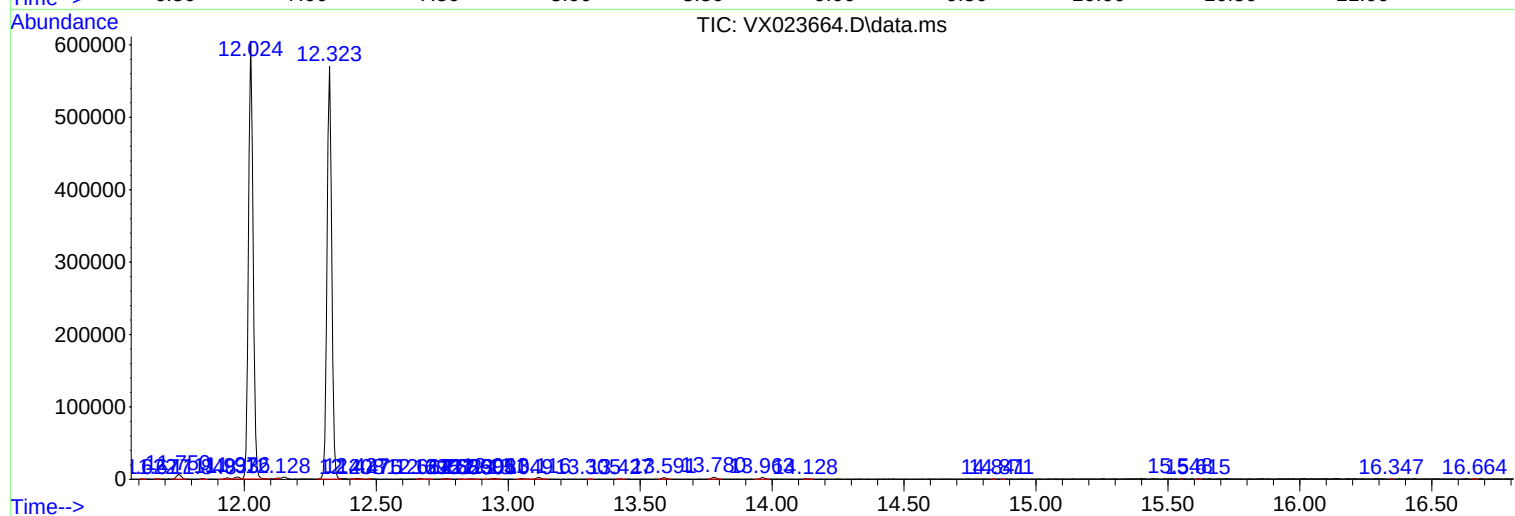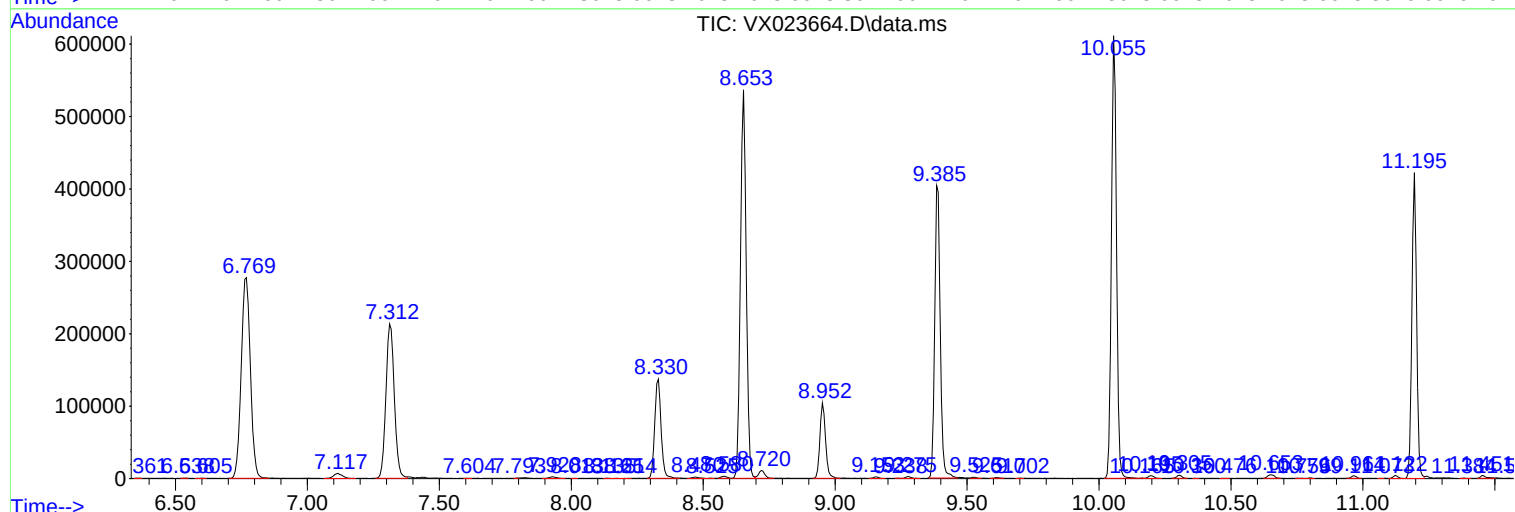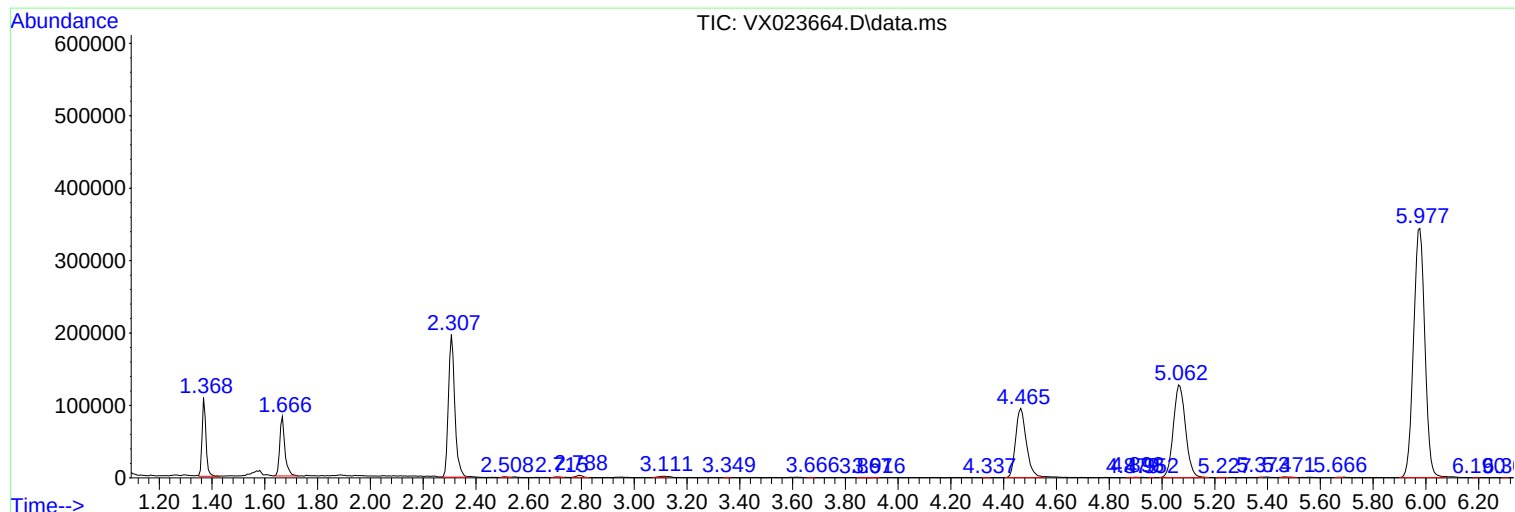

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023664.D
Acq On : 12 Aug 2021 10:51
Operator : JC/MD
Sample : VX0812WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK607

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023664.D
Acq On : 12 Aug 2021 10:51
Operator : JC/MD
Sample : VX0812WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK607

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
