

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023667.D
 Acq On : 12 Aug 2021 12:17
 Operator : JC/MD
 Sample : M3364-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rBV	111751	120414	11.14%	1.452%
2	1.666	90	95	105	rBV	91982	122635	11.34%	1.478%
3	2.306	194	200	209	rBV	217582	357455	33.06%	4.309%
4	2.581	243	245	249	rBV2	348	281	0.03%	0.003%
5	2.635	253	254	258	rBV3	203	270	0.02%	0.003%
6	2.788	277	279	285	rVB2	1387	1671	0.15%	0.020%
7	2.952	298	306	315	rVV2	2873	6774	0.63%	0.082%
8	3.056	317	323	325	rBV3	228	415	0.04%	0.005%
9	3.123	325	334	343	rVV3	25044	57670	5.33%	0.695%
10	3.221	347	350	352	rVB3	291	282	0.03%	0.003%
11	3.465	387	390	395	rBV3	244	467	0.04%	0.006%
12	3.806	444	446	448	rVB	412	311	0.03%	0.004%
13	3.830	448	450	454	rVB2	248	351	0.03%	0.004%
14	3.971	471	473	475	rBV3	254	311	0.03%	0.004%
15	4.263	519	521	524	rVB2	306	289	0.03%	0.003%
16	4.361	533	537	539	rBV2	213	271	0.03%	0.003%
17	4.464	543	554	568	rBV	88258	248624	23.00%	2.997%
18	4.733	595	598	600	rBV2	299	308	0.03%	0.004%
19	4.757	600	602	604	rVB2	344	277	0.03%	0.003%
20	5.068	639	653	667	rBV	136819	424885	39.30%	5.122%
21	5.342	696	698	701	rVB2	318	279	0.03%	0.003%
22	5.379	701	704	705	rBV2	282	329	0.03%	0.004%
23	5.976	788	802	818	rBV2	365393	1081195	100.00%	13.034%
24	6.336	852	861	868	rBV7	1366	4197	0.39%	0.051%
25	6.446	876	879	881	rBV	424	420	0.04%	0.005%
26	6.543	893	895	897	rBV2	359	320	0.03%	0.004%
27	6.769	920	932	948	rBV	305183	723110	66.88%	8.717%
28	6.982	963	967	968	rBV3	299	307	0.03%	0.004%
29	7.037	974	976	979	rVB3	270	278	0.03%	0.003%
30	7.122	982	990	995	rBV3	4240	9729	0.90%	0.117%
31	7.311	1013	1021	1033	rVV	228333	491875	45.49%	5.929%
32	7.482	1046	1049	1054	rVB4	802	1408	0.13%	0.017%
33	7.799	1098	1101	1108	rVB3	540	1005	0.09%	0.012%
34	7.848	1108	1109	1114	rBV3	274	408	0.04%	0.005%
35	7.933	1117	1123	1132	rBV5	1920	4143	0.38%	0.050%
36	8.189	1162	1165	1168	rBV	288	333	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023667.D
 Acq On : 12 Aug 2021 12:17
 Operator : JC/MD
 Sample : M3364-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.329	1181	1188	1199	rBV	133531	217124	20.08%	2.617%
38	8.470	1207	1211	1217	rVB4	1234	2326	0.22%	0.028%
39	8.653	1234	1241	1248	rVV	571781	876803	81.10%	10.570%
40	8.720	1248	1252	1259	rVB	7910	13789	1.28%	0.166%
41	8.951	1284	1290	1302	rBV	100678	148808	13.76%	1.794%
42	9.238	1333	1337	1339	rBV3	404	567	0.05%	0.007%
43	9.274	1339	1343	1350	rVB2	1064	1592	0.15%	0.019%
44	9.390	1355	1362	1375	rBV	381387	562441	52.02%	6.780%
45	9.726	1415	1417	1419	rVB	493	333	0.03%	0.004%
46	9.768	1419	1424	1426	rBV3	348	517	0.05%	0.006%
47	9.921	1448	1449	1452	rVB2	379	356	0.03%	0.004%
48	9.963	1455	1456	1459	rBV3	206	257	0.02%	0.003%
49	10.055	1465	1471	1478	rBV	655551	859063	79.45%	10.356%
50	10.305	1508	1512	1516	rBV3	1559	2007	0.19%	0.024%
51	10.646	1566	1568	1569	rBV2	418	406	0.04%	0.005%
52	10.756	1583	1586	1588	rBV2	194	312	0.03%	0.004%
53	10.957	1617	1619	1623	rVB3	317	439	0.04%	0.005%
54	11.122	1642	1646	1651	rVB2	3539	4310	0.40%	0.052%
55	11.195	1652	1658	1668	rVV	392315	493364	45.63%	5.947%
56	11.280	1670	1672	1675	rVV3	903	1161	0.11%	0.014%
57	11.305	1675	1676	1685	rVB3	1419	2402	0.22%	0.029%
58	11.390	1685	1690	1693	rBV2	480	888	0.08%	0.011%
59	11.451	1698	1700	1701	rBV	629	385	0.04%	0.005%
60	11.548	1713	1716	1723	rVB4	484	718	0.07%	0.009%
61	11.615	1725	1727	1731	rVV3	416	537	0.05%	0.006%
62	11.683	1735	1738	1741	rVB3	536	657	0.06%	0.008%
63	11.719	1741	1744	1745	rBV	400	427	0.04%	0.005%
64	11.750	1745	1749	1756	rVB2	3492	4458	0.41%	0.054%
65	11.847	1761	1765	1768	rVB4	675	844	0.08%	0.010%
66	11.939	1774	1780	1783	rBV5	1801	2520	0.23%	0.030%
67	11.969	1783	1785	1789	rBV3	299	363	0.03%	0.004%
68	12.024	1789	1794	1807	rBV	597568	723516	66.92%	8.722%
69	12.128	1807	1811	1812	rBV4	1125	1434	0.13%	0.017%
70	12.225	1823	1827	1828	rBV3	650	805	0.07%	0.010%
71	12.323	1837	1843	1850	rVB	556283	679263	62.83%	8.188%
72	12.426	1857	1860	1863	rVB4	1229	1327	0.12%	0.016%
73	12.481	1865	1869	1876	rVB4	816	1696	0.16%	0.020%
74	12.579	1884	1885	1887	rVB2	468	267	0.02%	0.003%
75	12.603	1887	1889	1891	rBV	328	357	0.03%	0.004%
76	12.670	1896	1900	1903	rBV3	675	961	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023667.D
 Acq On : 12 Aug 2021 12:17
 Operator : JC/MD
 Sample : M3364-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.768	1909	1916	1917	rBV4	416	687	0.06%	0.008%
78	12.865	1926	1932	1933	rBV3	276	432	0.04%	0.005%
79	12.951	1944	1946	1947	rBV	518	350	0.03%	0.004%
80	13.060	1959	1964	1968	rVV3	530	1004	0.09%	0.012%
81	13.115	1971	1973	1976	rBV3	320	374	0.03%	0.005%
82	13.286	1998	2001	2004	rBV	399	449	0.04%	0.005%
83	13.591	2049	2051	2055	rVB	626	493	0.05%	0.006%
84	13.633	2055	2058	2061	rVB	311	298	0.03%	0.004%
85	13.774	2078	2081	2085	rBV2	618	988	0.09%	0.012%
86	13.871	2094	2097	2101	rBV2	1234	1714	0.16%	0.021%
87	13.969	2106	2113	2114	rBV3	504	748	0.07%	0.009%
88	14.133	2138	2140	2142	rVB3	517	439	0.04%	0.005%
89	14.206	2150	2152	2154	rVB2	315	281	0.03%	0.003%
90	14.438	2188	2190	2193	rBV2	282	446	0.04%	0.005%
91	14.597	2214	2216	2221	rVB3	852	957	0.09%	0.012%
92	14.786	2242	2247	2253	rBV	6522	8579	0.79%	0.103%
93	15.206	2311	2316	2319	rBV2	1133	1763	0.16%	0.021%
94	15.505	2364	2365	2367	rBV	438	330	0.03%	0.004%
95	15.792	2410	2412	2414	rBV2	443	371	0.03%	0.004%
96	16.237	2483	2485	2487	rBV	384	260	0.02%	0.003%
97	16.359	2503	2505	2506	rBV	472	302	0.03%	0.004%
98	16.724	2563	2565	2567	rBV2	563	417	0.04%	0.005%
99	16.749	2567	2569	2570	rBV2	406	310	0.03%	0.004%
100	16.779	2573	2574	2575	rBV	544	380	0.04%	0.005%


Sum of corrected areas: 8295469

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023667.D
Acq On : 12 Aug 2021 12:17
Operator : JC/MD
Sample : M3364-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

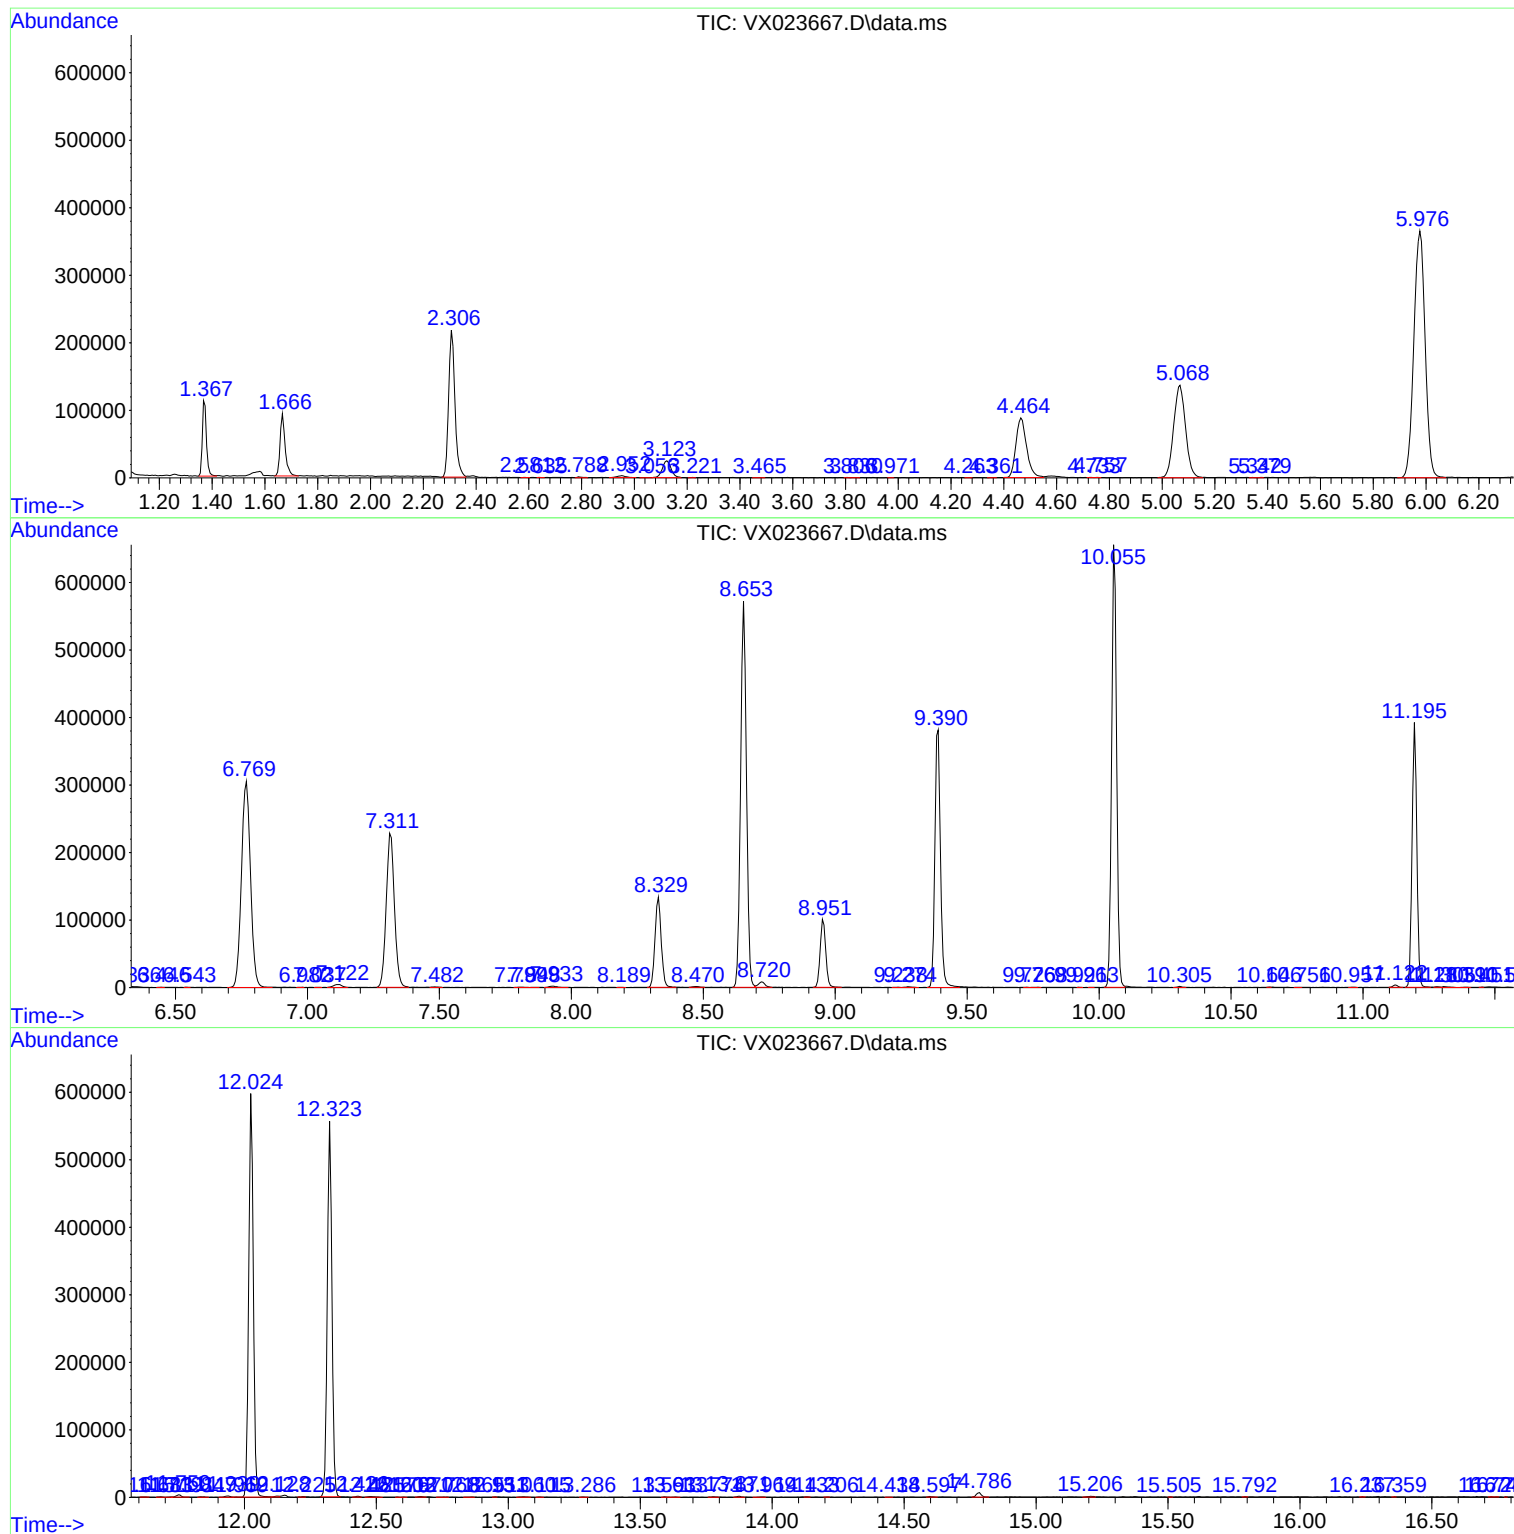

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023667.D
Acq On : 12 Aug 2021 12:17
Operator : JC/MD
Sample : M3364-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023667.D
Acq On : 12 Aug 2021 12:17
Operator : JC/MD
Sample : M3364-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
