

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023671.D
 Acq On : 12 Aug 2021 13:51
 Operator : JC/MD
 Sample : M3364-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

Signal : TIC: VX023671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	34	rBV	9557	16474	1.66%	0.205%
2	1.367	43	46	55	rVB	104493	106420	10.72%	1.321%
3	1.453	57	60	65	rBV	4191	4877	0.49%	0.061%
4	1.666	91	95	103	rVB	81783	107982	10.88%	1.341%
5	2.306	194	200	210	rBV	198190	324829	32.72%	4.033%
6	2.386	210	213	221	rVB	4315	6933	0.70%	0.086%
7	2.508	232	233	236	rBV2	469	349	0.04%	0.004%
8	2.794	275	280	286	rVB4	643	1172	0.12%	0.015%
9	2.946	298	305	315	rBV	4992	11751	1.18%	0.146%
10	3.227	350	351	355	rBV2	247	372	0.04%	0.005%
11	3.501	394	396	397	rVV	300	240	0.02%	0.003%
12	3.666	421	423	426	rBV2	210	303	0.03%	0.004%
13	3.837	449	451	452	rBV	319	268	0.03%	0.003%
14	4.221	510	514	515	rBV3	374	522	0.05%	0.006%
15	4.343	531	534	535	rBV3	309	341	0.03%	0.004%
16	4.464	543	554	567	rBV	85962	244992	24.68%	3.042%
17	4.696	590	592	595	rVB3	406	379	0.04%	0.005%
18	5.068	640	653	673	rBV	128550	391891	39.48%	4.866%
19	5.269	681	686	689	rBV2	342	539	0.05%	0.007%
20	5.483	718	721	722	rBV2	372	248	0.02%	0.003%
21	5.562	730	734	737	rBV	554	1068	0.11%	0.013%
22	5.647	746	748	751	rBV2	311	350	0.04%	0.004%
23	5.854	780	782	785	rVB2	355	295	0.03%	0.004%
24	5.976	790	802	817	rBV2	337909	992629	100.00%	12.325%
25	6.226	841	843	847	rVB2	288	305	0.03%	0.004%
26	6.428	873	876	881	rBV2	289	385	0.04%	0.005%
27	6.610	903	906	911	rBV2	261	478	0.05%	0.006%
28	6.769	922	932	946	rVV	309897	732068	73.75%	9.089%
29	6.891	950	952	954	rVV2	330	280	0.03%	0.003%
30	6.909	954	955	959	rVV2	295	351	0.04%	0.004%
31	6.958	961	963	966	rBV2	220	248	0.02%	0.003%
32	7.055	977	979	980	rBV	365	239	0.02%	0.003%
33	7.116	983	989	999	rVV4	3939	8845	0.89%	0.110%
34	7.318	1012	1022	1036	rBV	205839	458635	46.20%	5.694%
35	7.482	1044	1049	1052	rVV3	914	1557	0.16%	0.019%
36	7.720	1085	1088	1090	rBV2	196	232	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023671.D
 Acq On : 12 Aug 2021 13:51
 Operator : JC/MD
 Sample : M3364-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.805	1099	1102	1103	rBV2	320	396	0.04%	0.005%
38	7.818	1103	1104	1112	rVB2	939	991	0.10%	0.012%
39	7.885	1112	1115	1117	rBV3	285	324	0.03%	0.004%
40	7.933	1117	1123	1129	rBV3	2084	3859	0.39%	0.048%
41	8.013	1133	1136	1139	rBV	161	263	0.03%	0.003%
42	8.122	1150	1154	1156	rBV3	286	344	0.03%	0.004%
43	8.226	1169	1171	1177	rBV3	243	464	0.05%	0.006%
44	8.330	1182	1188	1200	rBV	136530	217262	21.89%	2.698%
45	8.470	1208	1211	1218	rVB5	1592	2591	0.26%	0.032%
46	8.653	1234	1241	1248	rBV	525773	805923	81.19%	10.006%
47	8.726	1248	1253	1259	rVB	7680	12486	1.26%	0.155%
48	8.951	1284	1290	1298	rBV	96071	143752	14.48%	1.785%
49	9.390	1356	1362	1375	rVV	397359	556101	56.02%	6.905%
50	9.805	1428	1430	1432	rVB2	268	237	0.02%	0.003%
51	9.835	1432	1435	1437	rBV	214	251	0.03%	0.003%
52	9.866	1439	1440	1442	rVV	315	245	0.02%	0.003%
53	9.896	1444	1445	1449	rVB	401	248	0.02%	0.003%
54	10.055	1465	1471	1482	rBV	646072	879424	88.60%	10.919%
55	10.305	1509	1512	1515	rVB2	1372	1418	0.14%	0.018%
56	10.585	1556	1558	1560	rVB	485	272	0.03%	0.003%
57	10.646	1564	1568	1569	rBV4	542	437	0.04%	0.005%
58	10.799	1590	1593	1595	rBV2	210	287	0.03%	0.004%
59	11.122	1642	1646	1652	rBV2	2860	4021	0.41%	0.050%
60	11.195	1653	1658	1667	rVV	403743	502107	50.58%	6.234%
61	11.366	1683	1686	1687	rBV2	257	237	0.02%	0.003%
62	11.451	1698	1700	1702	rVV2	696	552	0.06%	0.007%
63	11.488	1702	1706	1712	rVB3	884	1513	0.15%	0.019%
64	11.750	1746	1749	1754	rVB4	2955	4097	0.41%	0.051%
65	11.847	1762	1765	1769	rVB2	786	980	0.10%	0.012%
66	11.933	1776	1779	1782	rBV2	1844	1858	0.19%	0.023%
67	12.024	1789	1794	1805	rBV	633539	785026	79.09%	9.747%
68	12.128	1805	1811	1812	rBV4	1568	1980	0.20%	0.025%
69	12.225	1824	1827	1830	rVB4	551	774	0.08%	0.010%
70	12.323	1836	1843	1853	rBV	556456	689889	69.50%	8.566%
71	12.426	1858	1860	1864	rVV2	993	1147	0.12%	0.014%
72	12.481	1867	1869	1874	rVV3	654	745	0.08%	0.009%
73	12.530	1876	1877	1881	rVB	328	327	0.03%	0.004%
74	12.585	1881	1886	1888	rBV	226	323	0.03%	0.004%
75	12.664	1895	1899	1903	rBV4	672	1166	0.12%	0.014%
76	12.756	1911	1914	1919	rBV2	457	655	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023671.D
 Acq On : 12 Aug 2021 13:51
 Operator : JC/MD
 Sample : M3364-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBK97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.823	1922	1925	1928	rBV2	357	439	0.04%	0.005%
78	12.859	1928	1931	1937	rVB3	653	916	0.09%	0.011%
79	12.963	1944	1948	1951	rVB2	353	464	0.05%	0.006%
80	13.000	1951	1954	1957	rBV	346	353	0.04%	0.004%
81	13.054	1959	1963	1964	rBV3	497	624	0.06%	0.008%
82	13.262	1995	1997	1999	rBV	423	257	0.03%	0.003%
83	13.323	2005	2007	2009	rVB	323	307	0.03%	0.004%
84	13.426	2019	2024	2026	rBV2	270	363	0.04%	0.005%
85	13.591	2049	2051	2052	rBV	439	257	0.03%	0.003%
86	13.627	2055	2057	2059	rBV	382	364	0.04%	0.005%
87	13.780	2080	2082	2086	rVB3	647	600	0.06%	0.007%
88	13.823	2086	2089	2092	rBV2	311	411	0.04%	0.005%
89	13.877	2095	2098	2100	rVB2	423	458	0.05%	0.006%
90	13.951	2109	2110	2113	rVB2	468	396	0.04%	0.005%
91	14.091	2131	2133	2136	rVB2	362	293	0.03%	0.004%
92	14.121	2136	2138	2140	rBV	322	376	0.04%	0.005%
93	14.286	2164	2165	2168	rVB2	363	319	0.03%	0.004%
94	14.438	2187	2190	2192	rBV2	291	363	0.04%	0.005%
95	14.566	2210	2211	2215	rBV2	335	328	0.03%	0.004%
96	14.877	2258	2262	2266	rBV2	482	629	0.06%	0.008%
97	14.969	2275	2277	2279	rBV2	297	247	0.02%	0.003%
98	15.950	2436	2438	2440	rBV2	377	258	0.03%	0.003%
99	16.072	2456	2458	2461	rBV4	423	364	0.04%	0.005%
100	16.371	2504	2507	2512	rBV3	498	801	0.08%	0.010%

Sum of corrected areas: 8054006




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023671.D
Acq On : 12 Aug 2021 13:51
Operator : JC/MD
Sample : M3364-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

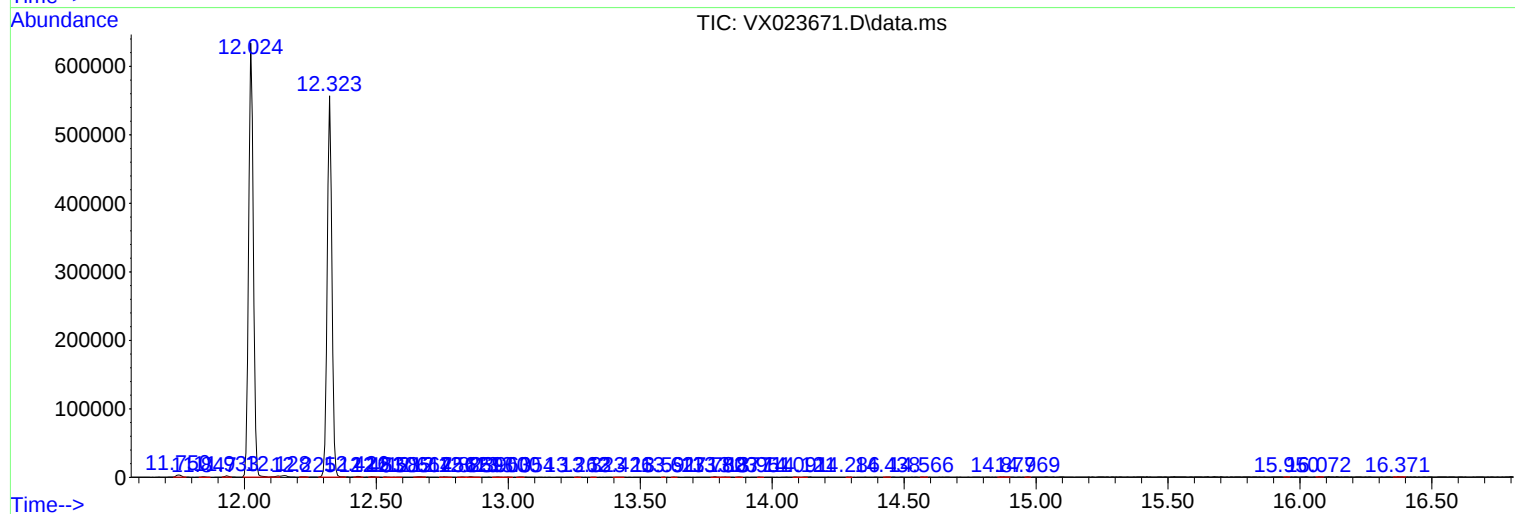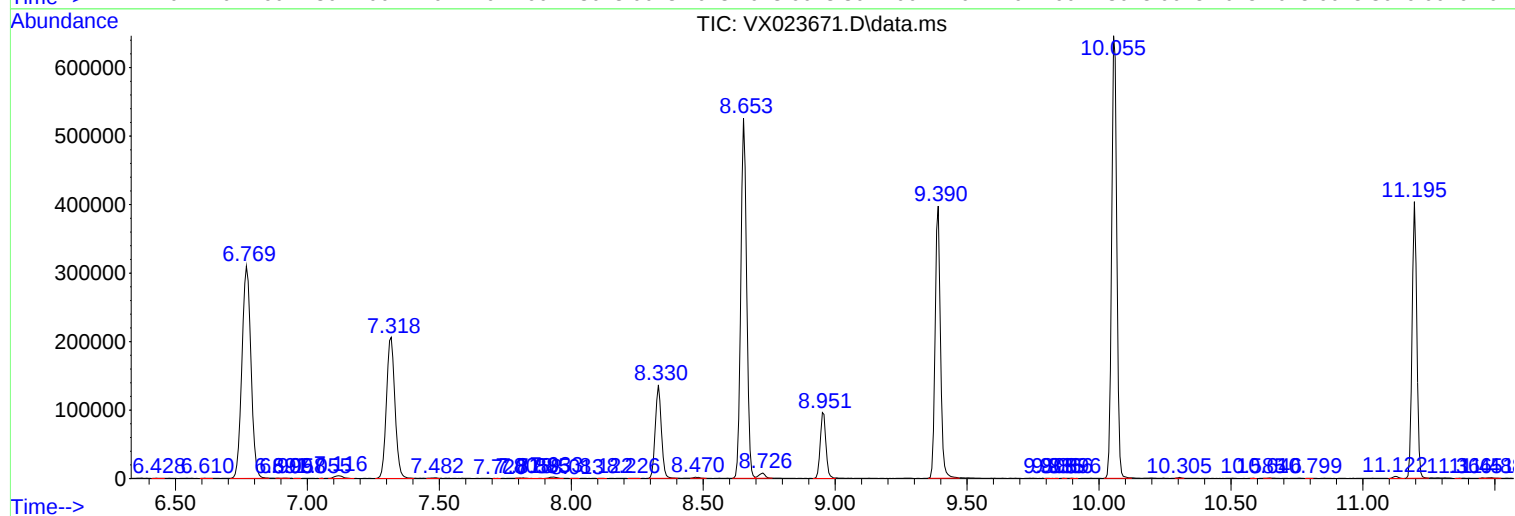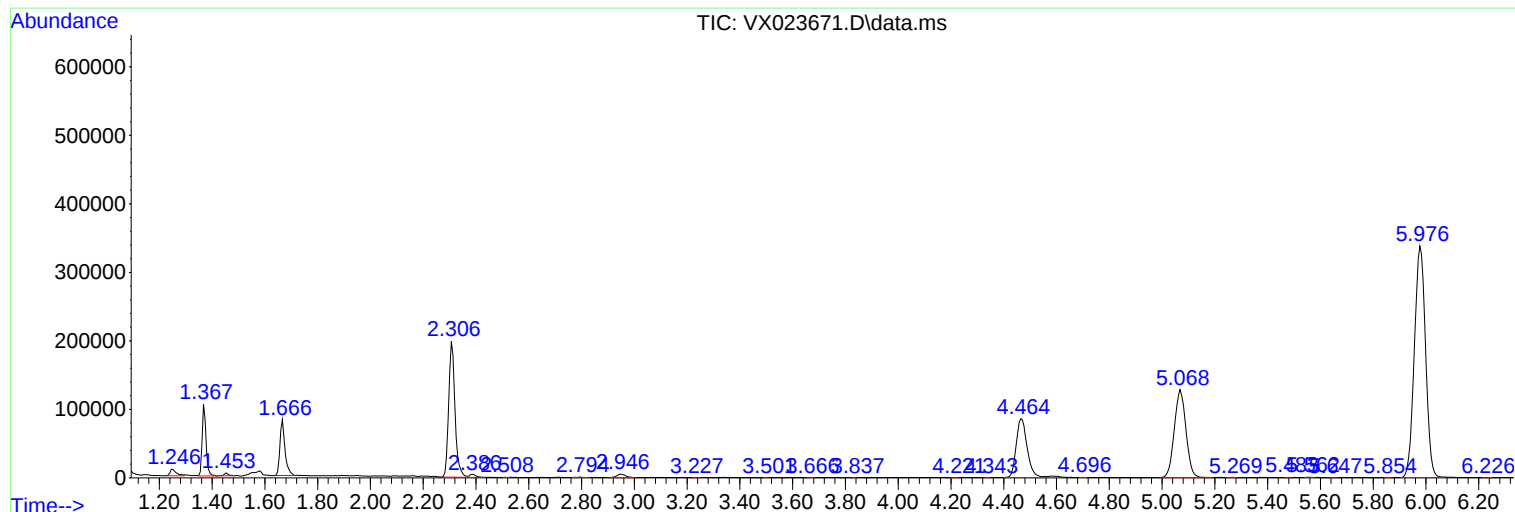

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023671.D
Acq On : 12 Aug 2021 13:51
Operator : JC/MD
Sample : M3364-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023671.D
Acq On : 12 Aug 2021 13:51
Operator : JC/MD
Sample : M3364-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBK97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
