

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023674.D
 Acq On : 12 Aug 2021 15:01
 Operator : JC/MD
 Sample : M3364-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBKA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M

Title : VOC Analysis

Signal : TIC: VX023674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV2	6158	7751	0.77%	0.096%
2	1.368	43	46	52	rVB	102682	106158	10.52%	1.314%
3	1.666	91	95	105	rVB	82531	109683	10.87%	1.358%
4	2.306	194	200	210	rBV	194903	327793	32.48%	4.058%
5	2.386	210	213	220	rVB	5671	9690	0.96%	0.120%
6	2.556	235	241	248	rVB4	1042	2476	0.25%	0.031%
7	2.611	248	250	255	rBV3	340	635	0.06%	0.008%
8	2.800	276	281	285	rVB3	805	1203	0.12%	0.015%
9	3.318	363	366	368	rBV3	441	556	0.06%	0.007%
10	3.373	374	375	378	rBV2	338	310	0.03%	0.004%
11	3.763	432	439	441	rBV	1297	2312	0.23%	0.029%
12	4.465	545	554	569	rBV	86786	242612	24.04%	3.004%
13	4.690	590	591	594	rVB	486	376	0.04%	0.005%
14	4.733	596	598	603	rVB3	379	566	0.06%	0.007%
15	4.885	621	623	626	rBV	275	304	0.03%	0.004%
16	5.068	640	653	667	rBV	130953	401911	39.82%	4.976%
17	5.251	682	683	688	rVB	430	328	0.03%	0.004%
18	5.428	710	712	715	rVB2	298	307	0.03%	0.004%
19	5.550	729	732	734	rBV3	453	564	0.06%	0.007%
20	5.976	788	802	819	rBV2	345732	1009339	100.00%	12.497%
21	6.543	892	895	896	rBV2	310	347	0.03%	0.004%
22	6.629	907	909	914	rVV3	507	692	0.07%	0.009%
23	6.769	922	932	944	rBV	316207	743670	73.68%	9.207%
24	7.110	983	988	998	rBV4	4238	9525	0.94%	0.118%
25	7.318	1010	1022	1035	rBV	216056	466830	46.25%	5.780%
26	7.482	1043	1049	1057	rBV4	719	1763	0.17%	0.022%
27	7.586	1062	1066	1074	rVB5	548	1188	0.12%	0.015%
28	7.763	1092	1095	1098	rBV3	270	312	0.03%	0.004%
29	7.812	1098	1103	1108	rBV2	794	1412	0.14%	0.017%
30	7.927	1116	1122	1127	rBV5	2140	4314	0.43%	0.053%
31	8.098	1146	1150	1154	rBV3	279	367	0.04%	0.005%
32	8.330	1181	1188	1197	rBV	132017	216749	21.47%	2.684%
33	8.397	1197	1199	1201	rVB3	533	414	0.04%	0.005%
34	8.476	1208	1212	1215	rVB3	1809	2285	0.23%	0.028%
35	8.586	1225	1230	1232	rBV4	419	634	0.06%	0.008%
36	8.653	1234	1241	1249	rVV	542465	820873	81.33%	10.163%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023674.D
 Acq On : 12 Aug 2021 15:01
 Operator : JC/MD
 Sample : M3364-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBKA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	8.726	1249	1253	1260	rVB	8183	13309	1.32%	0.165%
38	8.824	1267	1269	1271	rBV	402	326	0.03%	0.004%
39	8.952	1285	1290	1299	rBV	99221	144253	14.29%	1.786%
40	9.147	1318	1322	1325	rBV3	323	511	0.05%	0.006%
41	9.281	1337	1344	1349	rBV	1963	3295	0.33%	0.041%
42	9.391	1356	1362	1376	rBV	382469	547677	54.26%	6.781%
43	9.519	1381	1383	1388	rVB4	2474	3597	0.36%	0.045%
44	9.634	1398	1402	1404	rBV	340	440	0.04%	0.005%
45	9.768	1420	1424	1425	rVB2	297	316	0.03%	0.004%
46	10.055	1465	1471	1487	rVV	643965	889826	88.16%	11.017%
47	10.195	1492	1494	1499	rVB3	950	1372	0.14%	0.017%
48	10.238	1499	1501	1503	rBV	506	456	0.05%	0.006%
49	10.305	1509	1512	1517	rVB3	944	1196	0.12%	0.015%
50	10.415	1527	1530	1532	rBV3	348	412	0.04%	0.005%
51	10.482	1540	1541	1546	rBV2	243	313	0.03%	0.004%
52	10.646	1566	1568	1572	rVB	699	758	0.08%	0.009%
53	10.689	1572	1575	1578	rBV2	261	402	0.04%	0.005%
54	10.860	1600	1603	1608	rVB3	1042	1293	0.13%	0.016%
55	10.963	1616	1620	1622	rBV3	291	460	0.05%	0.006%
56	11.024	1627	1630	1633	rBV2	226	371	0.04%	0.005%
57	11.122	1643	1646	1650	rVB3	3465	4143	0.41%	0.051%
58	11.195	1652	1658	1669	rBV	406964	491946	48.74%	6.091%
59	11.317	1675	1678	1685	rVB4	2095	3310	0.33%	0.041%
60	11.457	1700	1701	1702	rBV	482	288	0.03%	0.004%
61	11.482	1702	1705	1714	rVB3	1223	1885	0.19%	0.023%
62	11.549	1714	1716	1720	rVB2	599	576	0.06%	0.007%
63	11.750	1746	1749	1756	rVB2	3370	4313	0.43%	0.053%
64	11.841	1761	1764	1769	rVB4	691	984	0.10%	0.012%
65	11.933	1773	1779	1782	rBV4	1919	2534	0.25%	0.031%
66	12.024	1789	1794	1801	rBV	620227	765643	75.86%	9.479%
67	12.128	1806	1811	1813	rBV4	1636	2688	0.27%	0.033%
68	12.152	1813	1815	1818	rVB3	2836	2787	0.28%	0.035%
69	12.225	1823	1827	1831	rBV4	1370	1973	0.20%	0.024%
70	12.323	1836	1843	1850	rBV	534493	664585	65.84%	8.228%
71	12.427	1857	1860	1863	rBV3	1000	1271	0.13%	0.016%
72	12.475	1864	1868	1876	rVB4	612	1234	0.12%	0.015%
73	12.573	1881	1884	1888	rBV2	441	781	0.08%	0.010%
74	12.762	1912	1915	1918	rBV4	664	832	0.08%	0.010%
75	12.823	1923	1925	1926	rBV2	428	332	0.03%	0.004%
76	12.969	1948	1949	1951	rVB	536	295	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023674.D
 Acq On : 12 Aug 2021 15:01
 Operator : JC/MD
 Sample : M3364-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DBKA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	13.054	1959	1963	1966	rBV2	878	1067	0.11%	0.013%
78	13.304	2001	2004	2007	rBV	263	313	0.03%	0.004%
79	13.402	2018	2020	2024	rBV2	306	387	0.04%	0.005%
80	13.597	2050	2052	2055	rVB	401	317	0.03%	0.004%
81	13.701	2066	2069	2071	rBV	374	326	0.03%	0.004%
82	13.780	2076	2082	2086	rBV	3592	4500	0.45%	0.056%
83	13.865	2093	2096	2099	rBV3	390	501	0.05%	0.006%
84	13.938	2105	2108	2109	rBV3	408	395	0.04%	0.005%
85	13.993	2115	2117	2119	rBV2	300	314	0.03%	0.004%
86	14.444	2189	2191	2195	rBV3	399	562	0.06%	0.007%
87	14.554	2206	2209	2214	rBV3	201	364	0.04%	0.005%
88	14.621	2217	2220	2222	rBV3	473	593	0.06%	0.007%
89	14.780	2242	2246	2250	rBV2	1167	1981	0.20%	0.025%
90	14.841	2255	2256	2258	rBV	334	301	0.03%	0.004%
91	15.207	2314	2316	2319	rBV2	490	546	0.05%	0.007%
92	15.347	2337	2339	2342	rBV3	633	640	0.06%	0.008%
93	15.426	2349	2352	2354	rBV3	384	421	0.04%	0.005%
94	15.469	2358	2359	2362	rBV2	410	394	0.04%	0.005%
95	15.737	2401	2403	2407	rBV3	526	643	0.06%	0.008%
96	15.865	2423	2424	2426	rBV2	517	371	0.04%	0.005%
97	15.999	2444	2446	2447	rBV	749	460	0.05%	0.006%
98	16.030	2447	2451	2452	rVV2	467	485	0.05%	0.006%
99	16.597	2540	2544	2545	rBV	393	520	0.05%	0.006%
100	16.688	2556	2559	2563	rBV3	797	1285	0.13%	0.016%




Sum of corrected areas: 8076918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023674.D
Acq On : 12 Aug 2021 15:01
Operator : JC/MD
Sample : M3364-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBKA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

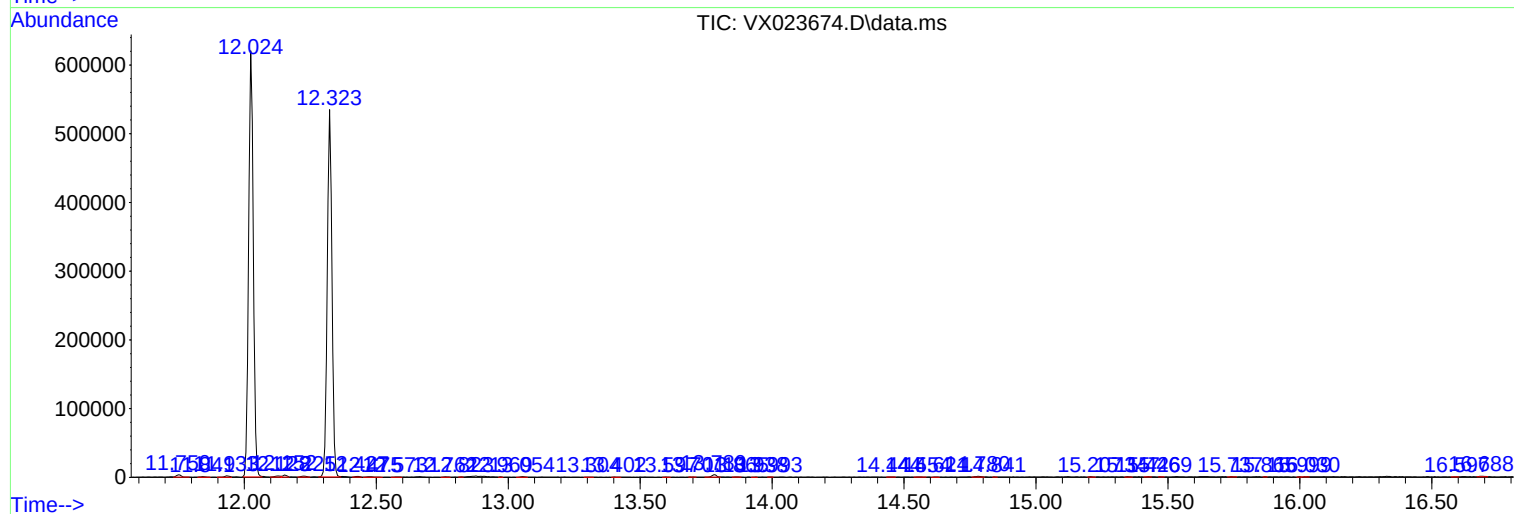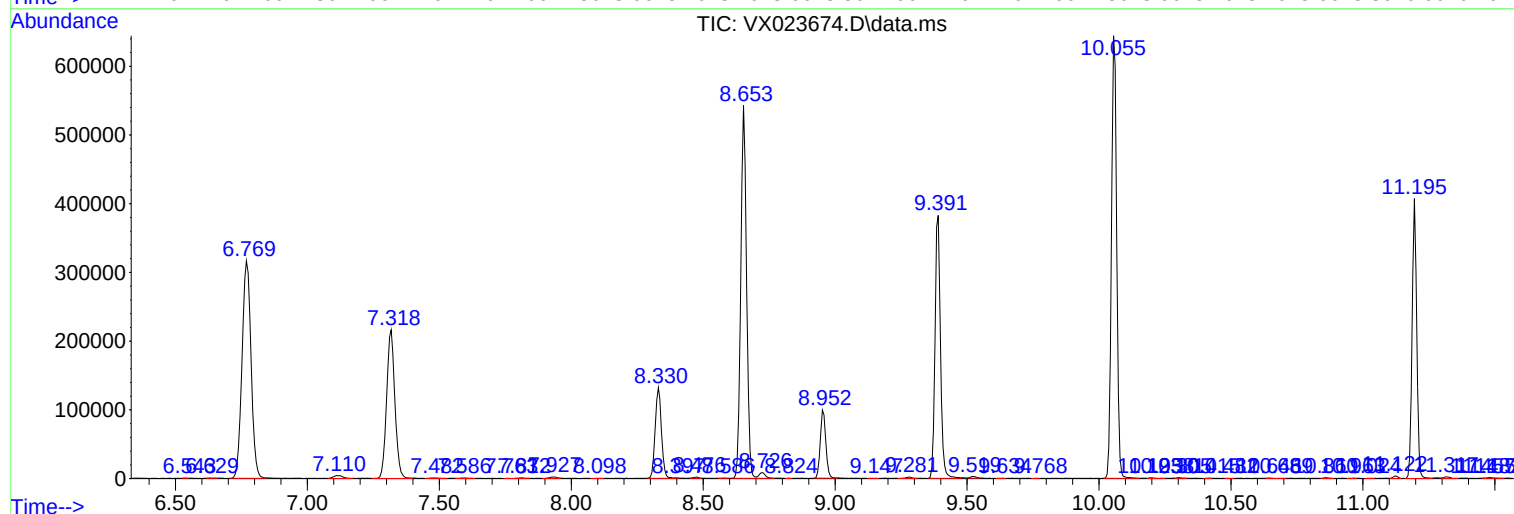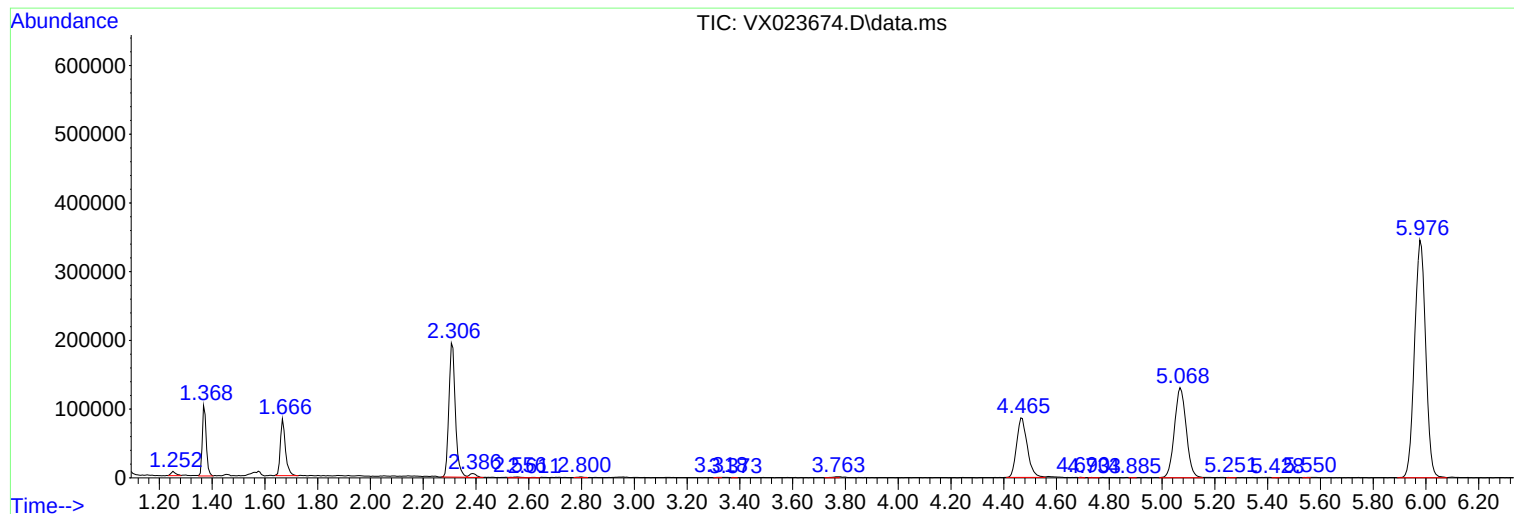

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023674.D
Acq On : 12 Aug 2021 15:01
Operator : JC/MD
Sample : M3364-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBKA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023674.D
Acq On : 12 Aug 2021 15:01
Operator : JC/MD
Sample : M3364-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DBKA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
