

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023675.D
 Acq On : 12 Aug 2021 15:35
 Operator : JC/MD
 Sample : M3364-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

Signal : TIC: VX023675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	101113	104365	10.53%	1.314%
2	1.666	90	95	106	rBV	82578	111753	11.27%	1.407%
3	2.306	194	200	211	rBV	199094	321093	32.39%	4.043%
4	2.514	233	234	237	rBV2	406	390	0.04%	0.005%
5	2.794	274	280	288	rVB3	3874	7040	0.71%	0.089%
6	3.008	314	315	317	rBV	407	290	0.03%	0.004%
7	3.117	331	333	339	rBV2	265	390	0.04%	0.005%
8	3.178	340	343	344	rBV2	281	242	0.02%	0.003%
9	3.337	365	369	370	rBV2	257	241	0.02%	0.003%
10	3.526	396	400	402	rVB2	225	306	0.03%	0.004%
11	3.934	466	467	471	rBV2	291	389	0.04%	0.005%
12	4.007	475	479	481	rVV3	245	390	0.04%	0.005%
13	4.172	504	506	508	rBV2	389	231	0.02%	0.003%
14	4.306	522	528	529	rBV2	248	287	0.03%	0.004%
15	4.465	544	554	569	rBV	83382	237241	23.93%	2.987%
16	4.690	589	591	594	rVB2	265	262	0.03%	0.003%
17	5.068	640	653	668	rBV	125116	394291	39.77%	4.965%
18	5.294	686	690	692	rBV2	238	261	0.03%	0.003%
19	5.477	718	720	725	rVB3	246	304	0.03%	0.004%
20	5.519	725	727	728	rBV	271	225	0.02%	0.003%
21	5.653	746	749	751	rVB	296	273	0.03%	0.003%
22	5.800	771	773	776	rVV2	184	241	0.02%	0.003%
23	5.977	790	802	817	rVV2	336579	991306	100.00%	12.482%
24	6.123	824	826	830	rVB2	343	404	0.04%	0.005%
25	6.166	830	833	838	rVB3	299	441	0.04%	0.006%
26	6.257	846	848	852	rBV2	256	287	0.03%	0.004%
27	6.464	879	882	886	rVV3	403	518	0.05%	0.007%
28	6.763	921	931	946	rBV	299275	711182	71.74%	8.955%
29	7.110	982	988	997	rVB2	5643	11228	1.13%	0.141%
30	7.184	997	1000	1002	rBV2	214	226	0.02%	0.003%
31	7.312	1012	1021	1034	rVV	213046	461218	46.53%	5.808%
32	7.403	1034	1036	1039	rVB3	450	390	0.04%	0.005%
33	7.525	1055	1056	1061	rBV2	187	286	0.03%	0.004%
34	7.610	1067	1070	1075	rBV2	375	498	0.05%	0.006%
35	7.763	1090	1095	1097	rBV2	318	645	0.07%	0.008%
36	7.799	1097	1101	1105	rBV2	447	849	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023675.D
 Acq On : 12 Aug 2021 15:35
 Operator : JC/MD
 Sample : M3364-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

37	7.927	1118	1122	1127	rVB4	1760	3190	0.32%	0.040%
38	8.196	1164	1166	1169	rVB2	276	287	0.03%	0.004%
39	8.330	1181	1188	1199	rBV	133832	217187	21.91%	2.735%
40	8.470	1206	1211	1216	rBV4	1682	2809	0.28%	0.035%
41	8.537	1219	1222	1225	rBV3	384	379	0.04%	0.005%
42	8.580	1225	1229	1231	rBV2	243	262	0.03%	0.003%
43	8.653	1234	1241	1249	rBV	522346	814011	82.12%	10.250%
44	8.720	1249	1252	1256	rVB	7184	10367	1.05%	0.131%
45	8.811	1265	1267	1271	rVB	477	498	0.05%	0.006%
46	8.952	1284	1290	1300	rBV	99310	144905	14.62%	1.825%
47	9.384	1356	1361	1378	rBV	372405	542098	54.69%	6.826%
48	9.842	1434	1436	1440	rVB2	289	293	0.03%	0.004%
49	10.055	1465	1471	1490	rVV	653696	870437	87.81%	10.960%
50	10.305	1509	1512	1516	rVB	734	932	0.09%	0.012%
51	10.860	1601	1603	1605	rVB	263	243	0.02%	0.003%
52	10.878	1605	1606	1609	rBV2	324	303	0.03%	0.004%
53	10.939	1611	1616	1618	rBV	251	309	0.03%	0.004%
54	10.970	1618	1621	1622	rBV2	412	301	0.03%	0.004%
55	11.091	1637	1641	1642	rBV2	284	267	0.03%	0.003%
56	11.122	1642	1646	1652	rVB3	3226	3940	0.40%	0.050%
57	11.195	1652	1658	1666	rBV	386741	492817	49.71%	6.205%
58	11.268	1669	1670	1675	rVV4	578	737	0.07%	0.009%
59	11.384	1686	1689	1691	rVV3	325	277	0.03%	0.003%
60	11.445	1697	1699	1700	rBV	510	332	0.03%	0.004%
61	11.476	1700	1704	1707	rVV5	949	1544	0.16%	0.019%
62	11.506	1707	1709	1712	rVV3	711	587	0.06%	0.007%
63	11.543	1712	1715	1716	rVV2	318	271	0.03%	0.003%
64	11.585	1719	1722	1725	rVB2	252	319	0.03%	0.004%
65	11.677	1735	1737	1739	rBV3	199	266	0.03%	0.003%
66	11.750	1745	1749	1755	rVB3	2703	3728	0.38%	0.047%
67	11.841	1762	1764	1770	rVB3	575	860	0.09%	0.011%
68	11.939	1773	1780	1784	rBV3	1498	2168	0.22%	0.027%
69	11.975	1784	1786	1789	rBV2	446	438	0.04%	0.006%
70	12.024	1789	1794	1804	rBV	627014	766935	77.37%	9.657%
71	12.134	1806	1812	1813	rBV3	1212	2115	0.21%	0.027%
72	12.323	1837	1843	1853	rVB	547208	681196	68.72%	8.578%
73	12.433	1856	1861	1864	rBV4	1111	1479	0.15%	0.019%
74	12.609	1887	1890	1893	rVV2	512	712	0.07%	0.009%
75	12.664	1896	1899	1902	rVV3	721	826	0.08%	0.010%
76	12.725	1908	1909	1912	rBV	285	239	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023675.D
 Acq On : 12 Aug 2021 15:35
 Operator : JC/MD
 Sample : M3364-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
 Title : VOC Analysis

77	12.768	1912	1916	1920	rVB4	548	831	0.08%	0.010%
78	12.859	1928	1931	1934	rBV2	571	735	0.07%	0.009%
79	12.951	1944	1946	1949	rBV2	267	246	0.02%	0.003%
80	13.055	1959	1963	1967	rVB4	617	930	0.09%	0.012%
81	13.244	1992	1994	1996	rBV2	267	295	0.03%	0.004%
82	13.304	2001	2004	2005	rVB3	279	257	0.03%	0.003%
83	13.445	2026	2027	2031	rVB2	279	243	0.02%	0.003%
84	13.487	2031	2034	2038	rBV2	406	535	0.05%	0.007%
85	13.530	2038	2041	2044	rBV2	276	350	0.04%	0.004%
86	13.591	2048	2051	2053	rVV2	230	263	0.03%	0.003%
87	13.780	2079	2082	2085	rVV4	590	734	0.07%	0.009%
88	13.896	2098	2101	2102	rBV2	207	259	0.03%	0.003%
89	13.975	2111	2114	2115	rBV2	304	359	0.04%	0.005%
90	14.140	2137	2141	2144	rVB4	468	772	0.08%	0.010%
91	14.286	2162	2165	2167	rVB2	280	322	0.03%	0.004%
92	14.317	2167	2170	2174	rBV3	267	483	0.05%	0.006%
93	14.737	2237	2239	2244	rVB4	422	402	0.04%	0.005%
94	14.774	2244	2245	2248	rBV2	274	271	0.03%	0.003%
95	14.908	2265	2267	2269	rBV	329	228	0.02%	0.003%
96	15.999	2444	2446	2449	rVB4	441	459	0.05%	0.006%
97	16.030	2449	2451	2453	rBV	600	421	0.04%	0.005%
98	16.054	2453	2455	2457	rBV3	428	419	0.04%	0.005%
99	16.267	2489	2490	2492	rBV	447	354	0.04%	0.004%
100	16.658	2552	2554	2558	rBV3	394	616	0.06%	0.008%


Sum of corrected areas: 7941631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023675.D
Acq On : 12 Aug 2021 15:35
Operator : JC/MD
Sample : M3364-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

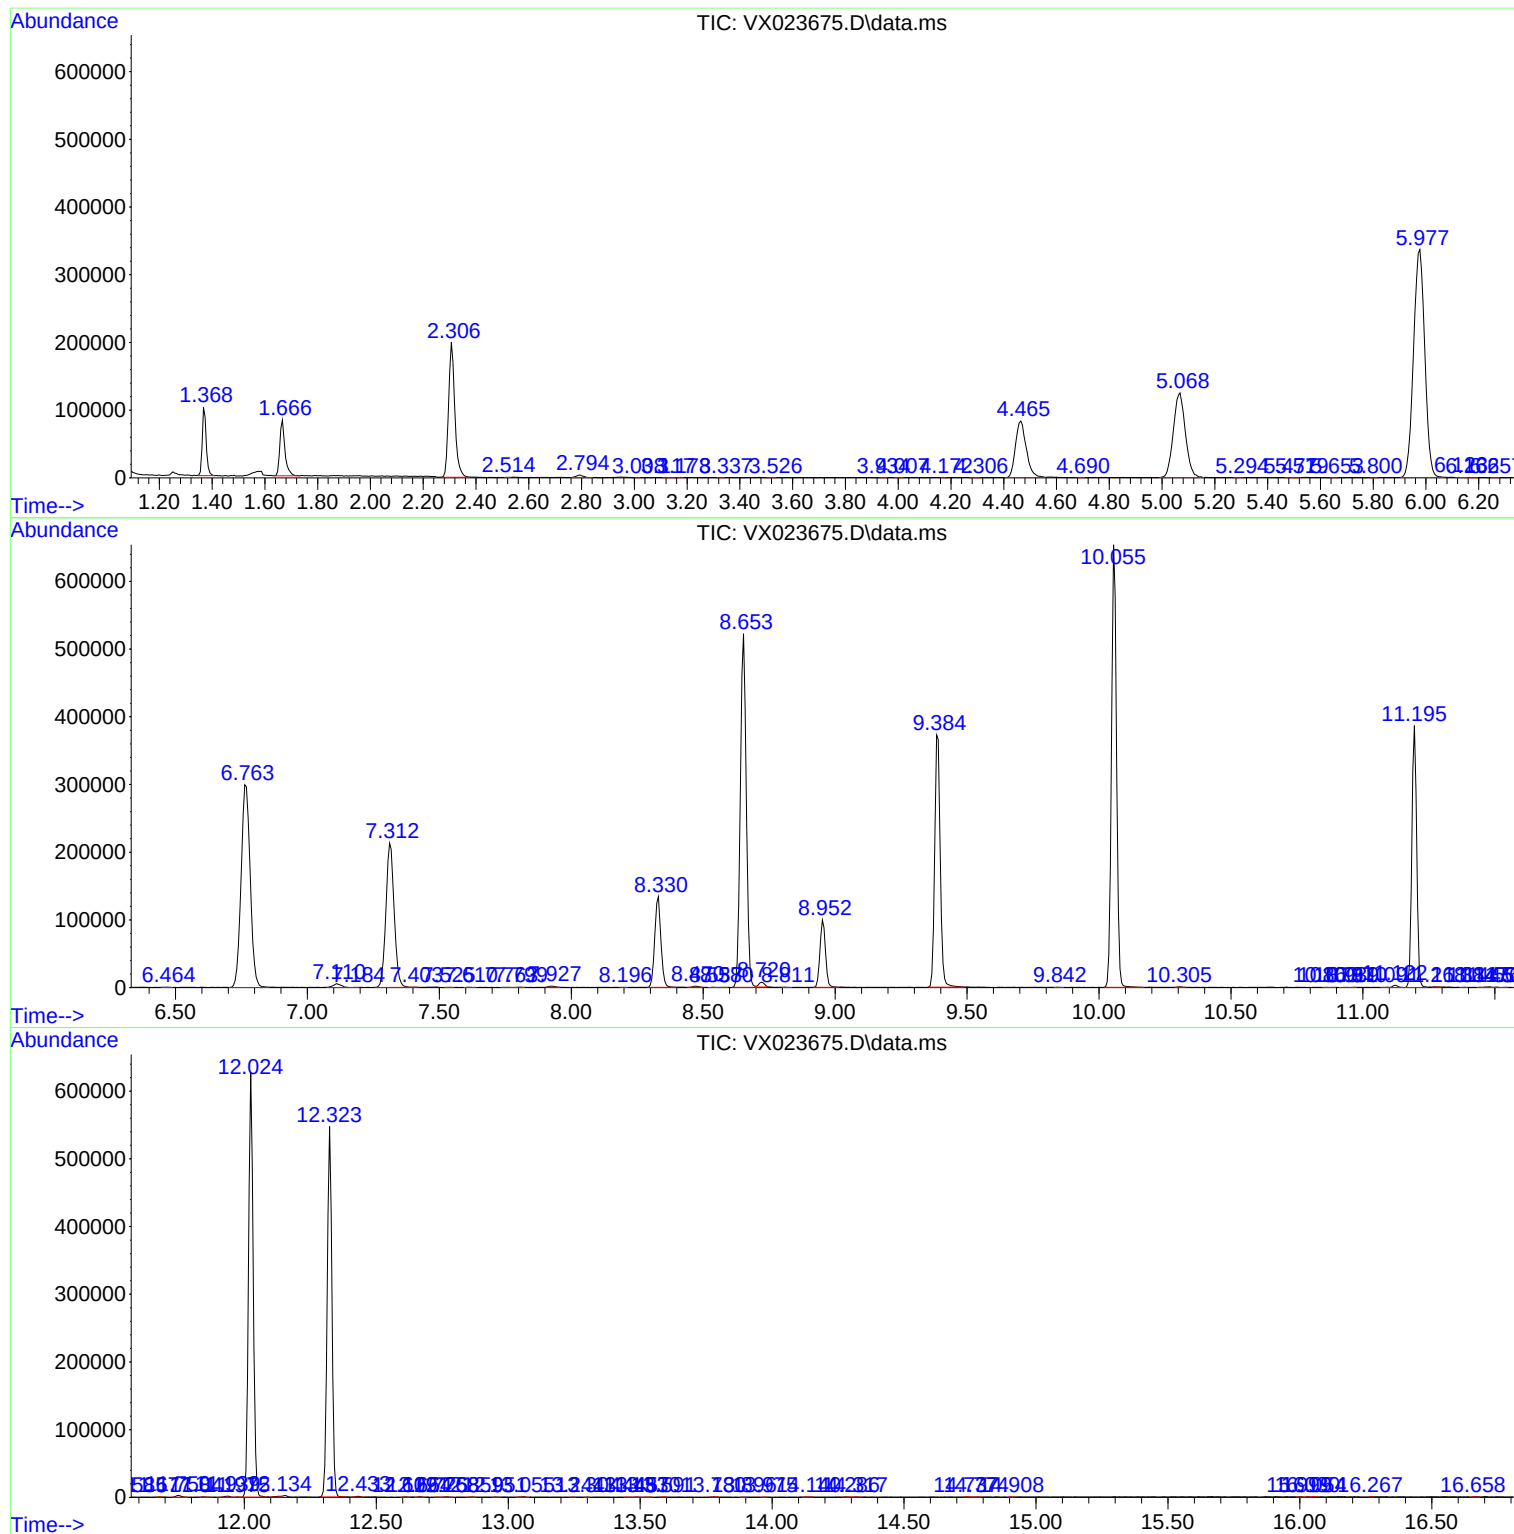

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023675.D
Acq On : 12 Aug 2021 15:35
Operator : JC/MD
Sample : M3364-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
Data File : VX023675.D
Acq On : 12 Aug 2021 15:35
Operator : JC/MD
Sample : M3364-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML081121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
