
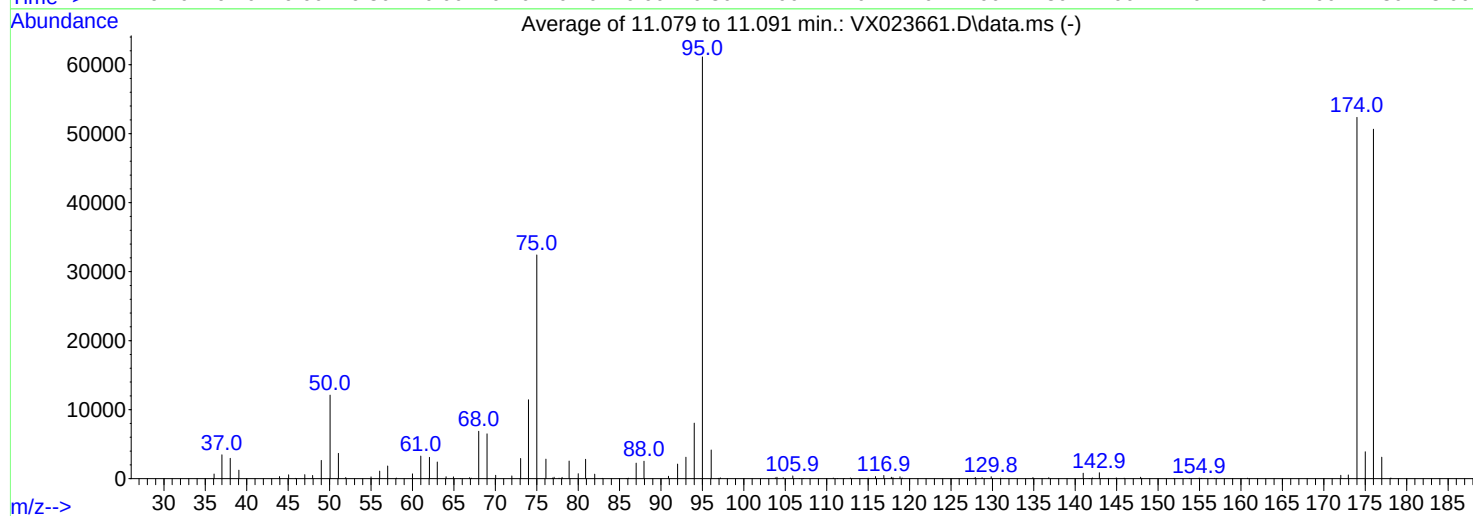


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081221\
 Data File : VX023661.D
 Acq On : 12 Aug 2021 08:54
 Operator : JC/MD
 Sample : BFB603
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB603

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM081121WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 13 01:00:38 2021

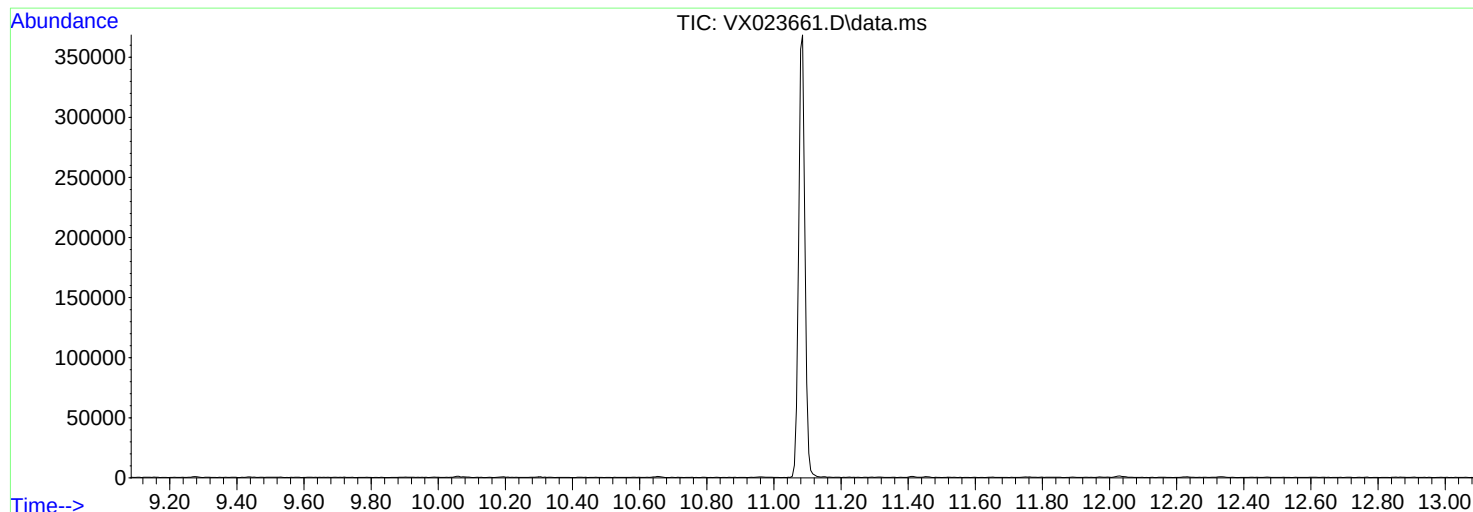

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12109	PASS
75	95	30	80	53.0	32427	PASS
95	95	100	100	100.0	61133	PASS
96	95	5	9	6.8	4155	PASS
173	174	0.00	2	1.0	540	PASS
174	95	50	120	85.7	52371	PASS
175	174	5	9	7.4	3901	PASS
176	174	95	101	96.7	50643	PASS
177	176	5	9	6.1	3098	PASS

Scan 1633 (11.043 min): VX023661.D\data.ms
BFB603

m/z	Abundance
40.00	315.0
44.10	271.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.00	692.0
37.00	4340.0
38.00	3529.0
39.10	1629.0
40.00	200.0
43.90	604.0
45.00	701.0
45.90	178.0
47.00	768.0
47.90	547.0
49.00	3314.0
50.10	15589.0
51.00	4684.0
52.00	216.0
55.10	245.0
56.10	1431.0
57.00	2157.0
58.10	132.0
60.00	849.0
61.00	4072.0
62.10	3919.0
63.00	2997.0
64.10	337.0
64.90	252.0
66.90	334.0
68.00	8153.0
69.00	7531.0
70.10	701.0
72.00	447.0
73.00	3623.0
74.00	13621.0
75.00	39104.0
76.10	3146.0
76.90	252.0
78.00	214.0
78.90	3030.0
80.00	823.0
80.90	3439.0
81.90	862.0
82.90	81.0
86.00	98.0
87.00	2576.0
88.00	2665.0
90.90	418.0
92.00	2353.0
93.00	3771.0
94.00	9546.0
95.00	70376.0
96.10	5119.0
97.10	127.0
103.80	370.0
104.80	112.0
105.90	432.0
107.20	60.0
110.80	100.0
112.90	139.0
115.00	76.0
115.90	319.0
116.90	510.0
117.80	383.0
118.80	470.0
127.80	192.0
128.90	190.0
129.80	306.0
131.00	153.0
134.90	180.0
136.80	162.0
141.00	904.0
142.10	135.0
142.90	966.0
144.00	54.0
145.00	117.0
146.00	83.0
148.00	180.0
151.90	127.0
155.20	176.0
157.10	120.0
159.00	70.0
172.00	502.0
173.00	646.0
174.00	53816.0
175.00	3780.0
176.00	51728.0
177.00	3349.0
178.10	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.00	771.0
37.00	3956.0
38.00	3741.0
39.10	1110.0
40.10	276.0
44.00	656.0
45.10	719.0
47.00	536.0
48.00	604.0
49.00	3072.0
50.00	13624.0
51.10	4071.0
52.00	153.0
54.90	238.0
56.00	1224.0
57.00	2195.0
58.00	129.0
60.00	786.0
61.00	3456.0
62.00	3568.0
63.00	2569.0
64.00	394.0
65.00	291.0
67.10	205.0
68.00	7934.0
69.00	7536.0
70.00	484.0
72.00	482.0
73.10	3150.0
74.00	13348.0
75.00	37616.0
76.10	3377.0
77.10	448.0
77.70	204.0
78.10	177.0
78.90	2929.0
80.00	902.0
80.90	3020.0
82.00	760.0
82.90	51.0
86.10	137.0
87.00	2656.0
87.90	3385.0
90.90	395.0
92.00	2548.0
93.00	3674.0
94.00	9207.0
95.00	72496.0
96.00	4795.0
97.20	228.0
104.00	474.0
104.80	166.0
105.90	518.0
106.70	64.0
110.80	126.0
111.30	65.0
112.10	53.0
112.80	105.0
115.00	95.0
115.90	411.0
116.90	579.0
118.00	393.0
118.90	379.0
128.00	239.0
128.70	125.0
129.90	310.0
131.00	72.0
135.00	185.0
136.80	151.0
140.90	867.0
142.00	94.0
142.90	950.0
144.00	90.0
145.00	164.0
145.90	50.0
147.90	257.0
153.80	60.0
154.90	163.0
156.80	138.0
160.80	137.0
172.10	429.0
172.90	671.0
174.00	61000.0
175.00	5098.0
176.00	59880.0
177.00	3605.0
178.10	102.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	524.0
37.10	2072.0
38.00	1598.0
39.00	922.0
39.90	141.0
44.00	429.0
45.00	269.0
46.90	407.0
48.10	216.0
49.00	1580.0
50.00	7113.0
51.10	2266.0
51.90	138.0
55.00	270.0
56.00	626.0
57.10	1143.0
60.00	442.0
61.00	2308.0
62.10	1758.0
63.00	1668.0
63.90	143.0
64.90	195.0
65.80	51.0
66.80	90.0
68.00	4542.0
69.00	4394.0
70.00	261.0
72.00	253.0
73.00	1987.0
74.00	7348.0
75.00	20560.0
76.00	1950.0
77.10	201.0
78.10	158.0
78.90	1666.0
79.90	460.0
80.90	1975.0
82.10	355.0
85.80	67.0
87.00	1499.0
88.00	1515.0
90.80	202.0
92.00	1412.0
93.00	1882.0
94.10	5425.0
95.00	40528.0
96.00	2550.0
96.90	158.0
103.90	154.0
104.70	121.0
105.90	207.0
110.80	68.0
112.90	58.0
114.90	54.0
115.80	180.0
116.90	280.0
117.80	213.0
119.10	286.0
127.90	237.0
128.70	137.0
129.80	232.0
134.80	148.0
136.90	96.0
141.00	608.0
141.70	78.0
142.10	108.0
142.90	696.0
144.90	99.0
145.80	103.0
147.80	170.0
153.80	76.0
155.00	95.0
160.80	77.0
172.00	551.0
173.00	304.0
174.00	42296.0
175.00	2826.0
176.00	40320.0
177.00	2340.0
178.10	93.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603