

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030591.D
 Acq On : 12 Aug 2022 14:00
 Operator : JC/MD
 Sample : N4144-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Aug 12 23:30:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 12 23:28:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	266254	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	242147	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	103595	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	72357	42.318	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.640%		
7) Chloroethane-d5	1.672	69	62116	51.534	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	103.060%		
11) 1,1-Dichloroethene-d2	2.307	63	114704	35.465	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.920%		
21) 2-Butanone-d5	4.471	46	201457	127.162	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	127.160%		
24) Chloroform-d	5.068	84	187477	53.264	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.520%		
26) 1,2-Dichloroethane-d4	5.964	65	137925	57.711	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	115.420%		
32) Benzene-d6	5.977	84	356362	51.377	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.760%		
36) 1,2-Dichloropropane-d6	7.312	67	121362	53.929	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	107.860%		
41) Toluene-d8	8.653	98	311421	47.631	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.260%		
43) trans-1,3-Dichloroprop...	8.952	79	54029	48.260	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.520%		
47) 2-Hexanone-d5	9.384	63	132789	115.763	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	115.760%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	167895	56.792	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	113.580%		
66) 1,2-Dichlorobenzene-d4	12.323	152	105849	52.679	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.360%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.958	75	2779	0.922	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030591.D
Acq On : 12 Aug 2022 14:00
Operator : JC/MD
Sample : N4144-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Aug 12 23:30:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 23:28:07 2022
Response via : Initial Calibration

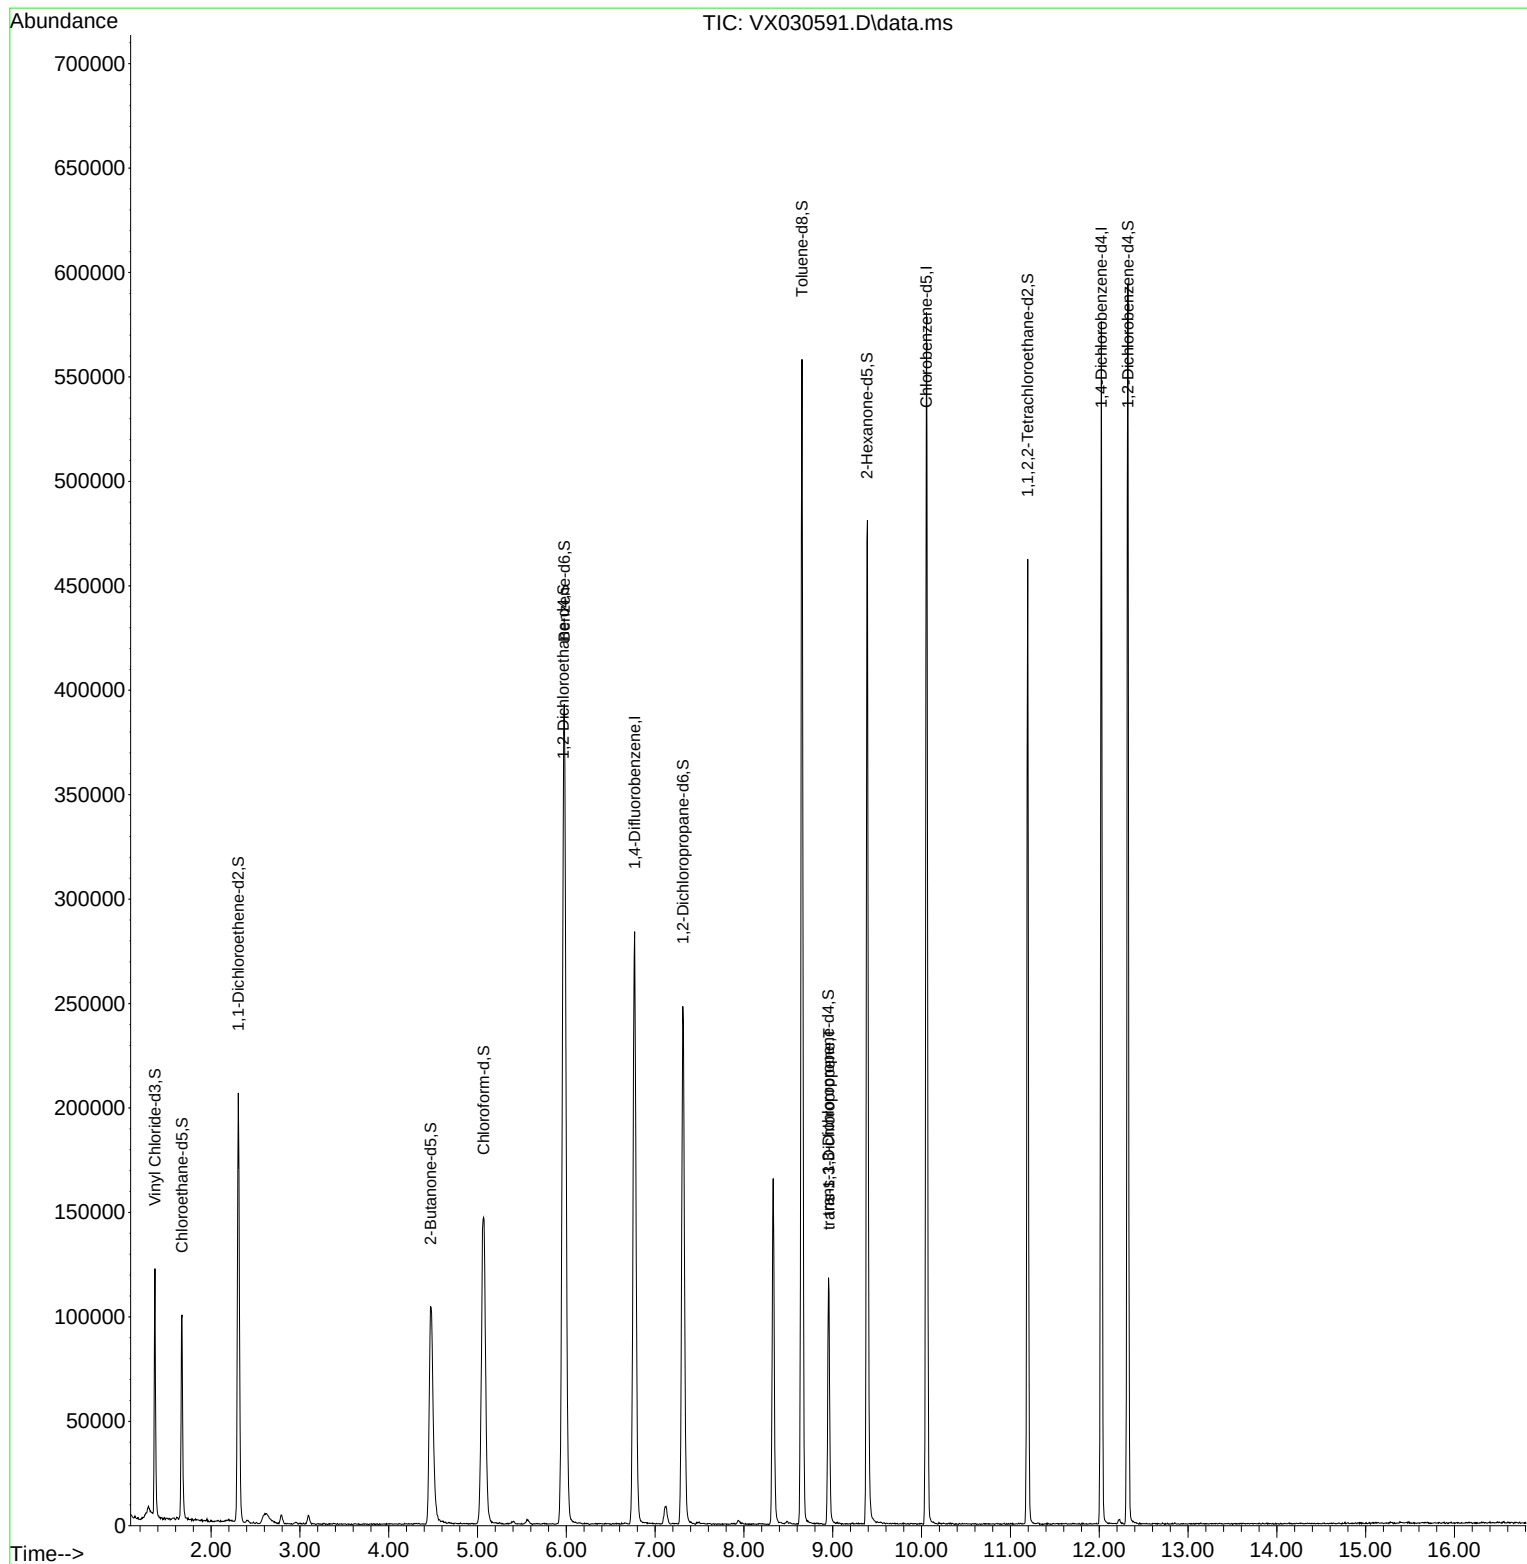

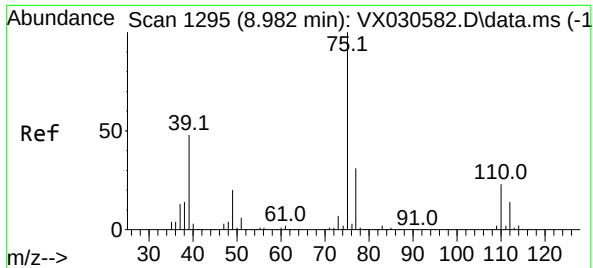

#44

trans-1,3-Dichloropropene

Concen: 0.922 ug/L

RT: 8.958 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX030591.D


Acq: 12 Aug 2022 14:00

Instrument :

MSVOA_X

ClientSampleId :

VHBLK001

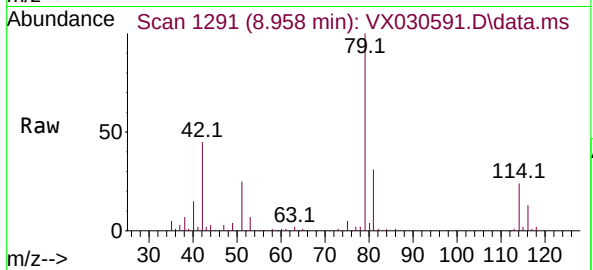

Tgt Ion: 75 Resp: 2779

Ion Ratio Lower Upper

75 100

77 38.5 22.5 41.7

