
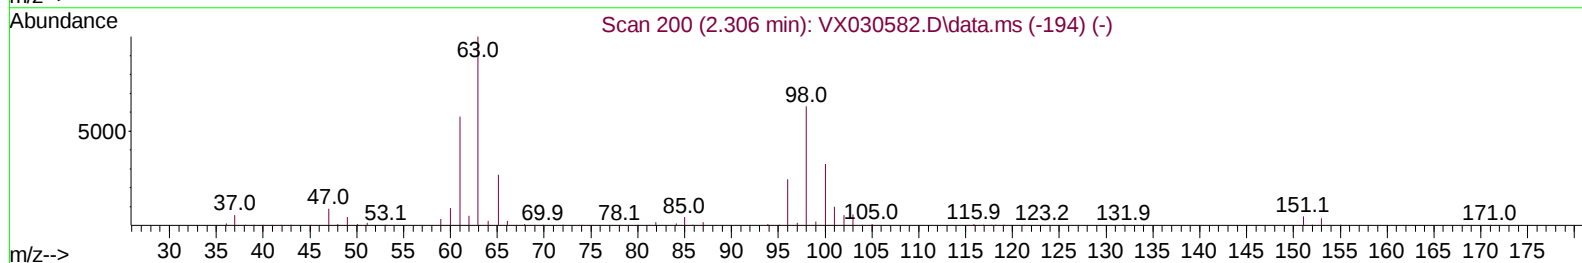
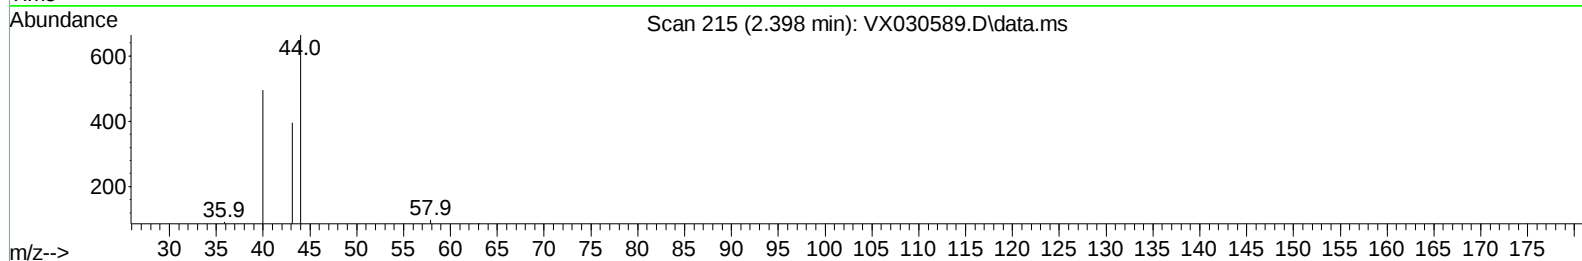


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 12 23:30:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 23:28:07 2022
Response via : Initial Calibration

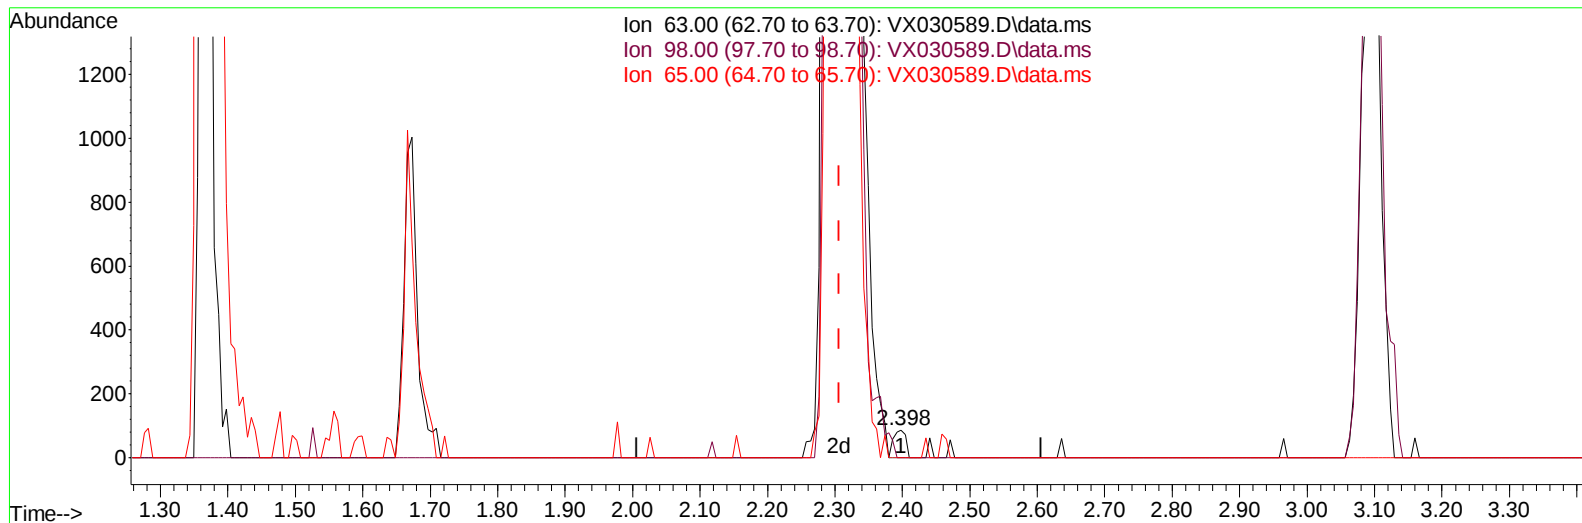

TIC: VX030589.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)




2.398min (+ 0.092) 0.03 ug/L

response 107

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.90	87.85
65.00	23.60	23.36
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 12 23:30:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 23:28:07 2022
Response via : Initial Calibration

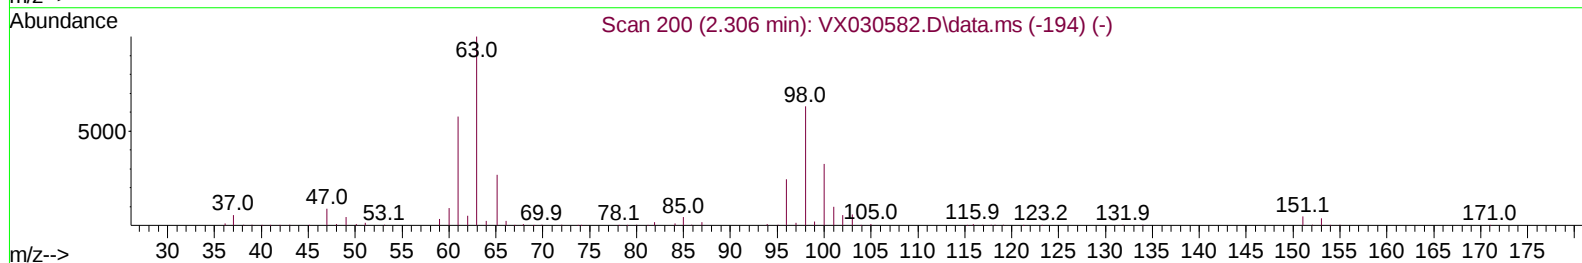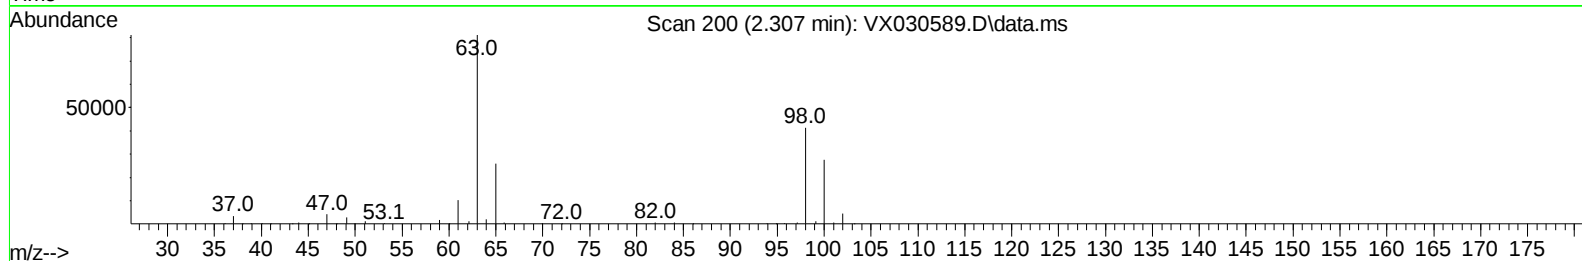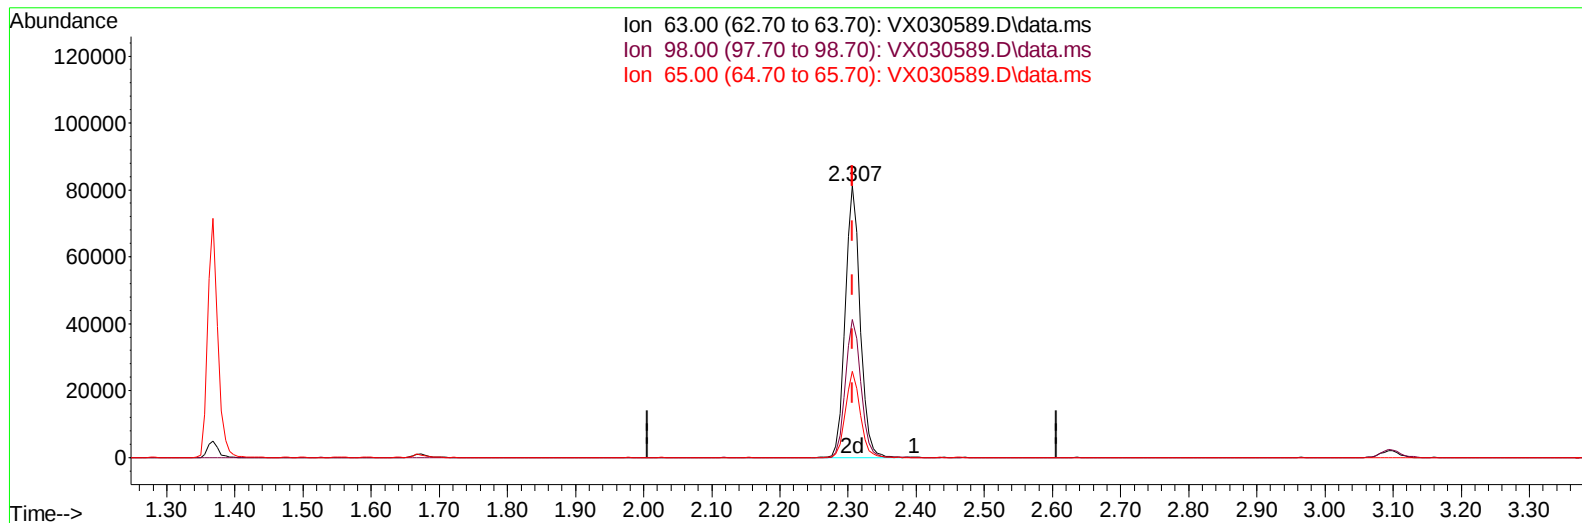

TIC: VX030589.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.307min (+ 0.000) 38.70 ug/L m

response 122788

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.90	0.08#
65.00	23.60	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030589.D
 Acq On : 12 Aug 2022 13:13
 Operator : JC/MD
 Sample : VIBLK672
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 12 23:30:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 12 23:28:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	261221	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	235465	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	104699	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	73070	43.558	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.120%		
7) Chloroethane-d5	1.673	69	64220	54.306	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	108.620%		
11) 1,1-Dichloroethene-d2	2.307	63	122788m	38.695	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.400%		
21) 2-Butanone-d5	4.477	46	204663	131.675	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	131.680%#		
24) Chloroform-d	5.062	84	192998	55.889	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	111.780%		
26) 1,2-Dichloroethane-d4	5.964	65	143371	61.146	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	122.300%		
32) Benzene-d6	5.983	84	365099	54.130	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.260%		
36) 1,2-Dichloropropane-d6	7.312	67	127349	58.195	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	116.400%		
41) Toluene-d8	8.653	98	321140	50.512	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.020%		
43) trans-1,3-Dichloroprop...	8.952	79	58525	53.759	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	107.520%		
47) 2-Hexanone-d5	9.391	63	134524	120.603	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	120.600%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	176215	61.298	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	122.600%#		
66) 1,2-Dichlorobenzene-d4	12.323	152	118101	58.156	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	116.320%		
Target Compounds						
17) trans-1,2-Dichloroethene	3.099	96	7270	4.292	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030589.D
Acq On : 12 Aug 2022 13:13
Operator : JC/MD
Sample : VIBLK672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 12 23:30:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 23:28:07 2022
Response via : Initial Calibration

