

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030584.D
 Acq On : 12 Aug 2022 10:55
 Operator : JC/MD
 Sample : N4114-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB	113946	120029	11.47%	1.513%
2	1.666	91	95	104	rBV	88609	113804	10.88%	1.435%
3	2.306	194	200	210	rVB	194985	297631	28.45%	3.753%
4	2.507	231	233	238	rBV	646	955	0.09%	0.012%
5	2.623	250	252	253	rBV	393	380	0.04%	0.005%
6	2.666	257	259	260	rBV2	445	427	0.04%	0.005%
7	2.745	270	272	274	rBV	470	453	0.04%	0.006%
8	2.788	274	279	286	rVB4	2695	4720	0.45%	0.060%
9	2.855	286	290	292	rBV2	472	696	0.07%	0.009%
10	2.940	299	304	314	rVB2	4538	11499	1.10%	0.145%
11	3.044	317	321	325	rBV3	473	699	0.07%	0.009%
12	3.178	341	343	346	rBV	567	446	0.04%	0.006%
13	3.343	368	370	373	rBV2	281	340	0.03%	0.004%
14	3.477	387	392	393	rBV	545	655	0.06%	0.008%
15	3.519	397	399	400	rBV	606	367	0.04%	0.005%
16	3.562	404	406	407	rBV2	505	435	0.04%	0.005%
17	3.599	409	412	415	rBV2	397	441	0.04%	0.006%
18	3.702	427	429	434	rBV2	269	357	0.03%	0.005%
19	3.824	446	449	450	rBV2	322	362	0.03%	0.005%
20	3.916	460	464	465	rVV2	241	350	0.03%	0.004%
21	4.093	491	493	496	rVV	385	399	0.04%	0.005%
22	4.190	507	509	510	rBV	521	380	0.04%	0.005%
23	4.282	521	524	528	rVB2	484	679	0.06%	0.009%
24	4.373	537	539	542	rBV	449	634	0.06%	0.008%
25	4.471	546	555	570	rBV	97616	289845	27.70%	3.654%
26	4.763	602	603	605	rVB	674	339	0.03%	0.004%
27	4.794	607	608	611	rBV2	774	504	0.05%	0.006%
28	5.062	638	652	671	rVV2	136264	435429	41.62%	5.490%
29	5.214	675	677	681	rBV2	426	356	0.03%	0.004%
30	5.300	689	691	692	rBV2	517	325	0.03%	0.004%
31	5.391	701	706	710	rVV4	753	1630	0.16%	0.021%
32	5.550	727	732	733	rBV	1123	1461	0.14%	0.018%
33	5.635	744	746	749	rBB	355	328	0.03%	0.004%
34	5.848	778	781	783	rBV3	471	574	0.05%	0.007%
35	5.970	789	801	814	rBV2	358087	1046281	100.00%	13.192%
36	6.348	861	863	866	rVB2	407	448	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030584.D
 Acq On : 12 Aug 2022 10:55
 Operator : JC/MD
 Sample : N4114-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	6.763	920	931	944	rBV	263350	611705	58.46%	7.712%
38	6.915	955	956	961	rVB3	810	931	0.09%	0.012%
39	7.055	976	979	980	rBV2	550	500	0.05%	0.006%
40	7.110	981	988	995	rVV3	8708	19218	1.84%	0.242%
41	7.311	1010	1021	1035	rBV	219068	490743	46.90%	6.187%
42	7.628	1070	1073	1076	rBV2	375	515	0.05%	0.006%
43	7.848	1105	1109	1111	rBV	627	576	0.06%	0.007%
44	7.903	1114	1118	1119	rBV	646	572	0.05%	0.007%
45	7.939	1120	1124	1132	rVV4	1251	2455	0.23%	0.031%
46	8.043	1136	1141	1143	rBV2	423	616	0.06%	0.008%
47	8.128	1154	1155	1158	rBV2	659	735	0.07%	0.009%
48	8.183	1162	1164	1165	rVV	330	310	0.03%	0.004%
49	8.214	1167	1169	1173	rBV	552	689	0.07%	0.009%
50	8.330	1181	1188	1198	rBV	145182	248055	23.71%	3.128%
51	8.452	1205	1208	1209	rBV2	897	767	0.07%	0.010%
52	8.653	1233	1241	1250	rBV	510103	792174	75.71%	9.988%
53	8.884	1277	1279	1282	rVB2	451	375	0.04%	0.005%
54	8.951	1284	1290	1304	rVV	110907	168367	16.09%	2.123%
55	9.140	1319	1321	1323	rBV	324	309	0.03%	0.004%
56	9.384	1356	1361	1375	rBV	432951	629866	60.20%	7.941%
57	9.701	1409	1413	1420	rBV4	4876	7160	0.68%	0.090%
58	9.781	1424	1426	1428	rVB2	628	464	0.04%	0.006%
59	9.805	1428	1430	1431	rBV2	463	486	0.05%	0.006%
60	10.055	1465	1471	1479	rBV	539273	707503	67.62%	8.920%
61	10.427	1530	1532	1535	rBV2	366	451	0.04%	0.006%
62	10.457	1535	1537	1539	rBV	413	327	0.03%	0.004%
63	10.738	1581	1583	1586	rBV2	534	688	0.07%	0.009%
64	10.884	1605	1607	1610	rBV2	423	372	0.04%	0.005%
65	11.012	1624	1628	1630	rBV2	331	469	0.04%	0.006%
66	11.195	1652	1658	1668	rBV	406900	529889	50.64%	6.681%
67	11.634	1728	1730	1732	rVB	672	474	0.05%	0.006%
68	11.658	1732	1734	1737	rVB2	362	390	0.04%	0.005%
69	11.695	1737	1740	1741	rBV	302	310	0.03%	0.004%
70	11.768	1751	1752	1754	rVB	662	415	0.04%	0.005%
71	11.792	1754	1756	1759	rBV2	281	403	0.04%	0.005%
72	11.841	1762	1764	1766	rBV2	613	349	0.03%	0.004%
73	11.926	1776	1778	1779	rVB	664	360	0.03%	0.005%
74	11.945	1779	1781	1784	rBV	298	397	0.04%	0.005%
75	11.975	1784	1786	1787	rBV	501	337	0.03%	0.004%
76	12.024	1788	1794	1800	rBV	537890	659290	63.01%	8.312%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
 Data File : VX030584.D
 Acq On : 12 Aug 2022 10:55
 Operator : JC/MD
 Sample : N4114-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.122	1808	1810	1813	rVB2	450	432	0.04%	0.005%
78	12.176	1818	1819	1822	rVB	500	315	0.03%	0.004%
79	12.225	1823	1827	1835	rBV4	1554	2795	0.27%	0.035%
80	12.323	1837	1843	1849	rBV	549779	702826	67.17%	8.861%
81	12.487	1868	1870	1874	rBV2	368	496	0.05%	0.006%
82	12.548	1878	1880	1884	rBV2	626	804	0.08%	0.010%
83	12.719	1906	1908	1909	rVV	609	329	0.03%	0.004%
84	12.762	1913	1915	1919	rVV2	472	498	0.05%	0.006%
85	12.792	1919	1920	1922	rVB	587	376	0.04%	0.005%
86	12.817	1922	1924	1925	rBV	377	325	0.03%	0.004%
87	13.006	1953	1955	1957	rBV	478	361	0.03%	0.005%
88	13.024	1957	1958	1961	rBV2	447	489	0.05%	0.006%
89	13.103	1968	1971	1972	rBV2	593	674	0.06%	0.008%
90	13.225	1989	1991	1994	rBV2	501	463	0.04%	0.006%
91	13.316	2004	2006	2007	rBV	704	494	0.05%	0.006%
92	13.377	2014	2016	2019	rBV	347	384	0.04%	0.005%
93	13.573	2045	2048	2049	rBV2	456	530	0.05%	0.007%
94	13.883	2097	2099	2101	rBV2	400	326	0.03%	0.004%
95	14.048	2122	2126	2127	rVB	709	572	0.05%	0.007%
96	14.304	2165	2168	2171	rBV3	642	881	0.08%	0.011%
97	14.664	2225	2227	2228	rBV	669	615	0.06%	0.008%
98	14.877	2260	2262	2263	rBV2	465	317	0.03%	0.004%
99	15.377	2342	2344	2347	rBV2	729	777	0.07%	0.010%
100	16.322	2497	2499	2500	rBV	723	644	0.06%	0.008%


Sum of corrected areas: 7931393

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030584.D
Acq On : 12 Aug 2022 10:55
Operator : JC/MD
Sample : N4114-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

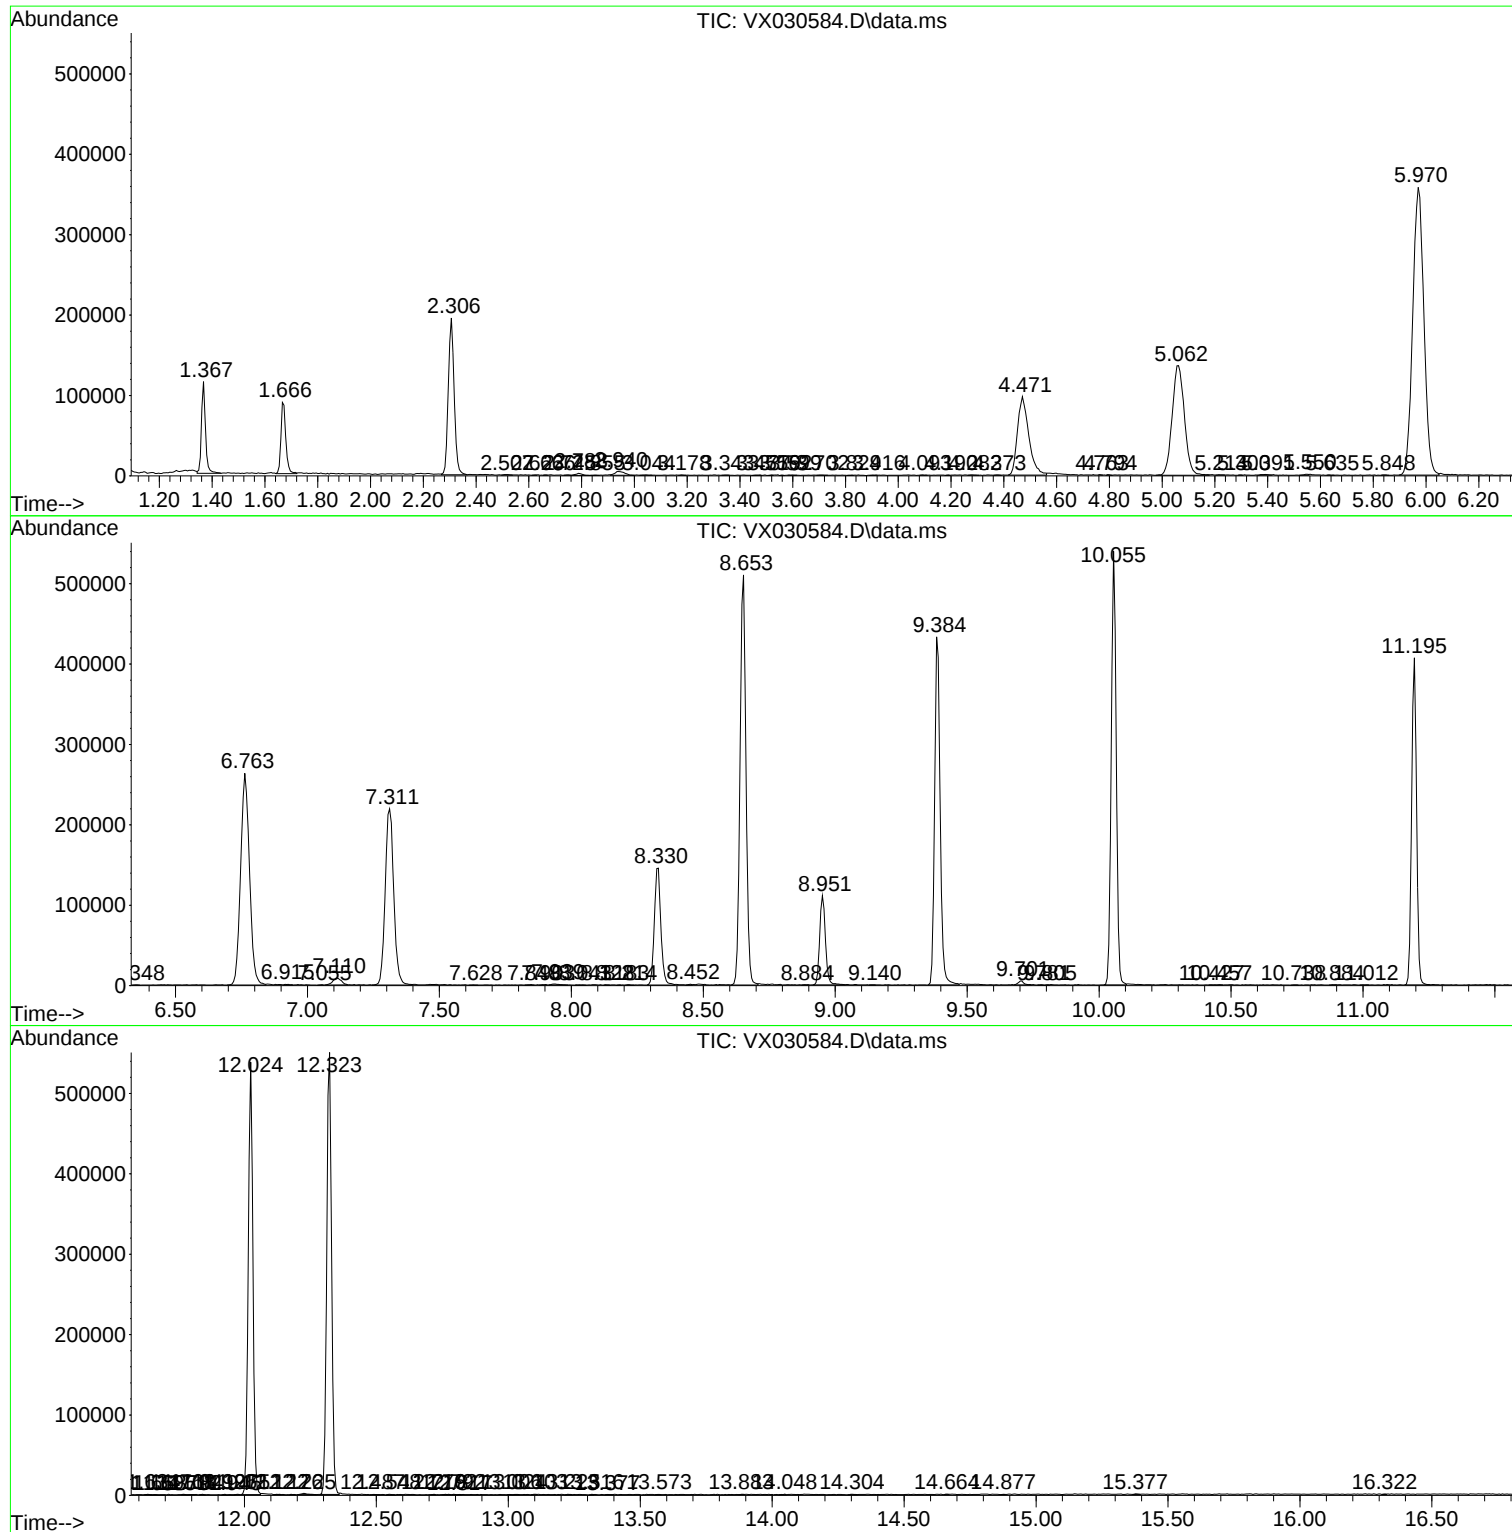

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030584.D
Acq On : 12 Aug 2022 10:55
Operator : JC/MD
Sample : N4114-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081222\
Data File : VX030584.D
Acq On : 12 Aug 2022 10:55
Operator : JC/MD
Sample : N4114-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc